

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
 Data File : BM010737.D
 Acq On : 24 Jun 2017 19:27
 Operator : SJ/JU
 Sample : I3653-09DL 2X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Quant Time: Jun 26 04:56:40 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 26 04:54:47 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 F5C52DL

Manual Integrations
 APPROVED

mohammad
 6/28/2017 7:43:04 AM

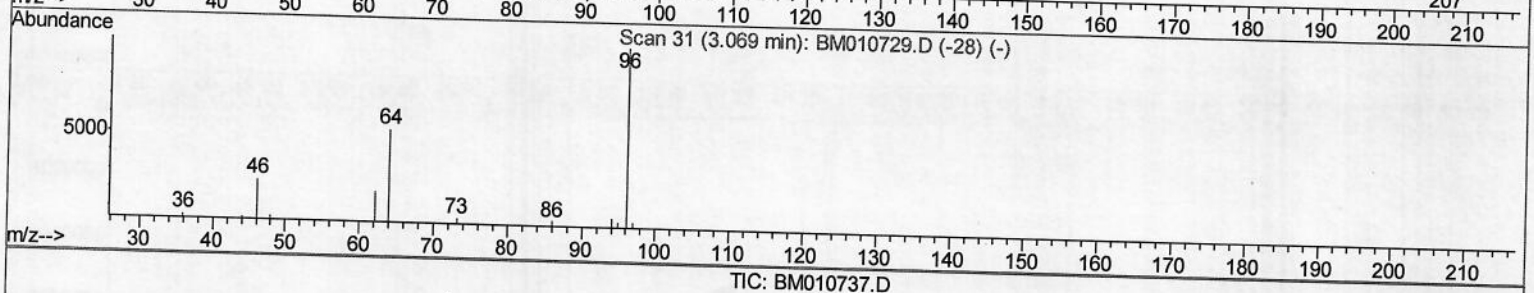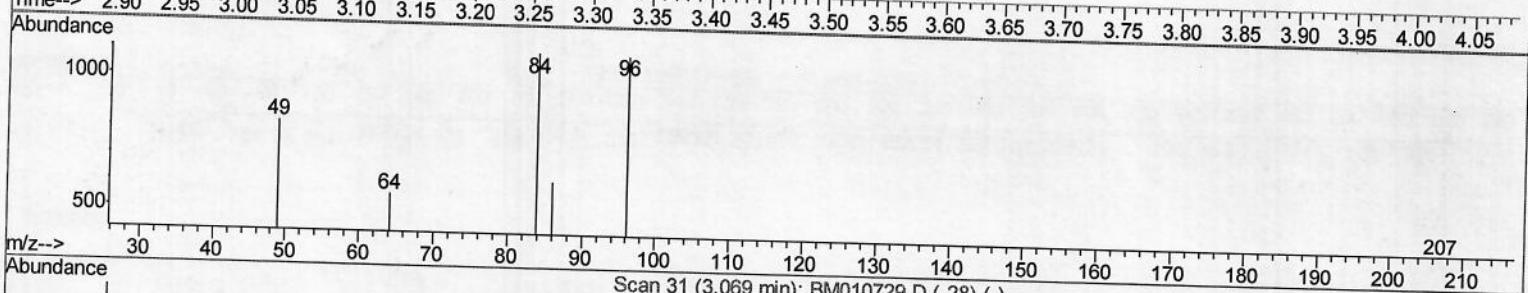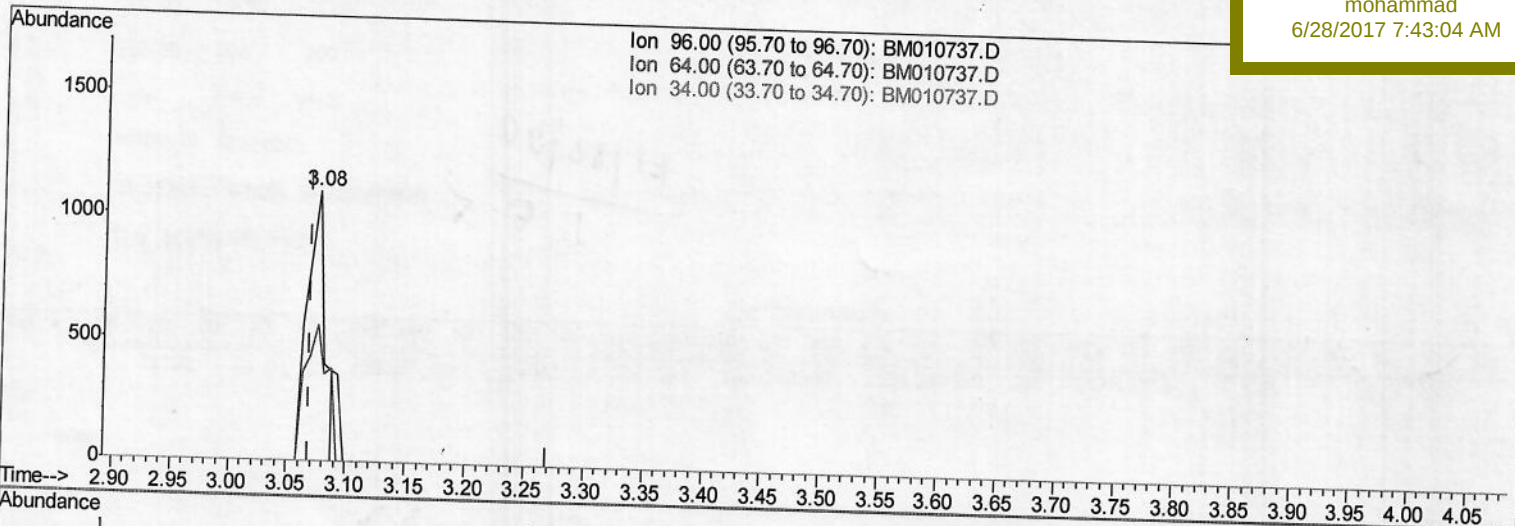

TIC: BM010737.D

(3) 1,4-Dioxane-d8 (S)

3.075min (+0.006) 1.13ng/uL

response 1154

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	64.47
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
 Data File : BM010737.D
 Acq On : 24 Jun 2017 19:27
 Operator : SJ/JU
 Sample : I3653-09DL 2X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Quant Time: Jun 26 04:56:40 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 26 04:54:47 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 Client Sampled :
 F5C52DL

Manual Integrations
 APPROVED

mohammad
 6/28/2017 7:43:04 AM

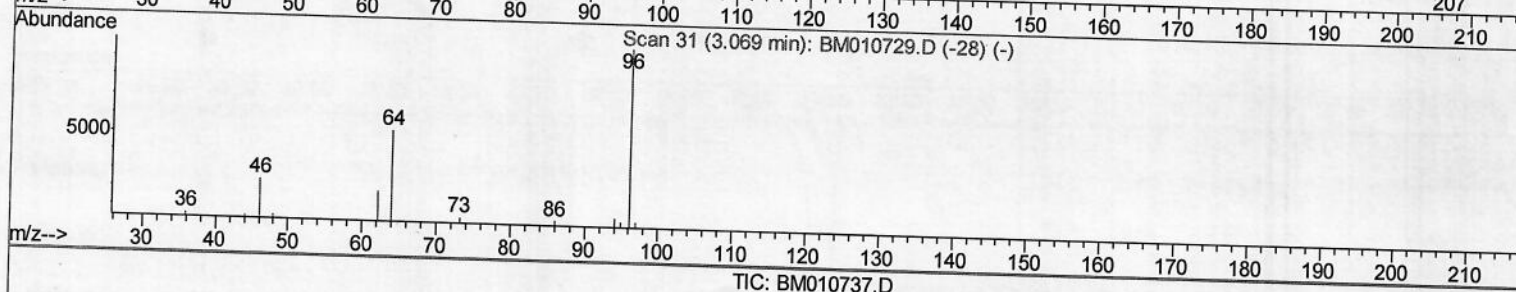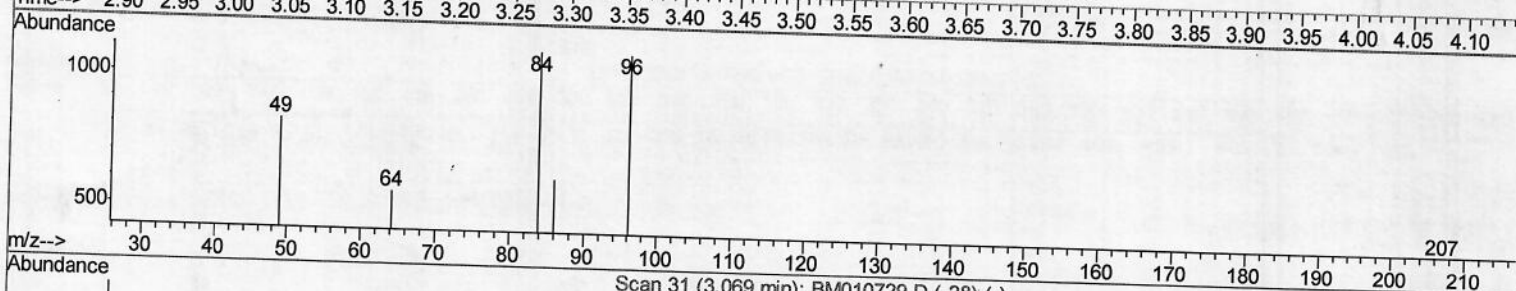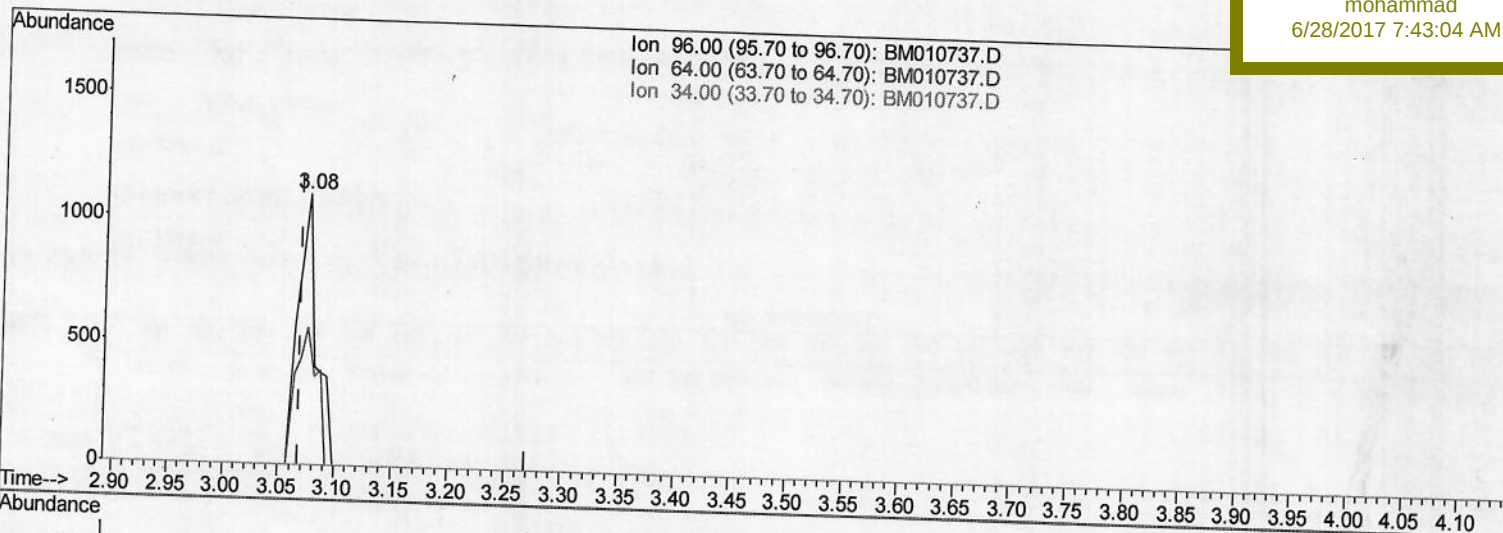

TIC: BM010737.D

(3) 1,4-Dioxane-d8 (S)

3.075min (+0.006) 1.25ng/uL m

response 1280

Ion	Exp%	Act%
96.00	100	100
64.00	74.90	58.13#
34.00	0.00	0.00
0.00	0.00	0.00

> S.J
 06/29/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
 Data File : BM010737.D
 Acq On : 24 Jun 2017 19:27
 Operator : SJ/JU
 Sample : I3653-09DL 2X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Quant Time: Jun 26 04:56:40 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 26 04:54:47 2017
 Response via : Initial Calibration

Instrument :
 BNA_M
 ClientSampleId :
 F5C52DL

Manual Integrations
 APPROVED

mohammad
 6/28/2017 7:43:04 AM

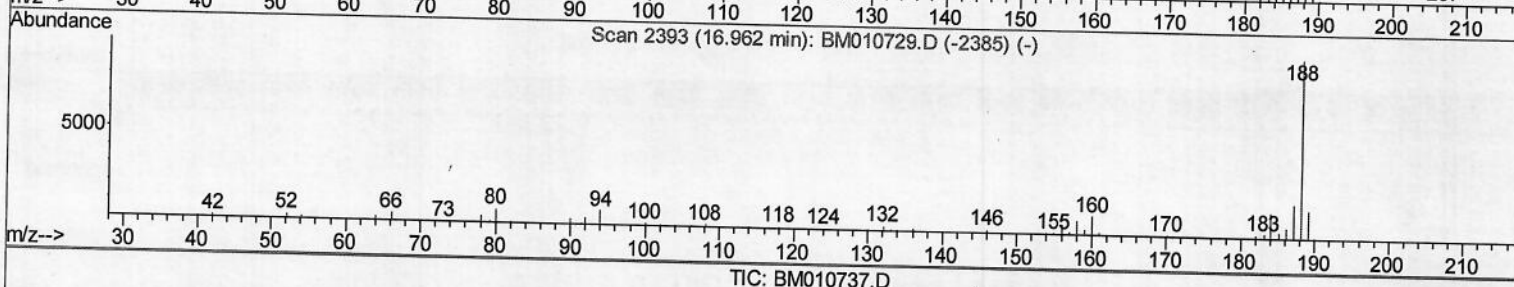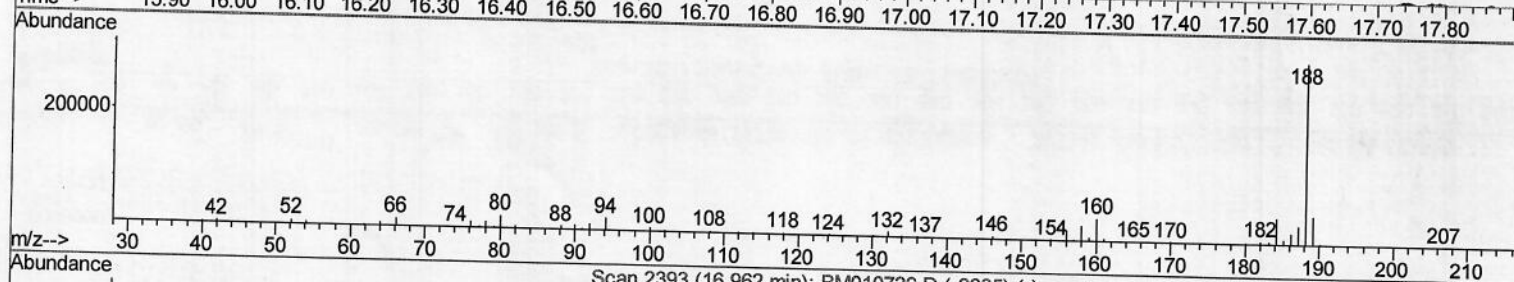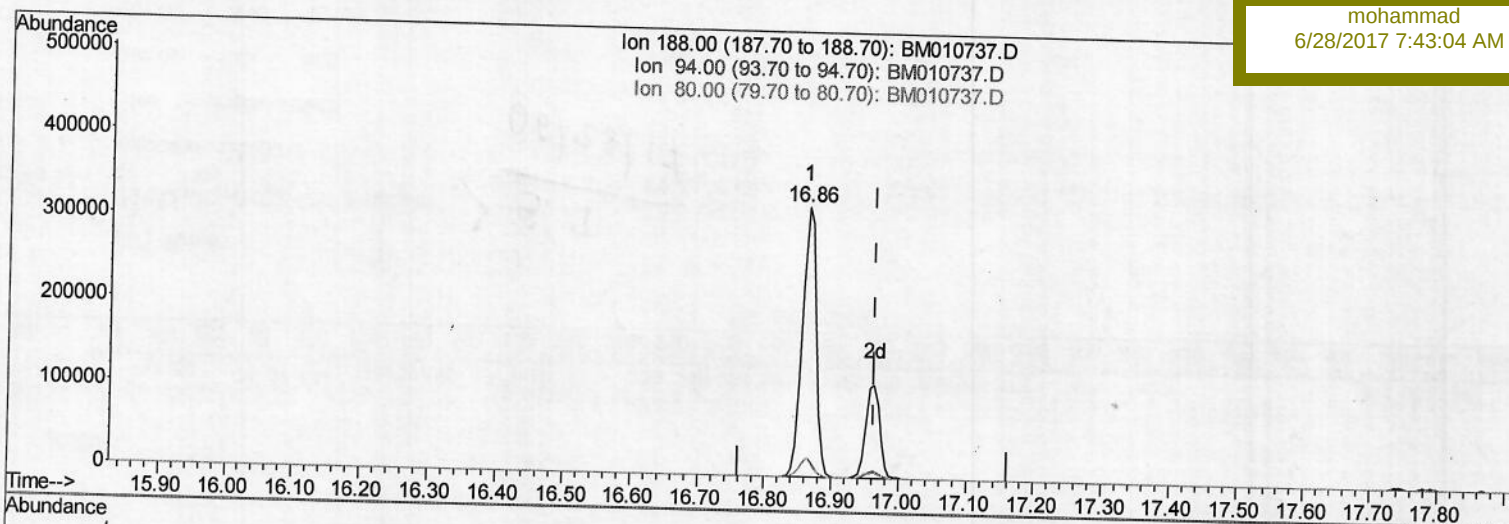

(70) Anthracene-d10 (S)
 16.863min (-0.100) 20.71ng/ul
 response 461177

Ion	Exp%	Act%
188.00	100	100
94.00	5.70	6.70
80.00	5.90	6.94
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
 Data File : BM010737.D
 Acq On : 24 Jun 2017 19:27
 Operator : SJ/JU
 Sample : I3653-09DL 2X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5C52DL

Quant Time: Jun 26 04:56:40 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 26 04:54:47 2017
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 6/28/2017 7:43:04 AM

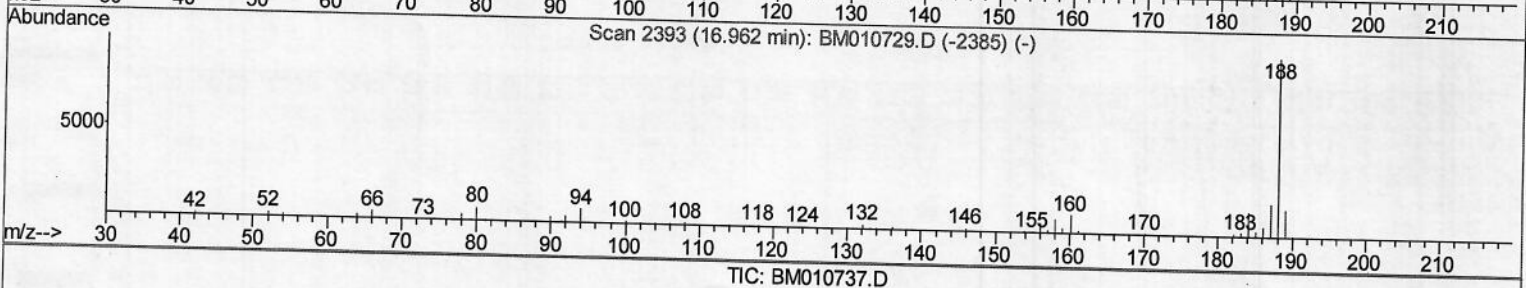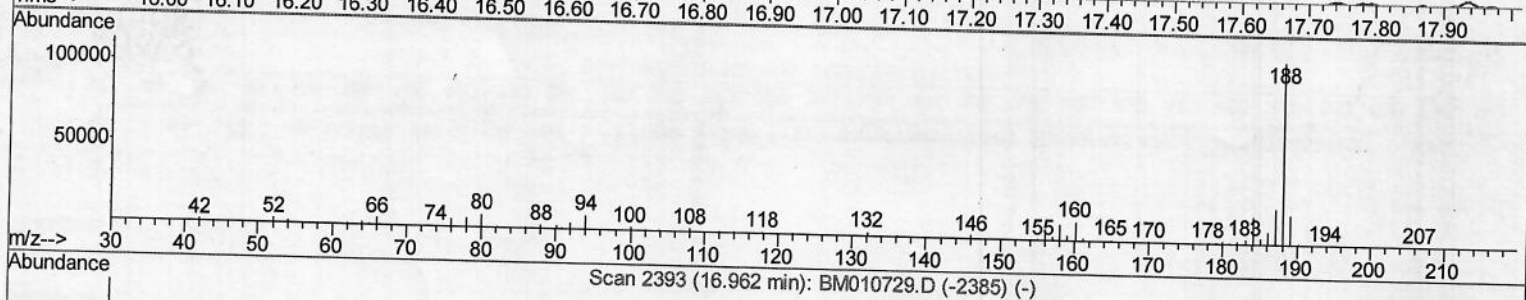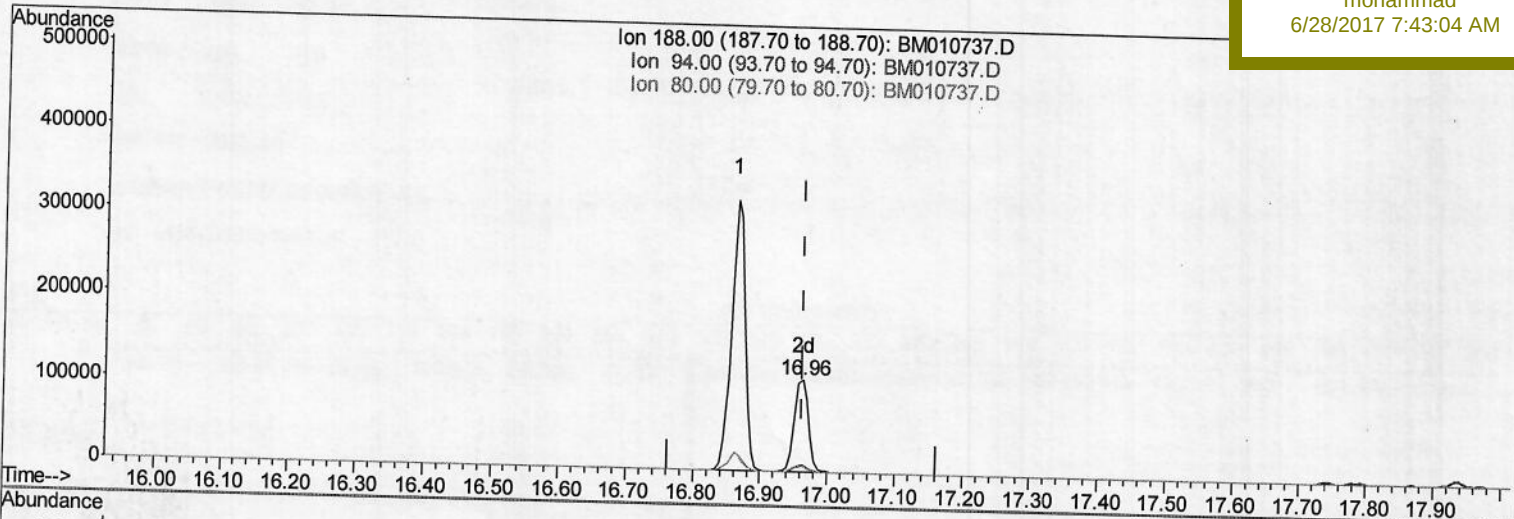

(70) Anthracene-d10 (S)

16.963min (+0.000) 7.27ng/ul m

response 161999

Ion	Exp%	Act%
188.00	100	100
94.00	5.70	7.83#
80.00	5.90	7.20#
0.00	0.00	0.00

Handwritten signature and date:
 > S.J
 06/29/17

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
 Data File : BM010737.D
 Acq On : 24 Jun 2017 19:27
 Operator : SJ/JU
 Sample : I3653-09DL 2X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
ClientSampleId :
 F5C52DL

Quant Time: Jun 26 04:56:40 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 26 04:54:47 2017
 Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
 6/28/2017 7:43:04 AM

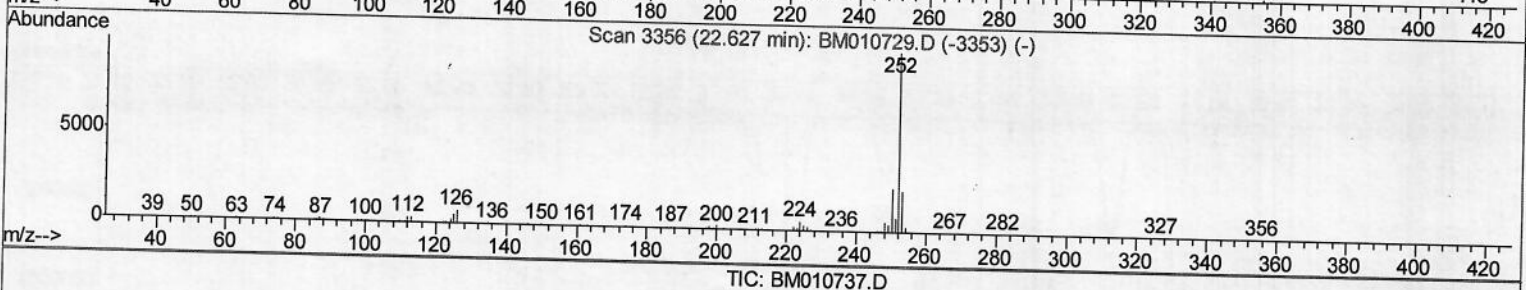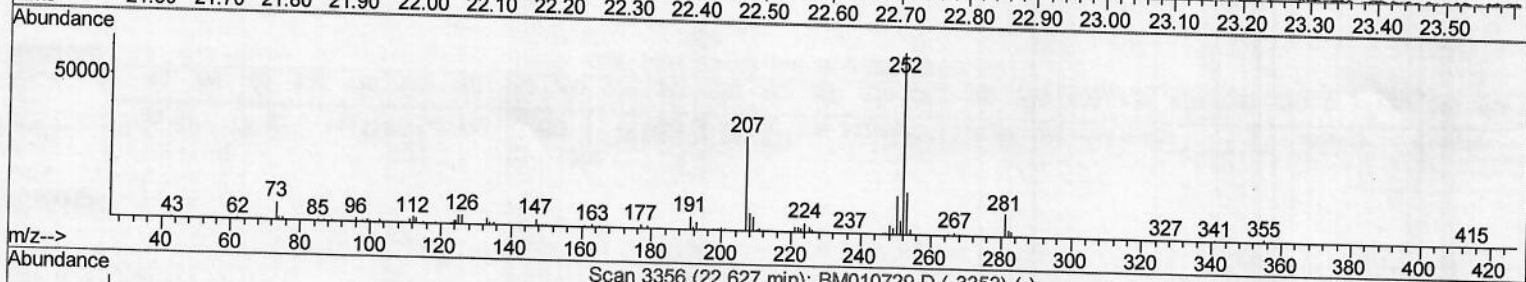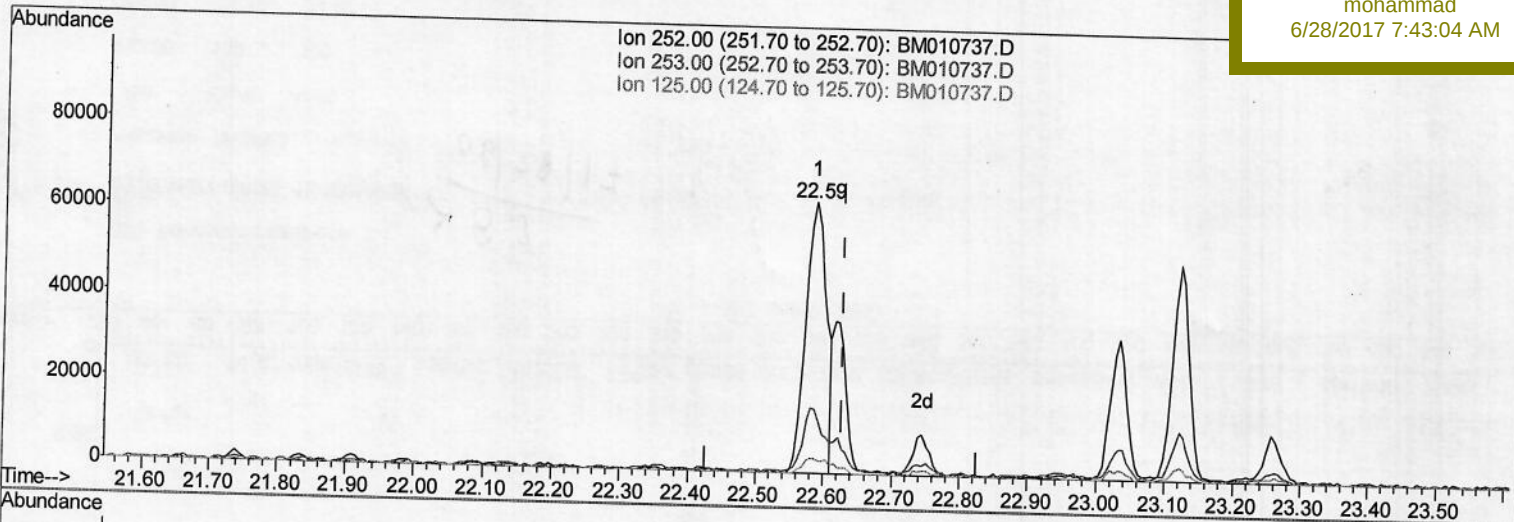

TIC: BM010737.D

(86) Benzo(k)fluoranthene
 22.586min (-0.041) 5.19ng/ul
 response 136229

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	23.78
125.00	4.30	5.31#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
 Data File : BM010737.D
 Acq On : 24 Jun 2017 19:27
 Operator : SJ/JU
 Sample : I3653-09DL 2X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :

BNA_M

Client Sampled :

F5C52DL

Manual Integrations

APPROVED

mohammad

6/28/2017 7:43:04 AM




Quant Time: Jun 26 04:56:40 2017

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M

Quant Title : SVOA CALIBRATION

QLast Update : Mon Jun 26 04:54:47 2017

Response via : Initial Calibration

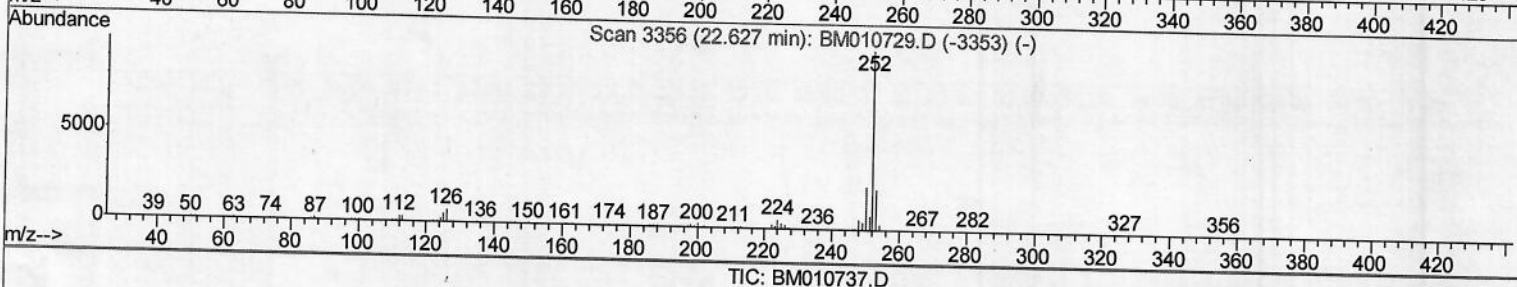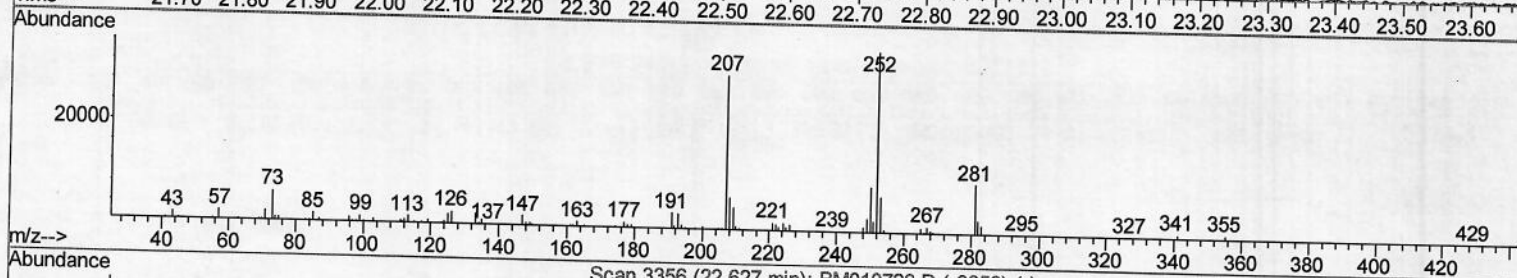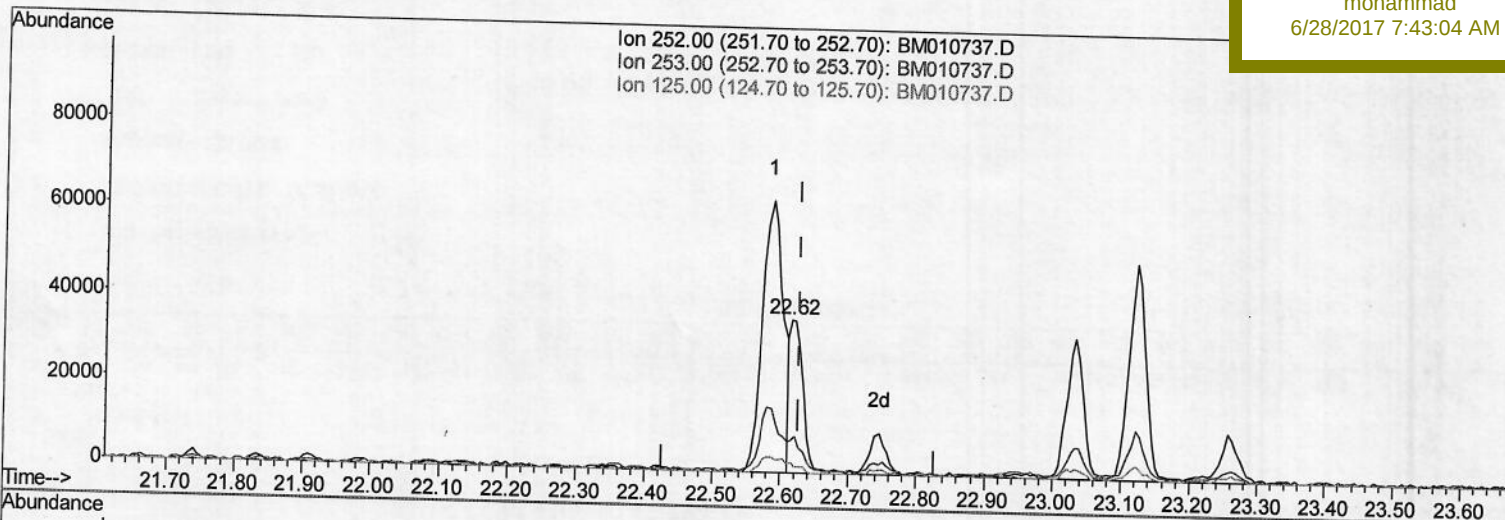

(86) Benzo(k)fluoranthene

22.615min (-0.012) 1.85ng/ul m

response 48591

Ion Exp% Act%

252.00 100 100

253.00 21.40 20.60

125.00 4.30 6.08#

0.00 0.00 0.00

> 5.9
06/29/17

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
 Data File : BM010737.D
 Acq On : 24 Jun 2017 19:27
 Operator : SJ/JU
 Sample : I3653-09DL 2X
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F5C52DL

Manual Integrations
 APPROVED

mohammad
 6/28/2017 7:43:04 AM

Quant Time: Jun 26 08:06:37 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 26 04:54:47 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	58467	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	268107	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.11	164	186588	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.86	188	461177	20.00	ng/ul	0.00
75) Chrysene-d12	21.08	240	560445	20.00	ng/ul	0.00
83) Perylene-d12	23.22	264	426546	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.08	96	1280m	1.25	ng/uL	0.00
5) Phenol-d5	6.65	99	31115	5.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.81	67	18350	5.77	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	24575	6.29	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	27313	5.91	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	13336	6.97	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	15339	6.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	29689	6.40	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	15412	3.15	ng/ul	0.00
43) Dimethylphthalate-d6	13.53	166	119464	7.29	ng/ul	0.00
46) Acenaphthylene-d8	13.80	160	130143	6.83	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	14019	4.86	ng/ul	-0.01
57) Fluorene-d10	15.11	176	100750	7.12	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.23	200	16822	5.94	ng/ul	0.00
70) Anthracene-d10	16.96	188	161999m	7.27	ng/ul	0.00
76) Pyrene-d10	19.27	212	212525	8.16	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.08	264	157358	7.63	ng/ul	0.00

Target Compounds

					Qvalue
28) Naphthalene	10.27	128	215974	16.19	ng/ul 98
34) 2-Methylnaphthalene	11.89	142	72198	6.73	ng/ul 100
40) 1,1'-Biphenyl	12.93	154	35110	2.41	ng/ul# 90
44) Dimethylphthalate	13.58	163	27912	1.74	ng/ul 96
49) Acenaphthene	14.17	153	147614	12.06	ng/ul 97
53) Dibenzofuran	14.51	168	185601	10.01	ng/ul 89
58) Fluorene	15.16	166	151977	9.79	ng/ul 98
69) Phenanthrene	16.91	178	1000886	40.82	ng/ul 98
71) Anthracene	17.00	178	146917	5.82	ng/ul 97
72) Carbazole	17.27	167	34564	1.57	ng/ul 96
74) Fluoranthene	18.94	202	755594	23.91	ng/ul 99
77) Pyrene	19.30	202	527318	16.29	ng/ul 98
80) Benzo(a)anthracene	21.06	228	209053	6.41	ng/ul 99
82) Chrysene	21.12	228	156506	5.38	ng/ul 99
85) Benzo(b)fluoranthene	22.59	252	136229	4.92	ng/ul 97
86) Benzo(k)fluoranthene	22.62	252	48591m	1.85	ng/ul
88) Benzo(a)pyrene	23.12	252	86805	3.41	ng/ul# 99
89) Indeno(1,2,3-cd)pyrene	25.33	276	33937	1.28	ng/ul 96
91) Benzo(g,h,i)perylene	25.96	276	23017	1.09	ng/ul# 92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
Data File : BM010737.D
Acq On : 24 Jun 2017 19:27
Operator : SJ/JU
Sample : I3653-09DL 2X
Misc :
ALS Vial : 52 Sample Multiplier: 1

Quant Time: Jun 26 08:06:37 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Jun 26 04:54:47 2017
Response via : Initial Calibration

Instrument :

BNA_M

Client Sampled :

F5C52DL

Manual Integrations
APPROVEDmohammad
6/28/2017 7:43:04 AM