

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
 Data File : BM010685.D
 Acq On : 23 Jun 2017 11:04
 Operator : SJ/JU
 Sample : I3767-01DL 2X
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BDC63DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.104	34	37	43	rVB	41543	50640	3.50%	0.390%
2	6.645	633	639	646	rBV	44164	61366	4.25%	0.473%
3	6.810	661	667	675	rVB	117244	168917	11.69%	1.301%
4	6.998	691	699	705	rBB	143766	212818	14.72%	1.639%
5	7.463	771	778	786	rVB	257528	393438	27.22%	3.031%
6	8.163	892	897	904	rVB	131742	190580	13.19%	1.468%
7	8.604	966	972	979	rVB	168005	268412	18.57%	2.068%
8	9.316	1087	1093	1100	rBB	155747	246446	17.05%	1.898%
9	9.845	1176	1183	1190	rBV	240072	372819	25.79%	2.872%
10	10.222	1240	1247	1255	rVB	392473	610192	42.22%	4.700%
11	13.533	1804	1810	1817	rBV	493998	668943	46.28%	5.153%
12	13.798	1849	1855	1864	rBV	507166	703298	48.66%	5.417%
13	14.110	1902	1908	1916	rVB2	618357	937512	64.86%	7.222%
14	14.321	1939	1944	1949	rBV	48582	69139	4.78%	0.533%
15	15.110	2072	2078	2087	rVB	663469	933343	64.57%	7.189%
16	15.233	2094	2099	2105	rVB	214932	293507	20.31%	2.261%
17	16.868	2370	2377	2383	rBV2	889710	1238550	85.69%	9.540%
18	16.962	2387	2393	2400	rVB	793807	1047547	72.48%	8.069%
19	19.274	2778	2786	2793	rVB	959425	1240255	85.81%	9.554%
20	21.080	3088	3093	3099	rVB	1248343	1445390	100.00%	11.134%
21	23.086	3428	3434	3441	rBV2	489676	850115	58.82%	6.548%
22	23.221	3450	3457	3464	rVB	549864	978806	67.72%	7.540%


Sum of corrected areas: 12982033

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
Data File : BM010685.D
Acq On : 23 Jun 2017 11:04
Operator : SJ/JU
Sample : I3767-01DL 2X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC63DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

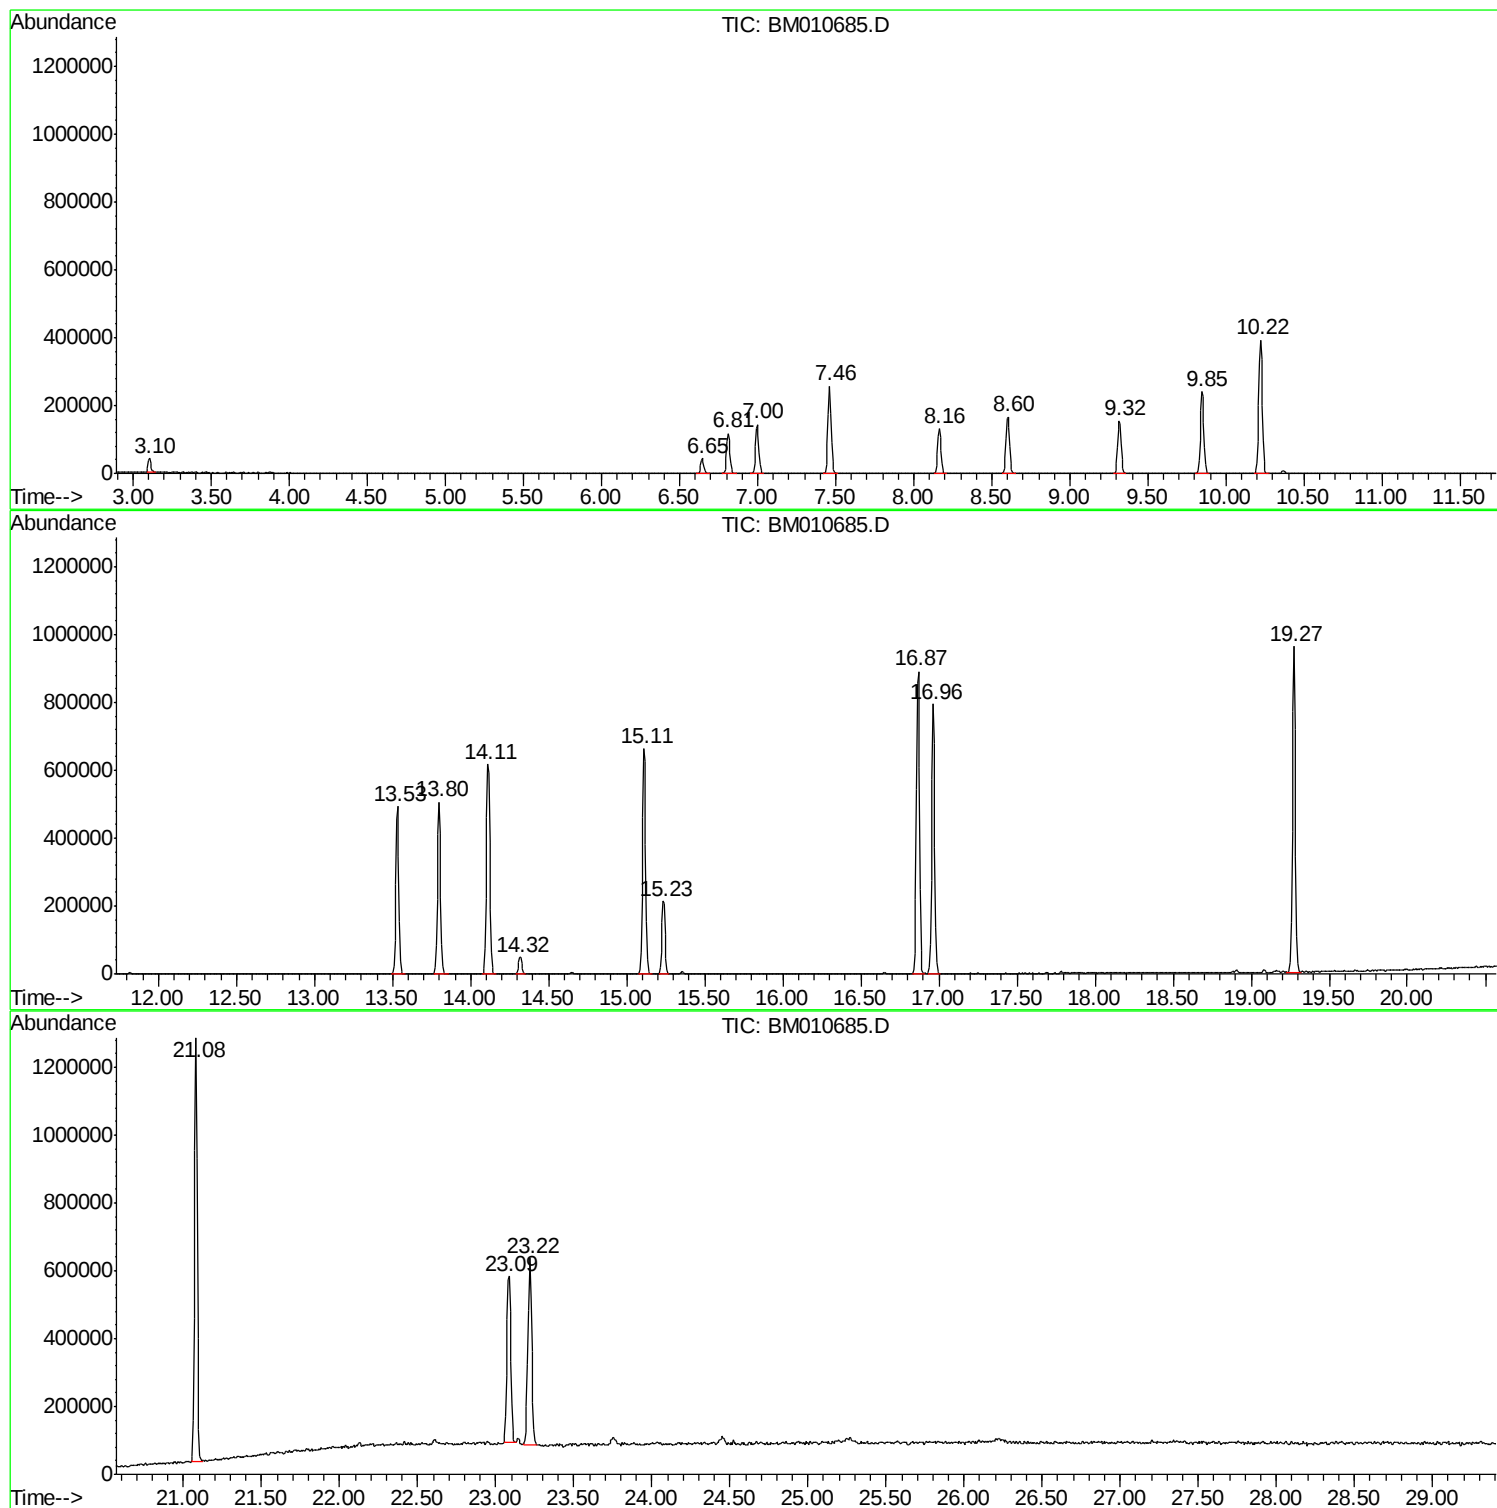

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
Data File : BM010685.D
Acq On : 23 Jun 2017 11:04
Operator : SJ/JU
Sample : I3767-01DL 2X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC63DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062317\
Data File : BM010685.D
Acq On : 23 Jun 2017 11:04
Operator : SJ/JU
Sample : I3767-01DL 2X
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDC63DL

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc