

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062319\
 Data File : BM021102.D
 Acq On : 22 Jun 2019 15:41
 Operator : HP/JU
 Sample : K3362-05
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A41X4

Quant Time: Jun 24 00:51:36 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 20 03:45:02 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	291032	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.56	136	1290709	20.00	ng/ul	-0.02
35) Acenaphthene-d10	14.42	164	863080	20.00	ng/ul	-0.01
61) Phenanthrene-d10	17.16	188	2139494	20.00	ng/ul	-0.01
77) Chrysene-d12	21.34	240	2057126	20.00	ng/ul	-0.01
85) Perylene-d12	23.62	264	2005967	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.29	96	31702	5.17	ng/uL	0.00
5) Phenol-d5	6.95	99	679005	26.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.12	67	456204	30.23	ng/ul	-0.01
9) 2-Chlorophenol-d4	7.31	132	594180	28.87	ng/ul	-0.01
13) 4-Methylphenol-d8	8.47	113	545516	25.80	ng/ul	-0.02
19) Nitrobenzene-d5	8.94	128	327840	31.28	ng/ul	-0.01
22) 2-Nitrophenol-d4	9.65	143	384214	33.02	ng/ul	-0.02
26) 2,4-Dichlorophenol-d3	10.18	165	715656	30.25	ng/ul	-0.02
29) 4-Chloroaniline-d4	10.71	131	775731	31.44	ng/ul	-0.01
43) Dimethylphthalate-d6	13.83	166	2620405	33.60	ng/ul	-0.01
46) Acenaphthylene-d8	14.11	160	2912514	30.51	ng/ul	-0.01
51) 4-Nitrophenol-d4	14.62	143	293316	23.12	ng/ul	-0.01
57) Fluorene-d10	15.41	176	2199587	32.43	ng/ul	-0.01
62) 4,6-Dinitro-2-methylphenol	15.54	200	334619	25.44	ng/ul	0.00
70) Anthracene-d10	17.26	188	3425274	30.81	ng/ul	-0.01
78) Pyrene-d10	19.56	212	3893239	31.54	ng/ul	-0.01
89) Benzo(a)pyrene-d12	23.48	264	3553613	30.03	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.87	163	616248	8.681	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062319\
Data File : BM021102.D
Acq On : 22 Jun 2019 15:41
Operator : HP/JU
Sample : K3362-05
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A41X4

Quant Time: Jun 24 00:51:36 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 20 03:45:02 2019
Response via : Initial Calibration

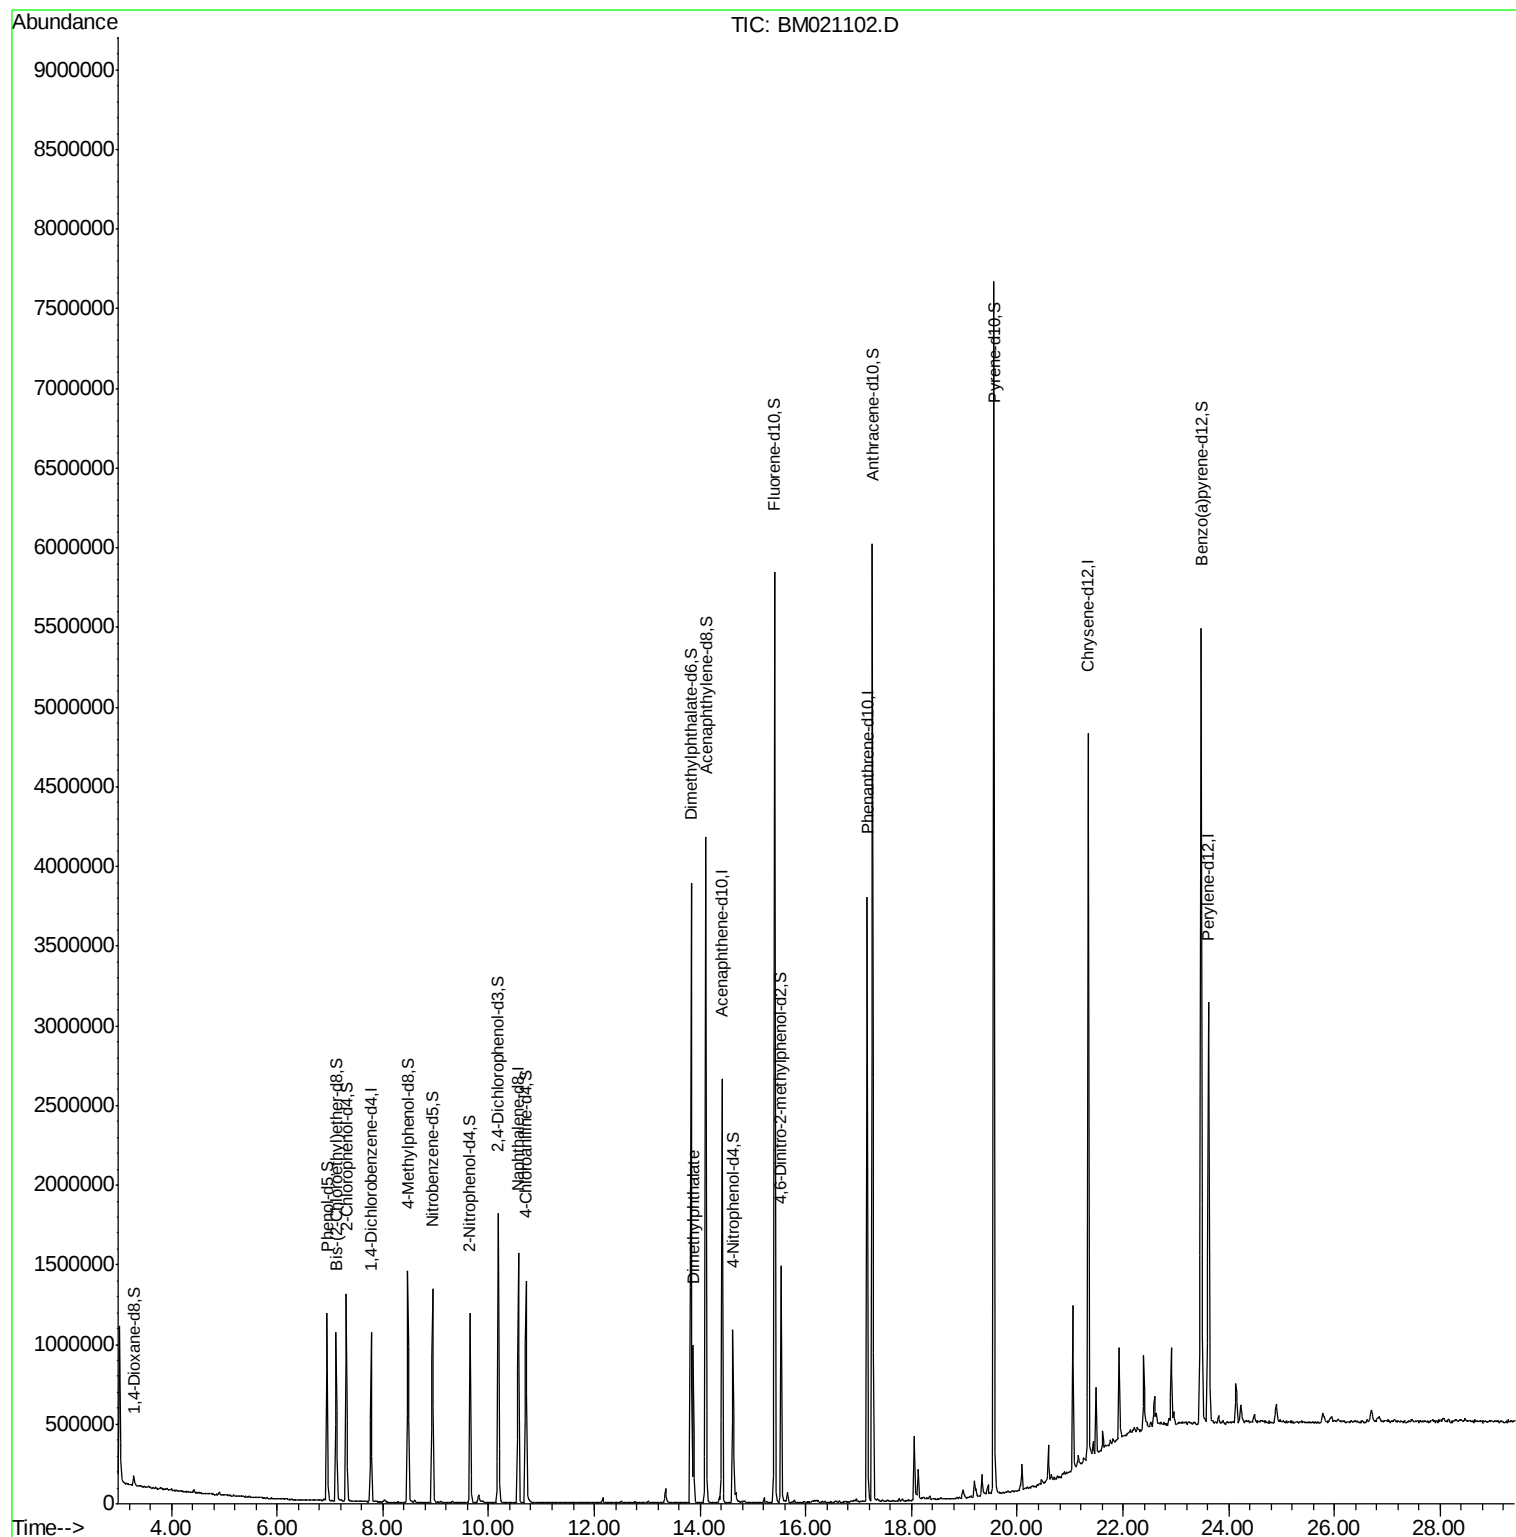


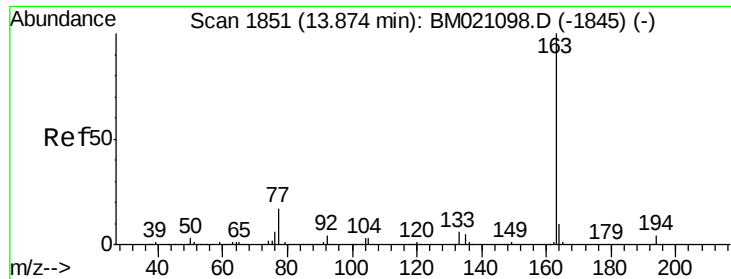

#44
 Dimethylphthalate
 Concen: 8.681 ng/ul
 RT: 13.87 min Scan# 1851
 Delta R.T. -0.01 min
 Lab File: BM021102.D
 Acq: 22 Jun 2019 15:41

Instrument :
 BNA_M
 ClientSampleId :
 A41X4

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.3	3.4	5.2
164	10.0	7.7	11.5

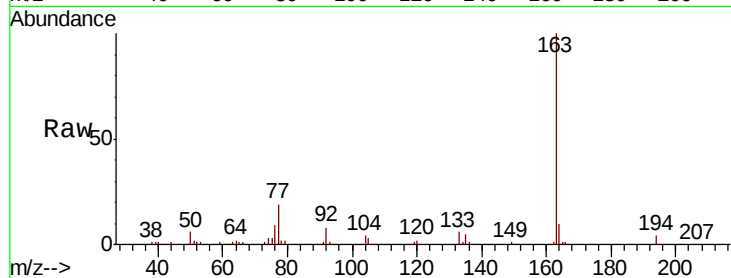

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

