

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062319\
 Data File : BM021123.D
 Acq On : 23 Jun 2019 06:06
 Operator : HP/JU
 Sample : PB120500BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK00

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.022	4	6	11	rVB	51438	64671	0.74%	0.075%
2	3.287	48	51	60	rVB	71378	97352	1.12%	0.114%
3	6.940	665	672	685	rVB	1321621	2028566	23.35%	2.366%
4	7.116	695	702	712	rBV	1055199	1636227	18.83%	1.909%
5	7.304	727	734	744	rVB	1404076	2164625	24.91%	2.525%
6	7.775	806	814	823	rVB	966977	1558162	17.93%	1.817%
7	8.475	924	933	948	rBV	1696234	2699633	31.07%	3.149%
8	8.934	1003	1011	1024	rBV	1366761	2234111	25.71%	2.606%
9	9.651	1125	1133	1146	rBV	1197966	1919457	22.09%	2.239%
10	10.181	1215	1223	1237	rBV	1845438	3052345	35.13%	3.560%
11	10.563	1280	1288	1300	rVB	1425648	2407936	27.71%	2.809%
12	10.704	1305	1312	1333	rVV	1744244	2998770	34.51%	3.498%
13	12.157	1553	1559	1566	rVB2	25916	42689	0.49%	0.050%
14	13.827	1836	1843	1853	rBV	3812987	5152274	59.30%	6.010%
15	14.104	1883	1890	1902	rBV	4225509	6094772	70.15%	7.109%
16	14.416	1936	1943	1954	rBV2	2381986	3677138	42.32%	4.289%
17	14.616	1970	1977	1999	rBV	1189882	1977854	22.76%	2.307%
18	15.204	2073	2077	2083	rBV	29901	40005	0.46%	0.047%
19	15.410	2104	2112	2120	rBV	5530929	7797681	89.75%	9.095%
20	15.533	2127	2133	2147	rBV	1365929	1918743	22.08%	2.238%
21	15.645	2147	2152	2160	rVB	59944	85523	0.98%	0.100%
22	16.945	2369	2373	2379	rVB2	9947	16366	0.19%	0.019%
23	17.162	2403	2410	2419	rBV	3203901	4485886	51.63%	5.232%
24	17.257	2419	2426	2438	rBV	5699438	8286536	95.37%	9.666%
25	19.186	2750	2754	2759	rBV	52610	67949	0.78%	0.079%
26	19.439	2793	2797	2803	rBV	44415	61907	0.71%	0.072%
27	19.556	2810	2817	2823	rBV	6326734	8688539	100.00%	10.134%
28	21.339	3115	3120	3130	rBV	3092005	3855615	44.38%	4.497%
29	23.468	3475	3482	3494	rVB	3922726	7008087	80.66%	8.174%
30	23.609	3500	3506	3521	rVB	1805184	3613472	41.59%	4.215%


Sum of corrected areas: 85732891

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062319\
Data File : BM021123.D
Acq On : 23 Jun 2019 06:06
Operator : HP/JU
Sample : PB120500BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK00

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

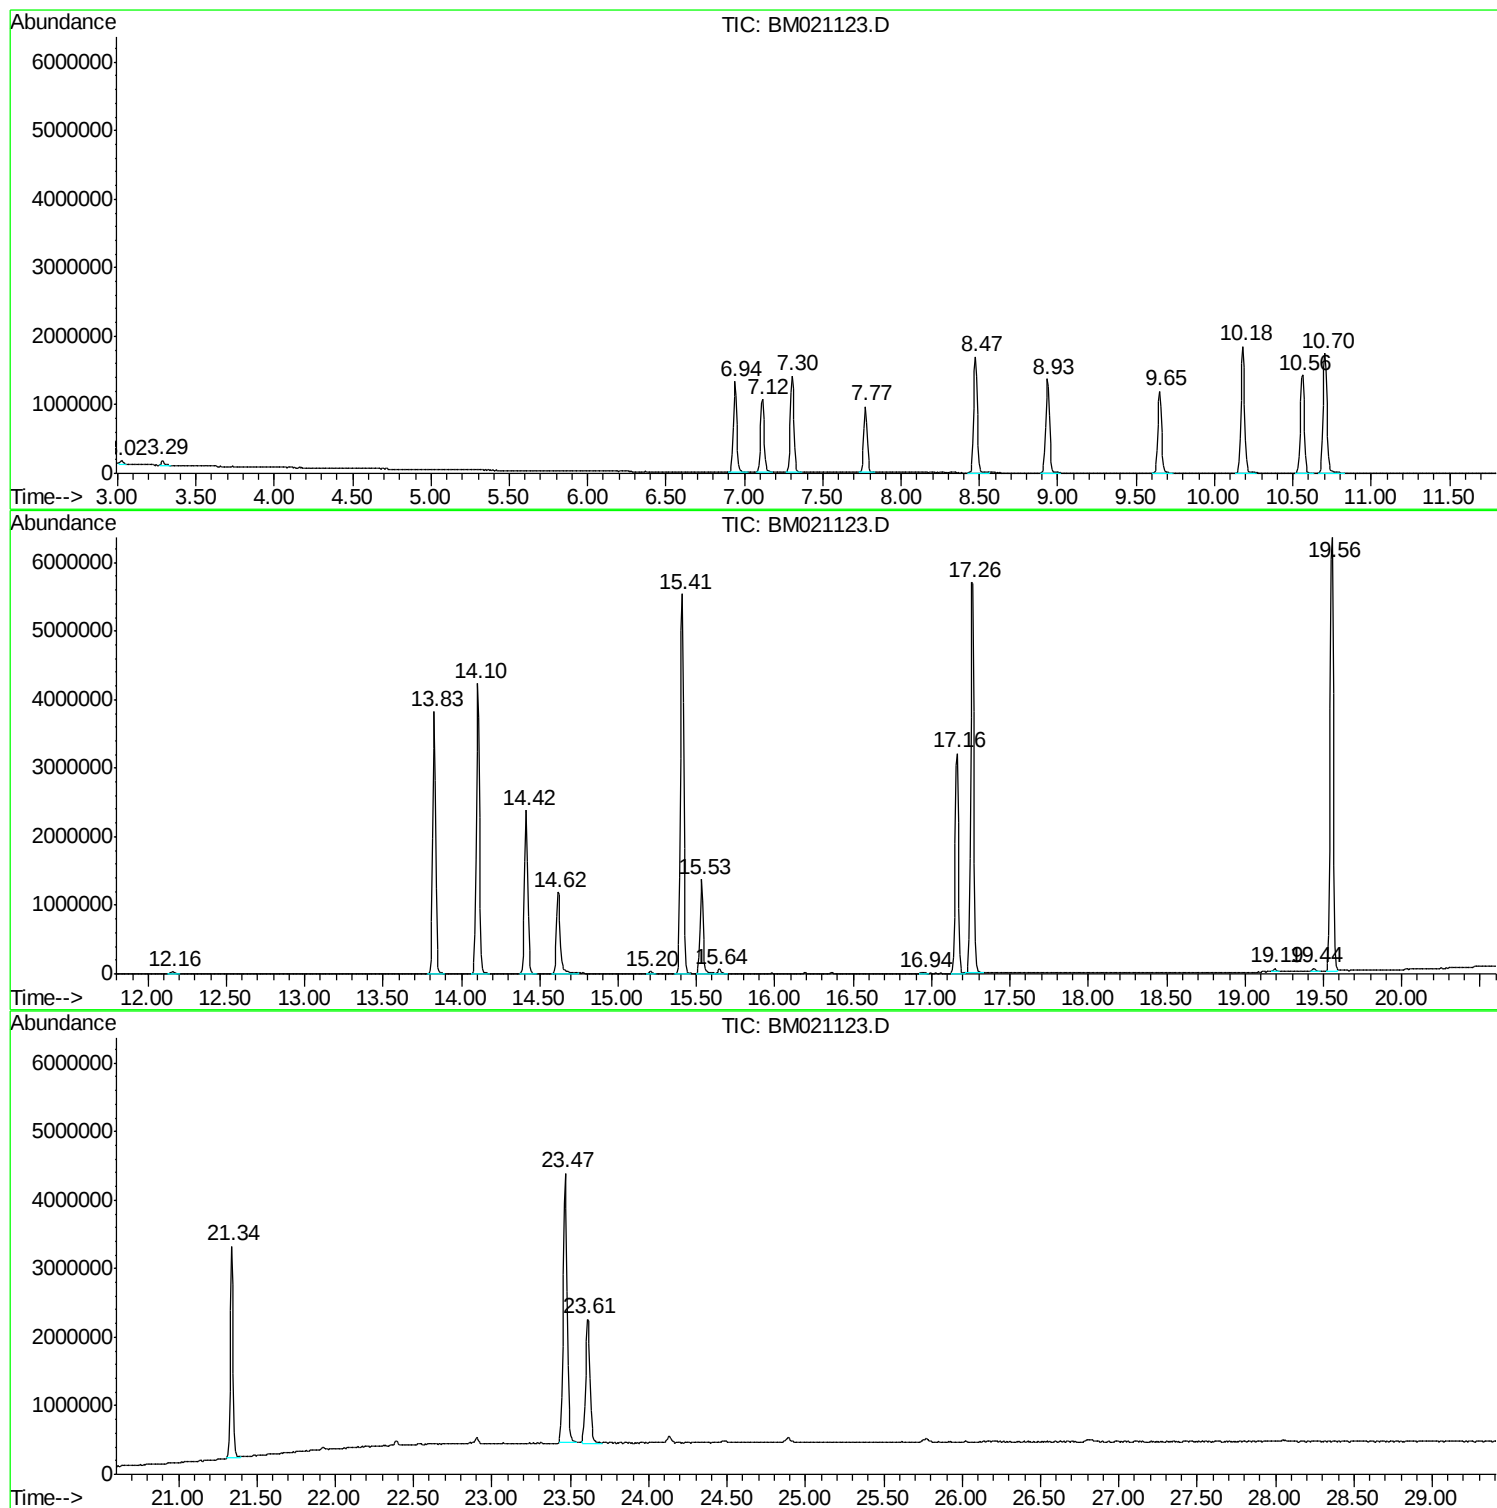

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062319\
Data File : BM021123.D
Acq On : 23 Jun 2019 06:06
Operator : HP/JU
Sample : PB120500BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK00

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062319\
Data File : BM021123.D
Acq On : 23 Jun 2019 06:06
Operator : HP/JU
Sample : PB120500BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK00

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc