

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062319\
 Data File : BM021126.D
 Acq On : 23 Jun 2019 09:42
 Operator : HP/JU
 Sample : K3226-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFCP1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.022	3	6	16	rVB	746708	990466	14.65%	1.367%
2	3.251	39	45	63	rVB	2470501	3989112	59.02%	5.506%
3	6.881	658	662	665	rVB2	8192	12570	0.19%	0.017%
4	6.939	666	672	682	rVB	244436	386541	5.72%	0.534%
5	7.116	695	702	717	rBV	795976	1264707	18.71%	1.746%
6	7.304	728	734	745	rVB	896806	1411038	20.88%	1.948%
7	7.775	807	814	822	rBV	1013833	1647763	24.38%	2.275%
8	8.475	925	933	947	rBV	741278	1185877	17.55%	1.637%
9	8.933	1004	1011	1022	rBV	1093380	1780844	26.35%	2.458%
10	9.310	1068	1075	1081	rVB	27201	40397	0.60%	0.056%
11	9.651	1125	1133	1146	rBV	918642	1491245	22.06%	2.058%
12	10.180	1216	1223	1237	rBV	1410024	2355995	34.86%	3.252%
13	10.563	1280	1288	1295	rBV	1452381	2506381	37.08%	3.460%
14	10.710	1307	1313	1324	rBV	100953	195018	2.89%	0.269%
15	11.798	1492	1498	1505	rVB2	25527	38135	0.56%	0.053%
16	12.157	1554	1559	1565	rVB2	21226	31276	0.46%	0.043%
17	13.827	1834	1843	1855	rBV	3029783	4233646	62.64%	5.844%
18	14.104	1883	1890	1901	rBV	3350703	4976097	73.63%	6.869%
19	14.410	1936	1942	1956	rBV2	2367012	3728010	55.16%	5.146%
20	14.627	1973	1979	1992	rBV	127734	270165	4.00%	0.373%
21	15.162	2064	2070	2075	rBV	121511	169928	2.51%	0.235%
22	15.204	2075	2077	2082	rVB	12039	13867	0.21%	0.019%
23	15.410	2105	2112	2123	rBV	4511963	6506190	96.27%	8.981%
24	15.533	2127	2133	2148	rVV	1078441	1531648	22.66%	2.114%
25	15.645	2148	2152	2156	rVB	48550	68955	1.02%	0.095%
26	16.192	2241	2245	2249	rVB4	5372	6975	0.10%	0.010%
27	16.951	2369	2374	2378	rVB2	9370	15079	0.22%	0.021%
28	17.162	2403	2410	2419	rBV	3044669	4291454	63.50%	5.924%
29	17.262	2419	2427	2442	rVV	4647303	6641214	98.26%	9.167%
30	18.045	2555	2560	2565	rBV2	41839	57760	0.85%	0.080%
31	19.186	2750	2754	2758	rBV	47299	61191	0.91%	0.084%
32	19.327	2774	2778	2784	rBV4	42577	59412	0.88%	0.082%
33	19.439	2793	2797	2801	rBV	36808	48557	0.72%	0.067%
34	19.474	2801	2803	2810	rVB7	14887	14329	0.21%	0.020%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062319\
Data File : BM021126.D
Acq On : 23 Jun 2019 09:42
Operator : HP/JU
Sample : K3226-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFCP1

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Title : SVOA CALIBRATION

35	19.550	2810	2816	2826	rBV	5129861	6758623	100.00%	9.329%
36	21.339	3115	3120	3131	rBV	2866562	3693728	54.65%	5.099%
37	22.391	3296	3299	3303	rVB	126258	149547	2.21%	0.206%
38	23.468	3475	3482	3497	rVB	3409188	6186285	91.53%	8.539%
39	23.615	3500	3507	3520	rVB2	1782560	3633868	53.77%	5.016%


Sum of corrected areas: 72443893

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062319\
Data File : BM021126.D
Acq On : 23 Jun 2019 09:42
Operator : HP/JU
Sample : K3226-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFCP1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

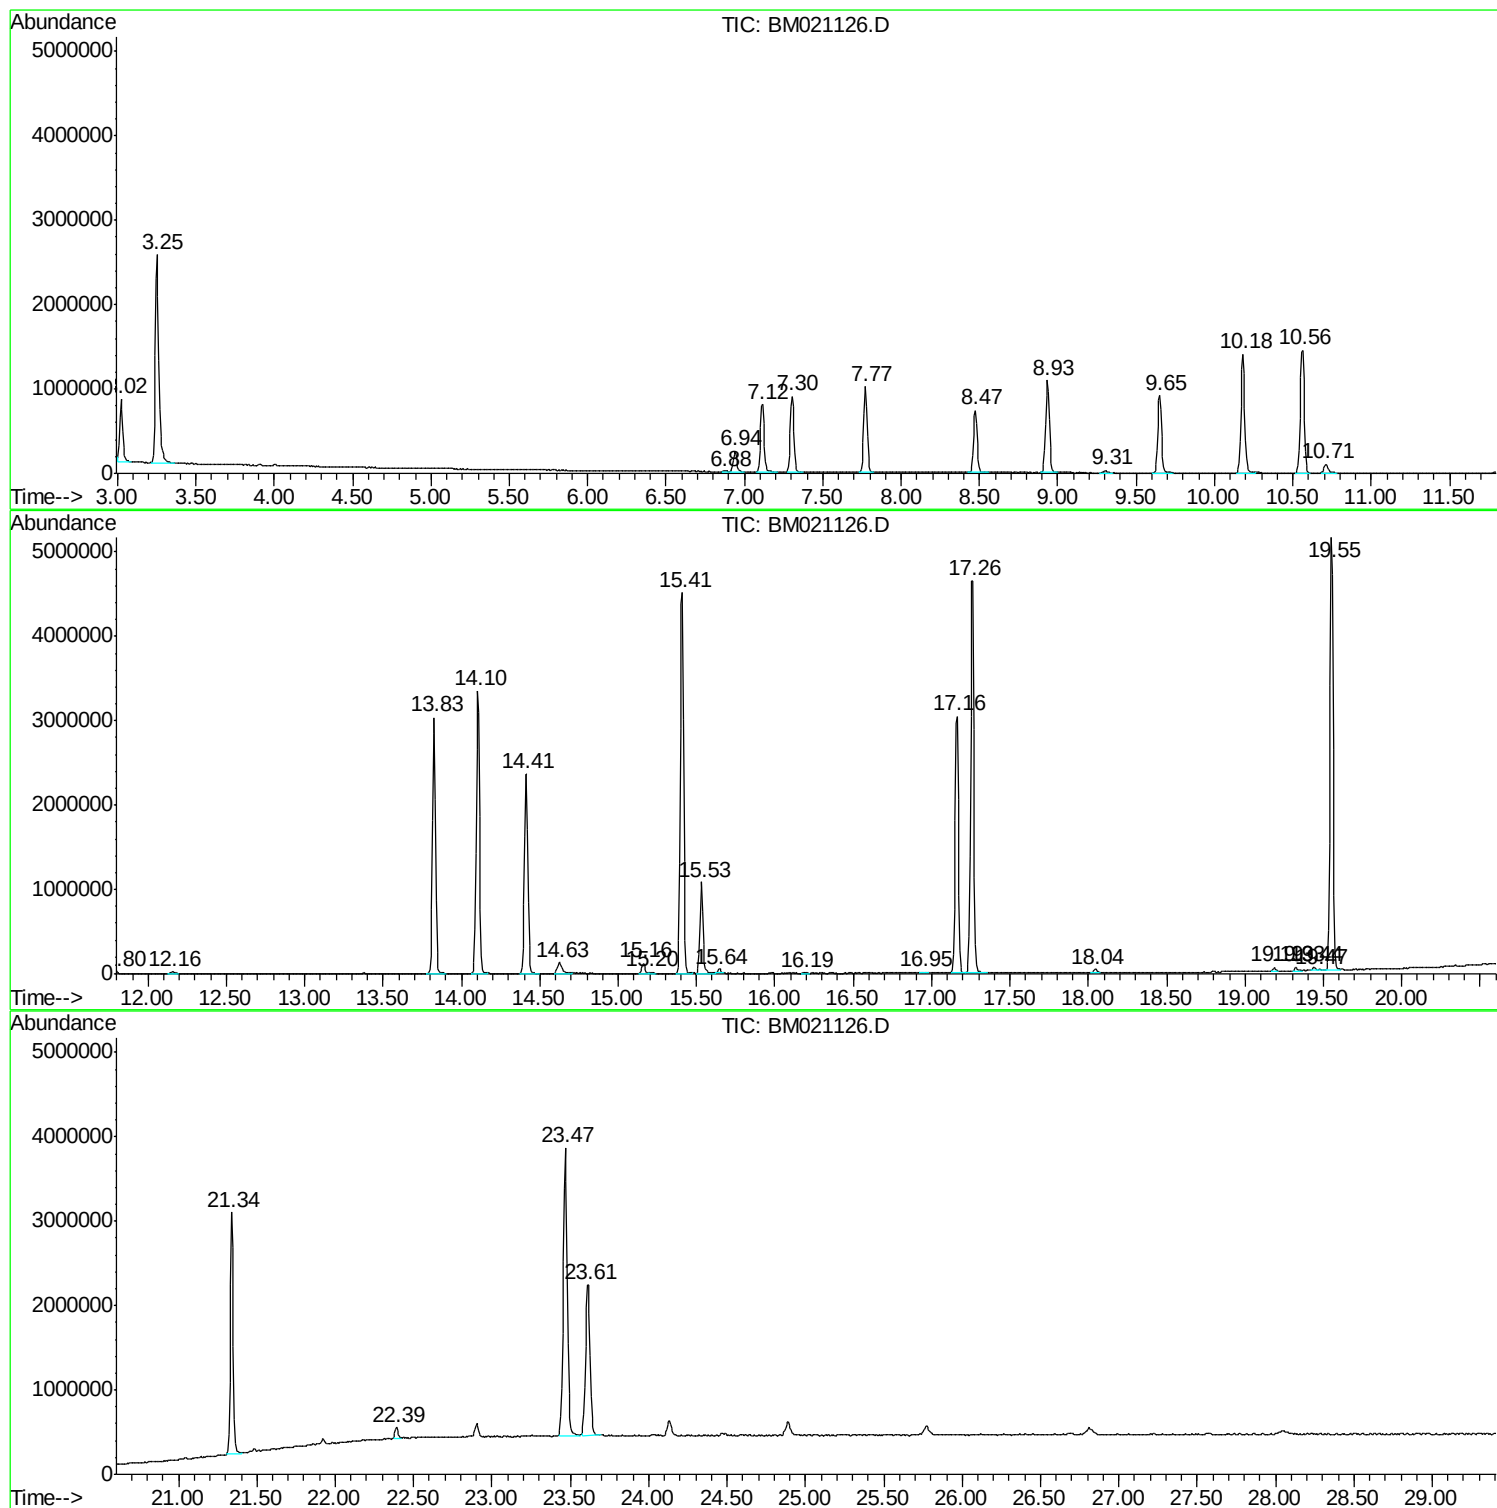

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062319\
Data File : BM021126.D
Acq On : 23 Jun 2019 09:42
Operator : HP/JU
Sample : K3226-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFCP1










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.02	12.02 ng/ul	990466	1,4-Dichlorobenzene-d4	7.77

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	86
2		Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	74
3		Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
4		Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9
5		Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

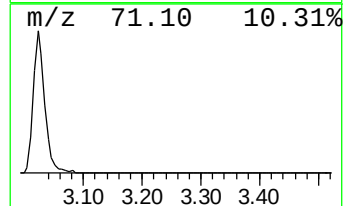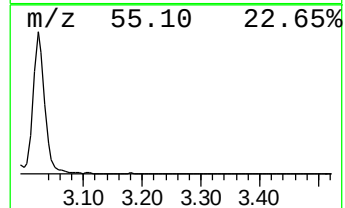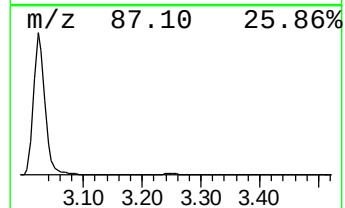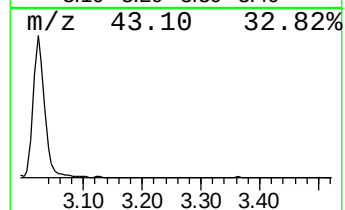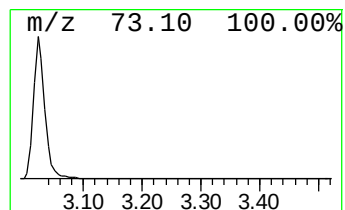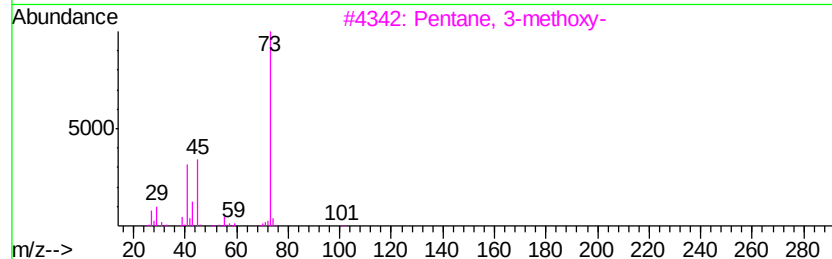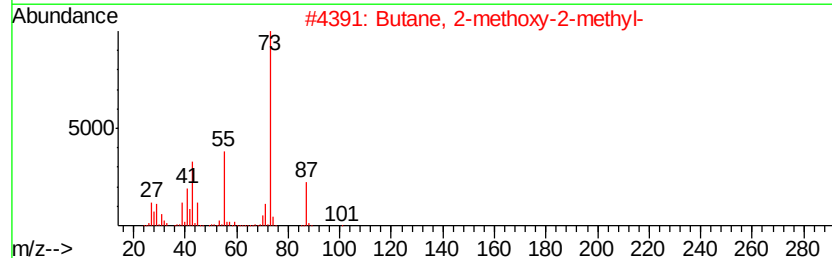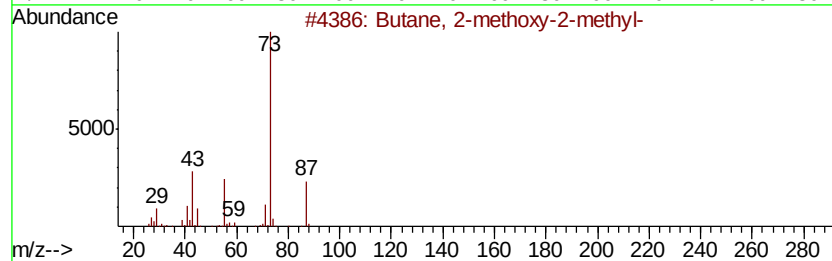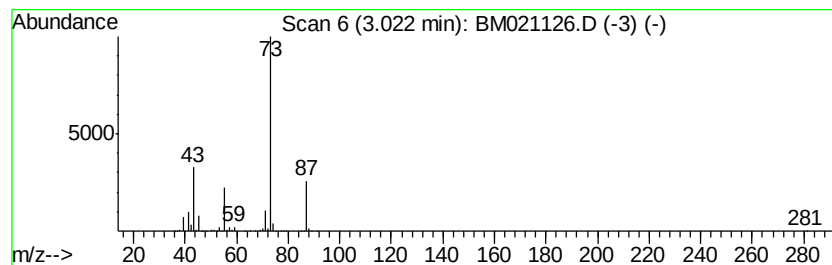

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062319\
Data File : BM021126.D
Acq On : 23 Jun 2019 09:42
Operator : HP/JU
Sample : K3226-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFCP1

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-methoxy...	3.02	12.0	ng/ul	990466	1	7.77	1647760	20.0