

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062319\
 Data File : BM021135.D
 Acq On : 23 Jun 2019 15:06
 Operator : HP/JU
 Sample : PB120468BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK68

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.022	4	6	11	rVB	52001	61685	0.76%	0.074%
2	3.287	47	51	59	rVB	78506	106176	1.30%	0.127%
3	6.939	666	672	682	rBV	1356489	2150678	26.34%	2.568%
4	7.110	695	701	714	rBV	1085094	1727058	21.15%	2.062%
5	7.304	727	734	747	rVB	1499060	2311400	28.31%	2.760%
6	7.769	806	813	823	rBV	1042847	1692796	20.73%	2.021%
7	8.475	925	933	943	rBV	1746464	2776150	34.00%	3.314%
8	8.933	1004	1011	1020	rBV	1378479	2285554	27.99%	2.729%
9	9.651	1125	1133	1140	rBV	1207902	1985438	24.32%	2.370%
10	10.180	1215	1223	1241	rBV	1874737	3108940	38.08%	3.712%
11	10.557	1280	1287	1297	rBV	1463615	2508118	30.72%	2.994%
12	10.704	1304	1312	1328	rBV	1729012	2981371	36.51%	3.560%
13	12.157	1554	1559	1567	rVB	24647	40455	0.50%	0.048%
14	13.827	1835	1843	1853	rBV	3461734	4641740	56.85%	5.542%
15	14.104	1883	1890	1900	rBV	3964597	5743116	70.34%	6.857%
16	14.415	1934	1943	1954	rBV2	2221215	3483265	42.66%	4.159%
17	14.621	1972	1978	1996	rBV	1071082	1784880	21.86%	2.131%
18	15.204	2073	2077	2082	rVB	24000	30478	0.37%	0.036%
19	15.409	2104	2112	2121	rBV	4793878	7032869	86.14%	8.397%
20	15.533	2127	2133	2146	rBV	1245048	1722785	21.10%	2.057%
21	15.645	2148	2152	2158	rVB	53779	81148	0.99%	0.097%
22	16.186	2242	2244	2253	rBV5	6182	8866	0.11%	0.011%
23	16.945	2369	2373	2378	rVB2	10277	14030	0.17%	0.017%
24	17.162	2403	2410	2420	rBV	2667444	3921896	48.03%	4.682%
25	17.256	2420	2426	2443	rVV	4861863	7178224	87.92%	8.570%
26	17.545	2473	2475	2482	rVB6	5242	9864	0.12%	0.012%
27	19.192	2750	2755	2762	rBV	44377	67148	0.82%	0.080%
28	19.439	2794	2797	2802	rBV	38321	47242	0.58%	0.056%
29	19.556	2810	2817	2826	rBV	5977795	7837029	95.99%	9.357%
30	21.344	3116	3121	3131	rBV	3294108	4071088	49.86%	4.861%
31	23.474	3476	3483	3495	rBV	4320496	8164801	100.00%	9.748%
32	23.621	3501	3508	3521	rVB	2163852	4181530	51.21%	4.992%

LSC Area Percent Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062319\
Data File : BM021135.D
Acq On : 23 Jun 2019 15:06
Operator : HP/JU
Sample : PB120468BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK68

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 83757818

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062319\
Data File : BM021135.D
Acq On : 23 Jun 2019 15:06
Operator : HP/JU
Sample : PB120468BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK68

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

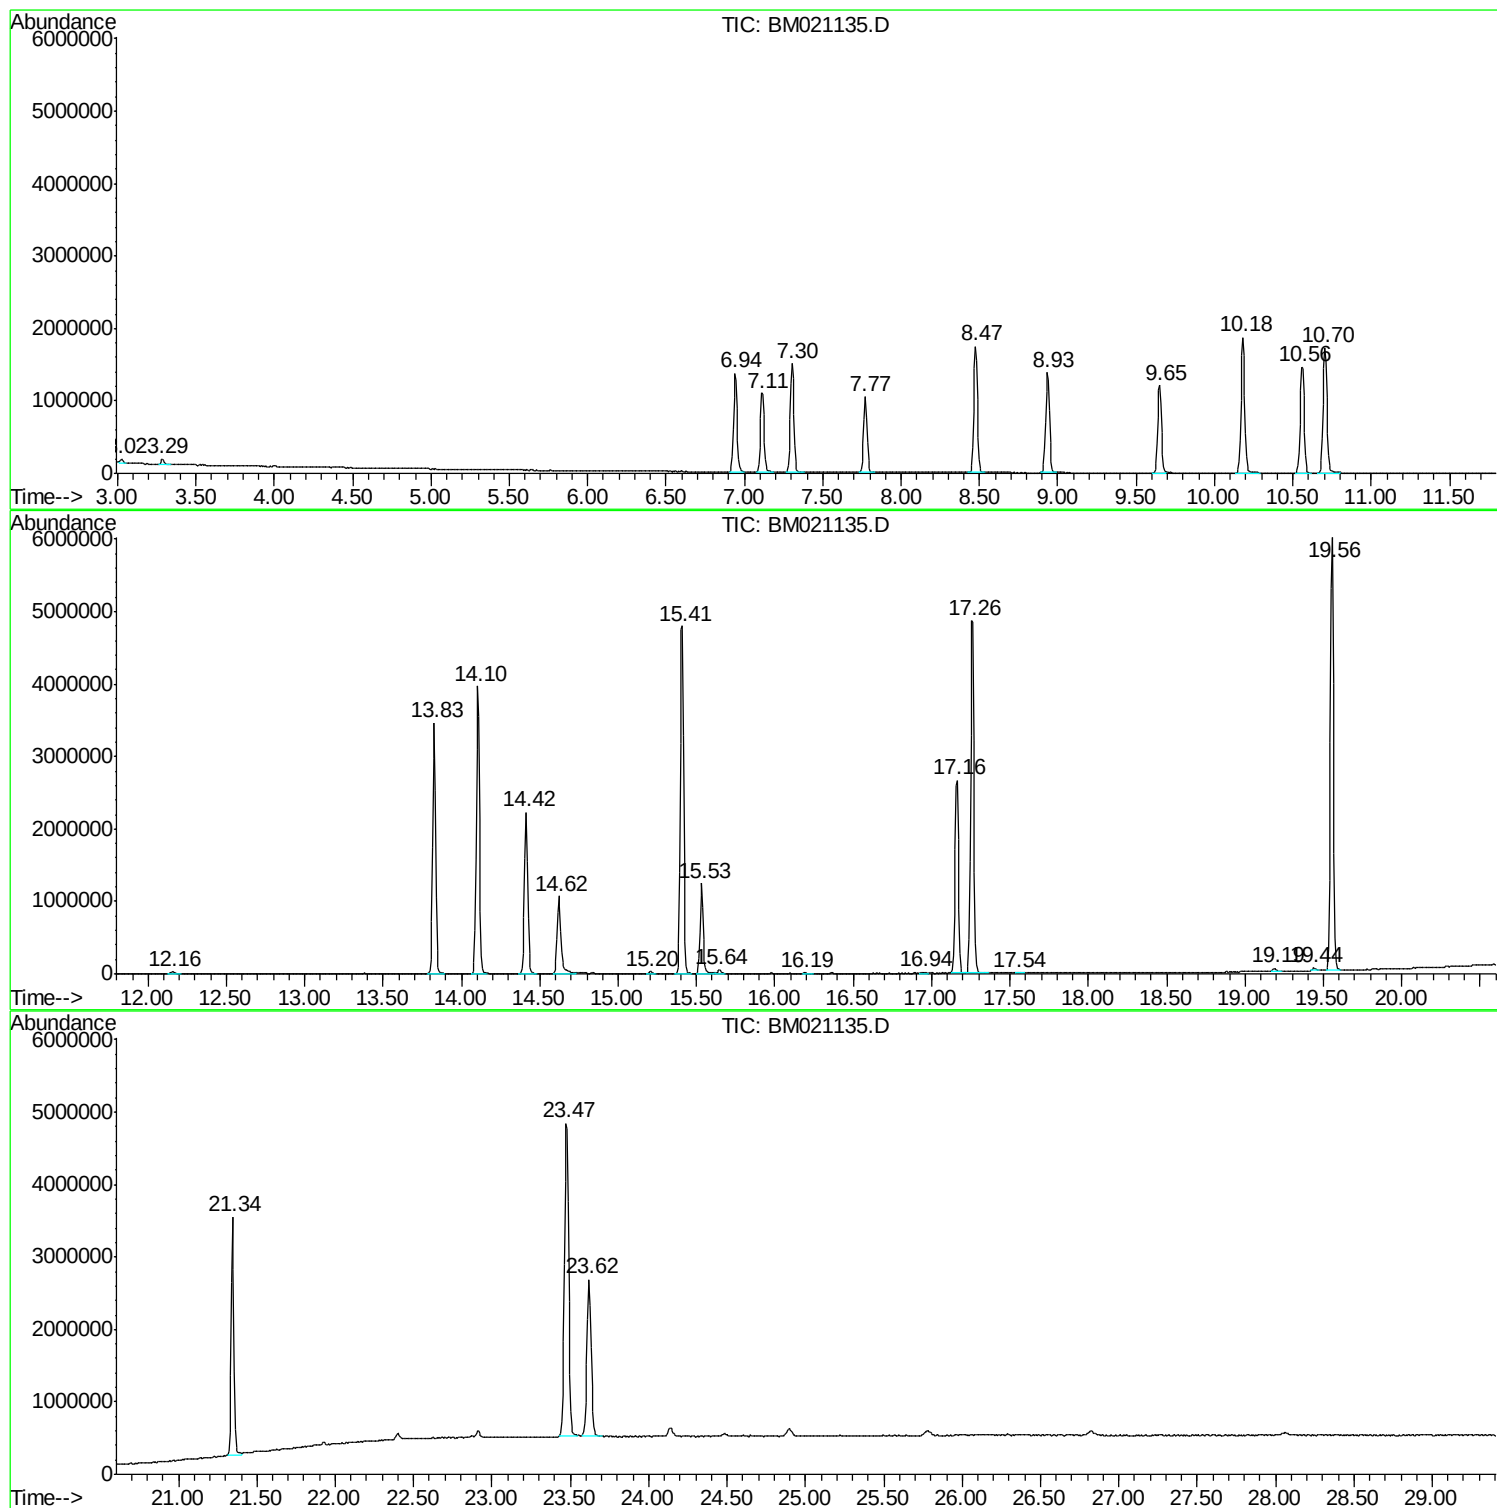

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062319\
Data File : BM021135.D
Acq On : 23 Jun 2019 15:06
Operator : HP/JU
Sample : PB120468BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK68

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062319\
Data File : BM021135.D
Acq On : 23 Jun 2019 15:06
Operator : HP/JU
Sample : PB120468BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK68

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc