

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
 Data File : BM026501.D
 Acq On : 23 Jun 2020 15:22
 Operator : JU/CG
 Sample : L3027-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG2K5

Quant Time: Jun 23 17:03:19 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 23 10:25:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	64816	20.00	ng/ul	0.00
18) Naphthalene-d8	10.14	136	294727	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.04	164	206084	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	497209	20.00	ng/ul	0.00
78) Chrysene-d12	21.01	240	573587	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	593182	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.97	96	6828	3.69	ng/uL	0.00
5) Phenol-d5	6.59	99	104909	17.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.74	67	78625	20.81	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	83216	17.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	88118	18.75	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	41494	15.85	ng/ul	0.00
22) 2-Nitrophenol-d4	9.25	143	46095	16.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	82218	15.50	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	113205	20.47	ng/ul	0.00
44) Dimethylphthalate-d6	13.47	166	327905	18.92	ng/ul	0.00
47) Acenaphthylene-d8	13.72	160	308413	14.84	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	30971	10.78	ng/ul	0.01
58) Fluorene-d10	15.04	176	222176	14.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	37825	11.62	ng/ul	0.00
71) Anthracene-d10	16.89	188	348672	13.78	ng/ul	0.00
79) Pyrene-d10	19.20	212	372415	11.84	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.97	264	328893	10.03	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.52	163	65267	3.627	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
Data File : BM026501.D
Acq On : 23 Jun 2020 15:22
Operator : JU/CG
Sample : L3027-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG2K5

Quant Time: Jun 23 17:03:19 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 23 10:25:31 2020
Response via : Initial Calibration

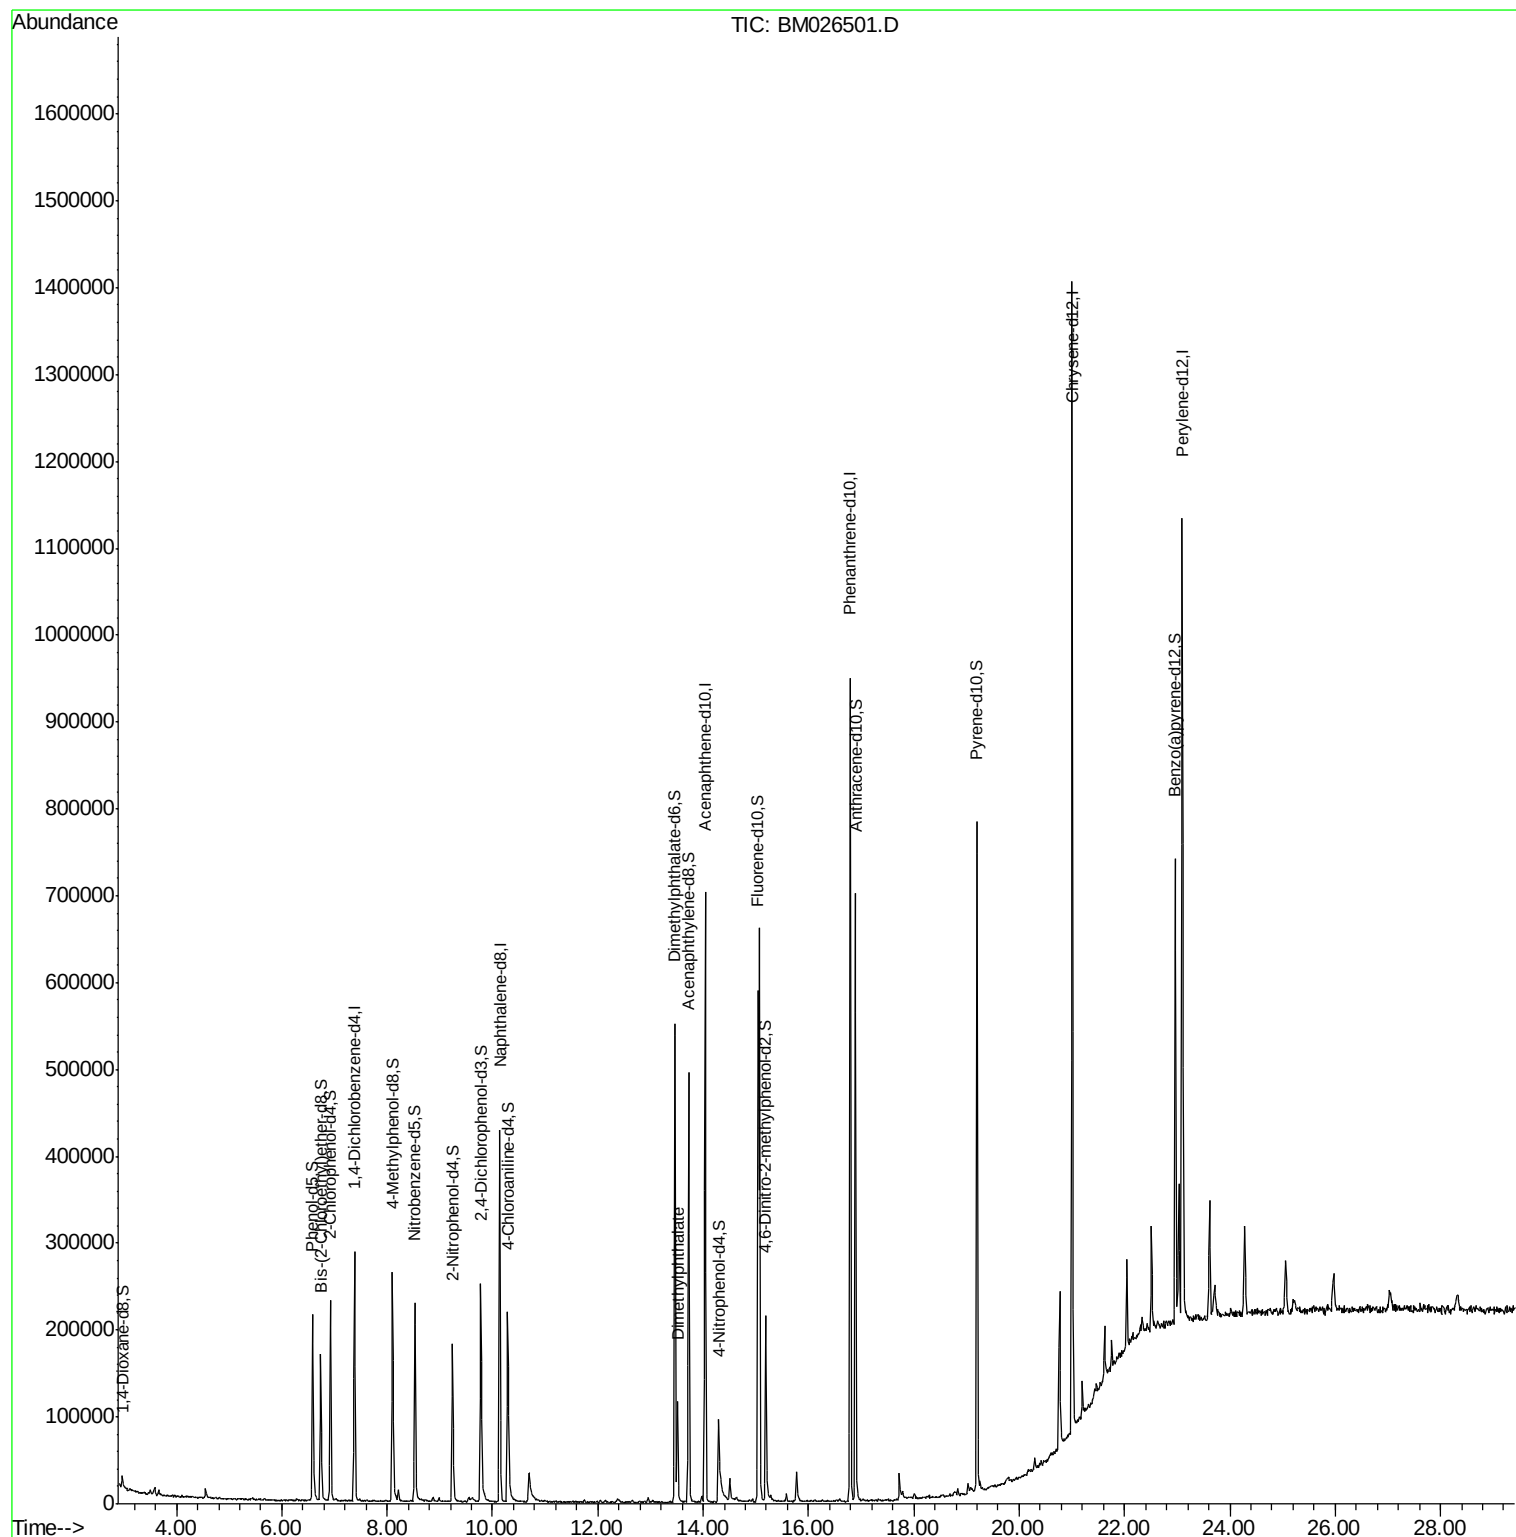

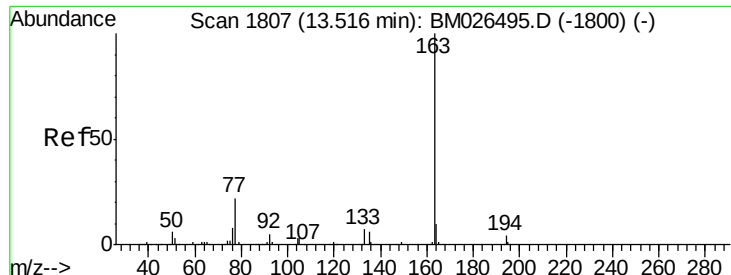

#45

Dimethylphthalate

Concen: 3.627 ng/ul

RT: 13.52 min Scan# 1807

Delta R.T. -0.00 min

Lab File: BM026501.D

Acq: 23 Jun 2020 15:22

Instrument :

BNA_M

ClientSampleId :

BG2K5


Tot Ion:163 Resp: 65267

Ion Ratio Lower Upper

163 100

194 3.7 3.4 5.2

164 10.5 7.8 11.6

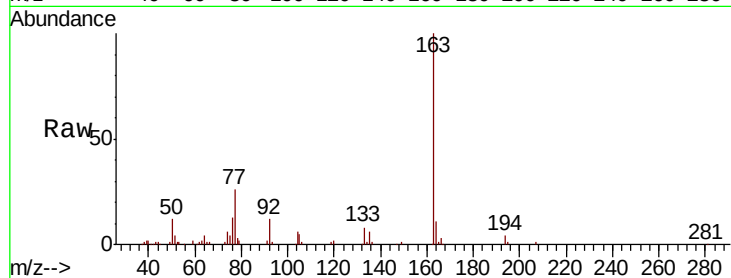

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

