

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
 Data File : BM026502.D
 Acq On : 23 Jun 2020 15:59
 Operator : JU/CG
 Sample : L3027-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG2L5

Quant Time: Jun 23 17:06:26 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 23 10:25:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	81607	20.00	ng/ul	0.00
18) Naphthalene-d8	10.14	136	363856	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.04	164	244670	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	579505	20.00	ng/ul	0.00
78) Chrysene-d12	21.01	240	694766	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	713961	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.97	96	13830	5.94	ng/uL	0.00
5) Phenol-d5	6.59	99	226530	30.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.74	67	160034	33.65	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	172551	28.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	190955	32.27	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	89480	27.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.24	143	95388	26.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	180041	27.49	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	231046	33.83	ng/ul	0.00
44) Dimethylphthalate-d6	13.47	166	594257	28.89	ng/ul	0.00
47) Acenaphthylene-d8	13.72	160	671848	27.23	ng/ul	0.00
52) 4-Nitrophenol-d4	14.28	143	85597	25.09	ng/ul	0.00
58) Fluorene-d10	15.04	176	477094	27.03	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	93205	24.57	ng/ul	0.00
71) Anthracene-d10	16.89	188	728317	24.69	ng/ul	0.00
79) Pyrene-d10	19.20	212	880501	23.11	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.97	264	867560	21.98	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.52	163	231330	10.828	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
Data File : BM026502.D
Acq On : 23 Jun 2020 15:59
Operator : JU/CG
Sample : L3027-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG2L5

Quant Time: Jun 23 17:06:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 23 10:25:31 2020
Response via : Initial Calibration

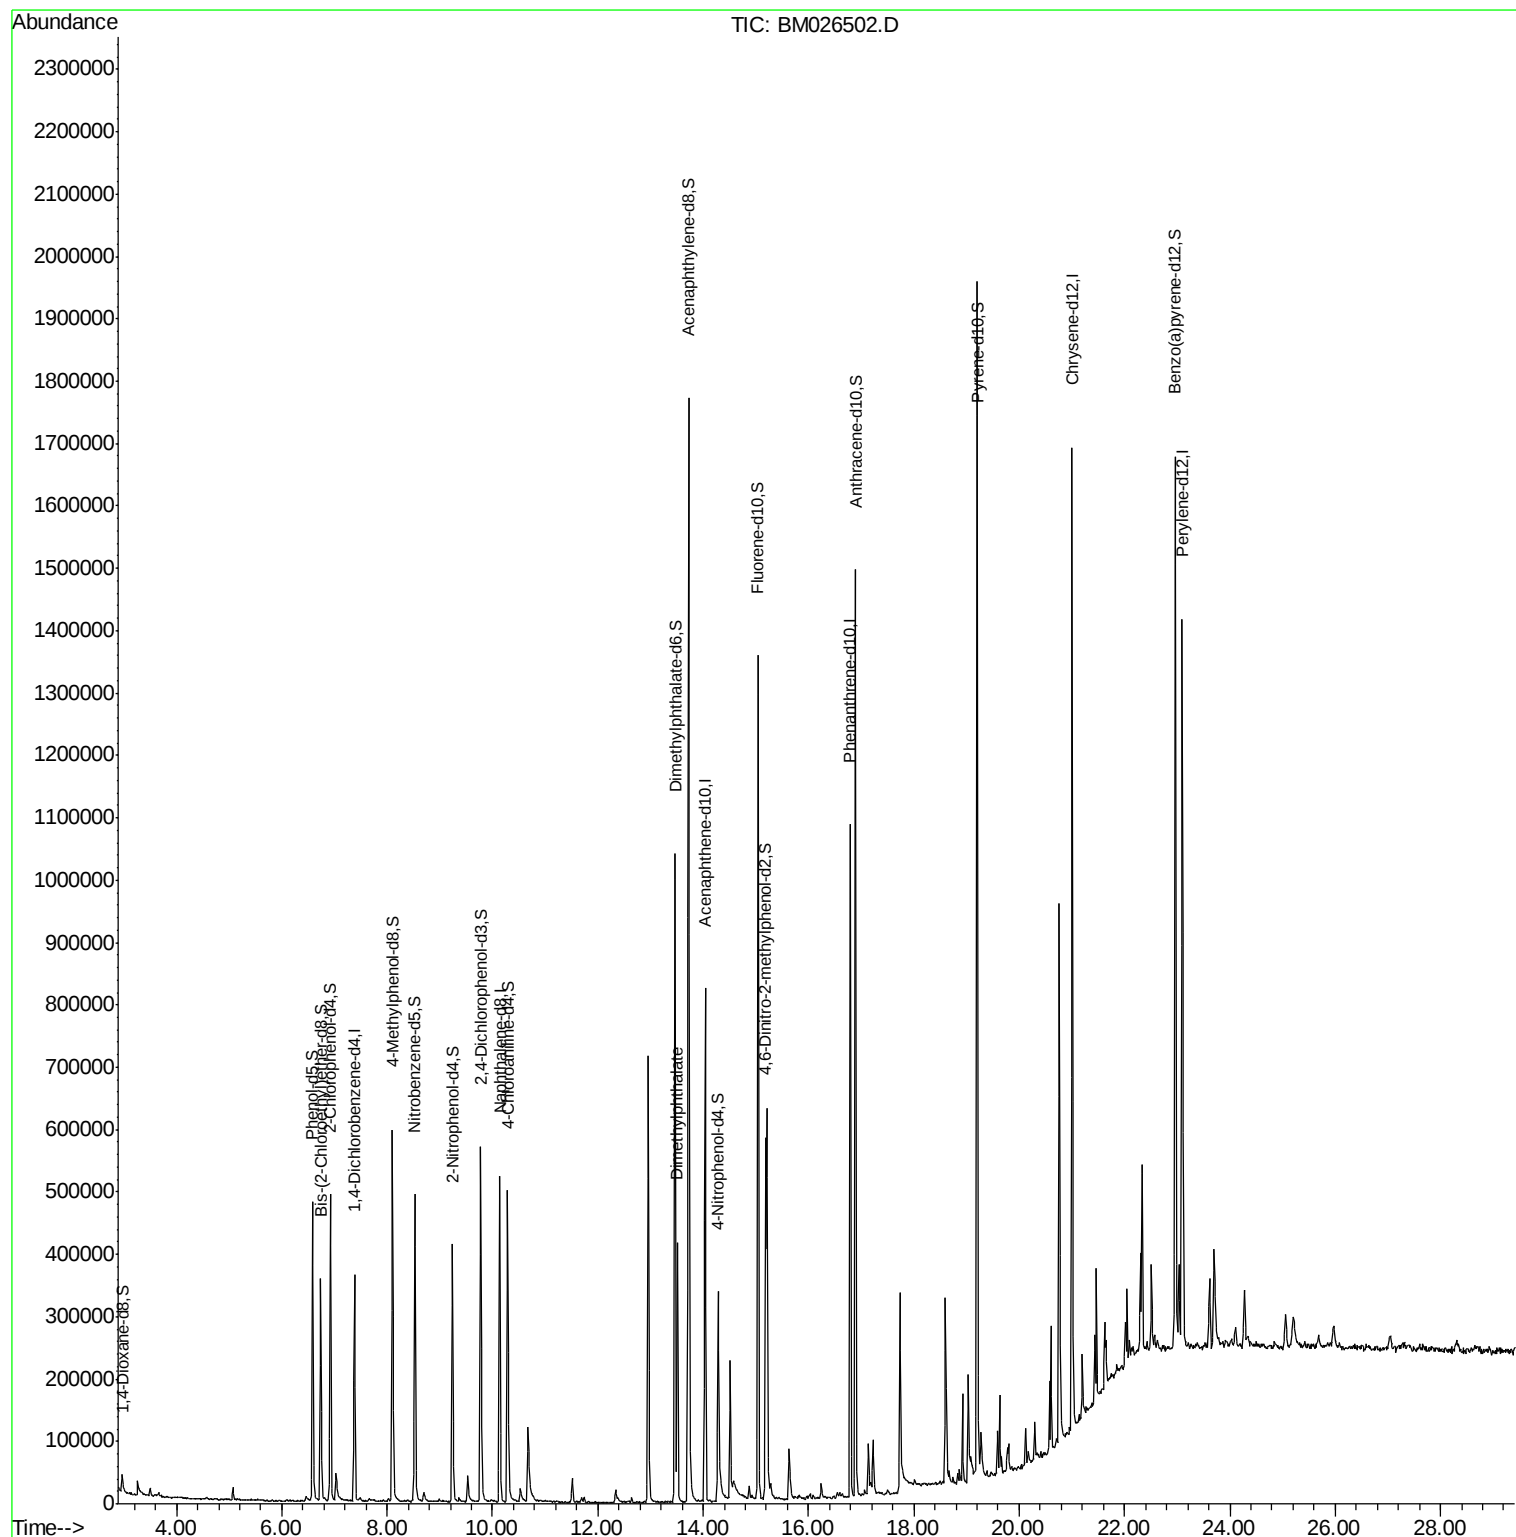

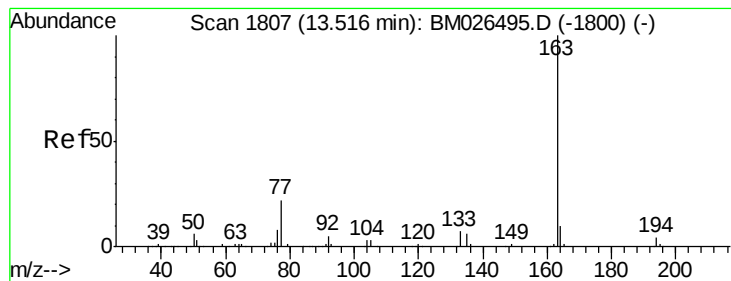

#45
 Dimethylphthalate
 Concen: 10.828 ng/ul
 RT: 13.52 min Scan# 1807
 Delta R.T. -0.00 min
 Lab File: BM026502.D
 Acq: 23 Jun 2020 15:59

Instrument :
 BNA_M
 ClientSampleId :
 BG2L5

Tot Ion	163	Resp: Lower	231330
	Ratio		Upper
163	100		
194	4.4	3.4	5.2
164	9.9	7.8	11.6

