

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
 Data File : BM026504.D
 Acq On : 23 Jun 2020 17:12
 Operator : JU/CG
 Sample : L3027-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG2K9

Quant Time: Jun 23 18:03:44 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 23 10:25:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	81542	20.00	ng/ul	0.00
18) Naphthalene-d8	10.14	136	375351	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.04	164	256647	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	605098	20.00	ng/ul	0.00
78) Chrysene-d12	21.01	240	710230	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	733149	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.97	96	8495	3.65	ng/uL	0.00
5) Phenol-d5	6.59	99	134124	17.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.74	67	95109	20.01	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	106034	17.32	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	113308	19.16	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	51272	15.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.24	143	53300	14.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	107972	15.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	149982	21.29	ng/ul	0.00
44) Dimethylphthalate-d6	13.46	166	385299	17.85	ng/ul	0.00
47) Acenaphthylene-d8	13.72	160	398773	15.41	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	40658	11.36	ng/ul	0.00
58) Fluorene-d10	15.04	176	286271	15.46	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	36647	9.25	ng/ul	0.00
71) Anthracene-d10	16.89	188	455573	14.79	ng/ul	0.00
79) Pyrene-d10	19.20	212	436236	11.20	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.96	264	454566	11.21	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.52	163	69535	3.103	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
Data File : BM026504.D
Acq On : 23 Jun 2020 17:12
Operator : JU/CG
Sample : L3027-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG2K9

Quant Time: Jun 23 18:03:44 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 23 10:25:31 2020
Response via : Initial Calibration

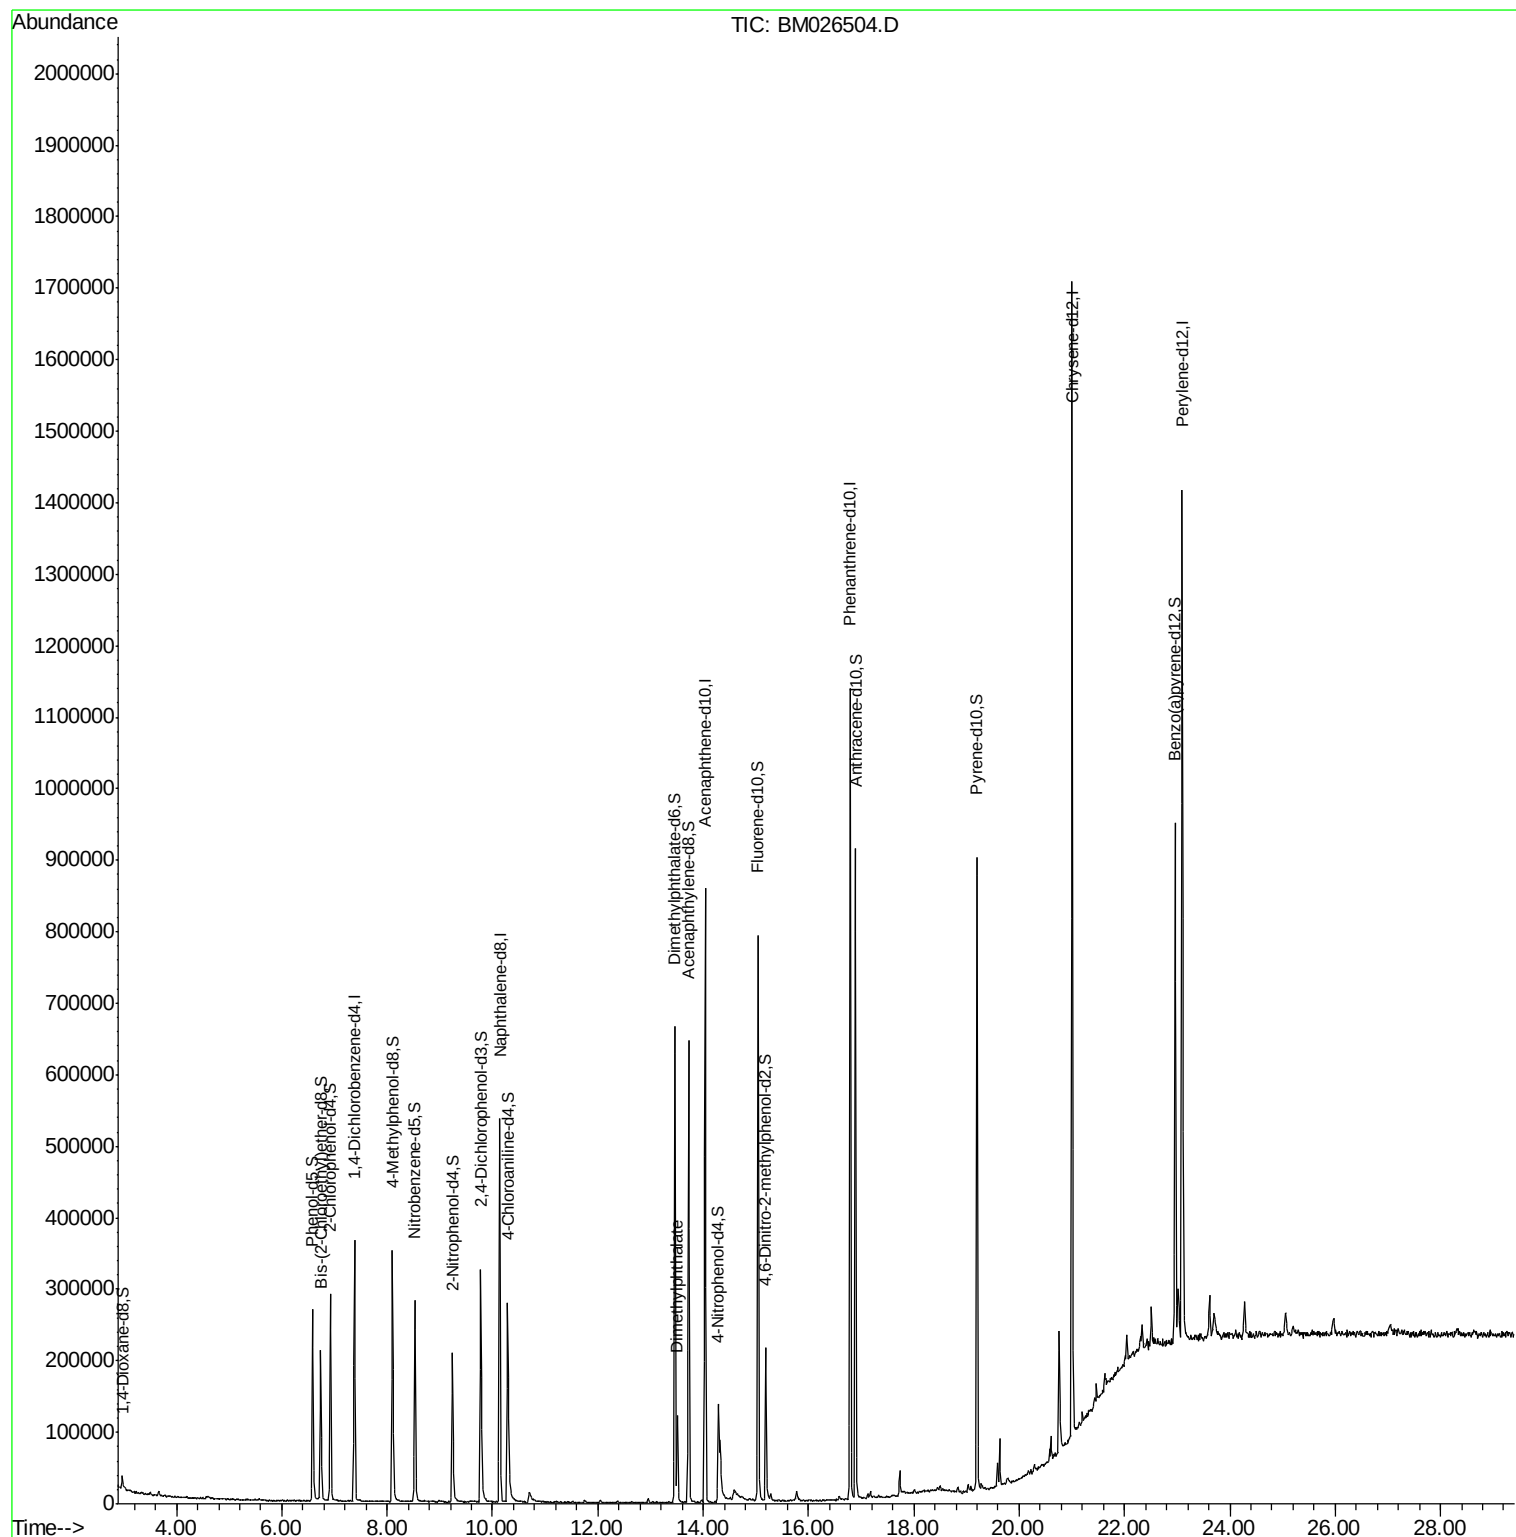

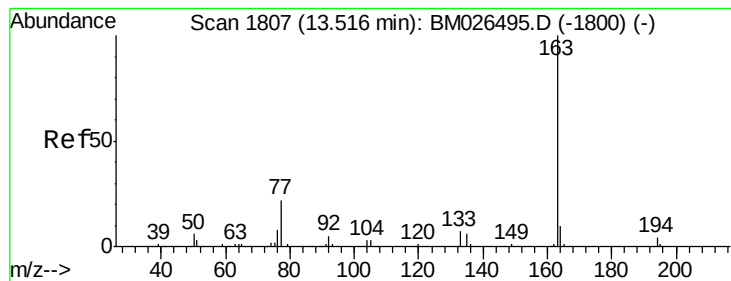

#45

Dimethylphthalate

Concen: 3.103 ng/ul

RT: 13.52 min Scan# 1807

Delta R.T. -0.00 min

Lab File: BM026504.D

Acq: 23 Jun 2020 17:12

Instrument :

BNA_M

ClientSampleId :

BG2K9


Tot Ion:163 Resp: 69535

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 10.7 7.8 11.6

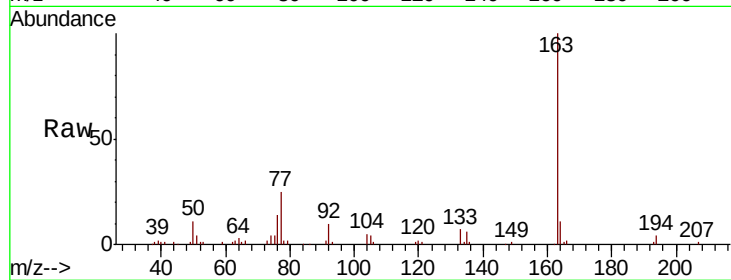

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

