

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
 Data File : BM026505.D
 Acq On : 23 Jun 2020 17:49
 Operator : JU/CG
 Sample : L3027-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG2L1

Quant Time: Jun 23 18:47:20 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 23 10:25:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	92033	20.00	ng/ul	0.00
18) Naphthalene-d8	10.14	136	428761	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.04	164	291017	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.80	188	700693	20.00	ng/ul	0.00
78) Chrysene-d12	21.01	240	836156	20.00	ng/ul	0.00
86) Perylene-d12	23.10	264	833281	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.98	96	8812	3.36	ng/uL	0.00
5) Phenol-d5	6.59	99	142247	16.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	101188	18.87	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	107040	15.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	121408	18.19	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	56086	14.72	ng/ul	0.00
22) 2-Nitrophenol-d4	9.24	143	59277	14.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	116304	15.07	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	150927	18.76	ng/ul	0.00
44) Dimethylphthalate-d6	13.47	166	446269	18.24	ng/ul	0.00
47) Acenaphthylene-d8	13.72	160	442918	15.09	ng/ul	0.00
52) 4-Nitrophenol-d4	14.28	143	54373	13.40	ng/ul	0.00
58) Fluorene-d10	15.04	176	322122	15.34	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	56298	12.28	ng/ul	0.00
71) Anthracene-d10	16.89	188	525439	14.73	ng/ul	0.00
79) Pyrene-d10	19.20	212	633922	13.82	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.97	264	568073	12.33	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.51	163	89053	3.505	ng/ul	97




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
Data File : BM026505.D
Acq On : 23 Jun 2020 17:49
Operator : JU/CG
Sample : L3027-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG2L1

Quant Time: Jun 23 18:47:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 23 10:25:31 2020
Response via : Initial Calibration

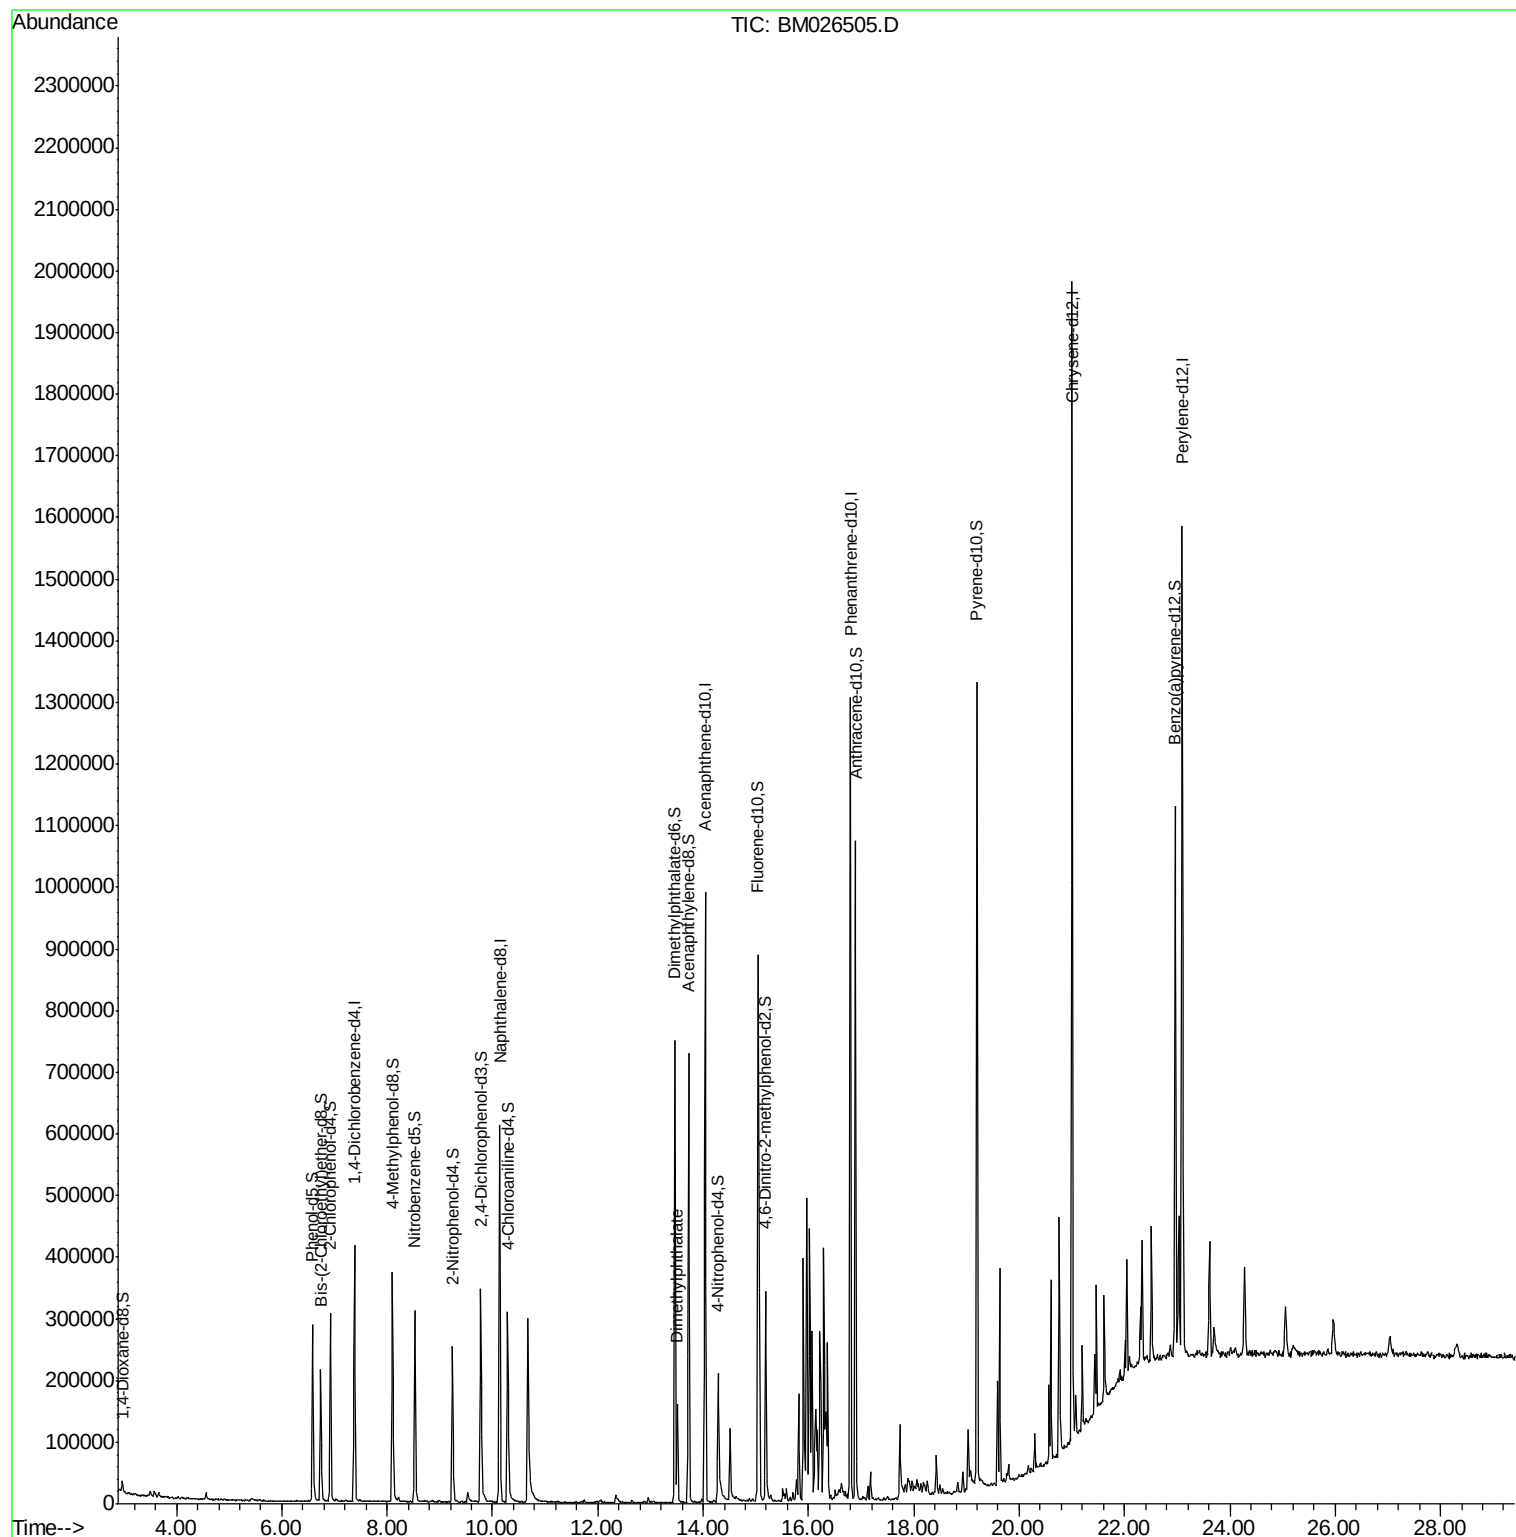

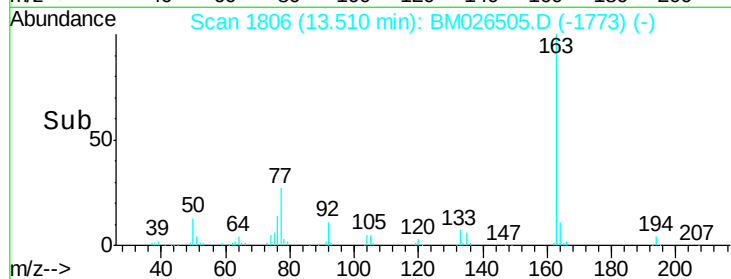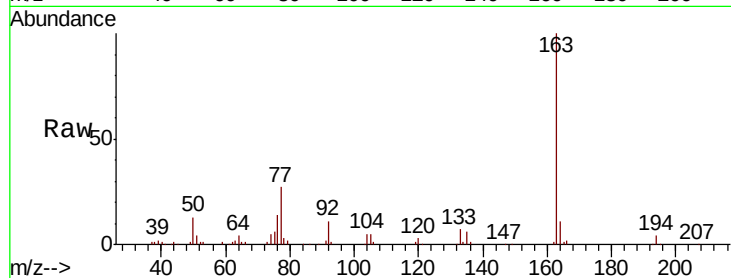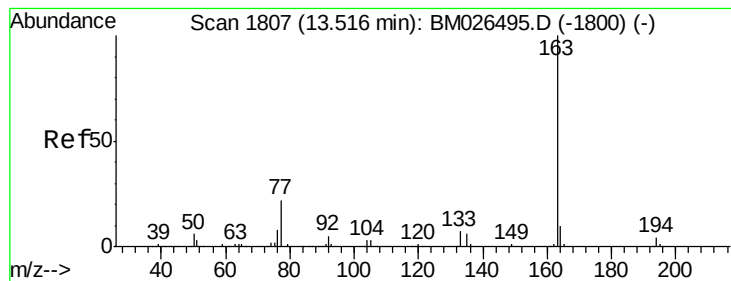

#45

Dimethylphthalate

Concen: 3.505 ng/ul

RT: 13.51 min Scan# 1806

Delta R.T. -0.01 min

Lab File: BM026505.D

Acq: 23 Jun 2020 17:49

Instrument :

BNA_M

ClientSampleId :

BG2L1

Tot Ion:163 Resp: 89053

Ion Ratio Lower Upper

163 100

194 3.8 3.4 5.2

164 10.9 7.8 11.6

