

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
 Data File : BM026507.D
 Acq On : 23 Jun 2020 19:38
 Operator : JU/CG
 Sample : L3027-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BG2L0

Quant Time: Jun 24 00:41:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 23 10:25:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	107678	20.00	ng/ul	0.00
18) Naphthalene-d8	10.14	136	480694	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.04	164	327824	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	768075	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	834685	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	775852	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.98	96	12605	4.11	ng/uL	0.00
5) Phenol-d5	6.59	99	216454	21.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	156075	24.87	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	165556	20.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	184003	23.57	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	86995	20.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.24	143	96162	20.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	167555	19.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	206899	22.93	ng/ul	0.00
44) Dimethylphthalate-d6	13.46	166	640230	23.23	ng/ul	0.00
47) Acenaphthylene-d8	13.72	160	653987	19.78	ng/ul	0.00
52) 4-Nitrophenol-d4	14.28	143	84334	18.45	ng/ul	0.00
58) Fluorene-d10	15.04	176	463471	19.59	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	92113	18.32	ng/ul	0.00
71) Anthracene-d10	16.89	188	774207	19.80	ng/ul	0.00
79) Pyrene-d10	19.20	212	837976	18.31	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.96	264	715745	16.68	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.51	163	81156	2.835	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
Data File : BM026507.D
Acq On : 23 Jun 2020 19:38
Operator : JU/CG
Sample : L3027-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BG2L0

Quant Time: Jun 24 00:41:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 23 10:25:31 2020
Response via : Initial Calibration

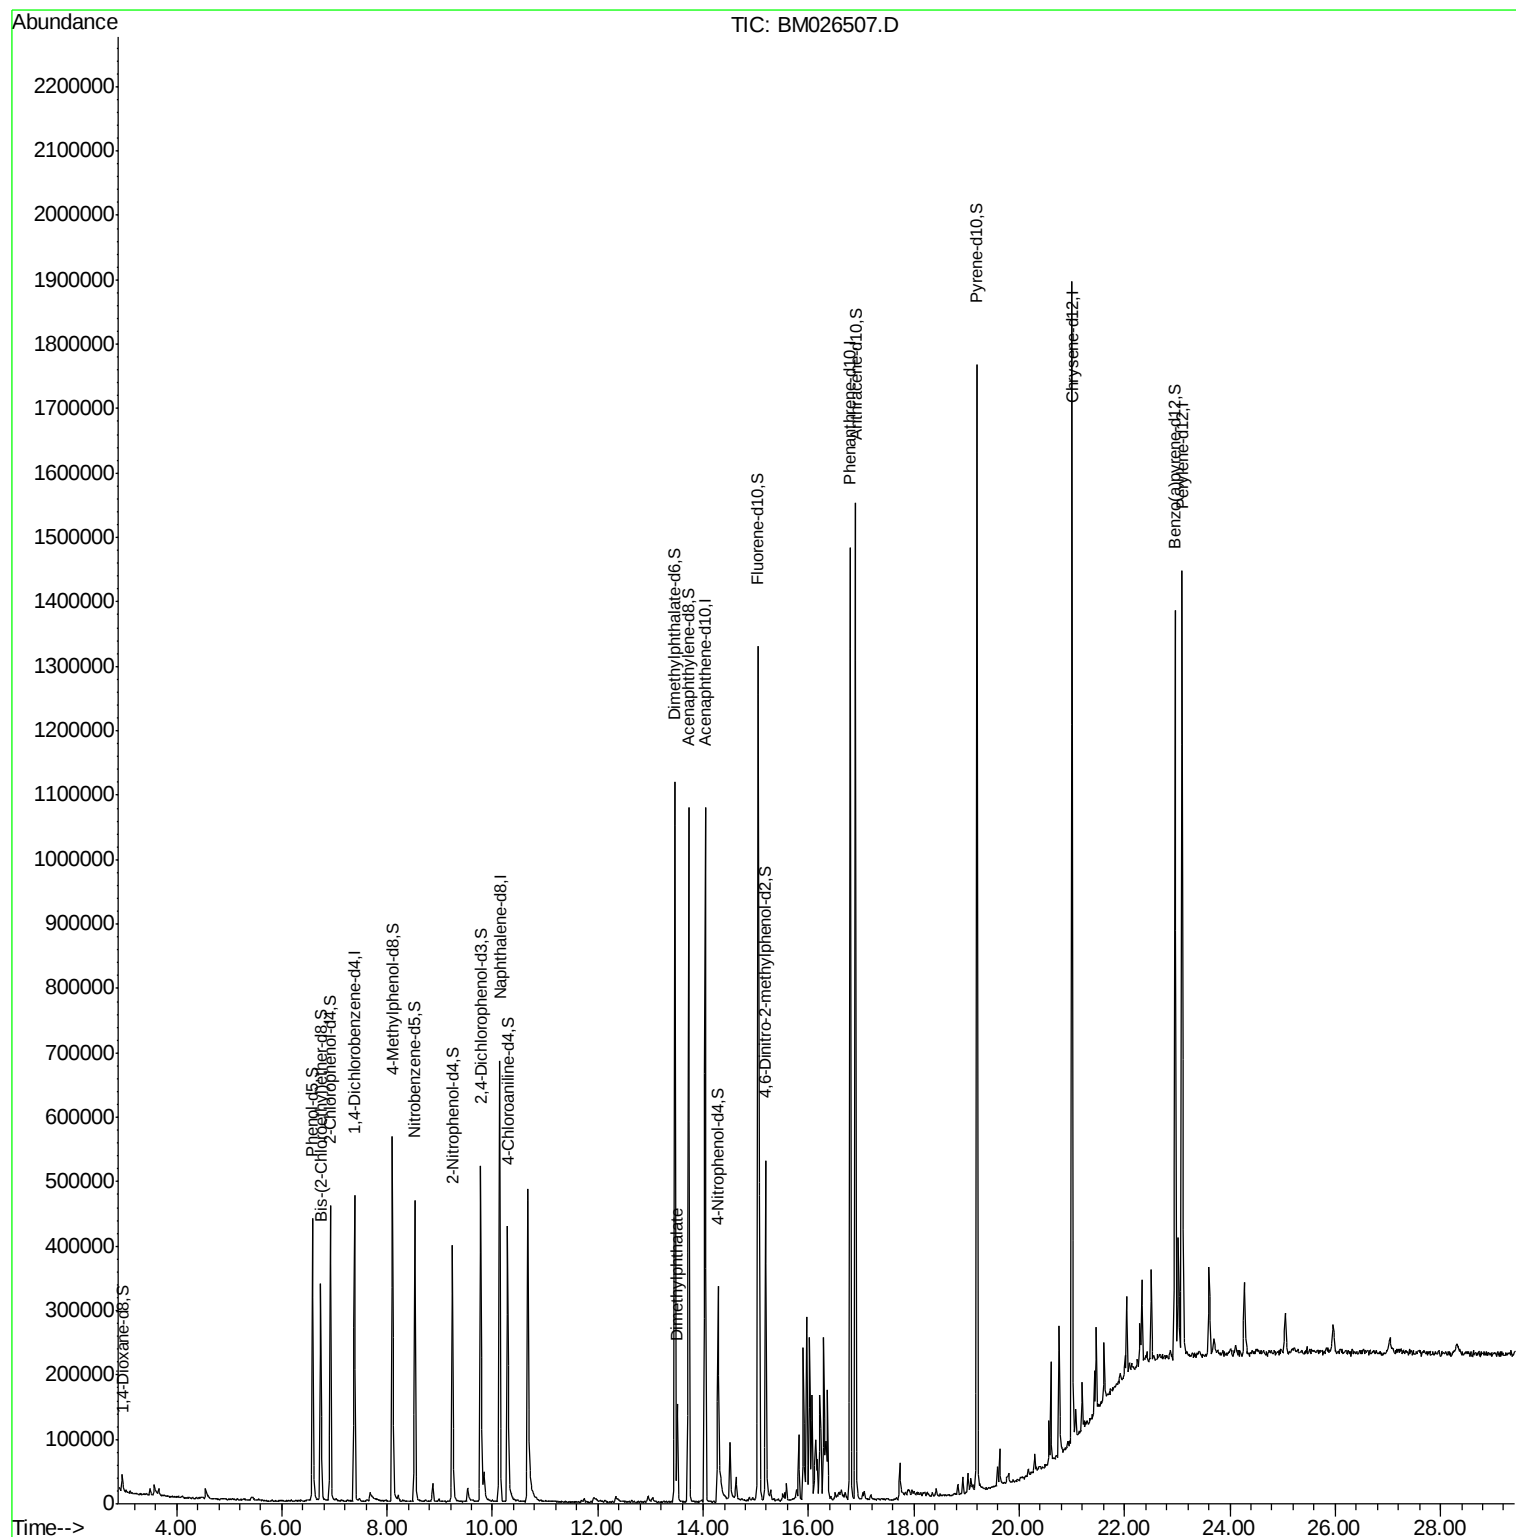

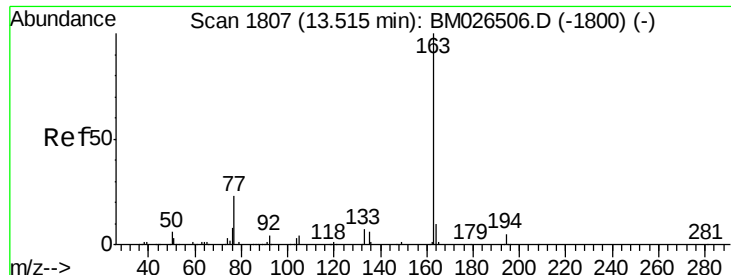

#45

Dimethylphthalate

Concen: 2.835 ng/ul

RT: 13.51 min Scan# 1806

Delta R.T. -0.01 min

Lab File: BM026507.D

Acq: 23 Jun 2020 19:38

Instrument :

BNA_M

ClientSampleId :

BG2L0

Tot Ion:163 Resp: 81156

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 9.6 7.8 11.6

