

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
 Data File : BM026526.D
 Acq On : 24 Jun 2020 08:56
 Operator : JU/CG
 Sample : L3069-08DL 2X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB7G2DL

Quant Time: Jun 24 10:33:08 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 23 10:25:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	133664	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	603534	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	395352	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	836884	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	695554	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	589905	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.97	96	8526	2.24	ng/uL	0.00
5) Phenol-d5	6.59	99	30876	2.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	71435	9.17	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	75105	7.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	56239	5.80	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	41133	7.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.24	143	47065	7.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	88810	8.18	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	116120	10.25	ng/ul	0.00
44) Dimethylphthalate-d6	13.46	166	286664	8.62	ng/ul	0.00
47) Acenaphthylene-d8	13.72	160	296151	7.43	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0d	0.00	ng/ul	0.00
58) Fluorene-d10	15.04	176	212338	7.44	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	22765	4.16	ng/ul	0.00
71) Anthracene-d10	16.89	188	320373	7.52	ng/ul	0.00
79) Pyrene-d10	19.20	212	332963	8.73	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.96	264	195223	5.99	ng/ul	0.00

Target Compounds


					Ovalue
2) 1,4-Dioxane	3.00	88	96572	22.854	ng/uL 96
45) Dimethylphthalate	13.51	163	91001	2.636	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
Data File : BM026526.D
Acq On : 24 Jun 2020 08:56
Operator : JU/CG
Sample : L3069-08DL 2X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB7G2DL

Quant Time: Jun 24 10:33:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 23 10:25:31 2020
Response via : Initial Calibration

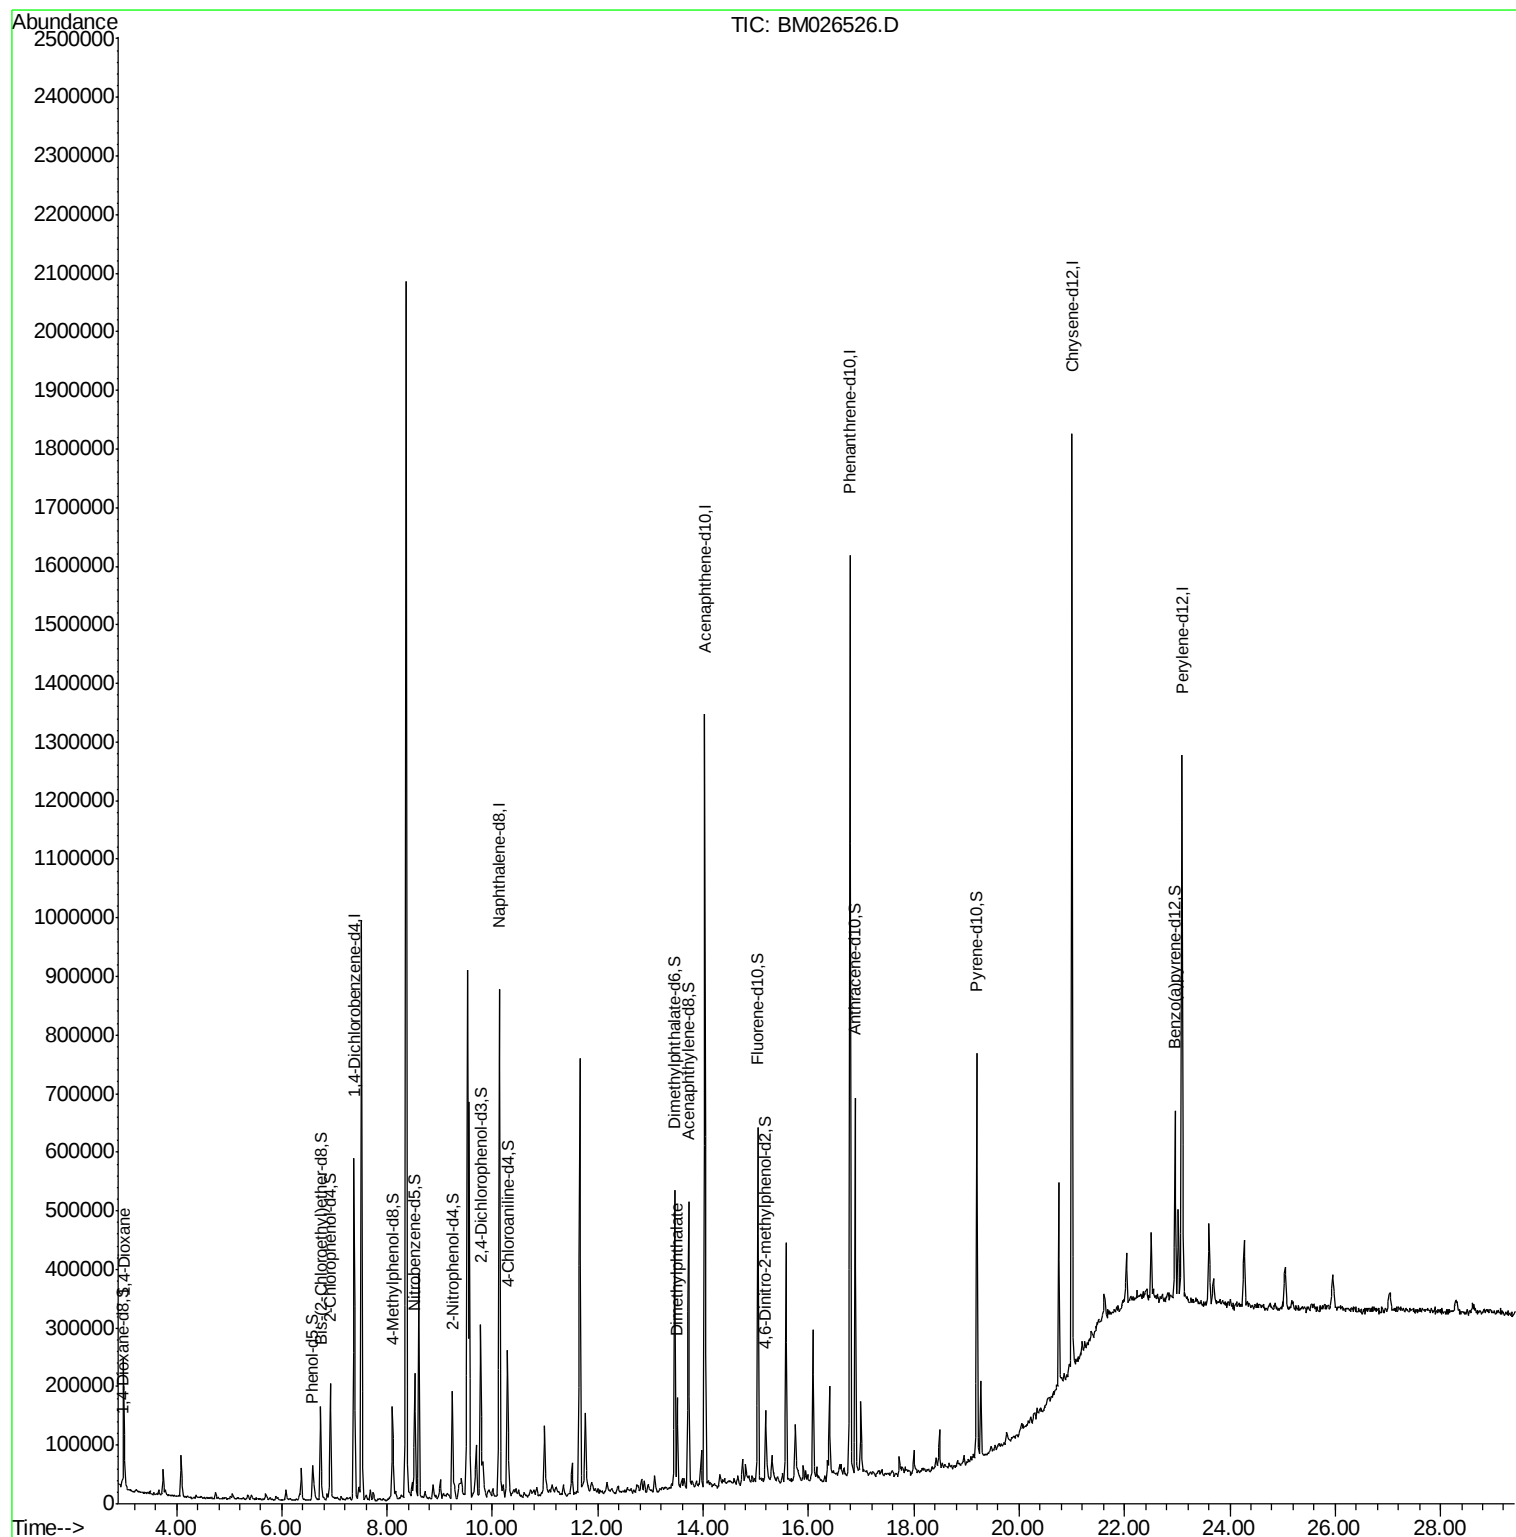

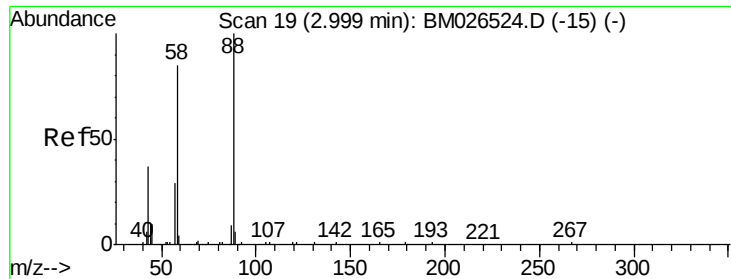

#2

1,4-Dioxane

Concen: 22.854 ng/uL

RT: 3.00 min Scan# 19

Delta R.T. -0.00 min

Lab File: BM026526.D

Acq: 24 Jun 2020 08:56

Instrument :

BNA_M

ClientSampleId :

CB7G2DL





Tot Ion: 88 Resp: 96572

Ion Ratio Lower Upper

88 100

43 37.1 33.2 49.8

58 87.3 67.8 101.6

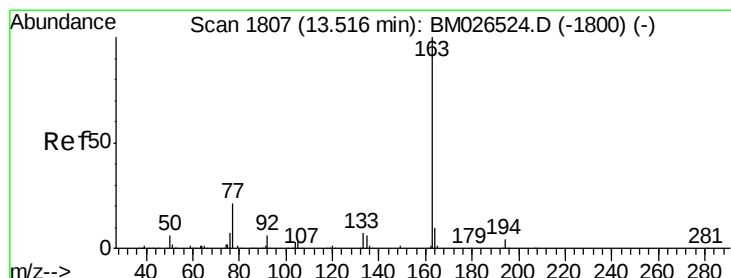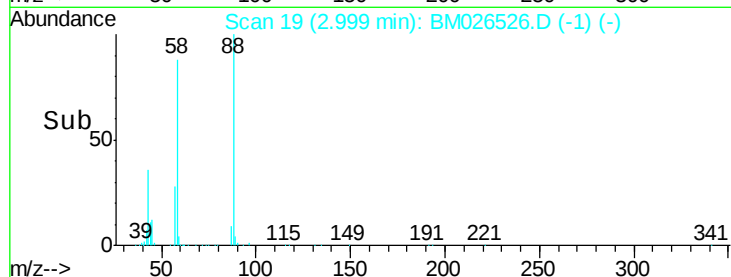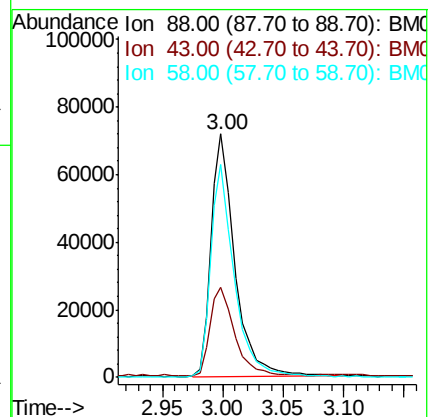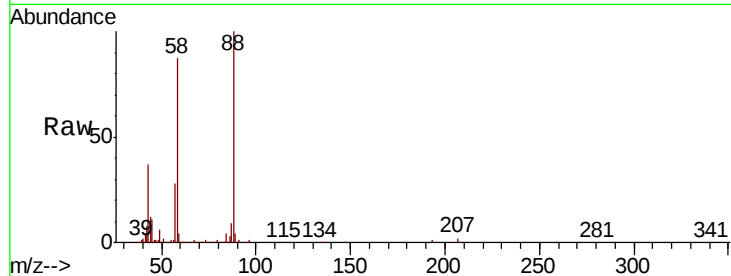

#45

Dimethylphthalate

Concen: 2.636 ng/uL

RT: 13.51 min Scan# 1806

Delta R.T. -0.01 min

Lab File: BM026526.D

Acq: 24 Jun 2020 08:56

Tgt Ion: 163 Resp: 91001

Ion Ratio Lower Upper

163 100

194 4.6 3.4 5.2

164 9.2 7.8 11.6

