

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
 Data File : BM026538.D
 Acq On : 24 Jun 2020 19:11
 Operator : JU/CG
 Sample : L3064-04
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET157

Manual Integrations
 APPROVED

Sohil
 6/25/2020 8:51:07 AM

Quant Time: Jun 25 03:53:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 23 10:25:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	95359	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	441321	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	305694	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	694172	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	754432	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	697908	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.97	96	4570	1.68	ng/uL	0.00
5) Phenol-d5	6.59	99	71185	8.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	62697	11.28	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	63936	8.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	68144	9.86	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	33163	8.46	ng/ul	0.00
22) 2-Nitrophenol-d4	9.24	143	30035	6.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	63674	8.02	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	87503	10.56	ng/ul	0.00
44) Dimethylphthalate-d6	13.46	166	257434	10.02	ng/ul	0.00
47) Acenaphthylene-d8	13.72	160	268008	8.69	ng/ul	0.00
52) 4-Nitrophenol-d4	14.31	143	12484m	2.93	ng/ul	0.03
58) Fluorene-d10	15.04	176	201504	9.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	13605	2.99	ng/ul	0.00
71) Anthracene-d10	16.89	188	341085	9.65	ng/ul	0.00
79) Pyrene-d10	19.20	212	403330	9.75	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.96	264	385789	10.00	ng/ul	-0.01

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.51	163	47954	1.797	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
Data File : BM026538.D
Acq On : 24 Jun 2020 19:11
Operator : JU/CG
Sample : L3064-04
Misc :
ALS Vial : 49 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
ET157

Manual Integrations
APPROVED

Sohil
6/25/2020 8:51:07 AM

Quant Time: Jun 25 03:53:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 23 10:25:31 2020
Response via : Initial Calibration

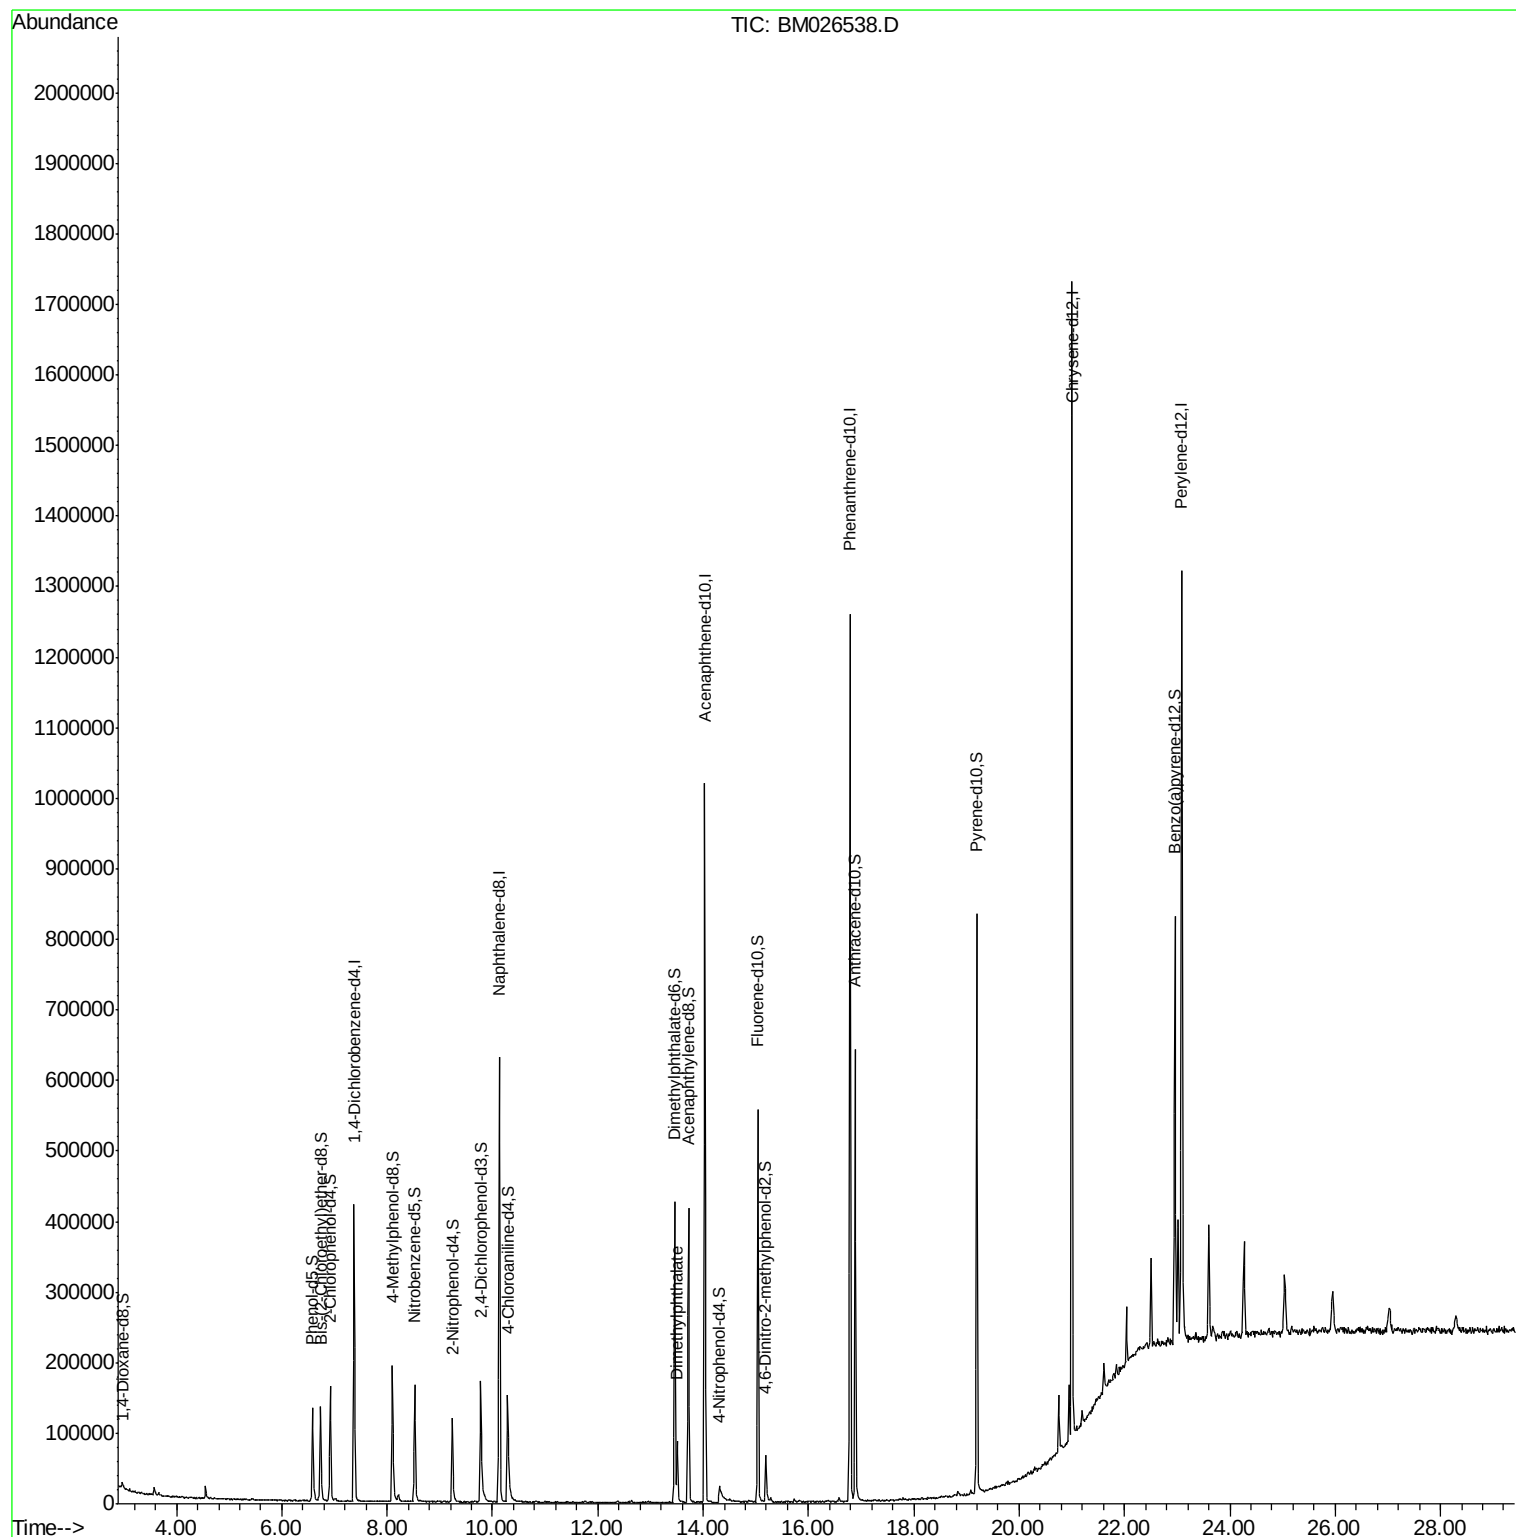

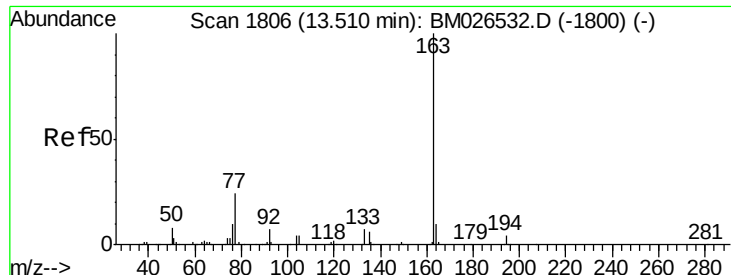

#45
 Dimethylphthalate
 Concen: 1.797 ng/ul
 RT: 13.51 min Scan# 1806
 Delta R.T. -0.01 min
 Lab File: BM026538.D
 Acq: 24 Jun 2020 19:11

Instrument :
 BNA_M
 ClientSampleId :
 ET157

Tot Ion:	163	Resp:	47954
Ion Ratio	Lower	Upper	
163	100		
194	4.4	3.4	5.2
164	10.4	7.8	11.6

Manual Integrations
 APPROVED

Sohil
 6/25/2020 8:51:07 AM

