

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
 Data File : BM026539.D
 Acq On : 24 Jun 2020 19:47
 Operator : JU/CG
 Sample : L3064-08
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET162

Manual Integrations
 APPROVED

Sohil
 6/25/2020 8:51:08 AM

Quant Time: Jun 25 03:59:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 23 10:25:31 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	89522	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	393009	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	264681	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	592652	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	624144	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	562966	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.98	96	2592	1.02	ng/uL	0.00
5) Phenol-d5	6.59	99	49990	6.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	37598	7.21	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	40320	6.00	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	42306	6.52	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	18502	5.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.24	143	18245	4.75	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.79	165	35223	4.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	47271	6.41	ng/ul	0.00
44) Dimethylphthalate-d6	13.46	166	146371	6.58	ng/ul	0.00
47) Acenaphthylene-d8	13.72	160	133114	4.99	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	5658m	1.53	ng/ul	0.04
58) Fluorene-d10	15.04	176	98859	5.18	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	6005	1.55	ng/ul	0.00
71) Anthracene-d10	16.89	188	144048	4.77	ng/ul	0.00
79) Pyrene-d10	19.20	212	153842	4.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.96	264	107946	3.47	ng/ul	0.00

Target Compounds					Ovalue	
45) Dimethylphthalate	13.51	163	47418	2.052	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062320\
Data File : BM026539.D
Acq On : 24 Jun 2020 19:47
Operator : JU/CG
Sample : L3064-08
Misc :
ALS Vial : 50 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
ET162

Quant Time: Jun 25 03:59:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 23 10:25:31 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
6/25/2020 8:51:08 AM

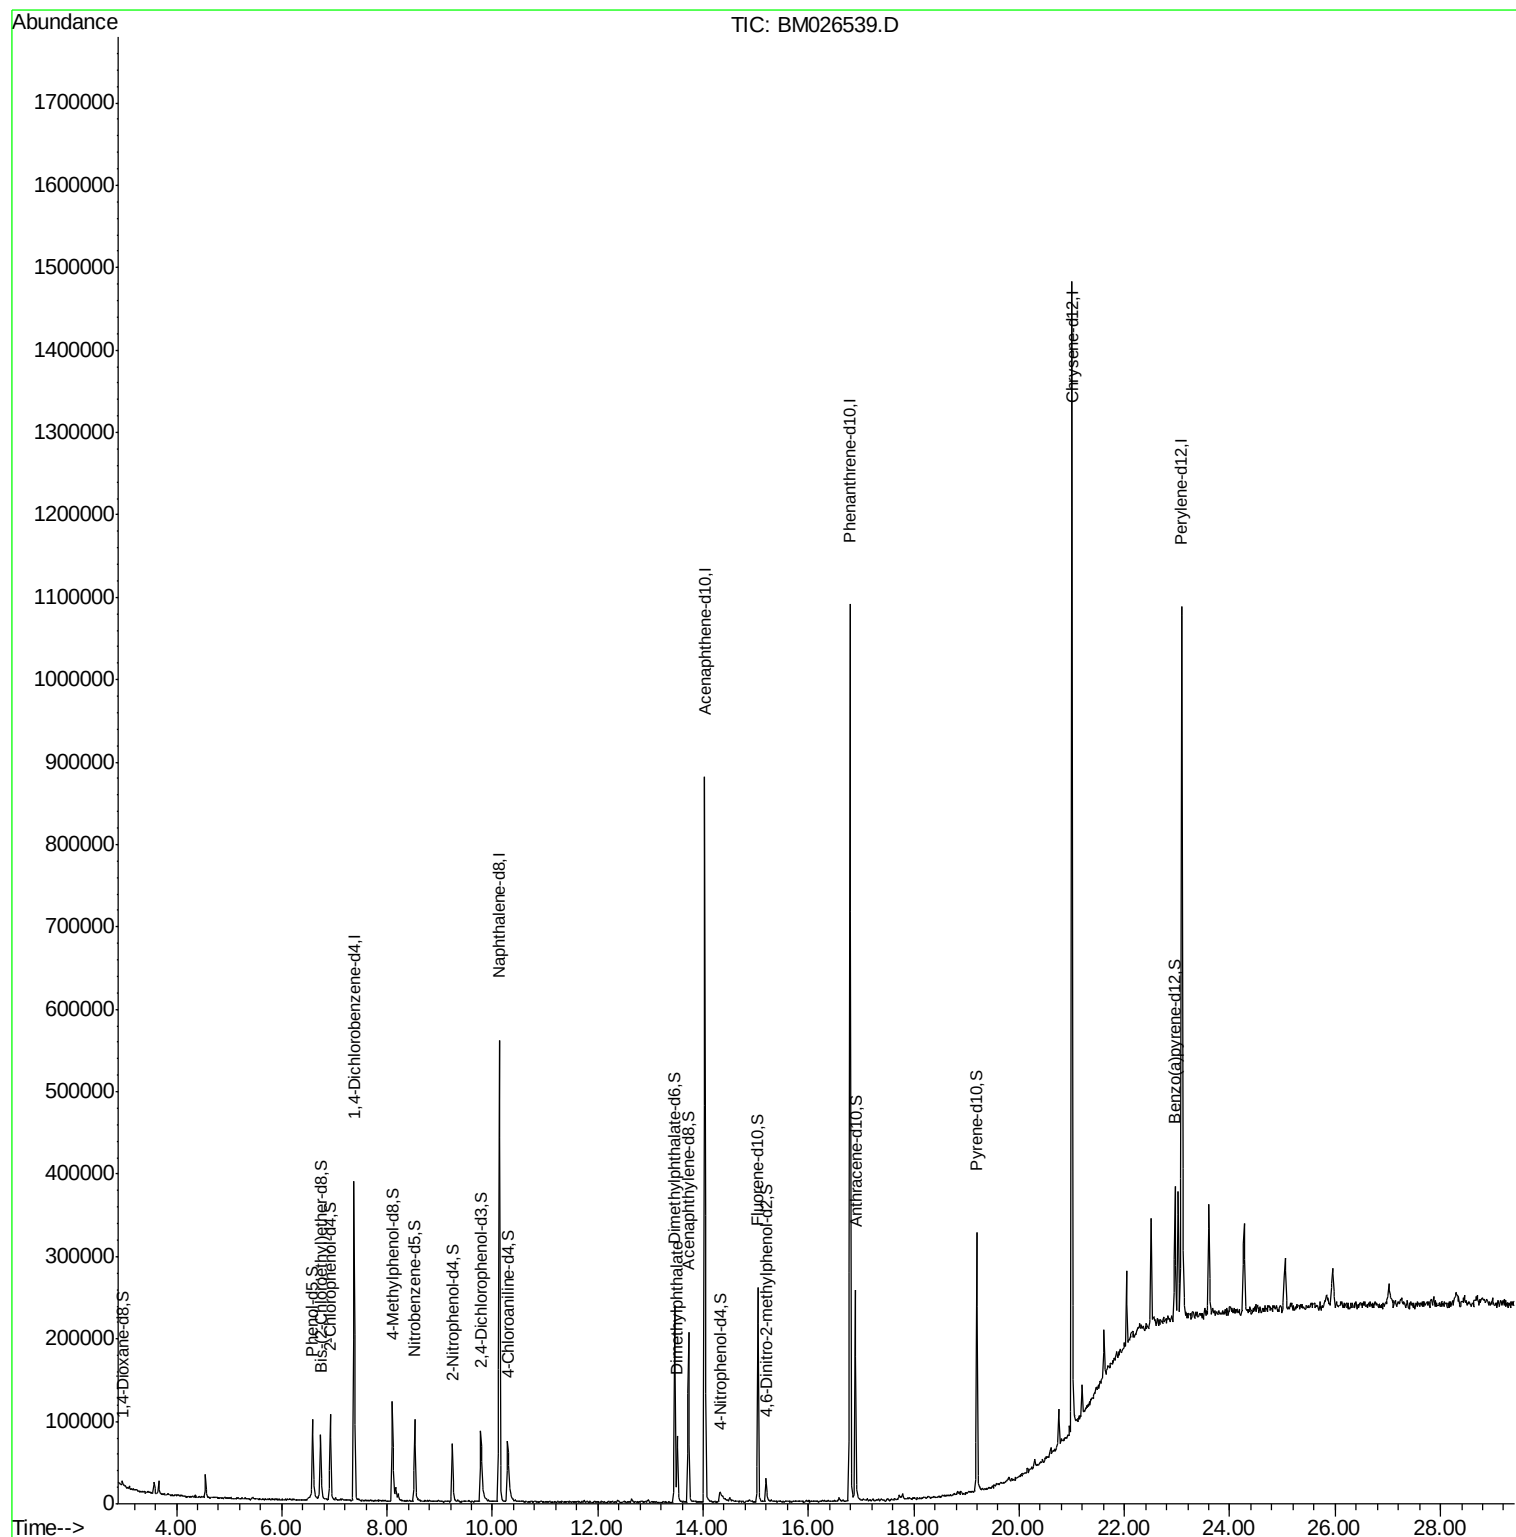

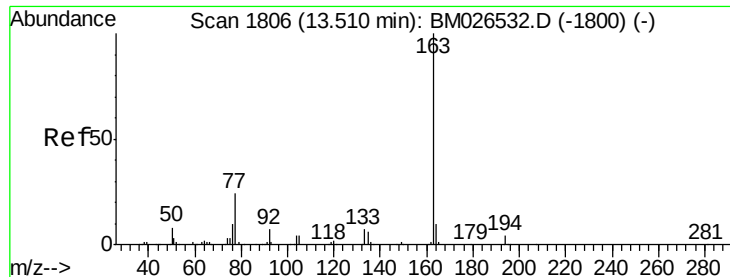

#45
 Dimethylphthalate
 Concen: 2.052 ng/ul
 RT: 13.51 min Scan# 1806
 Delta R.T. -0.01 min
 Lab File: BM026539.D
 Acq: 24 Jun 2020 19:47

Instrument :
 BNA_M
 ClientSampleId :
 ET162

Tot Ion	Ratio	Resp	Lower	Upper
163	100	47418		
194	3.9		3.4	5.2
164	10.8		7.8	11.6

Manual Integrations
 APPROVED

Sohil
 6/25/2020 8:51:08 AM

