

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062416\
 Data File : BM005965.D
 Acq On : 24 Jun 2016 13:18
 Operator : UM/SJ
 Sample : H3639-13
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9Z28

Quant Time: Jun 24 23:55:34 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 24 23:55:23 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	175623	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	769159	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.31	164	416403	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	882823	20.00	ng/ul	0.00
75) Chrysene-d12	21.25	240	955789	20.00	ng/ul	0.00
83) Perylene-d12	23.47	264	979782	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.19	96	7481	1.70	ng/uL	0.00
5) Phenol-d5	6.83	99	330626	21.86	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	218582	23.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	252811	21.23	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	274452	23.16	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	120534	21.30	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	128620	21.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	249075	21.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.58	131	363885	29.31	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	877919	26.54	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	1055005	25.53	ng/ul	0.00
51) 4-Nitrophenol-d4	14.50	143	127889	19.77	ng/ul	0.00
57) Fluorene-d10	15.30	176	761158	26.63	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	96450	21.93	ng/ul	0.00
70) Anthracene-d10	17.15	188	1188783	29.56	ng/ul	0.00
76) Pyrene-d10	19.45	212	1338321	30.17	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.33	264	1400832	31.73	ng/ul	0.00


Target Compounds						Qvalue
44) Dimethylphthalate	13.77	163	222905	6.68	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062416\
Data File : BM005965.D
Acq On : 24 Jun 2016 13:18
Operator : UM/SJ
Sample : H3639-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
D9Z28

Quant Time: Jun 24 23:55:34 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 24 23:55:23 2016
Response via : Initial Calibration

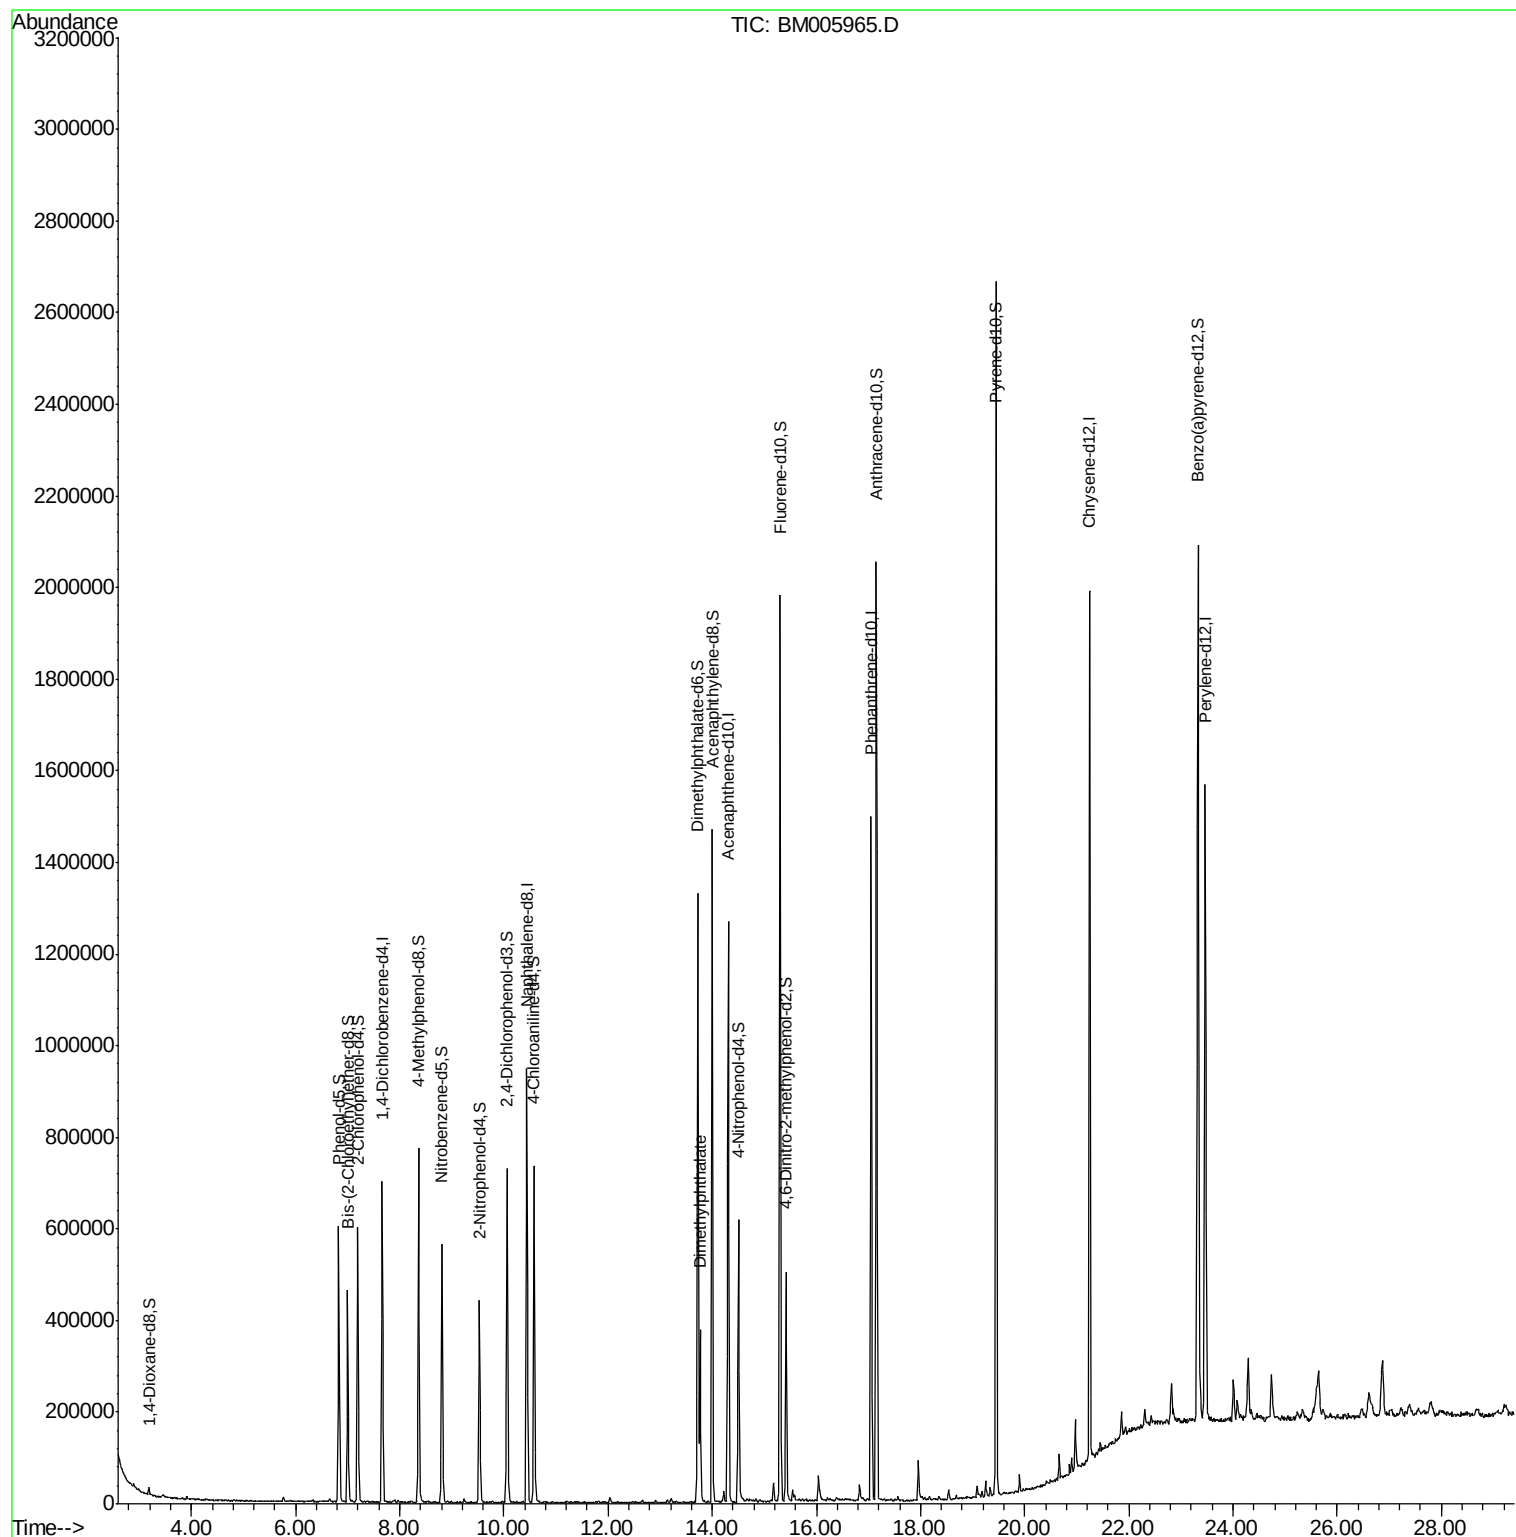


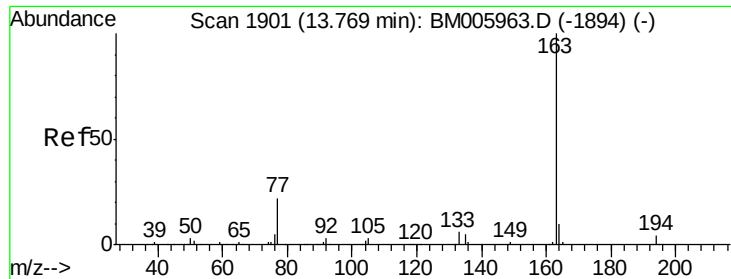

#44
 Dimethylphthalate
 Concen: 6.68 ng/ul
 RT: 13.77 min Scan# 1901
 Delta R.T. -0.00 min
 Lab File: BM005965.D
 Acq: 24 Jun 2016 13:18

Instrument :
 BNA_M
 ClientSampleId :
 D9Z28

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.1	4.7
164	9.8	7.9	11.9

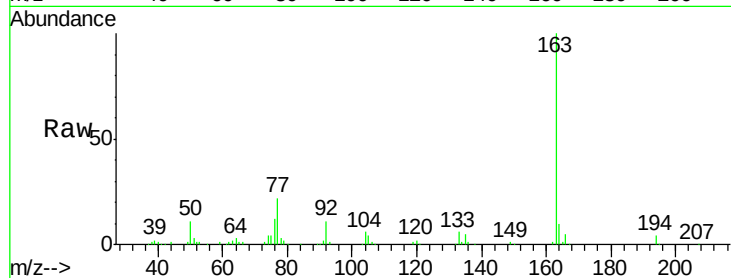

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

