

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062416\
 Data File : BM005970.D
 Acq On : 24 Jun 2016 17:49
 Operator : UM/SJ
 Sample : H3635-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C05D5

Quant Time: Jun 24 23:56:13 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 24 23:55:23 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	189540	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	817932	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	448736	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	1035083	20.00	ng/ul	0.00
75) Chrysene-d12	21.25	240	1216009	20.00	ng/ul	0.00
83) Perylene-d12	23.47	264	1200378	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.19	96	4571	0.96	ng/uL	0.00
5) Phenol-d5	6.83	99	174291	10.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	448433	44.90	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	459570	35.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	224271	17.54	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	272396	45.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	292432	46.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	504991	41.86	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	453	0.03	ng/ul	0.00
43) Dimethylphthalate-d6	13.72	166	1620521	45.45	ng/ul	0.00
46) Acenaphthylene-d8	14.00	160	2015003	45.25	ng/ul	0.00
51) 4-Nitrophenol-d4	14.53	143	78285	11.23	ng/ul	0.02
57) Fluorene-d10	15.30	176	1382624	44.89	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.42	200	239234	46.40	ng/ul	0.00
70) Anthracene-d10	17.16	188	2161997	45.85	ng/ul	0.00
76) Pyrene-d10	19.45	212	2403611	42.59	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.33	264	2397632	44.33	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
56) Diethylphthalate	15.14	149	70832	1.90	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062416\
Data File : BM005970.D
Acq On : 24 Jun 2016 17:49
Operator : UM/SJ
Sample : H3635-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C05D5

Quant Time: Jun 24 23:56:13 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062216.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 24 23:55:23 2016
Response via : Initial Calibration

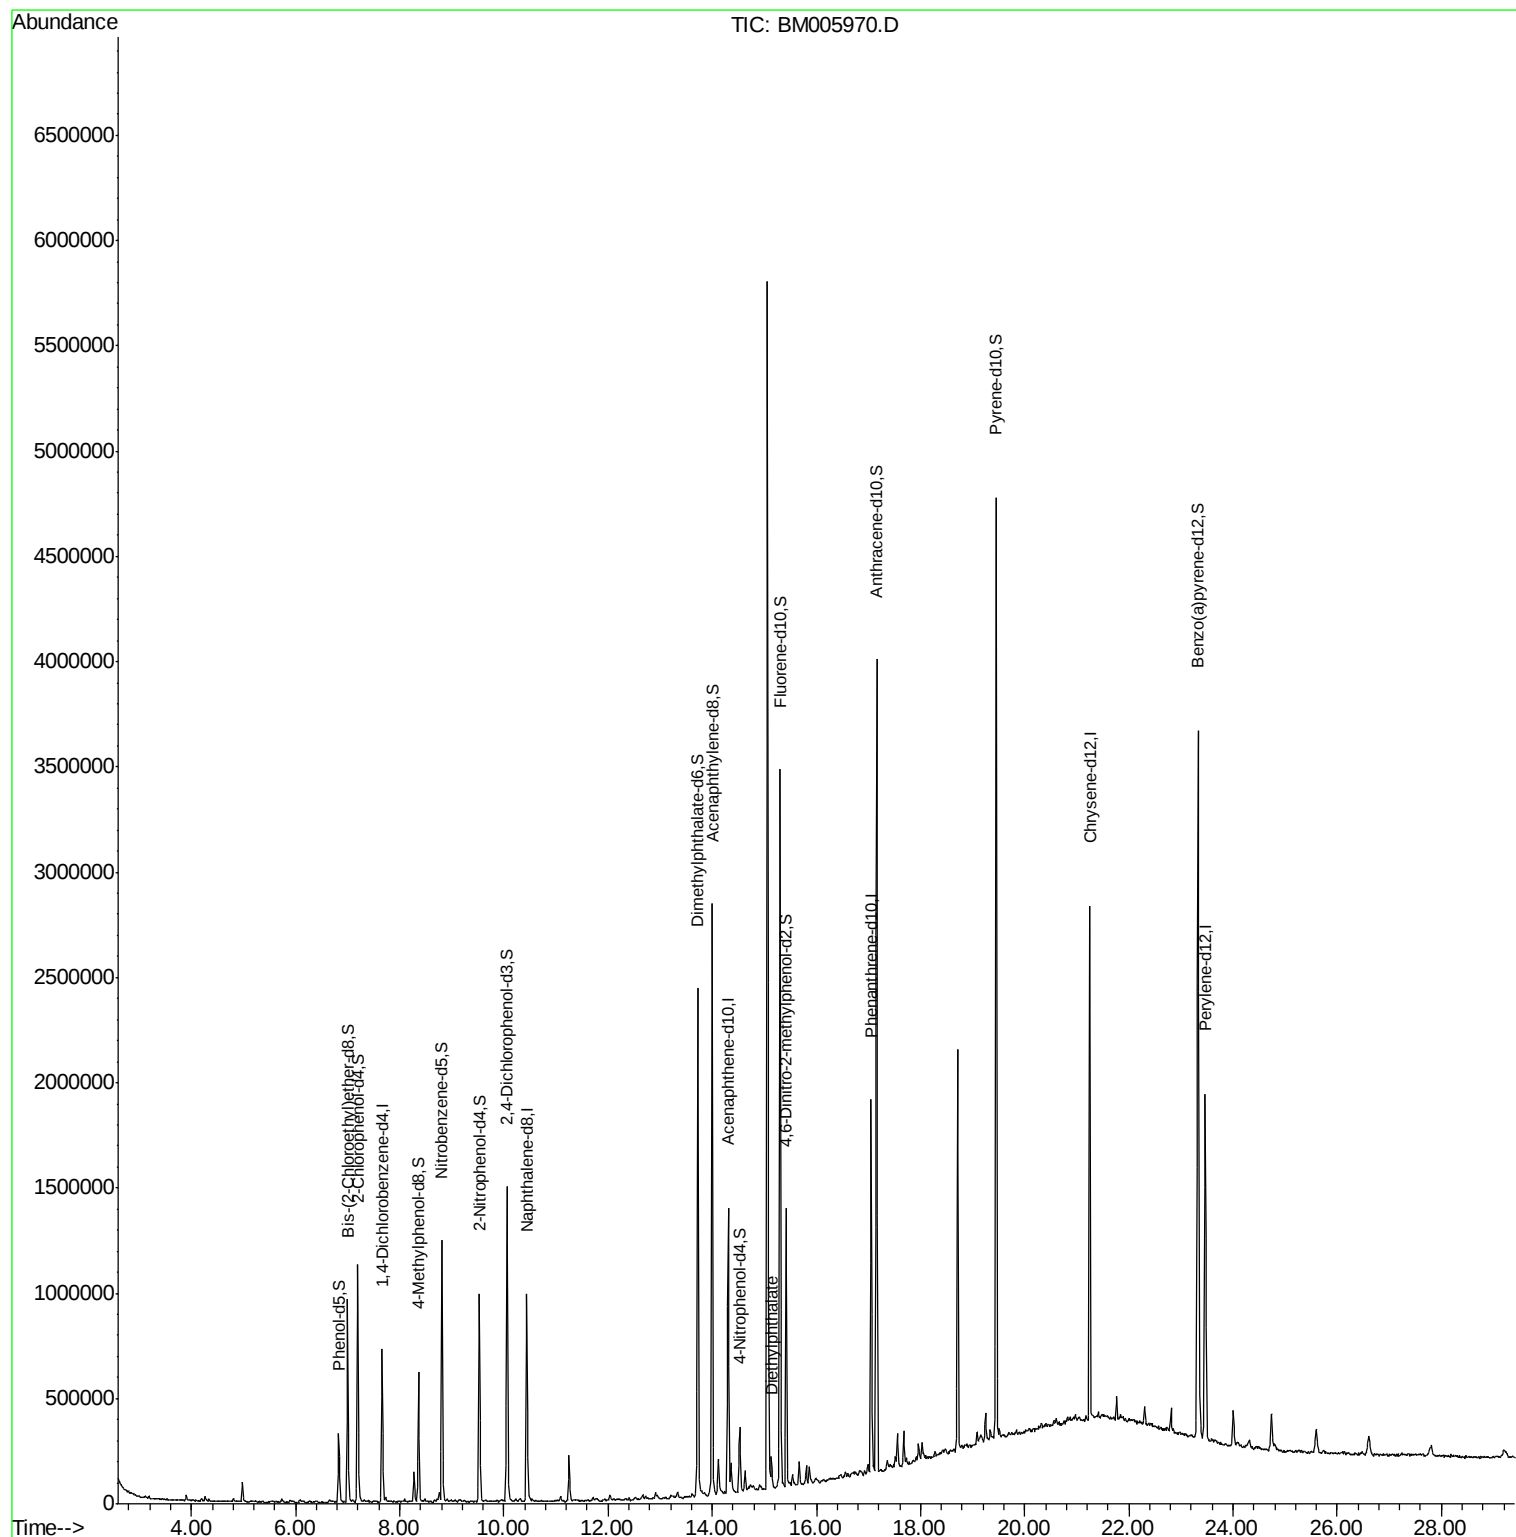

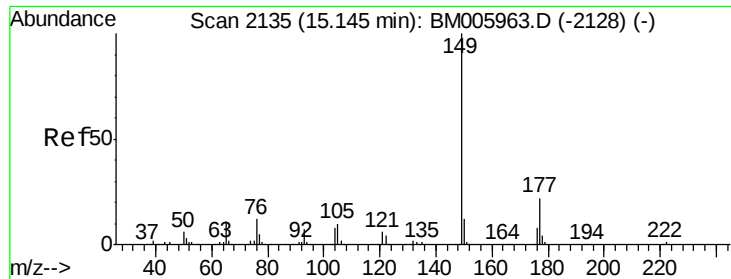

#56
 Diethylphthalate
 Concen: 1.90 ng/ul
 RT: 15.14 min Scan# 2134
 Delta R.T. -0.01 min
 Lab File: BM005970.D
 Acq: 24 Jun 2016 17:49

Instrument :
 BNA_M
 ClientSampleId :
 C05D5

Tgt Ion	Ratio	Lower	Upper
149	100		
177	21.1	17.4	26.0
150	11.1	9.7	14.5

