

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062424\
 Data File : BM046259.D
 Acq On : 24 Jun 2024 18:44
 Operator : MA/JU
 Sample : P2961-17
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1G72

Quant Time: Jun 25 02:26:47 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 24 02:25:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.404	152	1756	0.400	ng/ul	-0.06
4) Naphthalene-d8	10.172	136	5630	0.400	ng/ul	-0.08
9) Acenaphthene-d10	14.053	164	3219	0.400	ng/ul	#-0.06
13) Phenanthrene-d10	16.896	188	561755	0.400	ng/ul	# 0.04
17) Chrysene-d12	21.026	240	4698	0.400	ng/ul	-0.02
23) Perylene-d12	23.092	264	10880	0.400	ng/ul	#-0.05
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.021	96	9635	3.999	ng/ul	-0.03
6) 2-Methylnaphthalene-d10	11.811	152	2689	0.356	ng/ul	-0.05
18) Fluoranthene-d10	18.835	212	6076	0.432	ng/ul	-0.05
Target Compounds						
					Qvalue	
20) Pyrene	19.197	202	1305	0.059	ng/ul#	1
26) Benzo(a)pyrene	22.960	252	2821	0.078	ng/ul#	53


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062424\
Data File : BM046259.D
Acq On : 24 Jun 2024 18:44
Operator : MA/JU
Sample : P2961-17
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1G72

Quant Time: Jun 25 02:26:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration




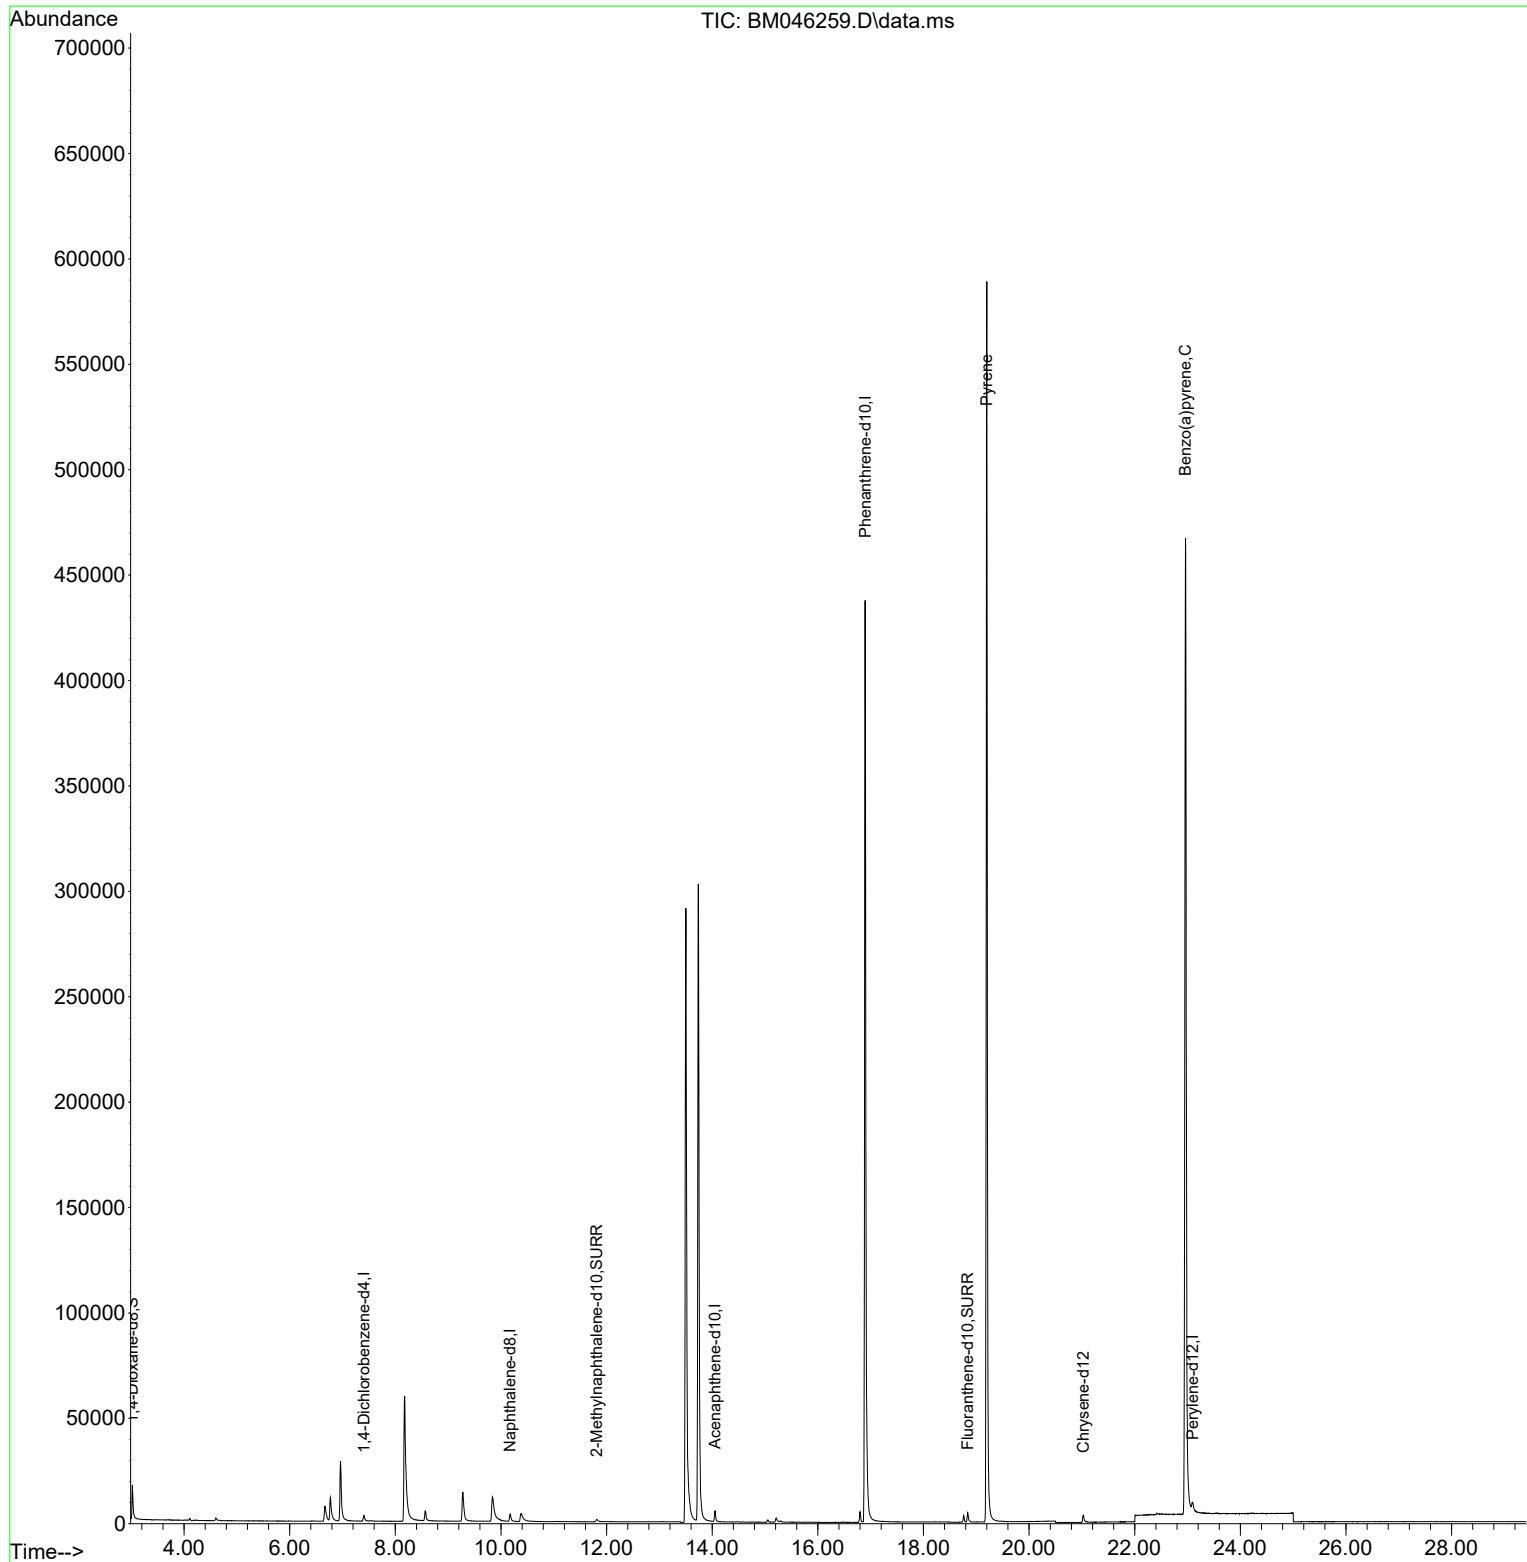


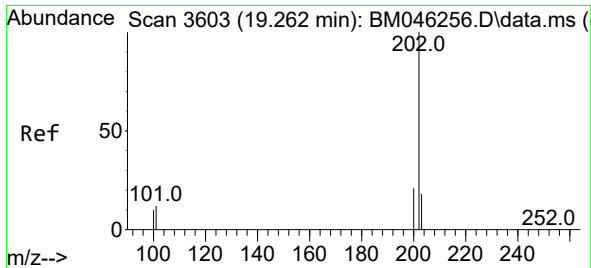

#20
Pyrene
Concen: 0.059 ng/ul
RT: 19.197 min Scan# 3589
Delta R.T. -0.078 min
Lab File: BM046259.D
Acq: 24 Jun 2024 18:44

Instrument :
BNA_M
ClientSampleId :
E1G72

Tgt Ion:202 Resp: 1305
Ion Ratio Lower Upper
202 100
101 203.0 11.3 16.9#
100 1547.0 9.8 14.6#

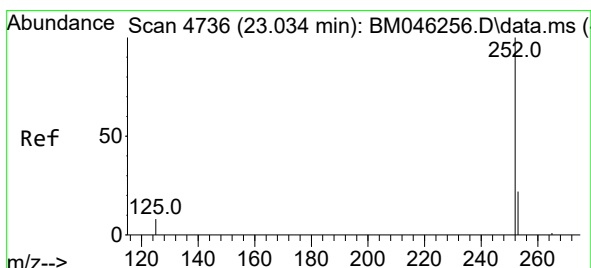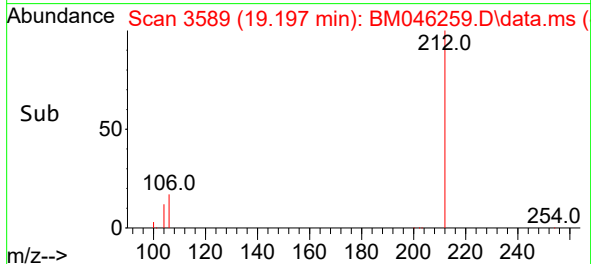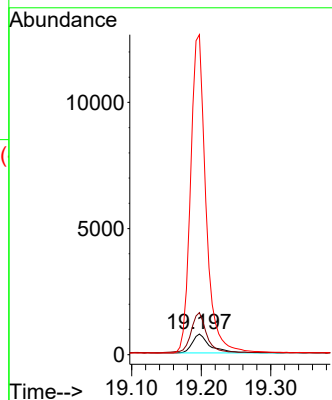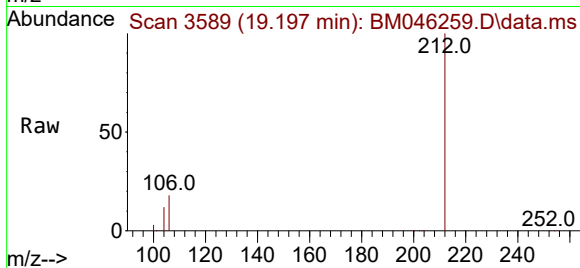

#26
Benzo(a)pyrene
Concen: 0.078 ng/ul
RT: 22.960 min Scan# 4711
Delta R.T. -0.094 min
Lab File: BM046259.D
Acq: 24 Jun 2024 18:44

Tgt Ion:252 Resp: 2821
Ion Ratio Lower Upper
252 100
253 64.1 32.1 48.1#
125 57.3 21.2 31.8#

