




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062424\
Data File : BM046265.D
Acq On : 24 Jun 2024 22:22
Operator : MA/JU
Sample : P2776-22DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C76DL

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:27:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/25/2024
Supervised By :mohammad ahmed 06/27/2024

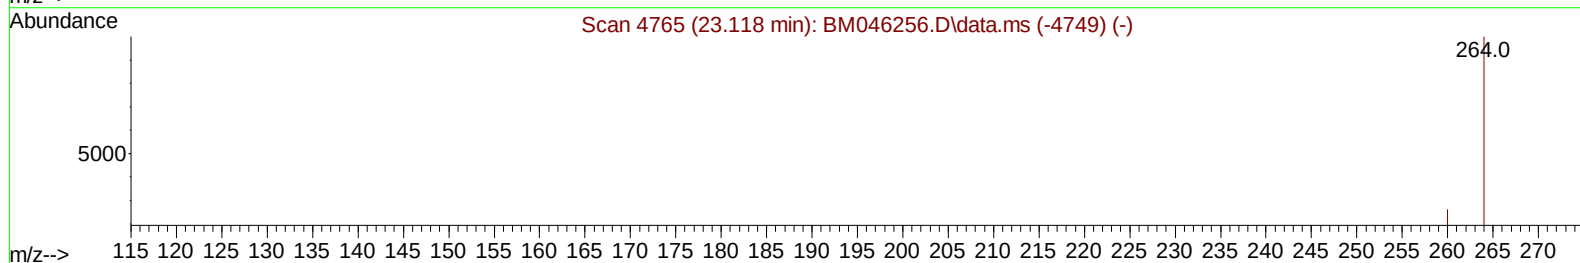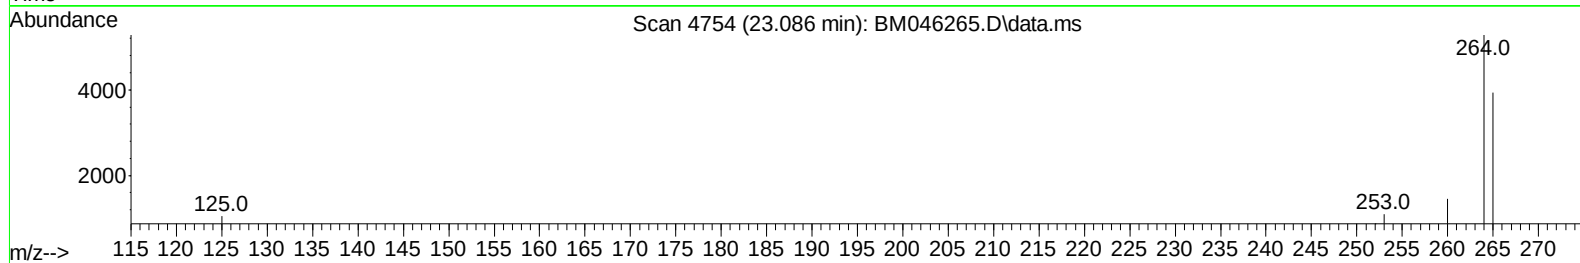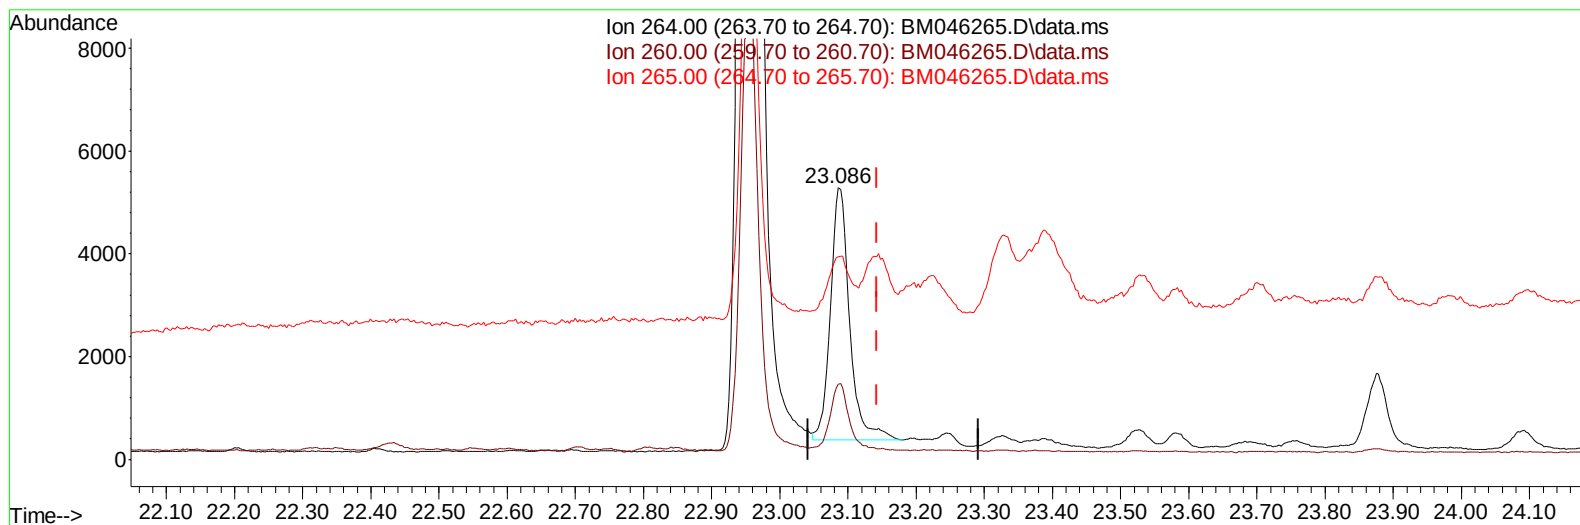

TIC: BM046265.D\data.ms

(23) Perylene-d12 (I)

23.086min (-0.056) 0.40 ng/u1

response 9542

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.20	27.61
265.00	110.60	74.55#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062424\
Data File : BM046265.D
Acq On : 24 Jun 2024 22:22
Operator : MA/JU
Sample : P2776-22DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C76DL

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:27:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/25/2024
Supervised By :mohammad ahmed 06/27/2024

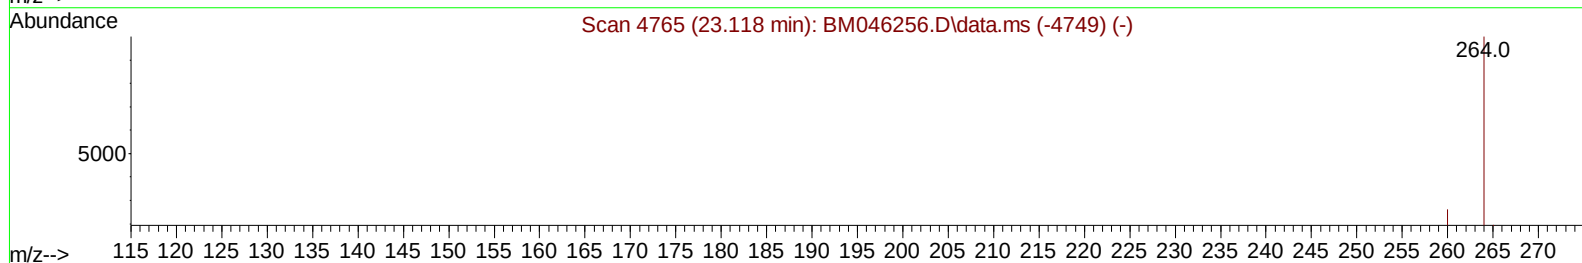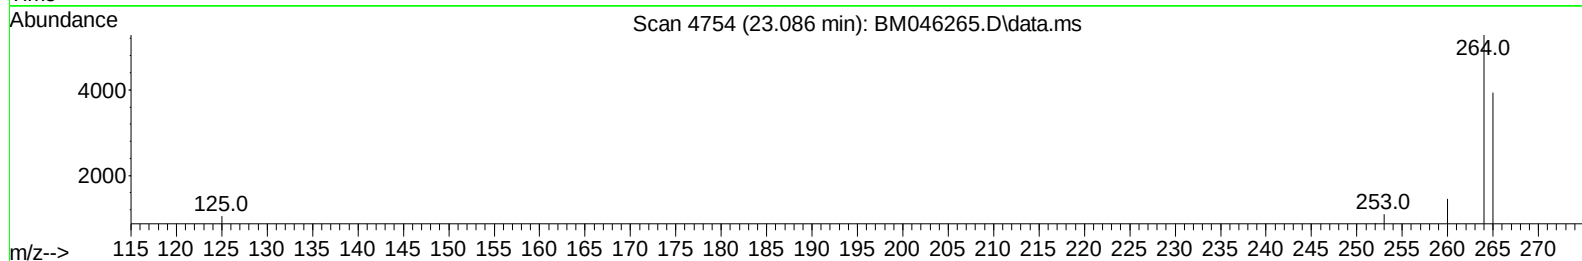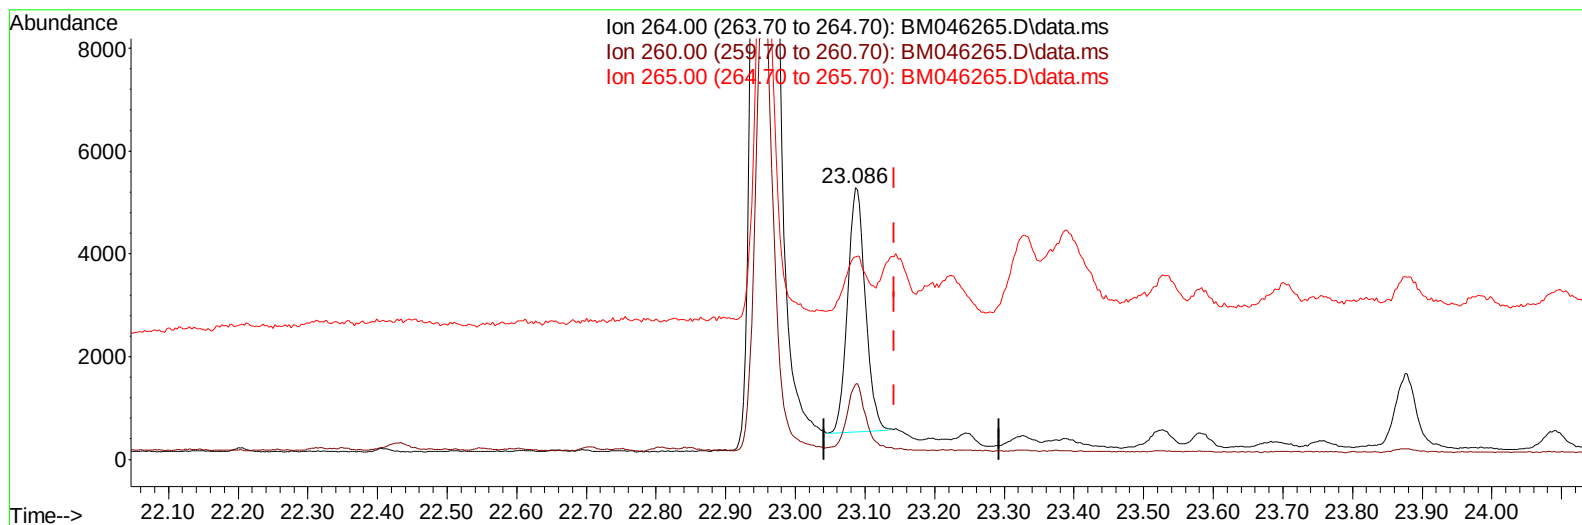

TIC: BM046265.D\data.ms

(23) Perylene-d12 (I)

23.086min (-0.056) 0.40 ng/ul m

response 8455

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	28.20	27.61
265.00	110.60	74.55#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062424\
Data File : BM046265.D
Acq On : 24 Jun 2024 22:22
Operator : MA/JU
Sample : P2776-22DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C76DL

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:27:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/25/2024
Supervised By :mohammad ahmed 06/27/2024

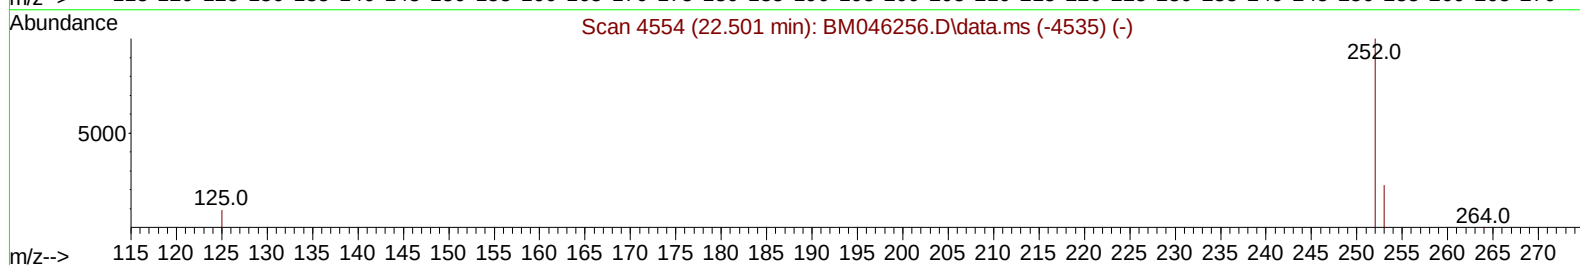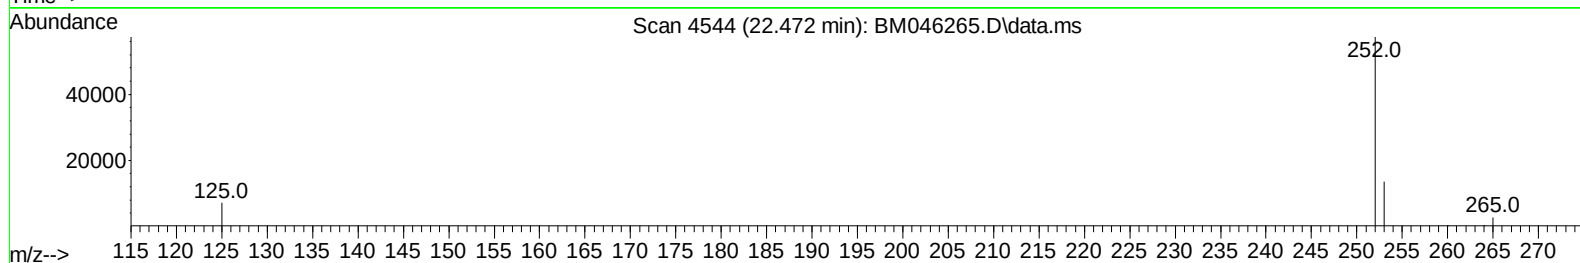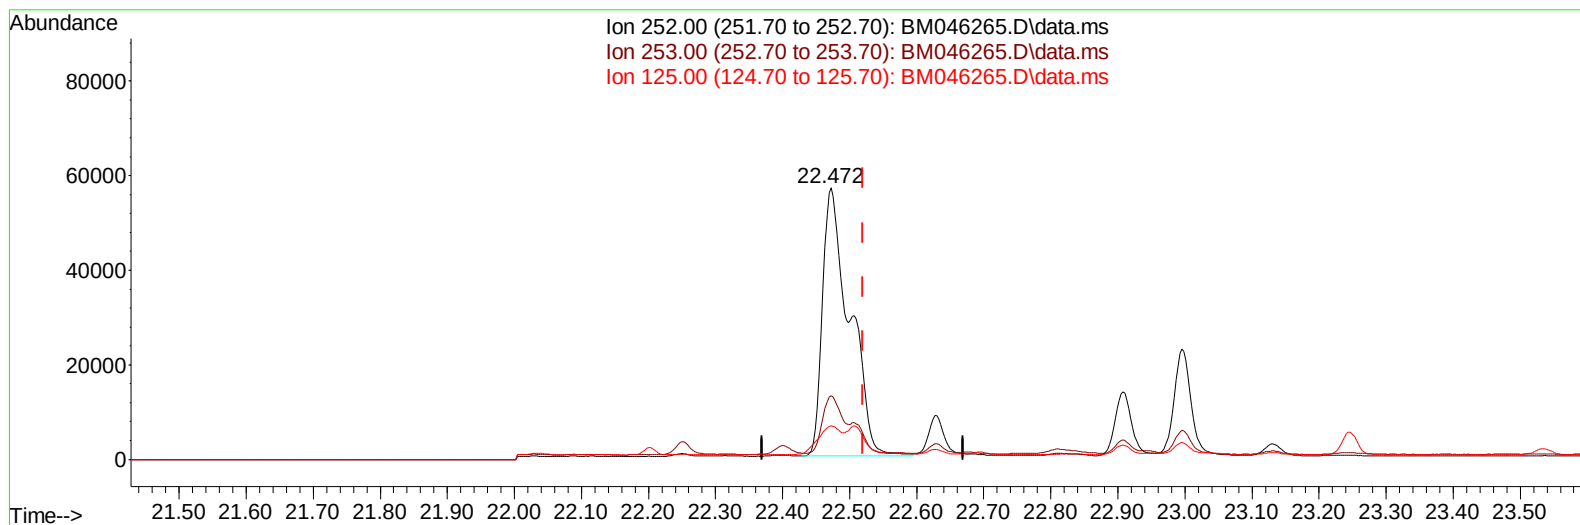

TIC: BM046265.D\data.ms

(24) Benzo(b)fluoranthene

22.472min (-0.047) 5.21 ng/u1

response 158699

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.90	23.57
125.00	20.10	12.46
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062424\
Data File : BM046265.D
Acq On : 24 Jun 2024 22:22
Operator : MA/JU
Sample : P2776-22DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C76DL

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:27:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/25/2024
Supervised By :mohammad ahmed 06/27/2024

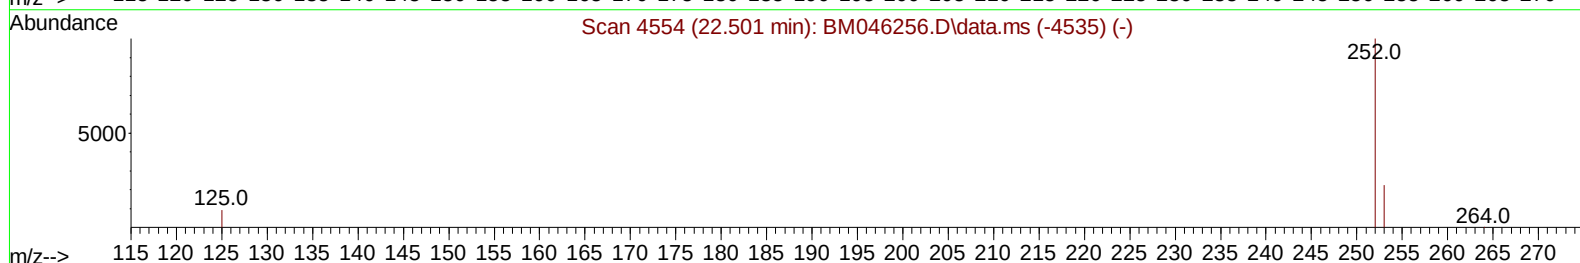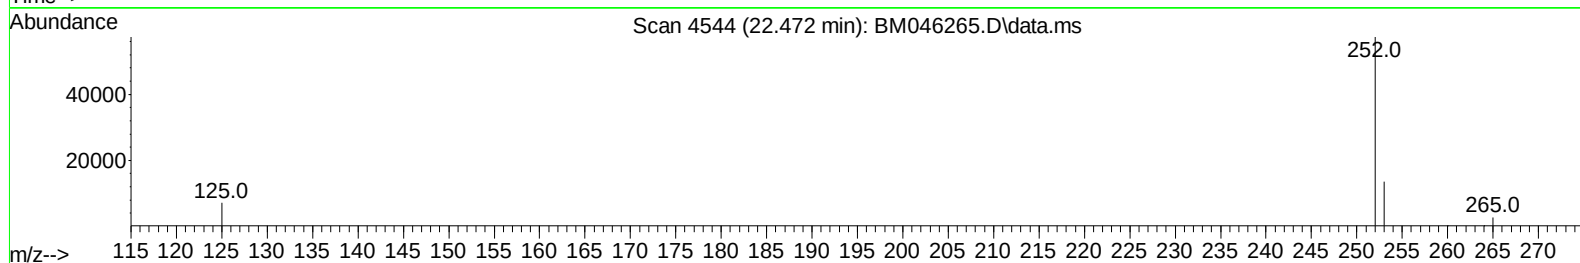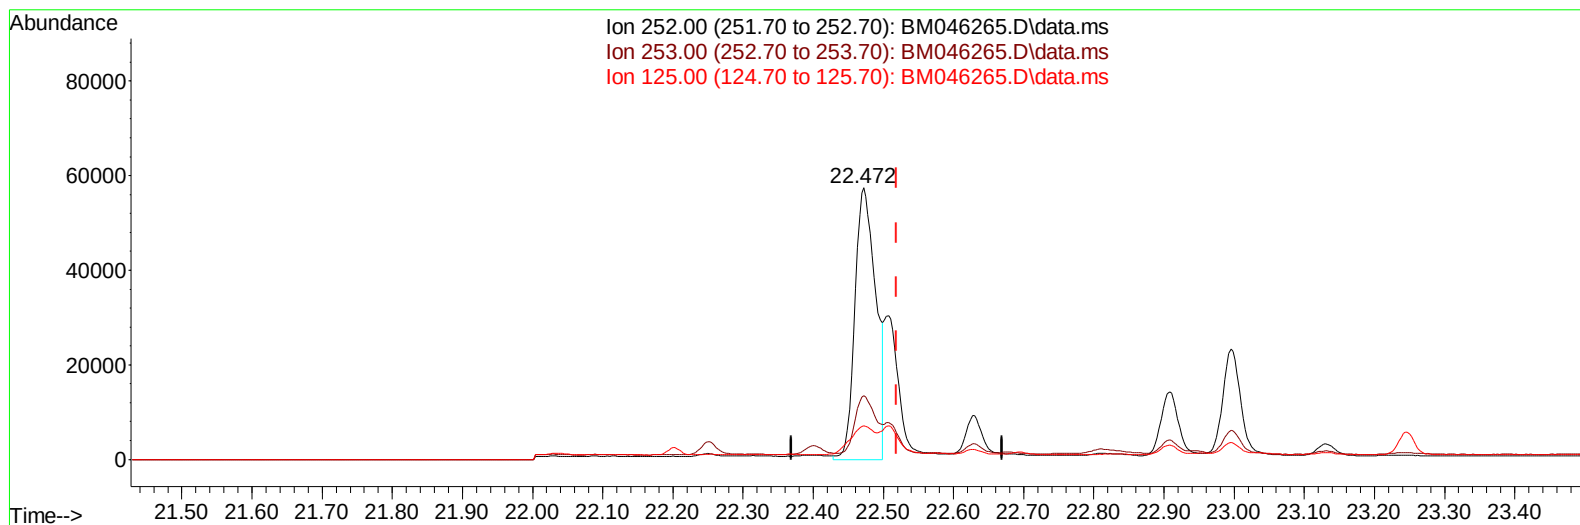

TIC: BM046265.D\data.ms

(24) Benzo(b)fluoranthene

22.472min (-0.047) 3.90 ng/ul m

response 118779

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	32.90	23.57
125.00	20.10	12.46
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062424\
Data File : BM046265.D
Acq On : 24 Jun 2024 22:22
Operator : MA/JU
Sample : P2776-22DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C76DL

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:27:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/25/2024
Supervised By :mohammad ahmed 06/27/2024

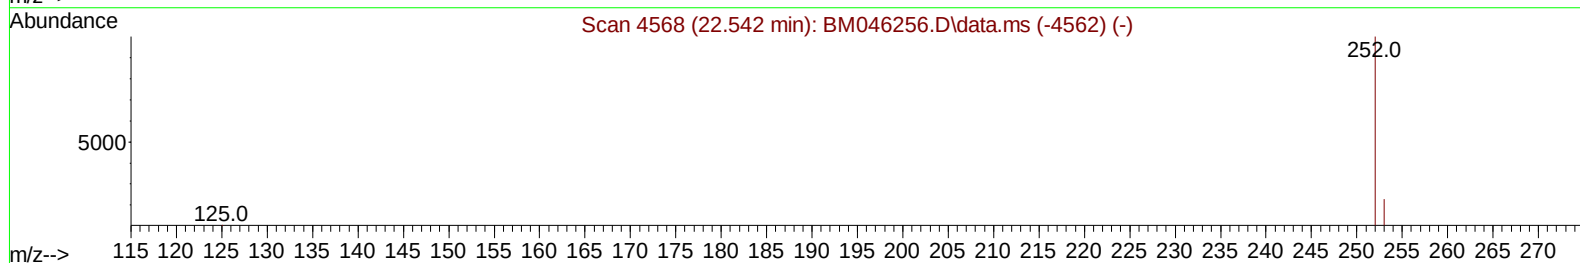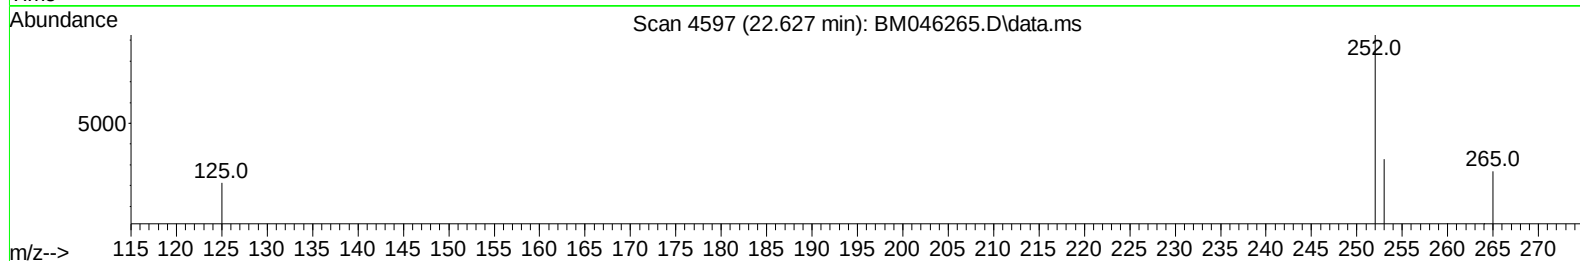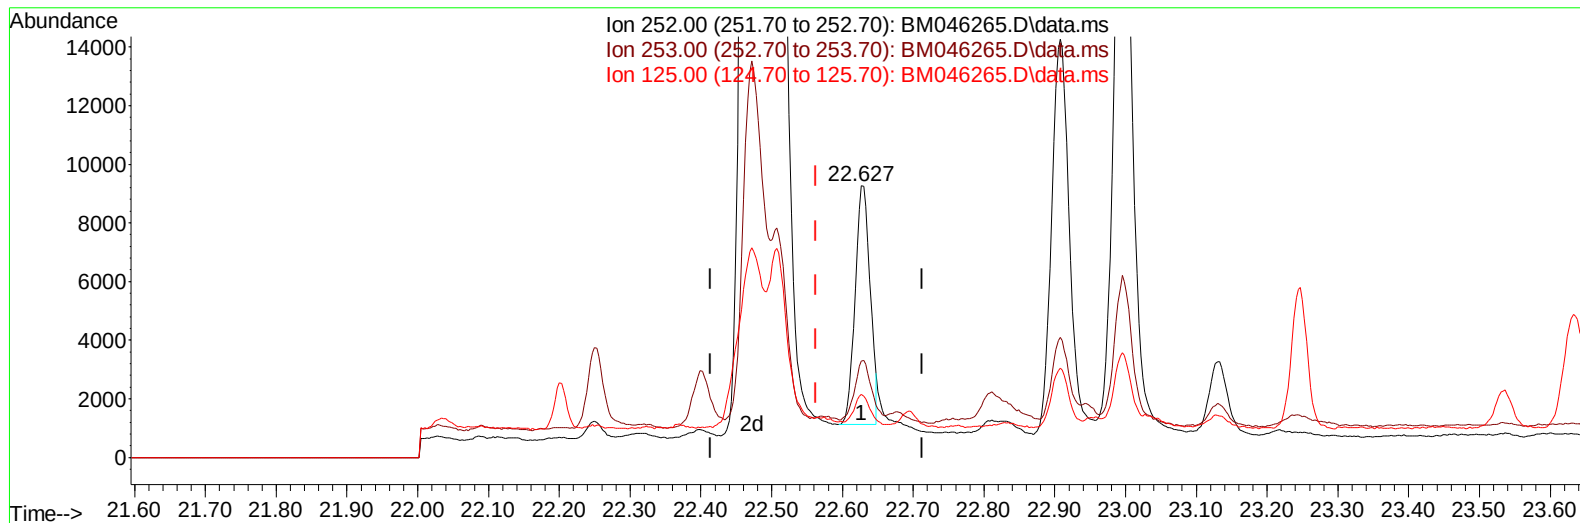

TIC: BM046265.D\data.ms

(25) Benzo(k)fluoranthene

22.627min (+ 0.064) 0.33 ng/u1

response 12025

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	34.00	35.48
125.00	20.80	23.16
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062424\
Data File : BM046265.D
Acq On : 24 Jun 2024 22:22
Operator : MA/JU
Sample : P2776-22DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C76DL

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:27:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/25/2024
Supervised By :mohammad ahmed 06/27/2024

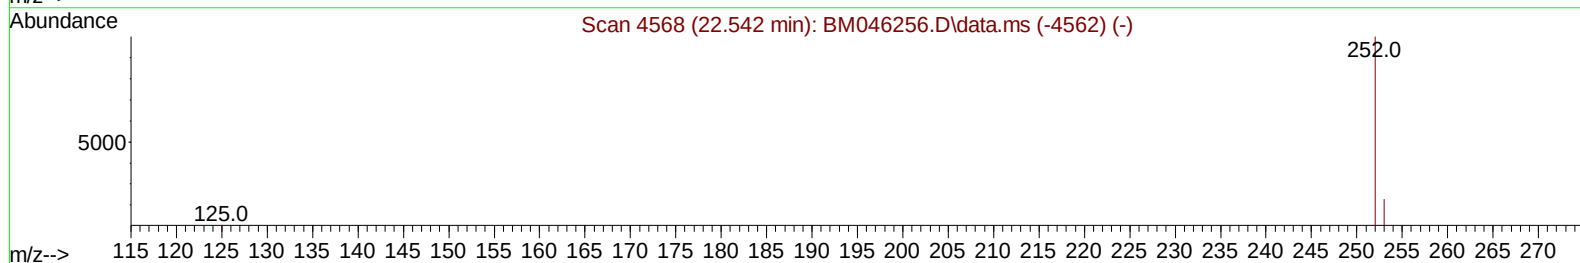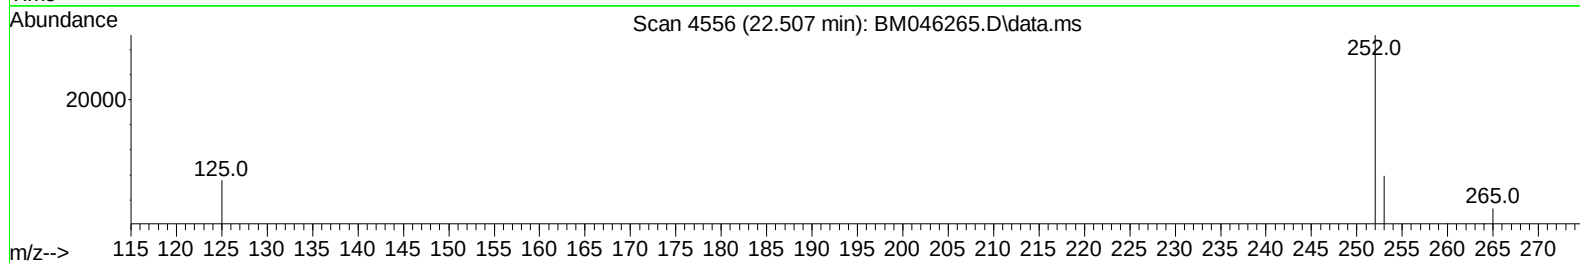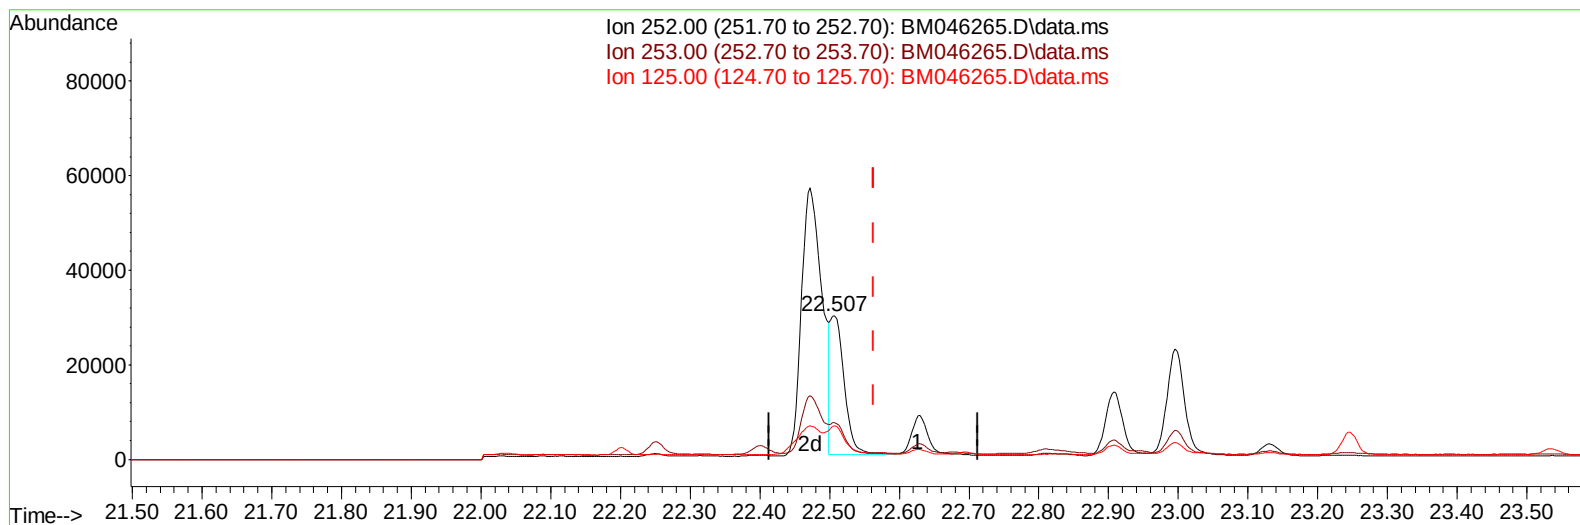

TIC: BM046265.D\data.ms

(25) Benzo(k)fluoranthene

22.507min (-0.056) 1.13 ng/ul m

response 40953

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	34.00	25.80#
125.00	20.80	23.47
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062424\
 Data File : BM046265.D
 Acq On : 24 Jun 2024 22:22
 Operator : MA/JU
 Sample : P2776-22DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4C76DL

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 06/25/2024
 Supervised By :mohammad ahmed 06/27/2024

Quant Time: Jun 25 02:27:49 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jun 24 02:25:34 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.413	152	2491	0.400	ng/ul	-0.05
4) Naphthalene-d8	10.210	136	7053	0.400	ng/ul	#-0.04
9) Acenaphthene-d10	14.058	164	4197	0.400	ng/ul	-0.05
13) Phenanthrene-d10	16.803	188	8455	0.400	ng/ul	-0.06
17) Chrysene-d12	21.000	240	7153	0.400	ng/ul	-0.04
23) Perylene-d12	23.086	264	8455m	0.400	ng/ul	-0.06
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.029	96	2564	0.750	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	11.838	152	568	0.060	ng/ul	-0.03
18) Fluoranthene-d10	18.830	212	1231	0.057	ng/ul	-0.05
Target Compounds						
					Qvalue	
5) Naphthalene	10.260	128	2008	0.102	ng/ul#	81
7) 2-Methylnaphthalene	11.904	142	744	0.067	ng/ul	93
8) 1-Methylnaphthalene	12.113	142	585	0.048	ng/ul	96
10) Acenaphthylene	13.780	152	6912	0.347	ng/ul	100
11) Acenaphthene	14.123	153	1968	0.137	ng/ul	98
12) Fluorene	15.122	166	2552	0.165	ng/ul#	97
15) Phenanthrene	16.846	178	59823	2.518	ng/ul	96
16) Anthracene	16.938	178	11904	0.673	ng/ul	97
19) Fluoranthene	18.863	202	151652	4.897	ng/ul	96
20) Pyrene	19.225	202	111816	3.338	ng/ul	95
21) Benzo(a)anthracene	20.982	228	65084	2.356	ng/ul	99
22) Chrysene	21.035	228	70747	2.006	ng/ul	99
24) Benzo(b)fluoranthene	22.472	252	118779m	3.899	ng/ul	
25) Benzo(k)fluoranthene	22.507	252	40953m	1.131	ng/ul	
26) Benzo(a)pyrene	22.995	252	39857	1.412	ng/ul#	78
27) Indeno(1,2,3-cd)pyrene	25.125	276	44564	0.965	ng/ul#	95
28) Dibenzo(a,h)anthracene	25.128	278	13850	0.403	ng/ul#	92
29) Benzo(g,h,i)perylene	25.748	276	6793	0.171	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062424\
Data File : BM046265.D
Acq On : 24 Jun 2024 22:22
Operator : MA/JU
Sample : P2776-22DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
A4C76DL

Manual IntegrationsAPPROVED

Quant Time: Jun 25 02:27:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM061824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jun 24 02:25:34 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 06/25/2024
Supervised By :mohammad ahmed 06/27/2024

