

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062515\
 Data File : BM001800.D
 Acq On : 25 Jun 2015 16:00
 Operator : TP/IZ
 Sample : G2760-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BK4

Quant Time: Jun 26 04:34:55 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 26 04:32:51 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	39833	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	157757	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	99617	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	237046	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	290796	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	285232	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	1103	1.32	ng/uL	0.00
5) Phenol-d5	6.83	99	20039	6.55	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	50355	29.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	61689	25.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	39693	16.16	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	36726	33.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	41925	35.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	79876	31.25	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	3641	1.40	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	247726	33.54	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	326089	33.67	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	8438	6.19	ng/ul	0.00
57) Fluorene-d10	15.31	176	236606	34.52	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	43300	29.90	ng/ul	0.00
70) Anthracene-d10	17.16	188	380620	34.47	ng/ul	0.00
78) Pyrene-d10	19.46	212	445535	36.17	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	436230	34.70	ng/ul	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	2.88	88	3730	3.91 ng/uL#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062515\
Data File : BM001800.D
Acq On : 25 Jun 2015 16:00
Operator : TP/IZ
Sample : G2760-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BK4

Quant Time: Jun 26 04:34:55 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 26 04:32:51 2015
Response via : Initial Calibration

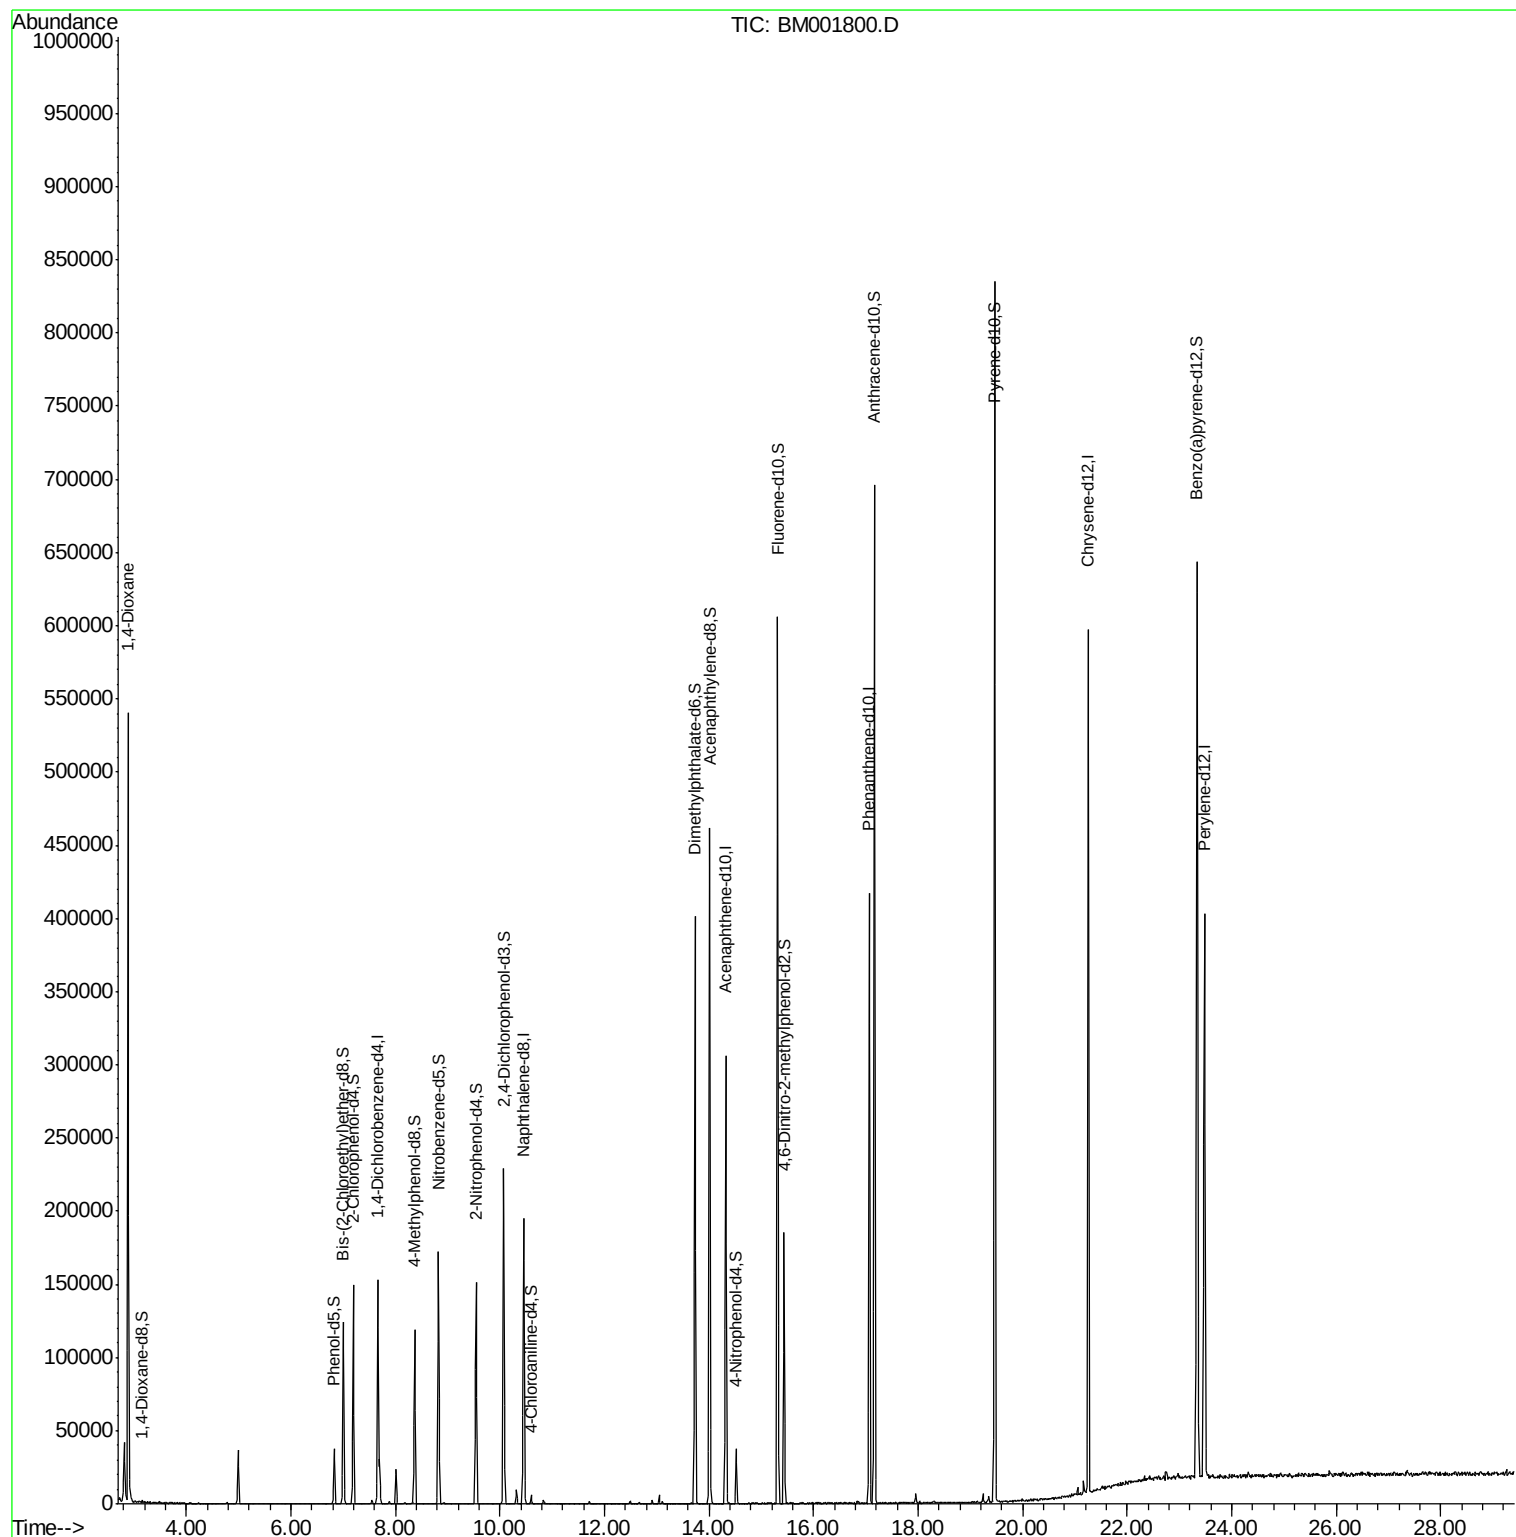

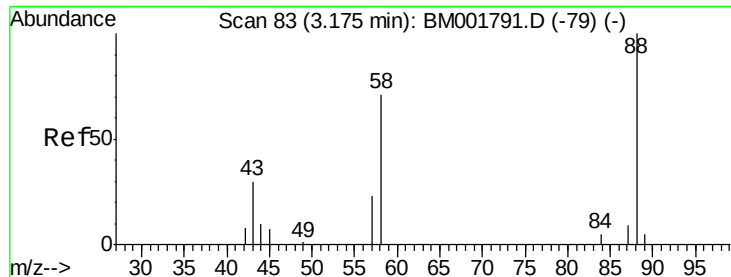

#2
 1,4-Dioxane
 Concen: 3.91 ng/uL
 RT: 2.88 min Scan# 33
 Delta R.T. -0.29 min
 Lab File: BM001800.D
 Acq: 25 Jun 2015 16:00

Instrument :
 BNA_M
 ClientSampleId :
 C0BK4

Tgt Ion: 88 Resp: 3730
 Ion Ratio Lower Upper
 88 100
 43 2414.0 24.2 36.4#
 58 30.4 56.2 84.2#

