

Data Path : Z:\HPCHEM1\BNA_M\Data\BM062515\
 Data File : BM001791.D
 Acq On : 25 Jun 2015 10:32
 Operator : TP/IZ
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP65

Quant Time: Jun 26 04:17:50 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 18 03:27:43 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	52248	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	201916	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	122093	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	279937	20.00	ng/ul	0.00
77) Chrysene-d12	21.26	240	345805	20.00	ng/ul	0.00
85) Perylene-d12	23.48	264	351456	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.14	96	7851	7.16	ng/uL	0.00
5) Phenol-d5	6.83	99	75660	18.85	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	40943	18.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	61867	19.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	61449	19.08	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	28580	20.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	32351	21.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	66935	20.46	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	78743	23.66	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	171630	18.96	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	229734	19.35	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	32215	19.29	ng/ul	0.00
57) Fluorene-d10	15.31	176	163037	19.41	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	29472	17.23	ng/ul	0.00
70) Anthracene-d10	17.16	188	256056	19.64	ng/ul	0.00
78) Pyrene-d10	19.46	212	291269	19.89	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.34	264	302405	19.52	ng/ul	0.00

Target Compounds

					Qvalue
2) 1,4-Dioxane	3.18	88	8596	6.87	ng/uL 98
4) Benzaldehyde	6.80	77	52214	19.90	ng/ul 98
6) Phenol	6.85	94	78826	19.03	ng/ul 99
8) Bis(2-Chloroethyl)ether	7.09	93	59168	19.02	ng/ul 97
10) 2-Chlorophenol	7.22	128	62439	19.01	ng/ul 99
11) 2-Methylphenol	8.10	108	59596	19.44	ng/ul 97
12) 2,2'-oxybis(1-Chloropropan	8.20	45	66417	17.44	ng/ul 95
14) Acetophenone	8.48	105	98079	19.18	ng/ul 99
15) N-Nitroso-di-n-propylamine	8.47	70	49138	19.67	ng/ul 99
16) 4-Methylphenol	8.43	108	63458	19.05	ng/ul 97
17) Hexachloroethane	8.73	117	25842	19.59	ng/ul 97
20) Nitrobenzene	8.86	77	72814	19.24	ng/ul 94
21) Isophorone	9.38	82	127478	20.17	ng/ul 99
23) 2-Nitrophenol	9.57	139	34527	20.63	ng/ul 98
24) 2,4-Dimethylphenol	9.63	107	74226	19.19	ng/ul 96
25) Bis(2-Chloroethoxy)methane	9.87	93	75124	19.05	ng/ul 98
27) 2,4-Dichlorophenol	10.10	162	64785	20.41	ng/ul 97
28) Naphthalene	10.50	128	194938	19.12	ng/ul 98
30) 4-Chloroaniline	10.62	127	77254	22.87	ng/ul 95
31) Hexachlorobutadiene	10.78	225	47616	19.59	ng/ul 93
32) Caprolactam	11.36	113	19473	20.54	ng/ul 92
33) 4-Chloro-3-methylphenol	11.74	107	66483	19.68	ng/ul 97
34) 2-Methylnaphthalene	12.12	142	141710	19.22	ng/ul 97


Data Path : Z:\HPCHEM1\BNA_M\Data\BM062515\
 Data File : BM001791.D
 Acq On : 25 Jun 2015 10:32
 Operator : TP/IZ
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP65

Quant Time: Jun 26 04:17:50 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 18 03:27:43 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
36) 1,2,4,5-Tetrachlorobenzene	12.49	216	87772	19.24	ng/ul	97
37) Hexachlorocyclopentadiene	12.47	237	46354	16.81	ng/ul	99
38) 2,4,6-Trichlorophenol	12.74	196	53307	20.08	ng/ul	95
39) 2,4,5-Trichlorophenol	12.80	196	57149	19.67	ng/ul	99
40) 1,1'-Biphenyl	13.14	154	186681	18.73	ng/ul	100
41) 2-Chloronaphthalene	13.19	162	147657	18.90	ng/ul	98
42) 2-Nitroaniline	13.40	65	41114	19.85	ng/ul	90
44) Dimethylphthalate	13.77	163	186639	18.86	ng/ul	99
45) 2,6-Dinitrotoluene	13.90	165	38513	20.70	ng/ul	97
47) Acenaphthylene	14.04	152	231671	19.15	ng/ul	100
48) 3-Nitroaniline	14.23	138	38894	22.37	ng/ul	95
49) Acenaphthene	14.38	153	154754	19.14	ng/ul	97
50) 2,4-Dinitrophenol	14.44	184	19660	17.05	ng/ul	89
52) 4-Nitrophenol	14.53	109	32620	18.90	ng/ul	96
53) Dibenzofuran	14.72	168	223126	19.27	ng/ul	100
54) 2,4-Dinitrotoluene	14.69	165	56186	20.48	ng/ul	99
55) 2,3,4,6-Tetrachlorophenol	14.94	232	50570	20.14	ng/ul	98
56) Diethylphthalate	15.14	149	181311	19.27	ng/ul	98
58) Fluorene	15.37	166	184787	19.17	ng/ul	99
59) 4-Chlorophenyl-phenylether	15.36	204	99897	19.23	ng/ul	98
60) 4-Nitroaniline	15.39	138	40648	20.60	ng/ul	98
63) 4,6-Dinitro-2-methylphenol	15.45	198	31892	17.51	ng/ul	97
64) N-Nitrosodiphenylamine	15.58	169	158028	19.32	ng/ul	99
65) 4-Bromophenyl-phenylether	16.26	248	61436	19.68	ng/ul	97
66) Hexachlorobenzene	16.37	284	68927	19.65	ng/ul	98
67) Atrazine	16.53	200	63912	19.40	ng/ul	95
68) Pentachlorophenol	16.71	266	41443	19.27	ng/ul	99
69) Phenanthrene	17.10	178	290996	19.17	ng/ul	99
71) Anthracene	17.20	178	301812	19.37	ng/ul	99
72) 1,2,3,4-Tetrachlorobenzene	13.11	216	84594	19.22	ng/uL	93
73) Pentachlorobenzene	14.63	250	80086	19.30	ng/uL	98
74) Carbazole	17.47	167	263338	19.26	ng/ul	99
75) Di-n-butylphthalate	18.03	149	295314	20.22	ng/ul	100
76) Fluoranthene	19.13	202	353277	19.46	ng/ul	98
79) Pyrene	19.49	202	375924	19.59	ng/ul	97
80) Butylbenzylphthalate	20.40	149	135057	21.58	ng/ul	98
81) 3,3'-Dichlorobenzidine	21.18	252	130383	21.22	ng/ul	97
82) Benzo(a)anthracene	21.24	228	389665	19.29	ng/ul	100
83) Bis(2-ethylhexyl)phthalate	21.17	149	198303	21.07	ng/ul	100
84) Chrysene	21.29	228	358799	18.73	ng/ul	99
86) Di-n-octyl phthalate	22.04	149	350064	20.27	ng/ul	100
87) Benzo(b)fluoranthene	22.81	252	400342	19.57	ng/ul	99
88) Benzo(k)fluoranthene	22.85	252	370053	18.72	ng/ul	99
90) Benzo(a)pyrene	23.38	252	377736	18.98	ng/ul	99
91) Indeno(1,2,3-cd)pyrene	25.72	276	463098	19.62	ng/ul	99
92) Dibenzo(a,h)anthracene	25.73	278	389837	19.58	ng/ul	100
93) Benzo(g,h,i)perylene	26.40	276	391514	19.73	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2

1,4-Dioxane

Concen: 6.87 ng/uL

RT: 3.18 min Scan# 83

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32

Instrument :

BNA_M

ClientSampleId :

DFTPP65


Tgt Ion: 88 Resp: 8596

Ion Ratio Lower Upper

88 100

43 28.8 24.2 36.4




58 71.5 56.2 84.2



Abundance Ion 88.00 (87.70 to 88.70): BM001791.D (-1) (-)

Ion 43.00 (42.70 to 43.70): BM001791.D (-1) (-)

Ion 58.00 (57.70 to 58.70): BM001791.D (-1) (-)

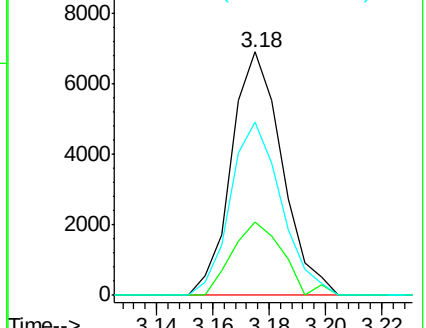

#4

Benzaldehyde

Concen: 19.90 ng/uL

RT: 6.80 min Scan# 700

Delta R.T. -0.01 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32


Tgt Ion: 77 Resp: 52214

Ion Ratio Lower Upper

77 100

105 97.6 79.3 118.9



106 92.5 72.8 109.2




Abundance Ion 77.00 (76.70 to 77.70): BM001791.D (-667) (-)

Ion 105.00 (104.70 to 105.70): BM001791.D (-667) (-)

Ion 106.00 (105.70 to 106.70): BM001791.D (-667) (-)

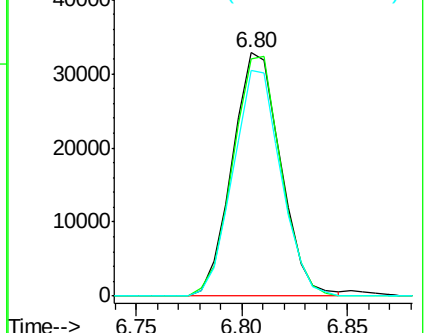

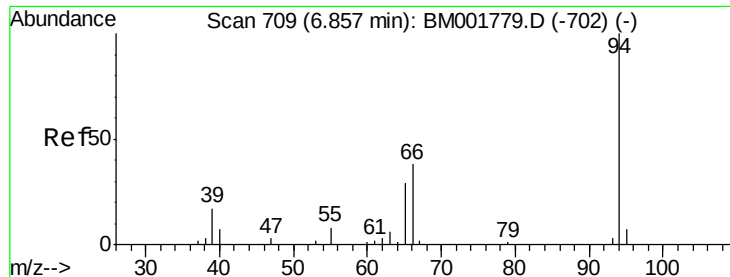

#6

Phenol

Concen: 19.03 ng/ul

RT: 6.85 min Scan# 708

Delta R.T. -0.01 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32

Instrument :

BNA_M

ClientSampleId :

DFTPP65


Tgt Ion: 94 Resp: 78826

Ion Ratio Lower Upper

94 100

65 31.8 26.1 39.1




66 45.9 35.9 53.9

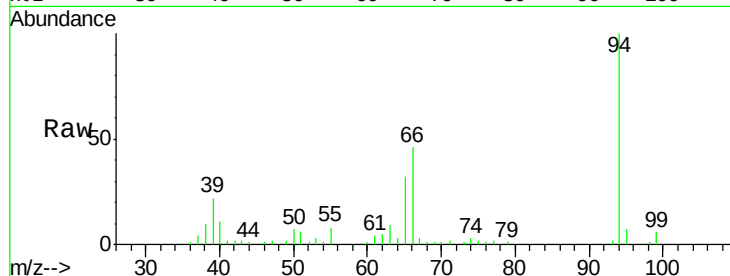

Abundance Ion 94.00 (93.70 to 94.70): BM001791.D (-702) (-)

Ion 65.00 (64.70 to 65.70): BM001791.D (-702) (-)

Ion 66.00 (65.70 to 66.70): BM001791.D (-702) (-)

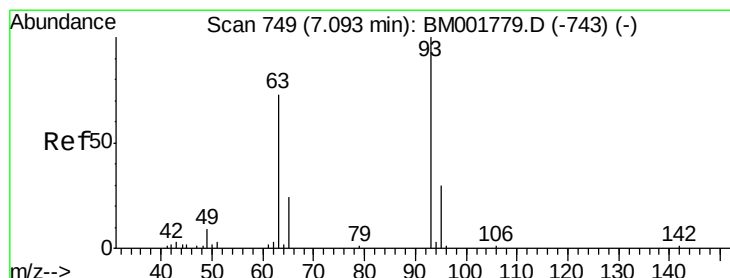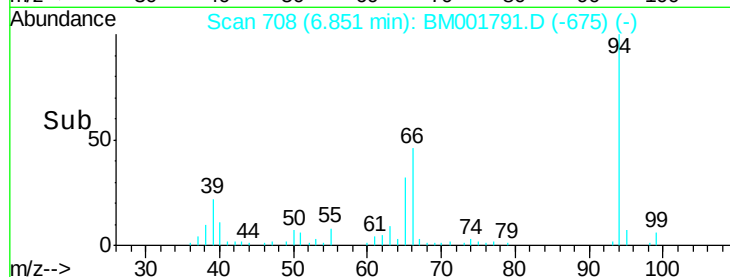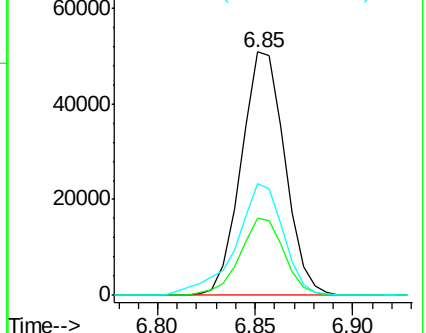

#8

Bis(2-Chloroethyl)ether

Concen: 19.02 ng/ul

RT: 7.09 min Scan# 749

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32


Tgt Ion: 93 Resp: 59168

Ion Ratio Lower Upper

93 100

63 69.9 58.7 88.1



95 33.8 27.0 40.6

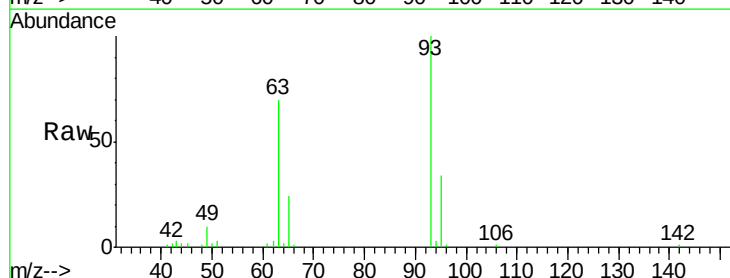


Abundance Ion 93.00 (92.70 to 93.70): BM001791.D (-743) (-)

Ion 63.00 (62.70 to 63.70): BM001791.D (-743) (-)

Ion 95.00 (94.70 to 95.70): BM001791.D (-743) (-)

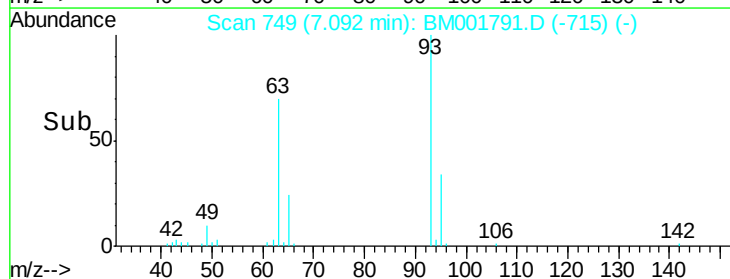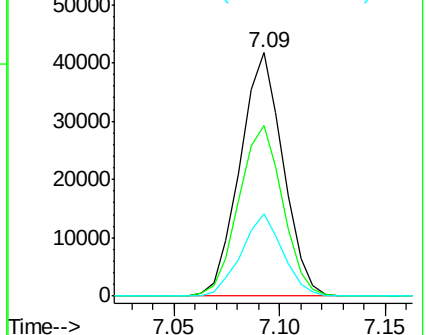







#10
2-Chlorophenol
Concen: 19.01 ng/ul
RT: 7.22 min Scan# 771
Delta R.T. -0.01 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32

Instrument :
BNA_M
ClientSampleId :
DFTPP65

Tgt Ion:128 Resp: 62439
Ion Ratio Lower Upper
128 100
64 47.5 37.4 56.2
130 32.8 25.4 38.0




Abundance Ion 128.00 (127.70 to 128.70): E
Ion 64.00 (63.70 to 64.70): BM0
Ion 130.00 (129.70 to 130.70): E

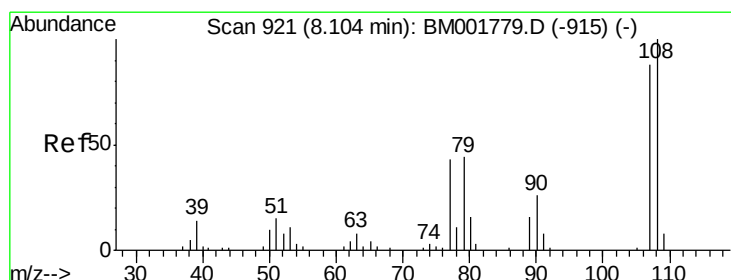
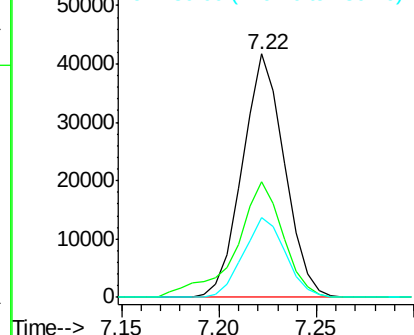



#11
2-Methylphenol
Concen: 19.44 ng/ul
RT: 8.10 min Scan# 921
Delta R.T. 0.00 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32

Tgt Ion:108 Resp: 59596
Ion Ratio Lower Upper
108 100
107 87.7 72.1 108.1



Abundance Ion 108.00 (107.70 to 108.70): E
Ion 107.00 (106.70 to 107.70): E




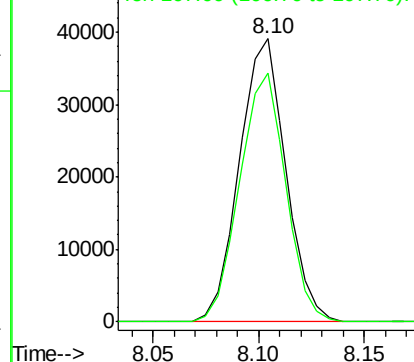


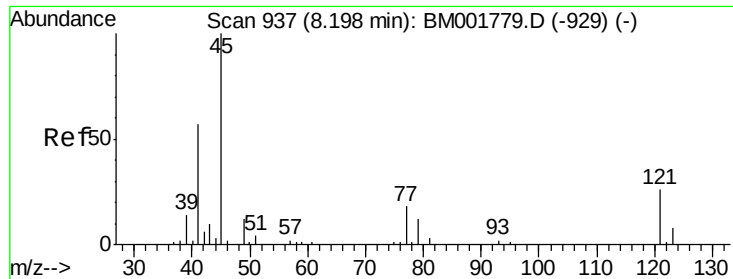

#12
2,2'-oxybis(1-Chloropropane)
Concen: 17.44 ng/ul
RT: 8.20 min Scan# 937
Delta R.T. 0.00 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32




Instrument :
BNA_M
ClientSampleId :
DFTPP65


Tgt Ion: 45 Resp: 66417
Ion Ratio Lower Upper
45 100
77 17.0 12.0 18.0
79 14.3 9.9 14.9

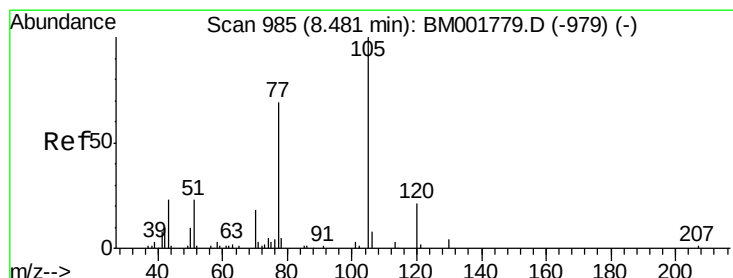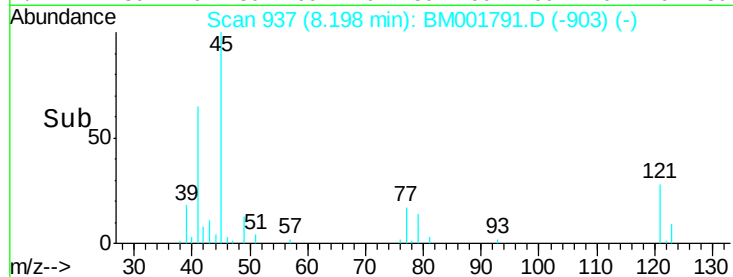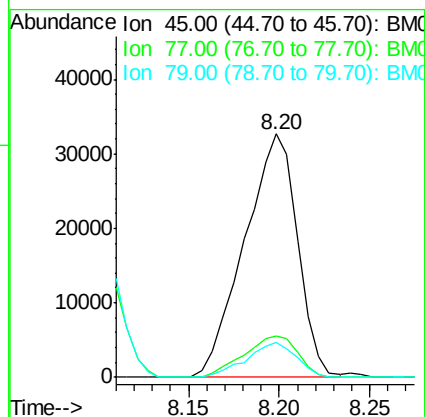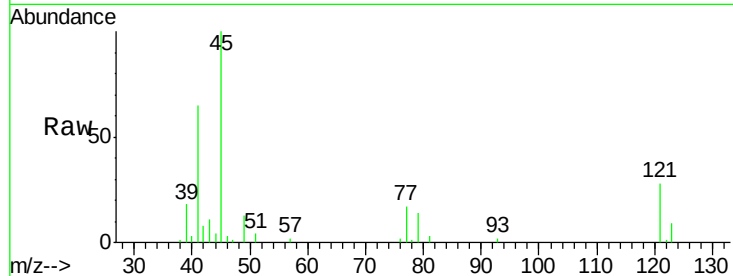

#14
Acetophenone
Concen: 19.18 ng/ul
RT: 8.48 min Scan# 985
Delta R.T. -0.01 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32

Tgt Ion: 105 Resp: 98079
Ion Ratio Lower Upper
105 100
77 81.4 64.2 96.4
51 27.7 22.0 33.0


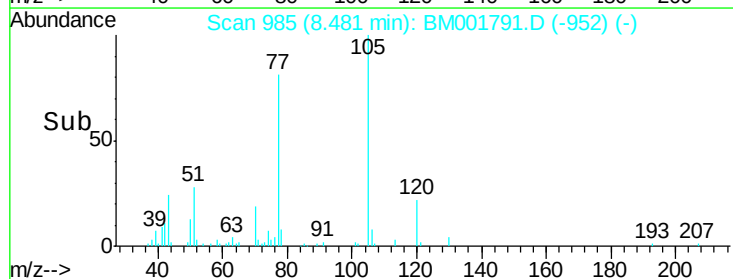
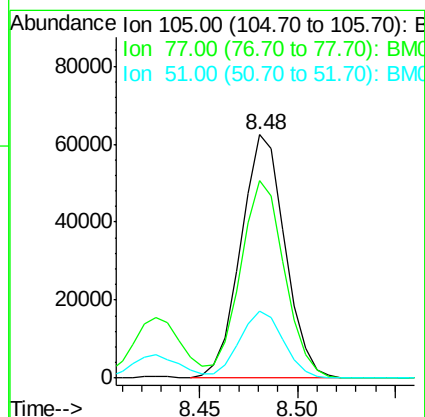
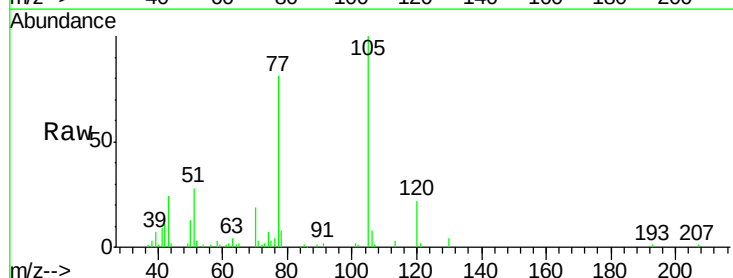




#15
N-Nitroso-di-n-propylamine
Concen: 19.67 ng/ul
RT: 8.47 min Scan# 983
Delta R.T. 0.00 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32




Instrument :
BNA_M
ClientSampleId :
DFTPP65


Tgt Ion: 70 Resp: 49138
Ion Ratio Lower Upper
70 100
42 56.3 45.2 67.8
101 9.2 7.8 11.6
130 21.3 15.5 23.3

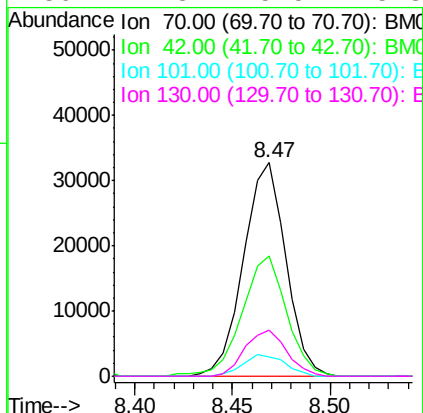

#16
4-Methylphenol
Concen: 19.05 ng/ul
RT: 8.43 min Scan# 976
Delta R.T. -0.01 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32

Tgt Ion: 108 Resp: 63458
Ion Ratio Lower Upper
108 100
107 115.8 89.9 134.9



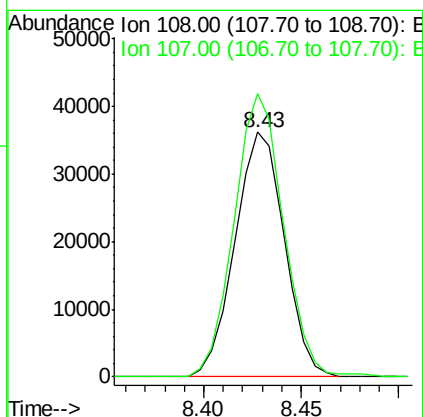



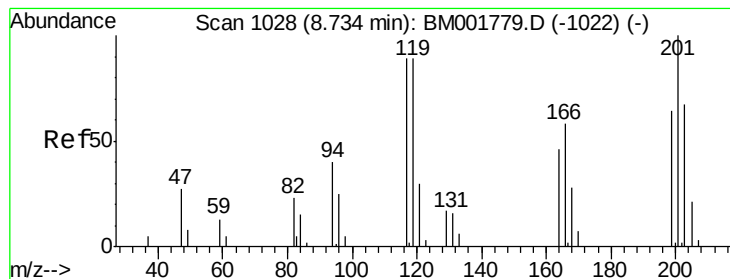

#17
 Hexachloroethane
 Concen: 19.59 ng/ul
 RT: 8.73 min Scan# 1028
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32




Instrument :
 BNA_M
 ClientSampleId :
 DFTPP65


Tgt Ion: 117 Resp: 25842
 Ion Ratio Lower Upper
 117 100
 201 114.0 92.1 138.1
 199 71.1 60.6 90.8

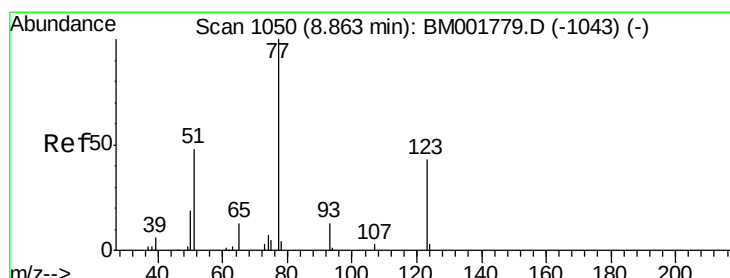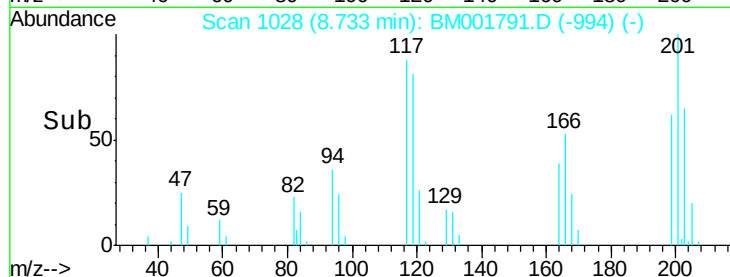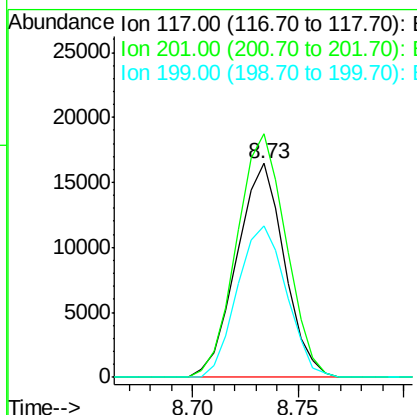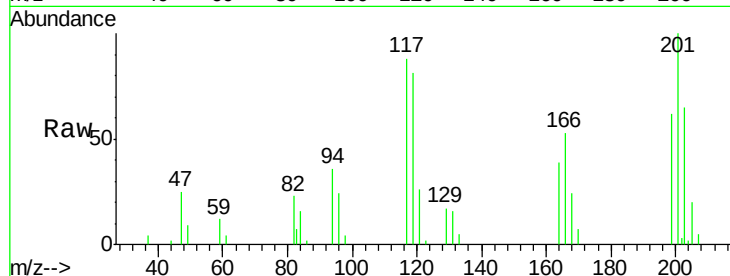

#20
 Nitrobenzene
 Concen: 19.24 ng/ul
 RT: 8.86 min Scan# 1050
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32

Tgt Ion: 77 Resp: 72814
 Ion Ratio Lower Upper
 77 100
 123 46.7 34.0 51.0
 65 15.2 11.3 16.9

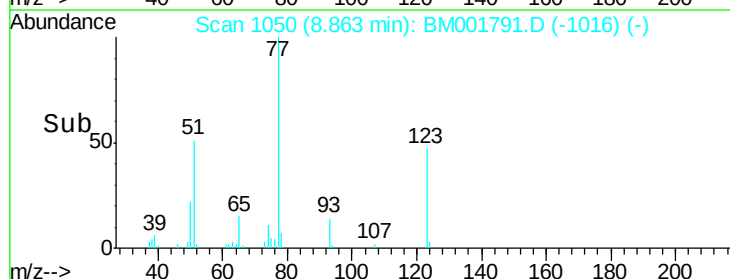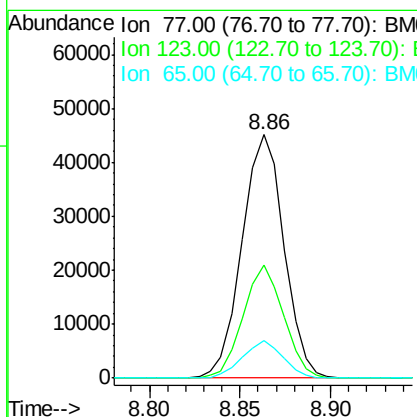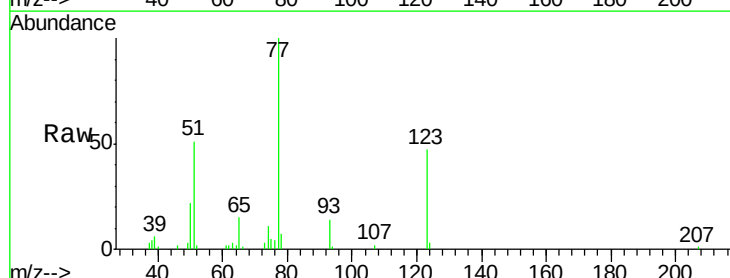



#21

Isophorone

Concen: 20.17 ng/ul

RT: 9.38 min Scan# 1138

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32

Instrument :

BNA_M

ClientSampleId :

DFTPP65


Tgt Ion: 82 Resp: 127478

Ion Ratio Lower Upper

82 100

95 8.9 6.3 9.5

138 18.5 14.9 22.3





Abundance Ion 82.00 (81.70 to 82.70): BM001791.D (-1131) (-)

Ion 95.00 (94.70 to 95.70): BM001791.D (-1131) (-)

Ion 138.00 (137.70 to 138.70): BM001791.D (-1131) (-)

Time-->



#23

2-Nitrophenol

Concen: 20.63 ng/ul

RT: 9.57 min Scan# 1170

Delta R.T. -0.01 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32


Tgt Ion: 139 Resp: 34527

Ion Ratio Lower Upper

139 100

65 55.3 45.4 68.0

109 37.5 31.6 47.4





Abundance Ion 139.00 (138.70 to 139.70): BM001791.D (-1164) (-)

Ion 65.00 (64.70 to 65.70): BM001791.D (-1164) (-)

Ion 109.00 (108.70 to 109.70): BM001791.D (-1164) (-)

Time-->







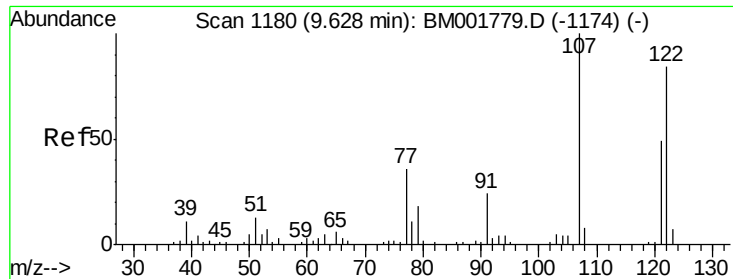

#24
 2,4-Dimethylphenol
 Concen: 19.19 ng/ul
 RT: 9.63 min Scan# 1180
 Delta R.T. -0.01 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32




Instrument :
 BNA_M
 ClientSampleId :
 DFTPP65


Tgt Ion: 107 Resp: 74226
 Ion Ratio Lower Upper
 107 100
 121 45.5 37.4 56.2
 122 78.4 59.2 88.8

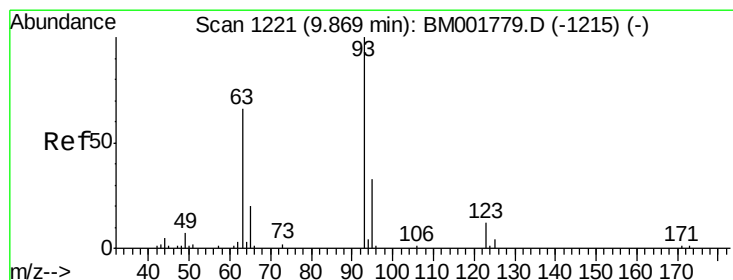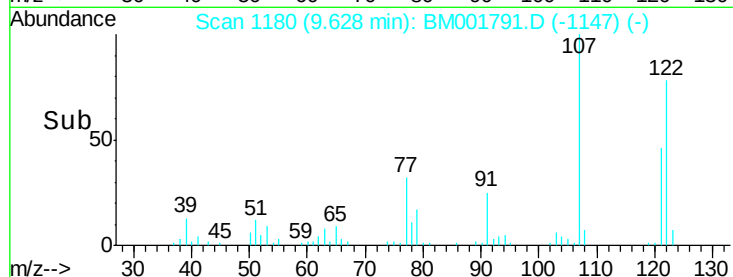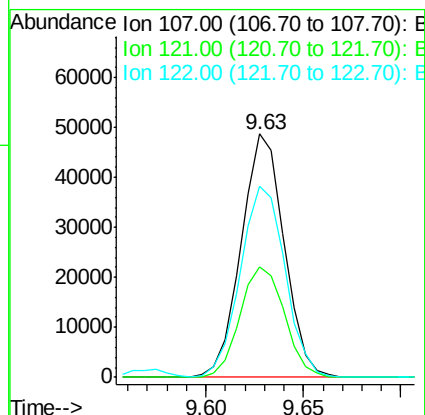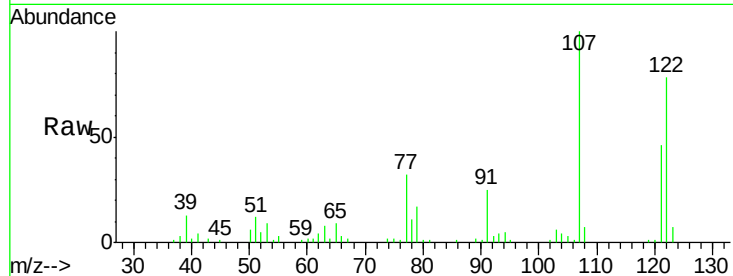

#25
 Bis(2-Chloroethoxy)methane
 Concen: 19.05 ng/ul
 RT: 9.87 min Scan# 1221
 Delta R.T. -0.01 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32

Tgt Ion: 93 Resp: 75124
 Ion Ratio Lower Upper
 93 100
 95 31.1 26.2 39.4
 123 11.5 9.1 13.7


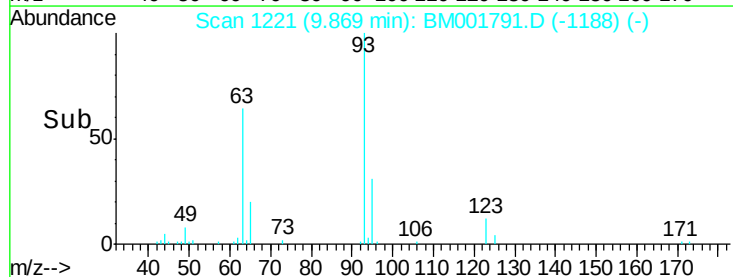
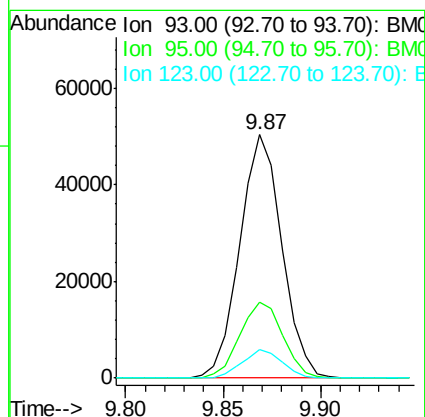
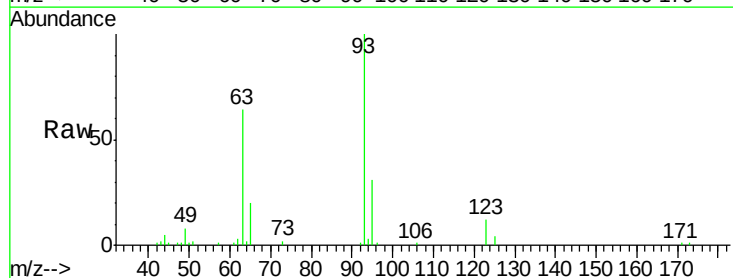




#27
 2,4-Dichlorophenol
 Concen: 20.41 ng/ul
 RT: 10.10 min Scan# 1260
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32




Instrument :
 BNA_M
 ClientSampleId :
 DFTPP65


Tgt Ion:162 Resp: 64785
 Ion Ratio Lower Upper
 162 100
 164 67.0 55.1 82.7
 98 35.7 30.8 46.2

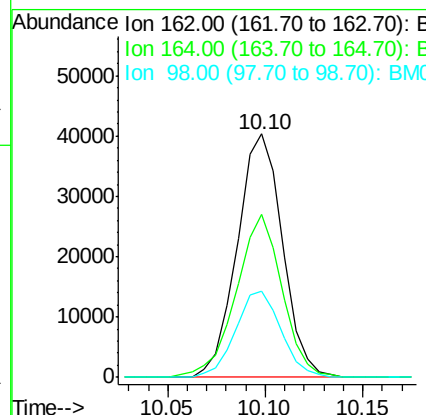

#28
 Naphthalene
 Concen: 19.12 ng/ul
 RT: 10.50 min Scan# 1328
 Delta R.T. -0.01 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32

Tgt Ion:128 Resp: 194938
 Ion Ratio Lower Upper
 128 100
 129 10.5 8.7 13.1
 127 13.9 10.0 15.0



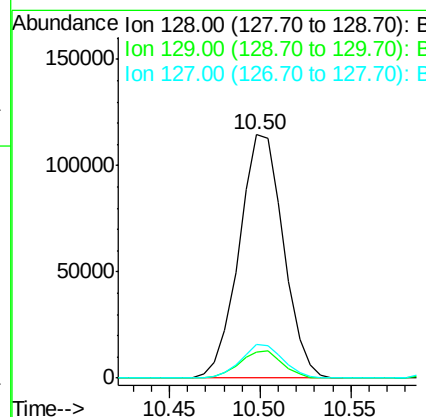



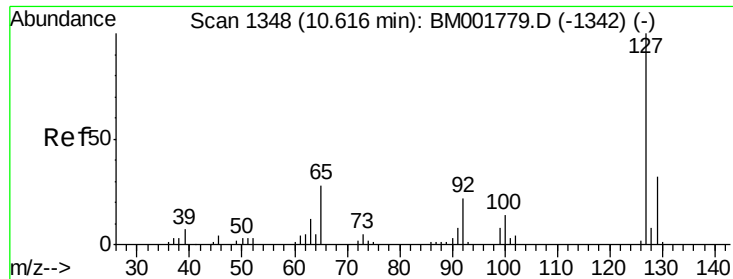

#30
4-Chloroaniline
Concen: 22.87 ng/ul
RT: 10.62 min Scan# 1348
Delta R.T. 0.00 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32




Instrument :
BNA_M
ClientSampleId :
DFTPP65


Tgt Ion:127 Resp: 77254
Ion Ratio Lower Upper
127 100
129 33.7 24.6 36.8

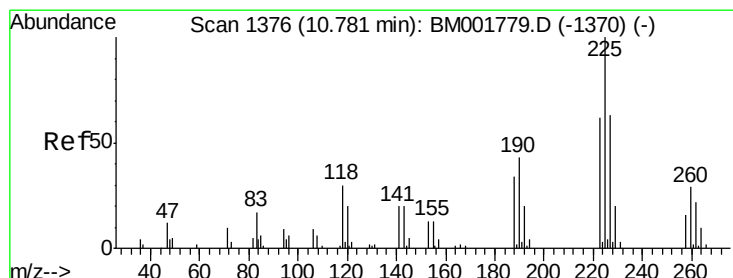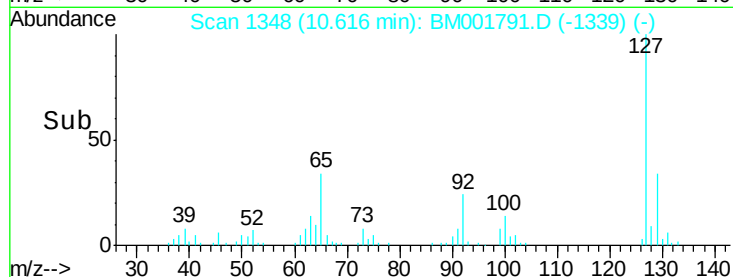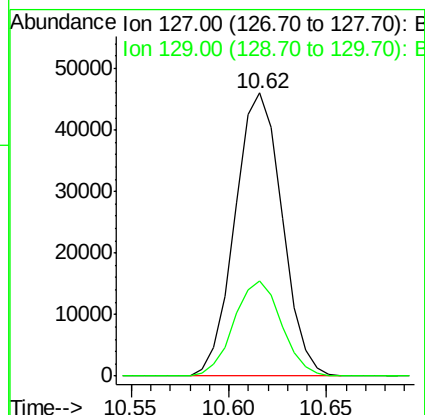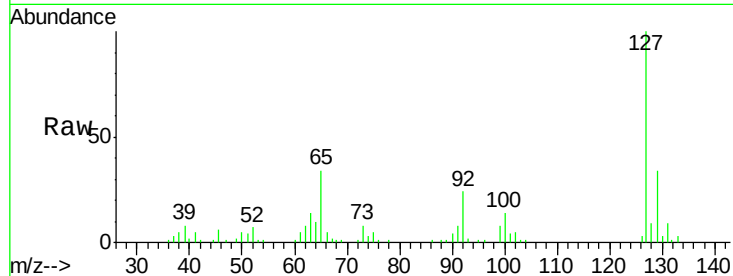

#31
Hexachlorobutadiene
Concen: 19.59 ng/ul
RT: 10.78 min Scan# 1376
Delta R.T. -0.01 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32

Tgt Ion:225 Resp: 47616
Ion Ratio Lower Upper
225 100
223 59.7 51.1 76.7
227 60.9 54.4 81.6


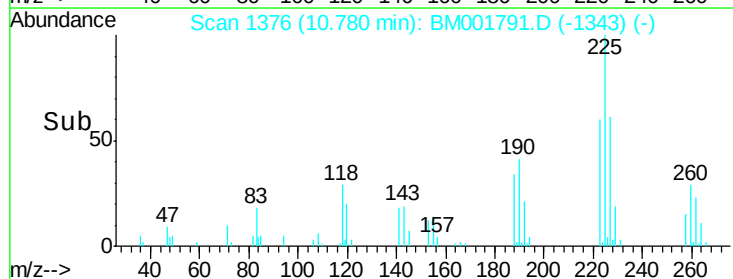
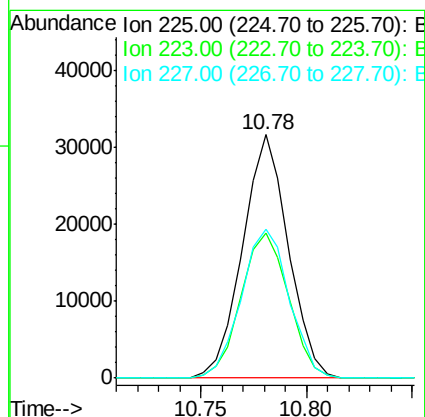
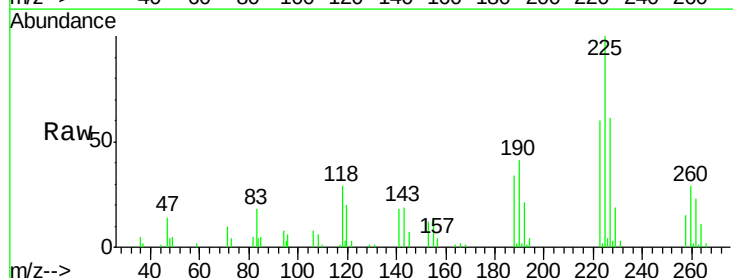




#32
 Caprolactam
 Concen: 20.54 ng/ul
 RT: 11.36 min Scan# 1475
 Delta R.T. -0.01 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32




Instrument :
 BNA_M
 ClientSampleId :
 DFTPP65


Tgt Ion:113 Resp: 19473
 Ion Ratio Lower Upper
 113 100
 55 136.4 123.3 184.9
 56 123.8 98.6 147.8

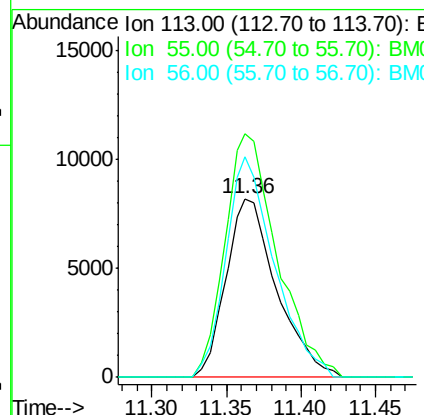

#33
 4-Chloro-3-methylphenol
 Concen: 19.68 ng/ul
 RT: 11.74 min Scan# 1539
 Delta R.T. -0.01 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32

Tgt Ion:107 Resp: 66483
 Ion Ratio Lower Upper
 107 100
 144 26.1 20.2 30.4
 142 75.3 57.7 86.5

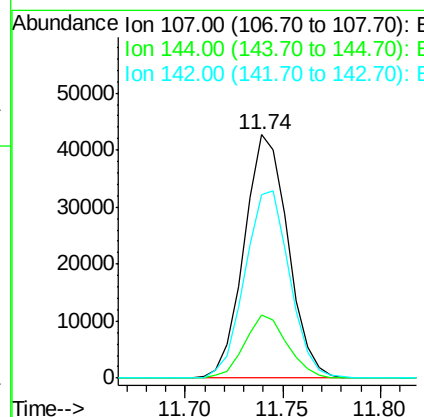

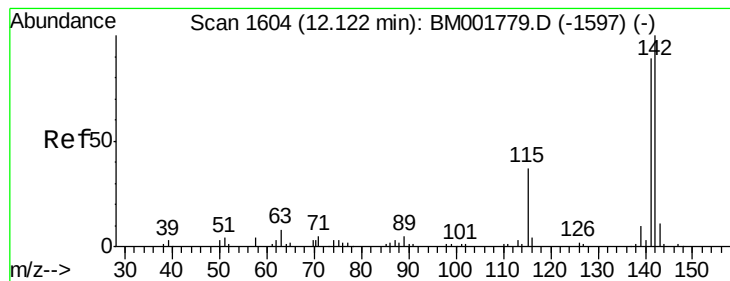

#34

2-Methylnaphthalene

Concen: 19.22 ng/ul

RT: 12.12 min Scan# 1604

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32

Instrument :

BNA_M

ClientSampleId :


DFTPP65

Tgt Ion:142 Resp: 141710

Ion Ratio Lower Upper




142 100

141 87.0 71.6 107.4

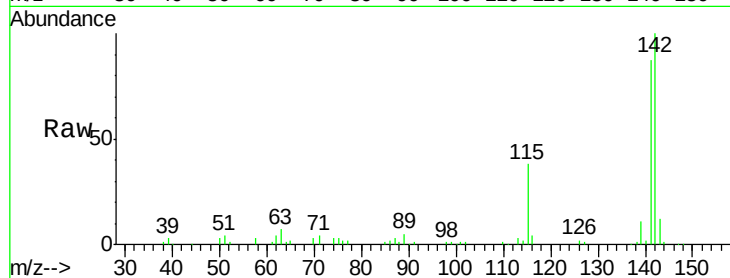

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

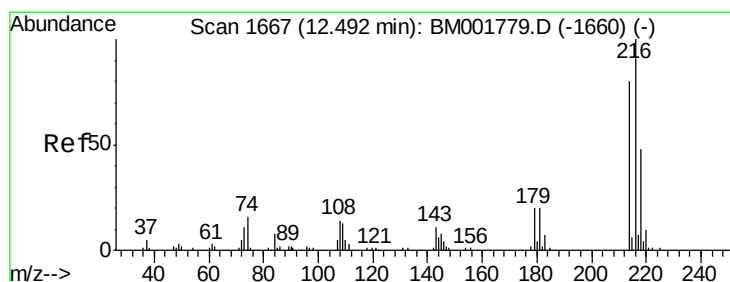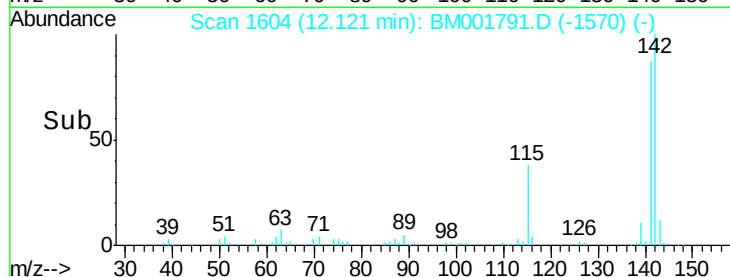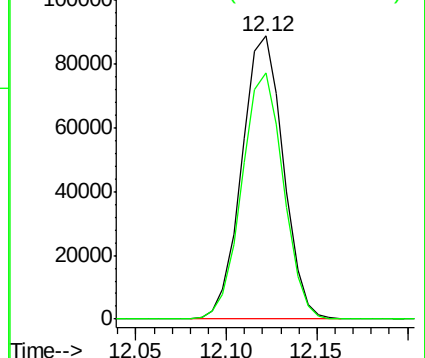

#36

1,2,4,5-Tetrachlorobenzene

Concen: 19.24 ng/ul

RT: 12.49 min Scan# 1667

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32

Tgt Ion:216 Resp: 87772


Ion Ratio Lower Upper

216 100

214 79.5 61.5 92.3

179 19.7 15.6 23.4

108 14.1 12.4 18.6


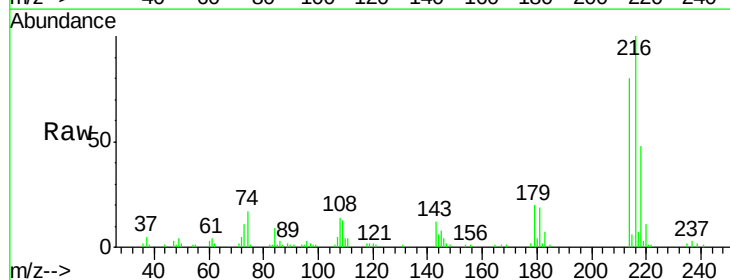



Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 108.00 (107.70 to 108.70): E

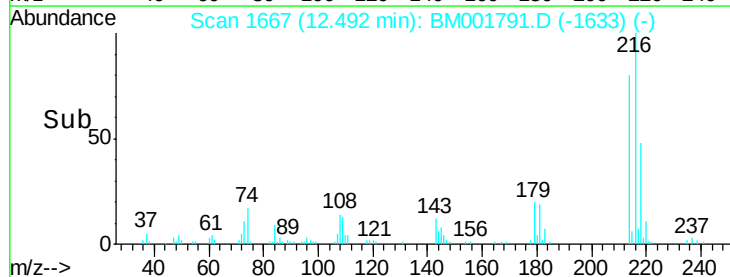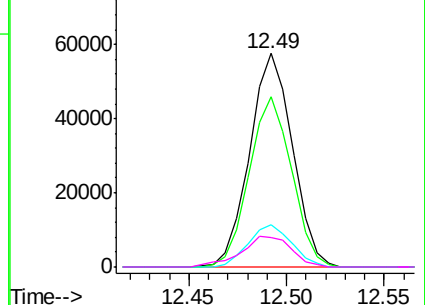

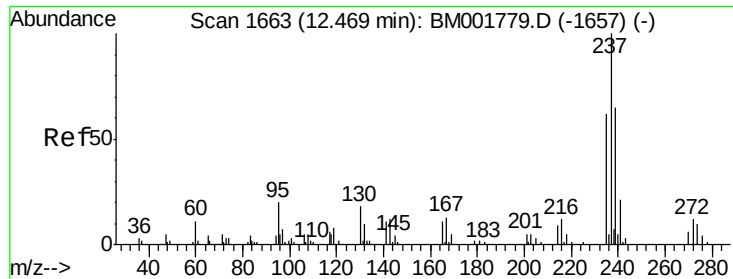

#37

Hexachlorocyclopentadiene

Concen: 16.81 ng/ul

RT: 12.47 min Scan# 1663

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32

Instrument :

BNA_M

ClientSampleId :

DFTPP65


Tgt Ion:237 Resp: 46354

Ion Ratio Lower Upper

237 100

235 62.0 49.2 73.8




272 12.5 8.8 13.2

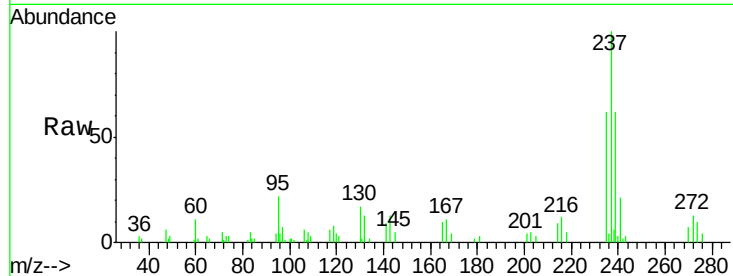

Abundance Ion 237.00 (236.70 to 237.70): E

Ion 235.00 (234.70 to 235.70): E

Ion 272.00 (271.70 to 272.70): E

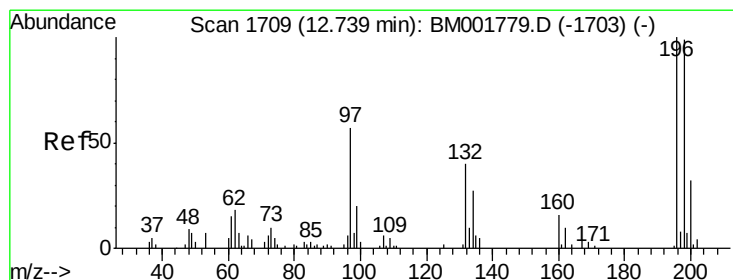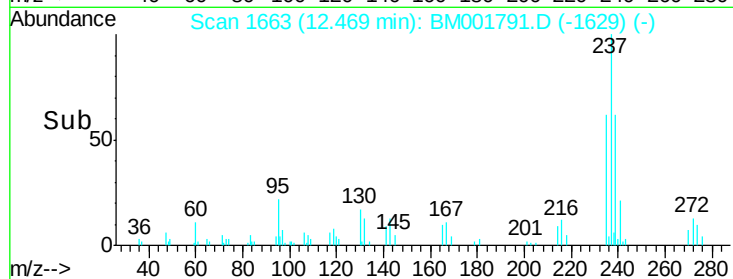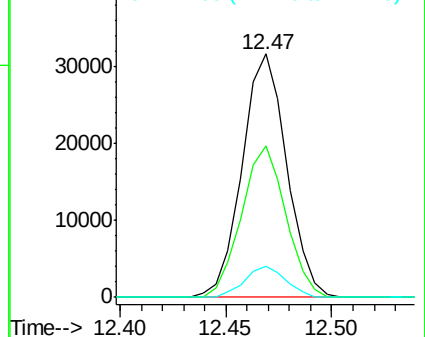

#38

2,4,6-Trichlorophenol

Concen: 20.08 ng/ul

RT: 12.74 min Scan# 1709

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32


Tgt Ion:196 Resp: 53307

Ion Ratio Lower Upper

196 100

198 99.3 74.4 111.6



200 31.4 25.0 37.4

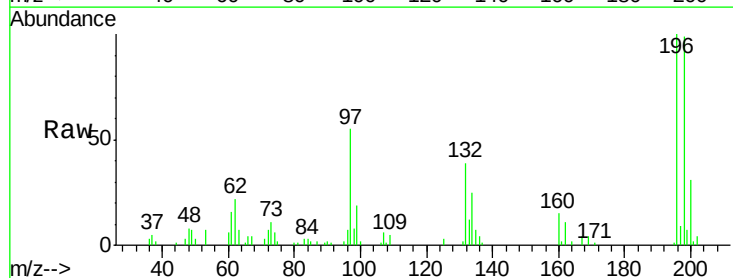


Abundance Ion 196.00 (195.70 to 196.70): E

Ion 198.00 (197.70 to 198.70): E

Ion 200.00 (199.70 to 200.70): E

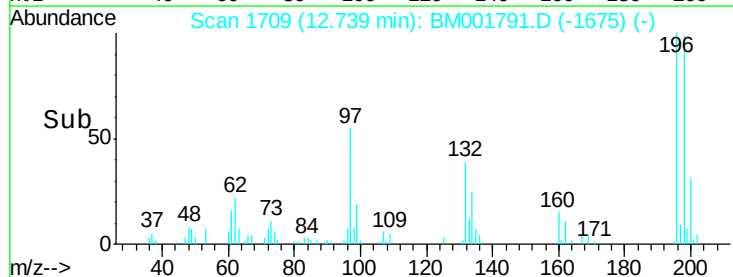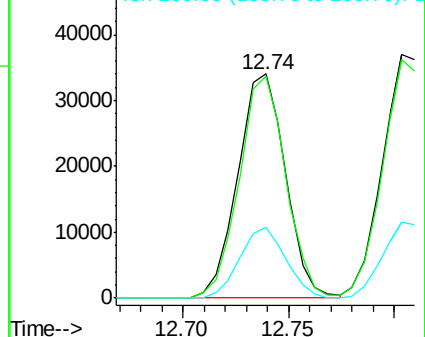


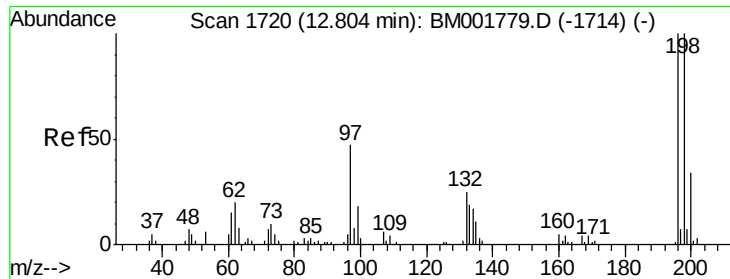




#39
 2,4,5-Trichlorophenol
 Concen: 19.67 ng/ul
 RT: 12.80 min Scan# 1720
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP65

Tgt Ion:196 Resp: 57149
 Ion Ratio Lower Upper
 196 100
 198 97.7 79.0 118.4
 200 31.3 26.2 39.4

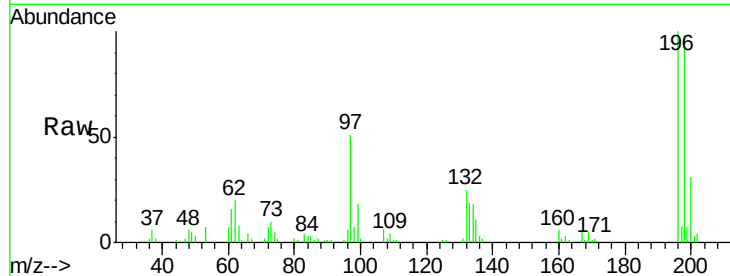


Abundance Ion 196.00 (195.70 to 196.70): E
 Ion 198.00 (197.70 to 198.70): E
 Ion 200.00 (199.70 to 200.70): E

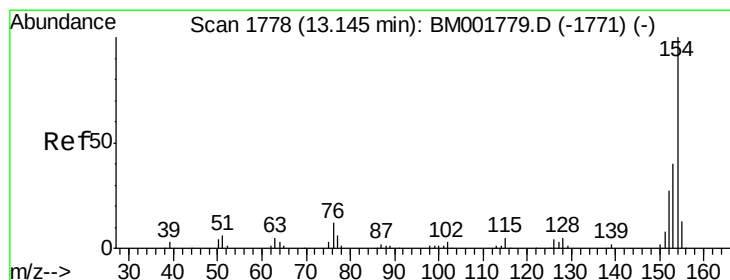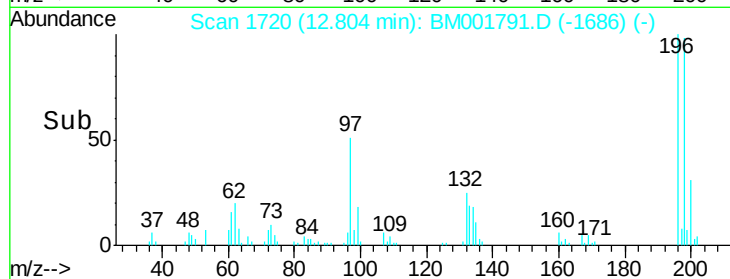
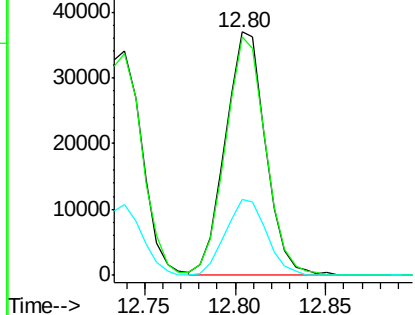



#40
 1,1'-Biphenyl
 Concen: 18.73 ng/ul
 RT: 13.14 min Scan# 1778
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32

Tgt Ion:154 Resp: 186681
 Ion Ratio Lower Upper
 154 100
 153 40.7 32.5 48.7
 76 10.9 9.0 13.6

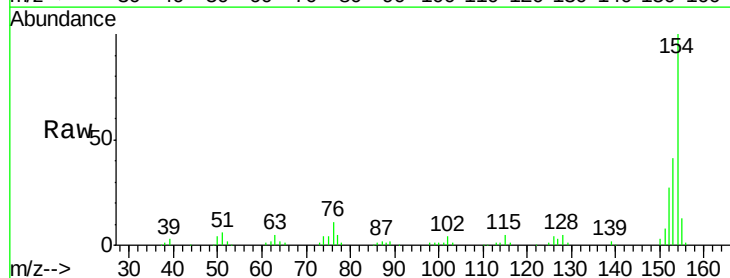

Abundance Ion 154.00 (153.70 to 154.70): E
 Ion 153.00 (152.70 to 153.70): E
 Ion 76.00 (75.70 to 76.70): BM



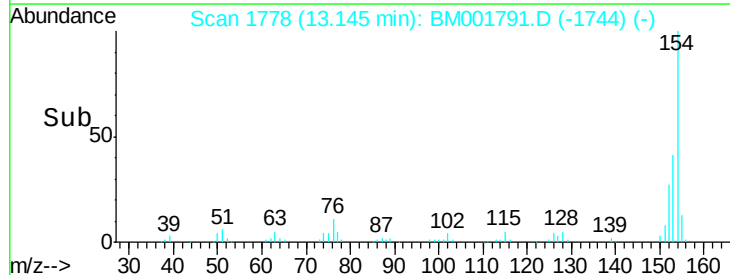
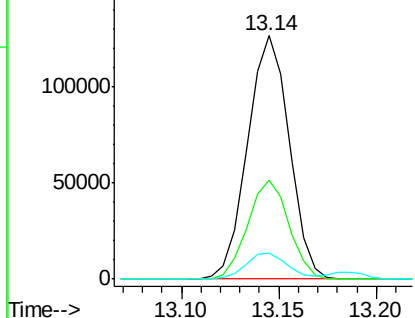




#41
 2-Chloronaphthalene
 Concen: 18.90 ng/ul
 RT: 13.19 min Scan# 1785
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32




Instrument :
 BNA_M
 ClientSampleId :
 DFTPP65


Tgt Ion: 162 Resp: 147657
 Ion Ratio Lower Upper
 162 100
 164 34.7 27.2 40.8
 127 39.1 32.6 49.0

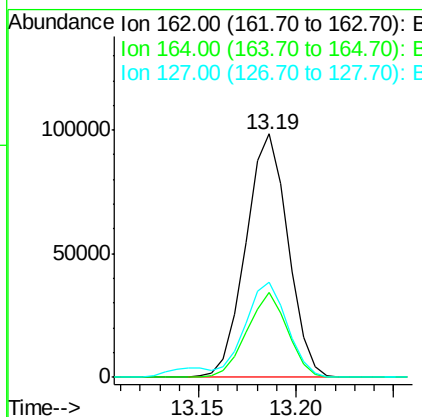

#42
 2-Nitroaniline
 Concen: 19.85 ng/ul
 RT: 13.40 min Scan# 1821
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32

Tgt Ion: 65 Resp: 41114
 Ion Ratio Lower Upper
 65 100
 92 69.8 52.1 78.1
 138 110.8 78.8 118.2

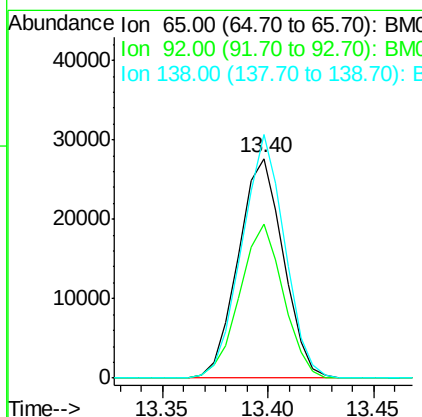

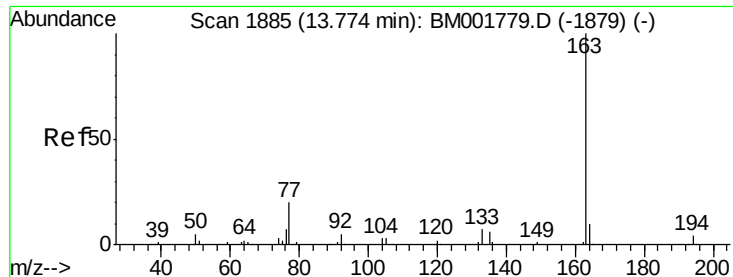

#44

Dimethylphthalate

Concen: 18.86 ng/ul

RT: 13.77 min Scan# 1885

Delta R.T. -0.01 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32

Instrument :

BNA_M

ClientSampleId :

DFTPP65


Tgt Ion:163 Resp: 186639

Ion Ratio Lower Upper

163 100

194 4.1 3.6 5.4




164 9.9 8.0 12.0

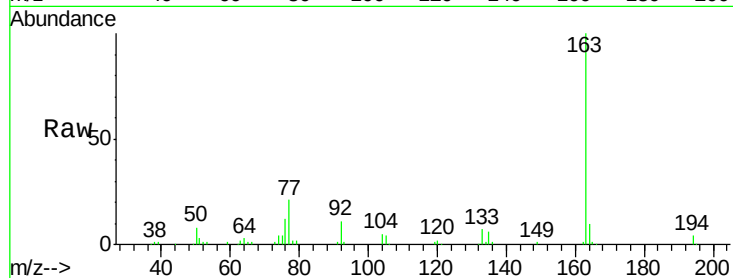

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

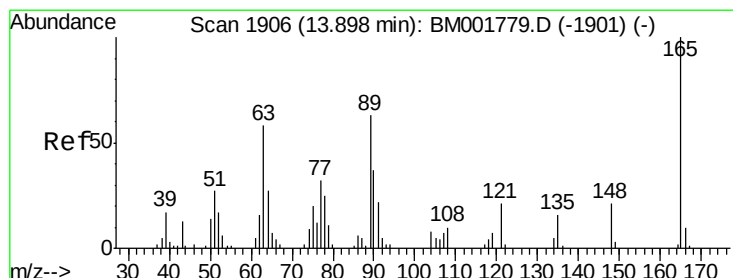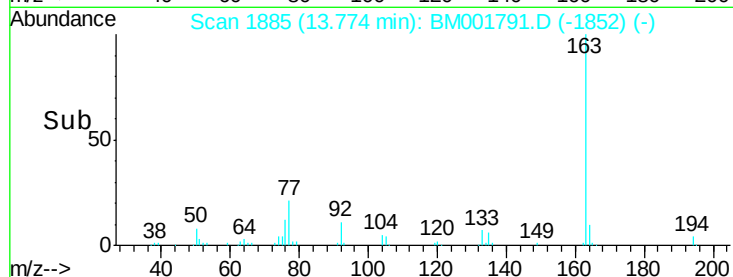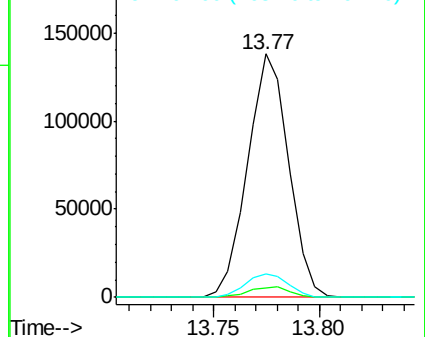

#45

2,6-Dinitrotoluene

Concen: 20.70 ng/ul

RT: 13.90 min Scan# 1906

Delta R.T. -0.01 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32


Tgt Ion:165 Resp: 38513

Ion Ratio Lower Upper

165 100

89 63.7 49.1 73.7



121 21.0 17.4 26.2

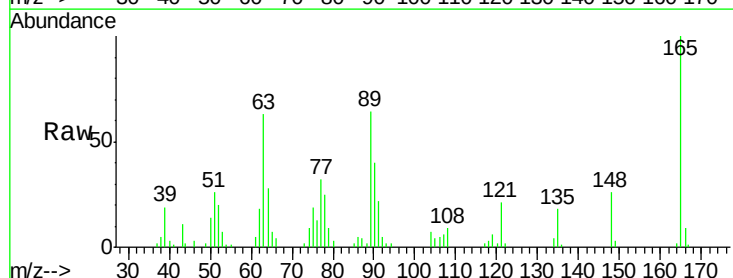


Abundance Ion 165.00 (164.70 to 165.70): E

Ion 89.00 (88.70 to 89.70): BM0

Ion 121.00 (120.70 to 121.70): E

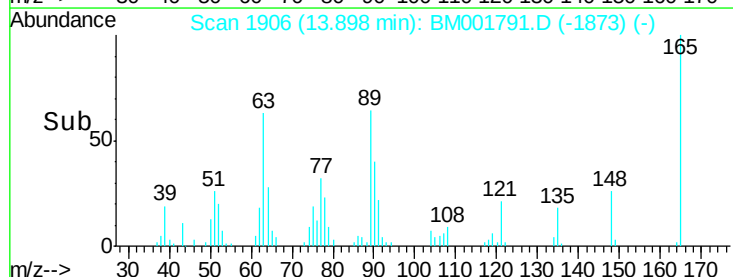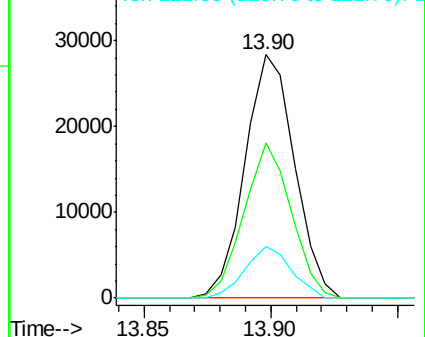



#47

Acenaphthylene

Concen: 19.15 ng/ul

RT: 14.04 min Scan# 1930

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32

Instrument :

BNA_M

ClientSampleId :

DFTPP65


Tgt Ion:152 Resp: 231671

Ion Ratio Lower Upper

152 100

151 19.6 15.9 23.9




153 12.6 10.0 15.0



Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

Ion 153.00 (152.70 to 153.70): E

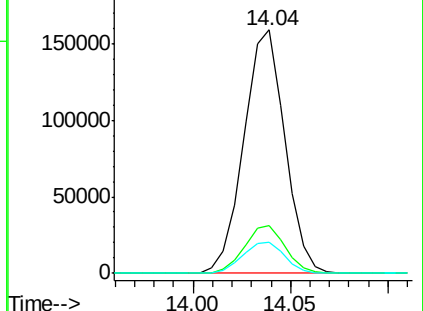

#48

3-Nitroaniline

Concen: 22.37 ng/ul

RT: 14.23 min Scan# 1962

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32


Tgt Ion:138 Resp: 38894

Ion Ratio Lower Upper

138 100

108 12.1 10.0 15.0



92 118.9 100.4 150.6




Abundance Ion 138.00 (137.70 to 138.70): E

Ion 108.00 (107.70 to 108.70): E

Ion 92.00 (91.70 to 92.70): BM

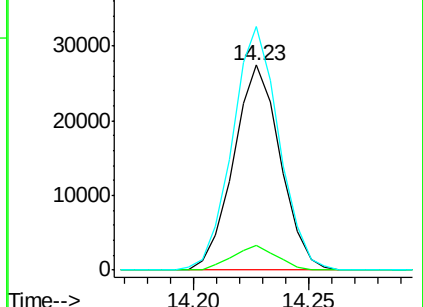



#49

Acenaphthene

Concen: 19.14 ng/ul

RT: 14.38 min Scan# 1988

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32

Instrument :

BNA_M

ClientSampleId :

DFTPP65


Tgt Ion:153 Resp: 154754

Ion Ratio Lower Upper

153 100

152 46.8 36.6 55.0




154 87.2 72.6 108.8



Abundance Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

Ion 154.00 (153.70 to 154.70): E

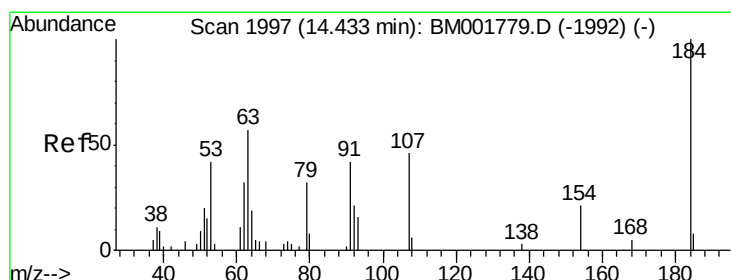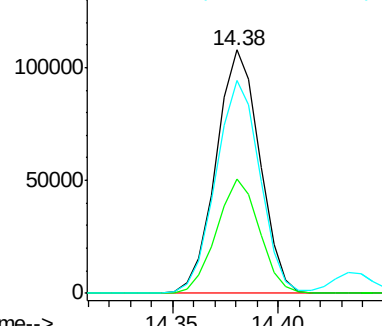

#50

2,4-Dinitrophenol

Concen: 17.05 ng/ul

RT: 14.44 min Scan# 1998

Delta R.T. 0.01 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32


Tgt Ion:184 Resp: 19660

Ion Ratio Lower Upper

184 100

63 54.6 51.0 76.6



154 65.6 46.9 70.3

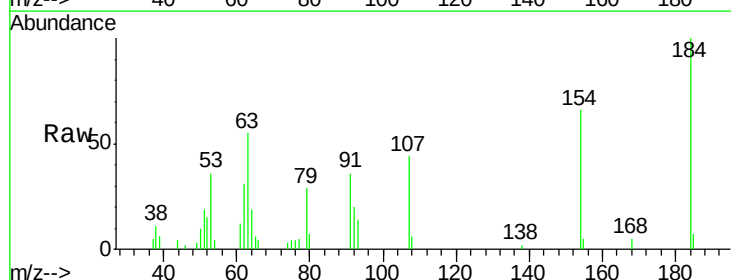


Abundance Ion 184.00 (183.70 to 184.70): E

Ion 63.00 (62.70 to 63.70): BM0

Ion 154.00 (153.70 to 154.70): E

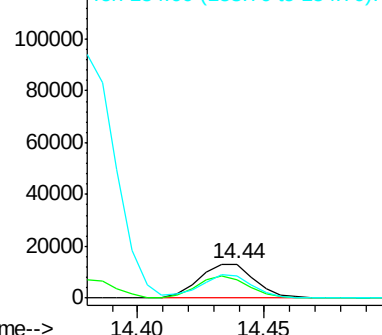


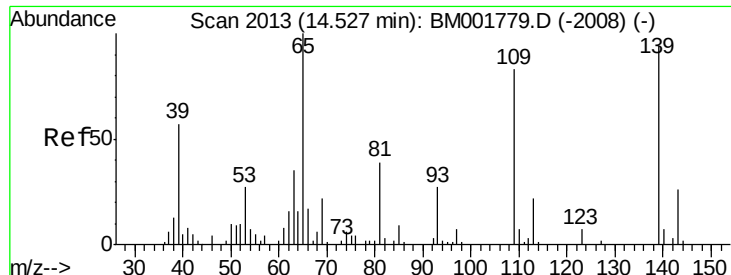




#52
4-Nitrophenol
Concen: 18.90 ng/ul
RT: 14.53 min Scan# 2014
Delta R.T. 0.00 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32

Instrument :
BNA_M
ClientSampleId :
DFTPP65

Tgt Ion:109 Resp: 32620
Ion Ratio Lower Upper
109 100
139 104.0 81.7 122.5
65 111.0 94.3 141.5




Abundance Ion 109.00 (108.70 to 109.70): E
Ion 139.00 (138.70 to 139.70): E
Ion 65.00 (64.70 to 65.70): BM


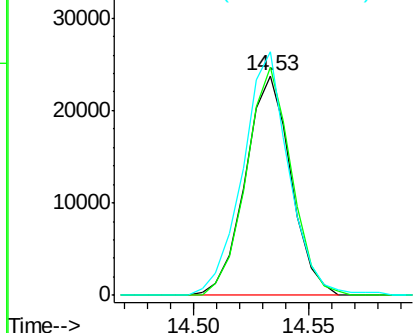



#53
Dibenzofuran
Concen: 19.27 ng/ul
RT: 14.72 min Scan# 2045
Delta R.T. 0.00 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32

Tgt Ion:168 Resp: 223126
Ion Ratio Lower Upper
168 100
139 37.6 30.1 45.1



Abundance Ion 168.00 (167.70 to 168.70): E
Ion 139.00 (138.70 to 139.70): E




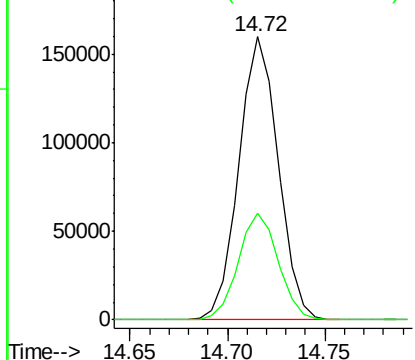




#54
 2,4-Dinitrotoluene
 Concen: 20.48 ng/ul
 RT: 14.69 min Scan# 2040
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32




Instrument :
 BNA_M
 ClientSampleId :
 DFTPP65


Tgt Ion:165 Resp: 56186
 Ion Ratio Lower Upper
 165 100
 63 43.6 35.4 53.2
 182 2.4 2.1 3.1

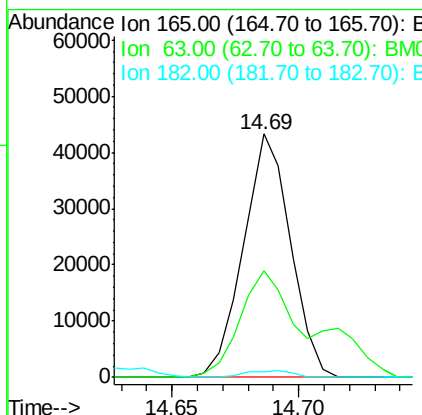

#55
 2,3,4,6-Tetrachlorophenol
 Concen: 20.14 ng/ul
 RT: 14.94 min Scan# 2084
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32

Tgt Ion:232 Resp: 50570
 Ion Ratio Lower Upper
 232 100
 131 42.3 32.9 49.3
 130 2.3 1.8 2.8
 166 30.2 23.0 34.4

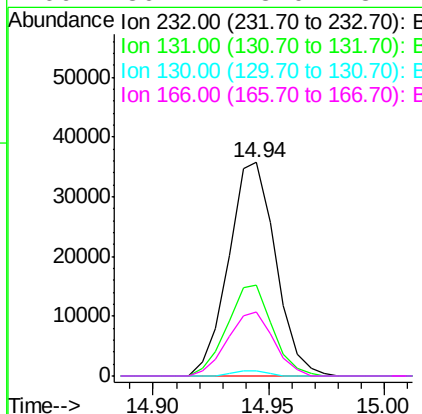







#56
Diethylphthalate
Concen: 19.27 ng/ul
RT: 15.14 min Scan# 2118
Delta R.T. -0.01 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32

Instrument :
BNA_M
ClientSampleId :
DFTPP65

Tgt Ion:149 Resp: 181311
Ion Ratio Lower Upper
149 100
177 22.7 17.3 25.9
150 13.0 10.1 15.1




Abundance Ion 149.00 (148.70 to 149.70): E
Ion 177.00 (176.70 to 177.70): E
Ion 150.00 (149.70 to 150.70): E


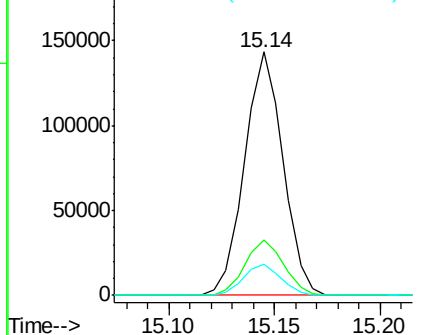



#58
Fluorene
Concen: 19.17 ng/ul
RT: 15.37 min Scan# 2156
Delta R.T. 0.00 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32

Tgt Ion:166 Resp: 184787
Ion Ratio Lower Upper
166 100
165 95.7 77.4 116.2
167 12.7 11.3 16.9



Abundance Ion 166.00 (165.70 to 166.70): E
Ion 165.00 (164.70 to 165.70): E
Ion 167.00 (166.70 to 167.70): E




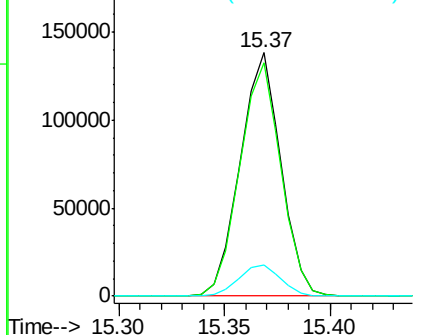


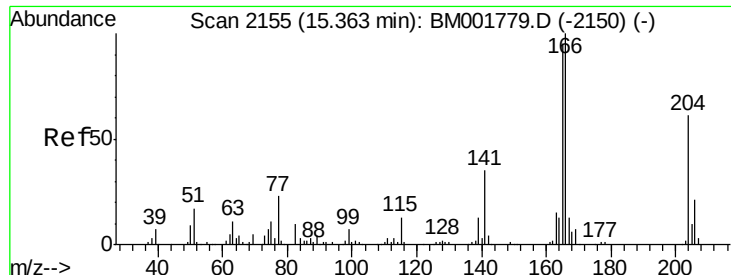

#59
 4-Chlorophenyl-phenylether
 Concen: 19.23 ng/ul
 RT: 15.36 min Scan# 2155
 Delta R.T. -0.01 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32




Instrument :
 BNA_M
 ClientSampleId :
 DFTPP65


Tgt Ion:204 Resp: 99897
 Ion Ratio Lower Upper
 204 100
 206 33.7 25.8 38.6
 141 57.3 46.6 69.8

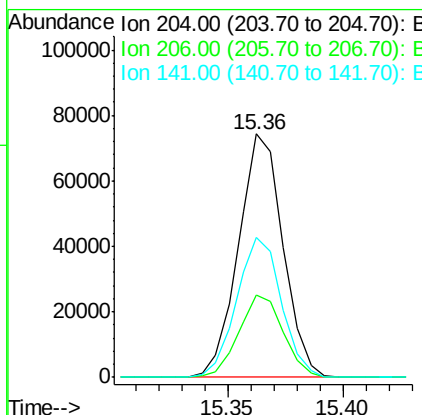

#60
 4-Nitroaniline
 Concen: 20.60 ng/ul
 RT: 15.39 min Scan# 2160
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32

Tgt Ion:138 Resp: 40648
 Ion Ratio Lower Upper
 138 100
 92 56.0 45.6 68.4
 108 110.2 89.6 134.4

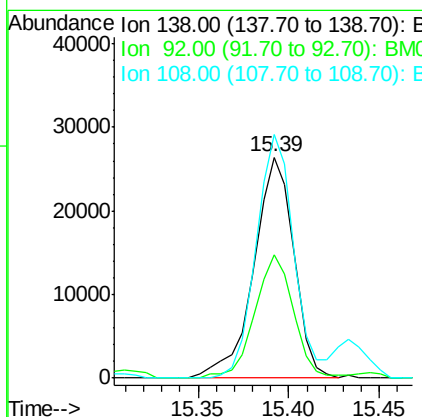







#63
 4,6-Dinitro-2-methylphenol
 Concen: 17.51 ng/ul
 RT: 15.45 min Scan# 2170
 Delta R.T. 0.01 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP65

Tgt Ion:198 Resp: 31892
 Ion Ratio Lower Upper
 198 100
 182 3.4 2.9 4.3
 77 26.0 19.4 29.2




Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 182.00 (181.70 to 182.70): E
 Ion 77.00 (76.70 to 77.70): B


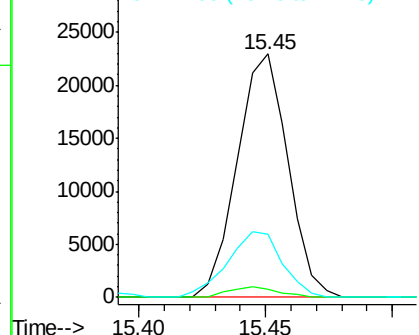



#64
 N-Nitrosodiphenylamine
 Concen: 19.32 ng/ul
 RT: 15.58 min Scan# 2192
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32

Tgt Ion:169 Resp: 158028
 Ion Ratio Lower Upper
 169 100
 168 65.5 52.9 79.3
 167 34.7 27.5 41.3



Abundance Ion 169.00 (168.70 to 169.70): E
 Ion 168.00 (167.70 to 168.70): E
 Ion 167.00 (166.70 to 167.70): E

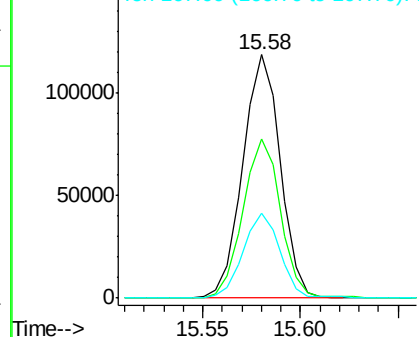


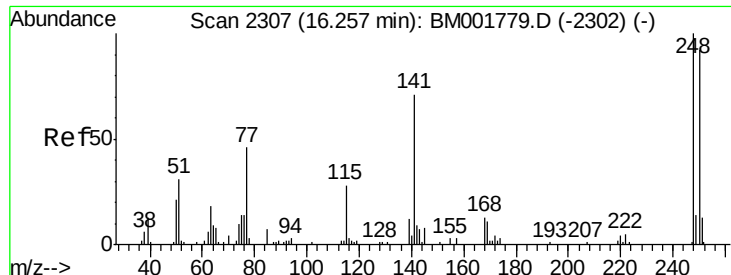




#65
4-Bromophenyl-phenylether
Concen: 19.68 ng/ul
RT: 16.26 min Scan# 2307
Delta R.T. -0.01 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32

Instrument :
BNA_M
ClientSampleId :
DFTPP65

Tgt Ion:248 Resp: 61436
Ion Ratio Lower Upper
248 100
250 98.7 82.2 123.4
141 74.6 60.7 91.1




Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E


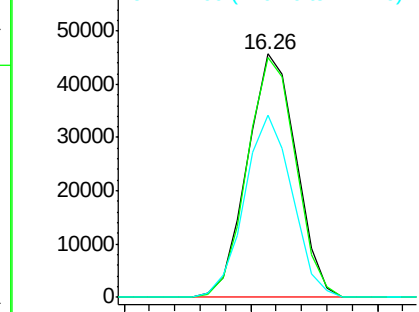



#66
Hexachlorobenzene
Concen: 19.65 ng/ul
RT: 16.37 min Scan# 2326
Delta R.T. 0.00 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32

Tgt Ion:284 Resp: 68927
Ion Ratio Lower Upper
284 100
142 32.7 26.6 39.8
249 32.8 27.7 41.5



Abundance Ion 284.00 (283.70 to 284.70): E
Ion 142.00 (141.70 to 142.70): E
Ion 249.00 (248.70 to 249.70): E




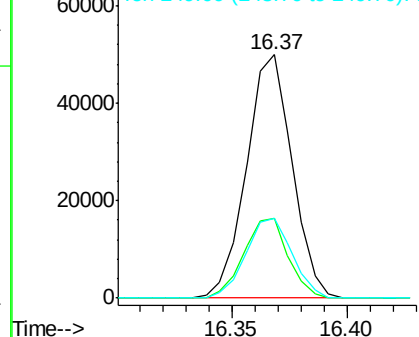


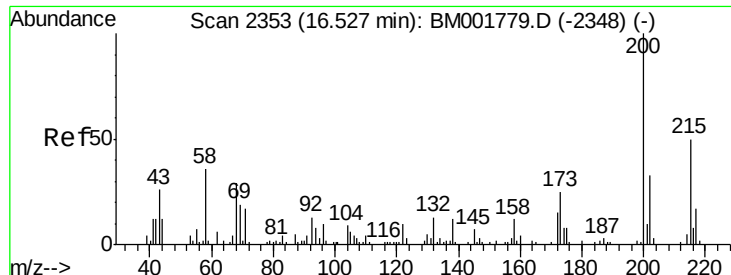

#67
 Atrazine
 Concen: 19.40 ng/ul
 RT: 16.53 min Scan# 2354
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32




Instrument :
 BNA_M
 ClientSampled :
 DFTPP65


Tgt Ion	Ratio	Lower	Upper
200	100		
173	23.6	19.6	29.4
215	49.8	36.2	54.4

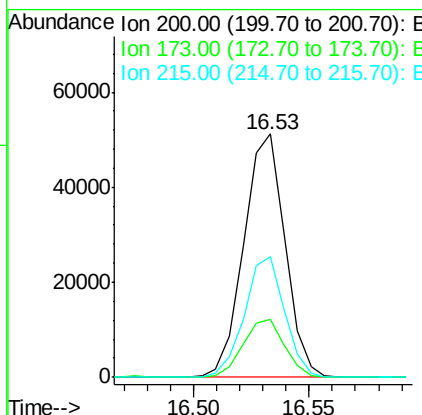

#68
 Pentachlorophenol
 Concen: 19.27 ng/ul
 RT: 16.71 min Scan# 2384
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32

Tgt Ion	Ratio	Lower	Upper
266	100		
264	65.7	50.8	76.2
268	65.0	52.0	78.0

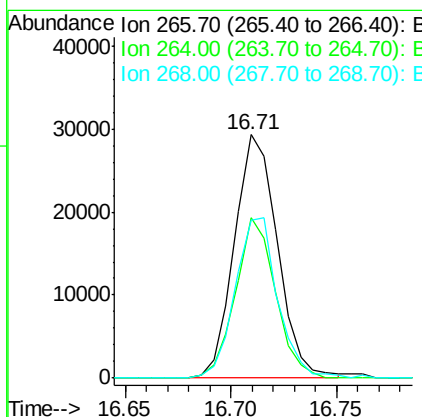



#69

Phenanthrene

Concen: 19.17 ng/ul

RT: 17.10 min Scan# 2451

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32

Instrument :

BNA_M

ClientSampleId :

DFTPP65


Tgt Ion:178 Resp: 290996

Ion Ratio Lower Upper

178 100

179 15.1 11.9 17.9




176 18.4 15.2 22.8



Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

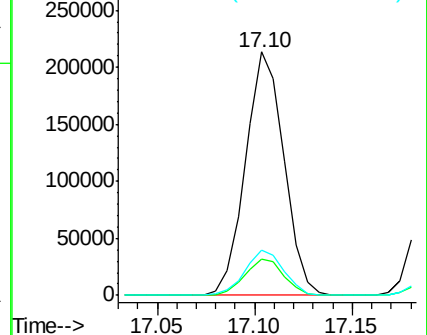

#71

Anthracene

Concen: 19.37 ng/ul

RT: 17.20 min Scan# 2467

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32


Tgt Ion:178 Resp: 301812

Ion Ratio Lower Upper

178 100

179 15.2 11.8 17.8



176 17.8 14.4 21.6




Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

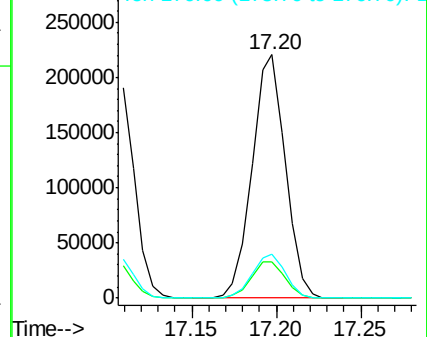



#72

1,2,3,4-Tetrachlorobenzene

Concen: 19.22 ng/uL

RT: 13.11 min Scan# 1772

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32

Instrument :

BNA_M

ClientSampled :

DFTPP65


Tgt Ion:216 Resp: 84594

Ion Ratio Lower Upper

216 100

214 74.8 65.1 97.7




218 47.8 42.2 63.4



Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

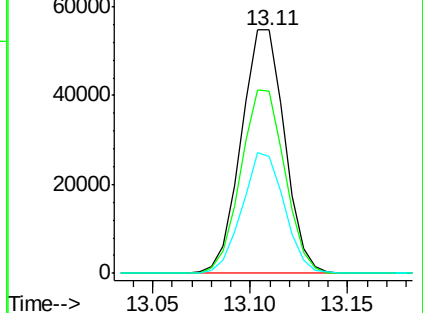

#73

Pentachlorobenzene

Concen: 19.30 ng/uL

RT: 14.63 min Scan# 2031

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32


Tgt Ion:250 Resp: 80086

Ion Ratio Lower Upper

250 100

248 62.8 48.4 72.6



252 63.3 49.9 74.9




Abundance Ion 250.00 (249.70 to 250.70): E

Ion 248.00 (247.70 to 248.70): E

Ion 252.00 (251.70 to 252.70): E

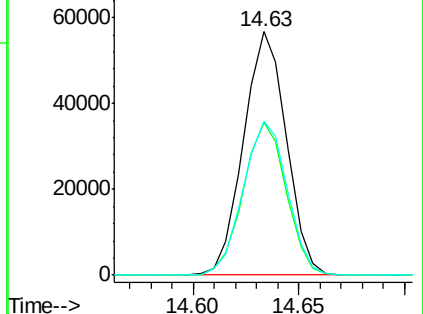



#74

Carbazole

Concen: 19.26 ng/ul

RT: 17.47 min Scan# 2513

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32

Instrument :

BNA_M

ClientSampleId :

DFTPP65


Tgt Ion:167 Resp: 263338

Ion Ratio Lower Upper

167 100

166 21.5 17.4 26.2


139 12.8 10.1 15.1





Abundance Ion 167.00 (166.70 to 167.70): E

Ion 166.00 (165.70 to 166.70): E

Ion 139.00 (138.70 to 139.70): E

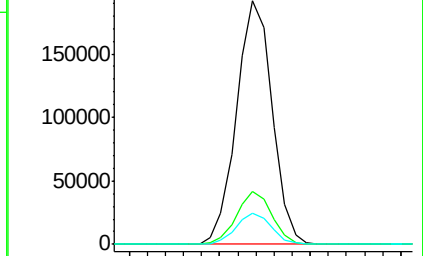

Time--> 17.40 17.45 17.50



#75

Di-n-butylphthalate

Concen: 20.22 ng/ul

RT: 18.03 min Scan# 2609

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32


Tgt Ion:149 Resp: 295314

Ion Ratio Lower Upper

149 100

150 9.1 7.4 11.0


104 6.0 4.7 7.1




Abundance Ion 149.00 (148.70 to 149.70): E


Ion 150.00 (149.70 to 150.70): E

Ion 104.00 (103.70 to 104.70): E

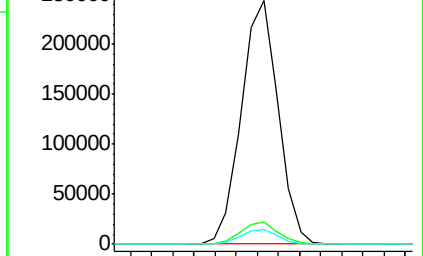

Time--> 18.00 18.05









#76
 Fluoranthene
 Concen: 19.46 ng/ul
 RT: 19.13 min Scan# 2795
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP65

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	353277		
101	7.1		6.1	9.1
100	5.3		4.8	7.2




Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B


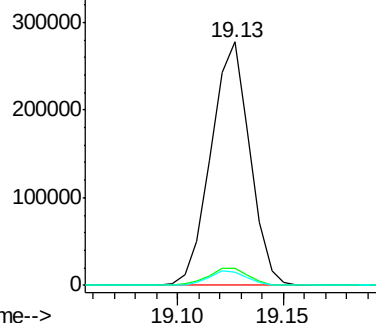



#79
 Pyrene
 Concen: 19.59 ng/ul
 RT: 19.49 min Scan# 2857
 Delta R.T. 0.00 min
 Lab File: BM001791.D
 Acq: 25 Jun 2015 10:32

Tgt Ion	Ratio	Resp	Lower	Upper
202	100	375924		
101	7.9		6.9	10.3
100	6.4		6.2	9.2



Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B



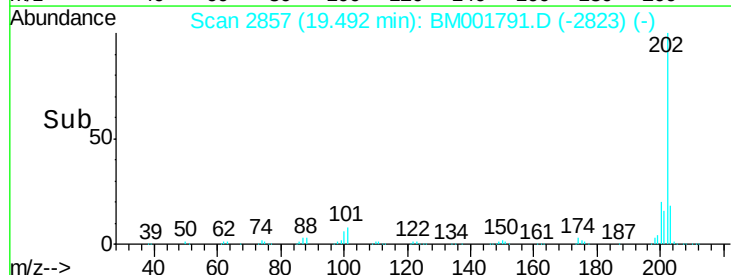
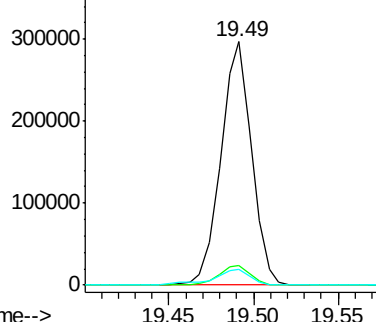




#80
Butylbenzylphthalate
Concen: 21.58 ng/ul
RT: 20.40 min Scan# 3011
Delta R.T. 0.00 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32




Instrument :
BNA_M
ClientSampleId :
DFTPP65


Tgt Ion	Ratio	Lower	Upper
149	100		
91	66.9	55.0	82.6
206	25.0	20.8	31.2

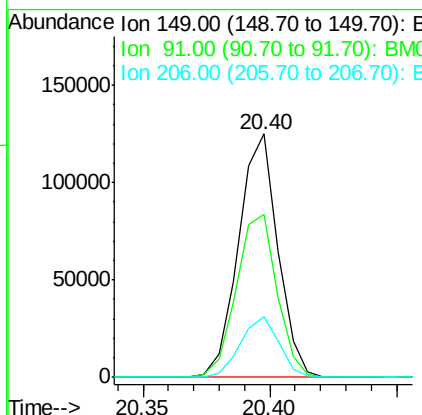

#81
3,3'-Dichlorobenzidine
Concen: 21.22 ng/ul
RT: 21.18 min Scan# 3144
Delta R.T. 0.00 min
Lab File: BM001791.D
Acq: 25 Jun 2015 10:32

Tgt Ion	Ratio	Lower	Upper
252	100		
254	65.6	50.9	76.3
126	7.5	7.0	10.6

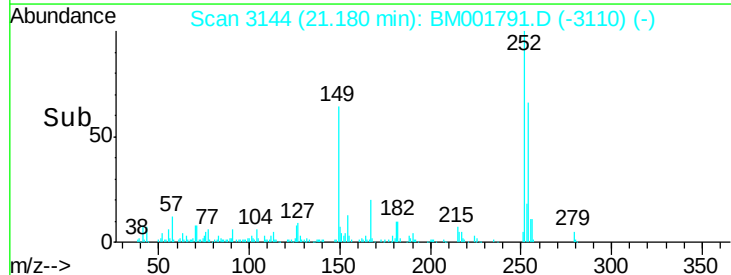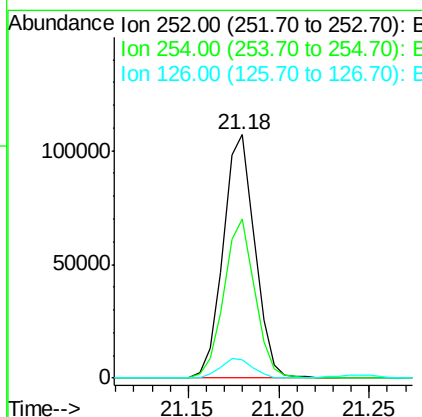



#82

Benzo(a)anthracene

Concen: 19.29 ng/ul

RT: 21.24 min Scan# 3154

Delta R.T. 0.00 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32

Instrument :

BNA_M

ClientSampleId :

DFTPP65


Tgt Ion:228 Resp: 389665

Ion Ratio Lower Upper




228 100

229 19.2 15.4 23.0

226 25.9 20.6 30.8



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

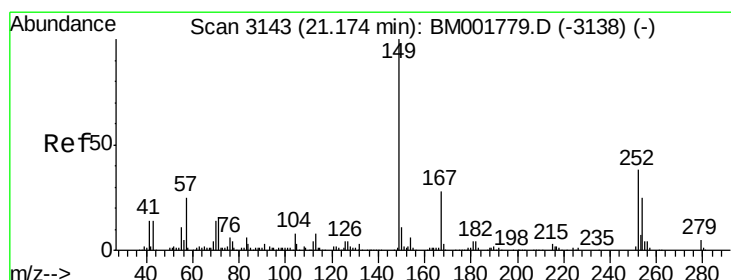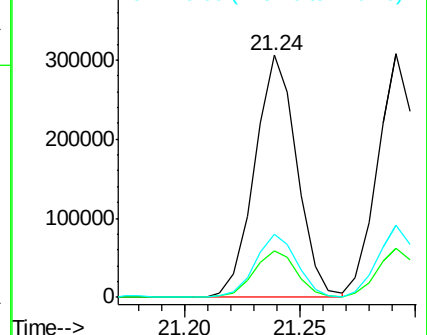

#83

Bis(2-ethylhexyl)phthalate

Concen: 21.07 ng/ul

RT: 21.17 min Scan# 3142

Delta R.T. -0.01 min

Lab File: BM001791.D

Acq: 25 Jun 2015 10:32


Tgt Ion:149 Resp: 198303

Ion Ratio Lower Upper

149 100

167 28.3 22.7 34.1

279 5.1 3.8 5.8



Abundance Ion 149.00 (148.70 to 149.70): E
Ion 167.00 (166.70 to 167.70): E
Ion 279.00 (278.70 to 279.70): E

