

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062515\
 Data File : BM001798.D
 Acq On : 25 Jun 2015 14:47
 Operator : TP/IZ
 Sample : G2760-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BK2

Quant Time: Jun 26 05:15:41 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 26 04:32:51 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	42144	20.00	ng/ul	0.00
18) Naphthalene-d8	10.45	136	170733	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.32	164	108020	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.06	188	256944	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	313446	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	309905	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.14	96	1410	1.60	ng/uL	0.00
5) Phenol-d5	6.83	99	24672	7.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	56437	31.13	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	70541	27.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	35463	13.65	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	41496	35.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.54	143	49258	38.12	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	88548	32.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.60	131	3417	1.21	ng/ul	0.00
43) Dimethylphthalate-d6	13.73	166	274377	34.25	ng/ul	0.00
46) Acenaphthylene-d8	14.01	160	365099	34.77	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	10850	7.34	ng/ul	0.00
57) Fluorene-d10	15.31	176	267131	35.94	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	46902	29.88	ng/ul	0.00
70) Anthracene-d10	17.16	188	418019	34.92	ng/ul	0.00
78) Pyrene-d10	19.46	212	483792	36.44	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	445671	32.63	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
20) Nitrobenzene	8.86	77	39922	12.48	ng/ul	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062515\
Data File : BM001798.D
Acq On : 25 Jun 2015 14:47
Operator : TP/IZ
Sample : G2760-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BK2

Quant Time: Jun 26 05:15:41 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM061515.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 26 04:32:51 2015
Response via : Initial Calibration

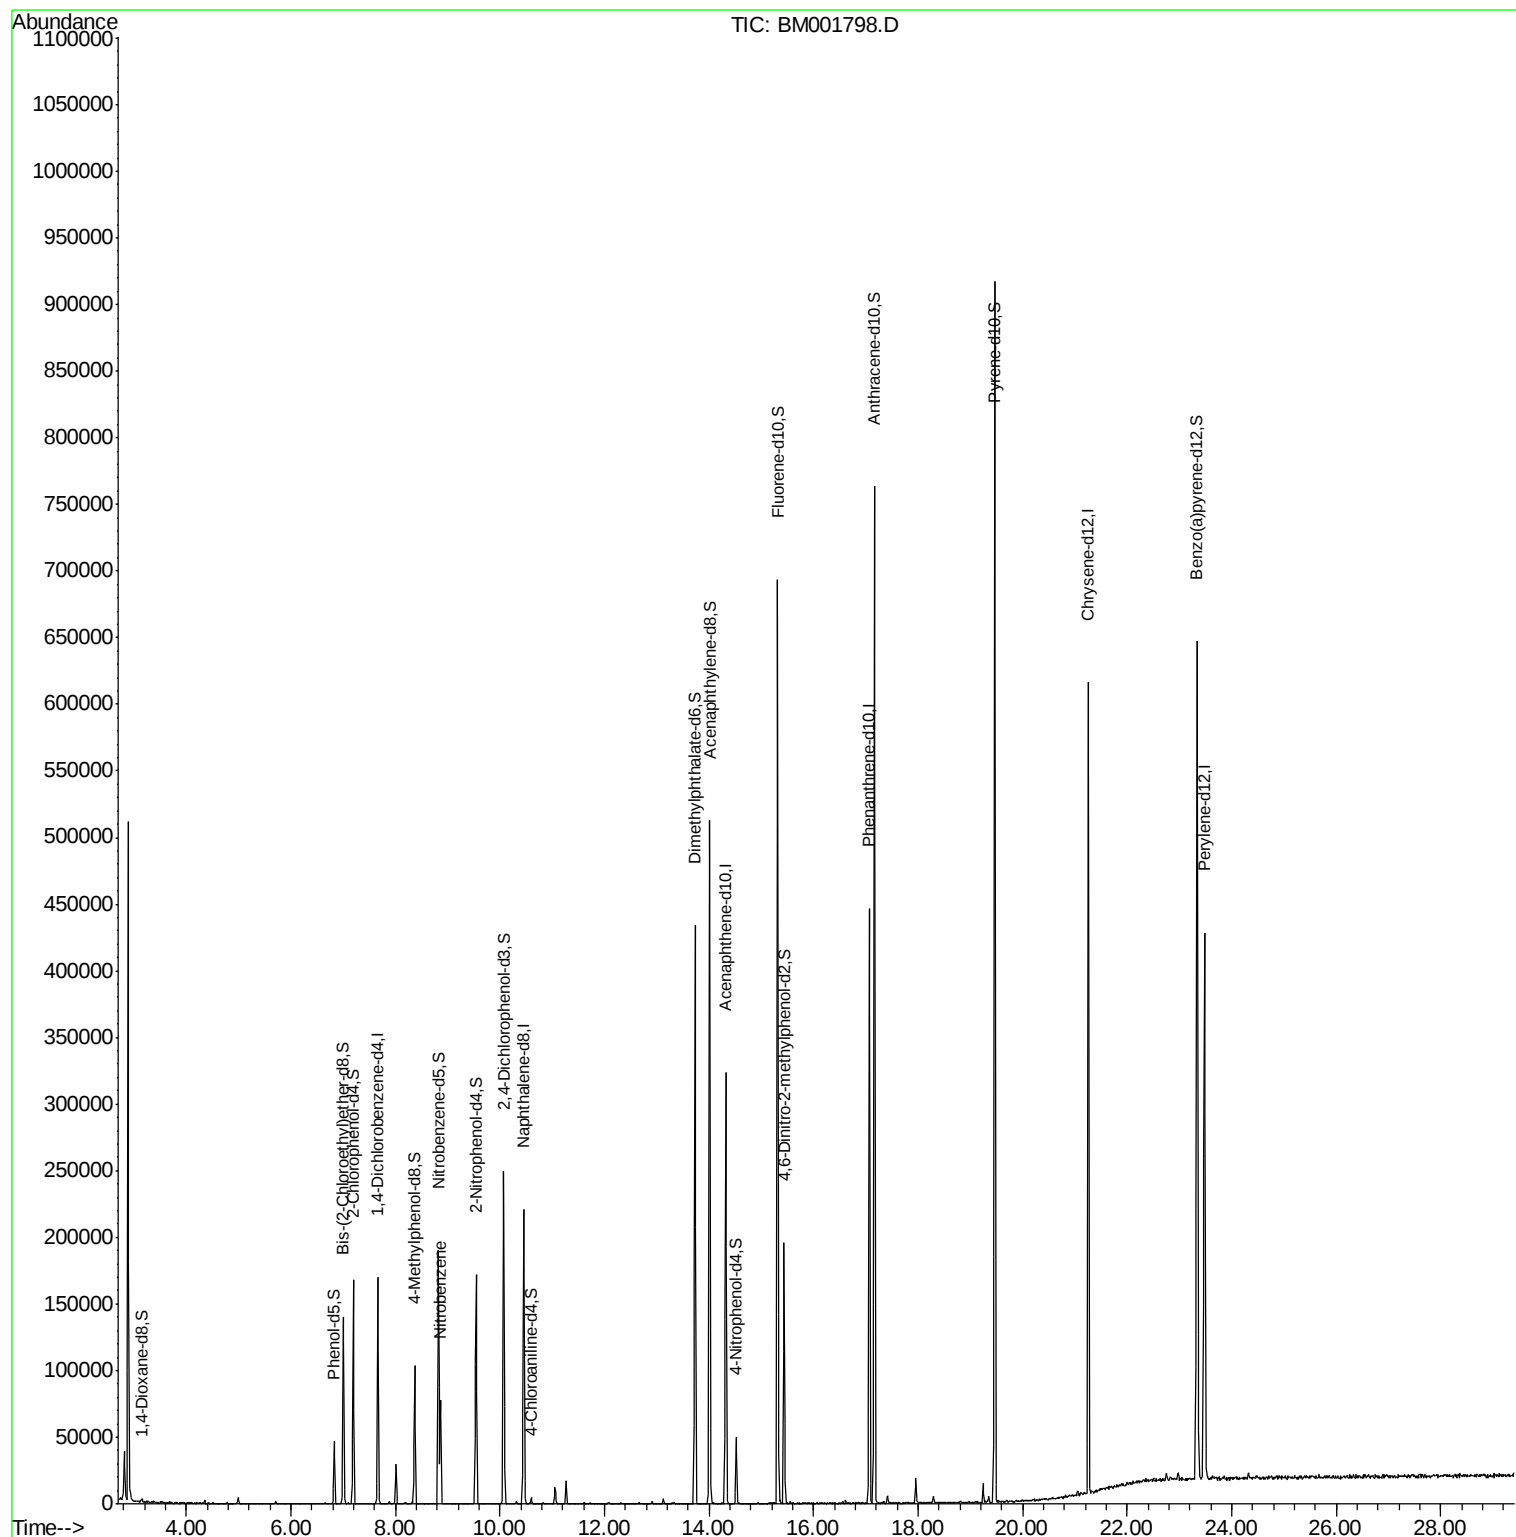

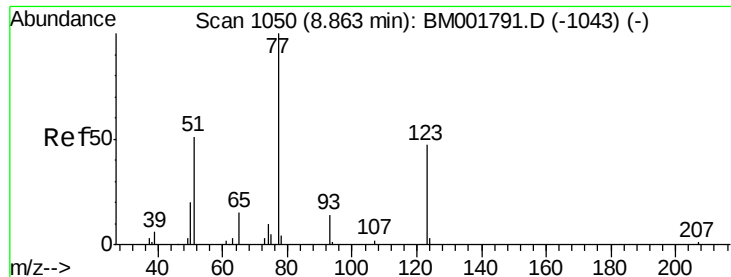

#20

Nitrobenzene

Concen: 12.48 ng/ul

RT: 8.86 min Scan# 1050

Delta R.T. -0.00 min

Lab File: BM001798.D

Acq: 25 Jun 2015 14:47

Instrument :

BNA_M

ClientSampleId :

C0BK2


Tgt Ion: 77 Resp: 39922

Ion Ratio Lower Upper

77 100

123 48.3 34.0 51.0

65 16.0 11.3 16.9

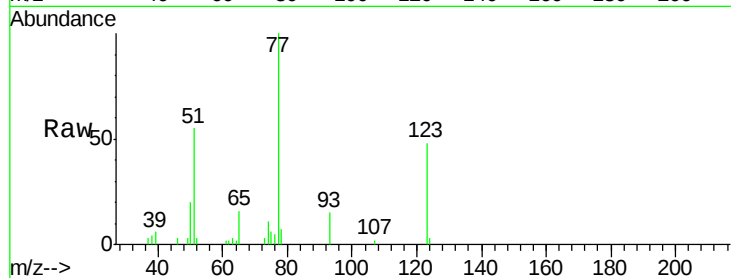

Abundance Ion 77.00 (76.70 to 77.70): BM001798.D (-1016) (-)

