


Data Path : Z:\HPCHEM1\BNA_M\Data\BM062515\
 Data File : BM001790.D
 Acq On : 25 Jun 2015 09:56
 Operator : TP/IZ
 Sample : DFTPP65
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP65

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM042815.M
 Title : SVOA CALIBRATION
 Last Update : Tue Apr 28 06:36:34 2015

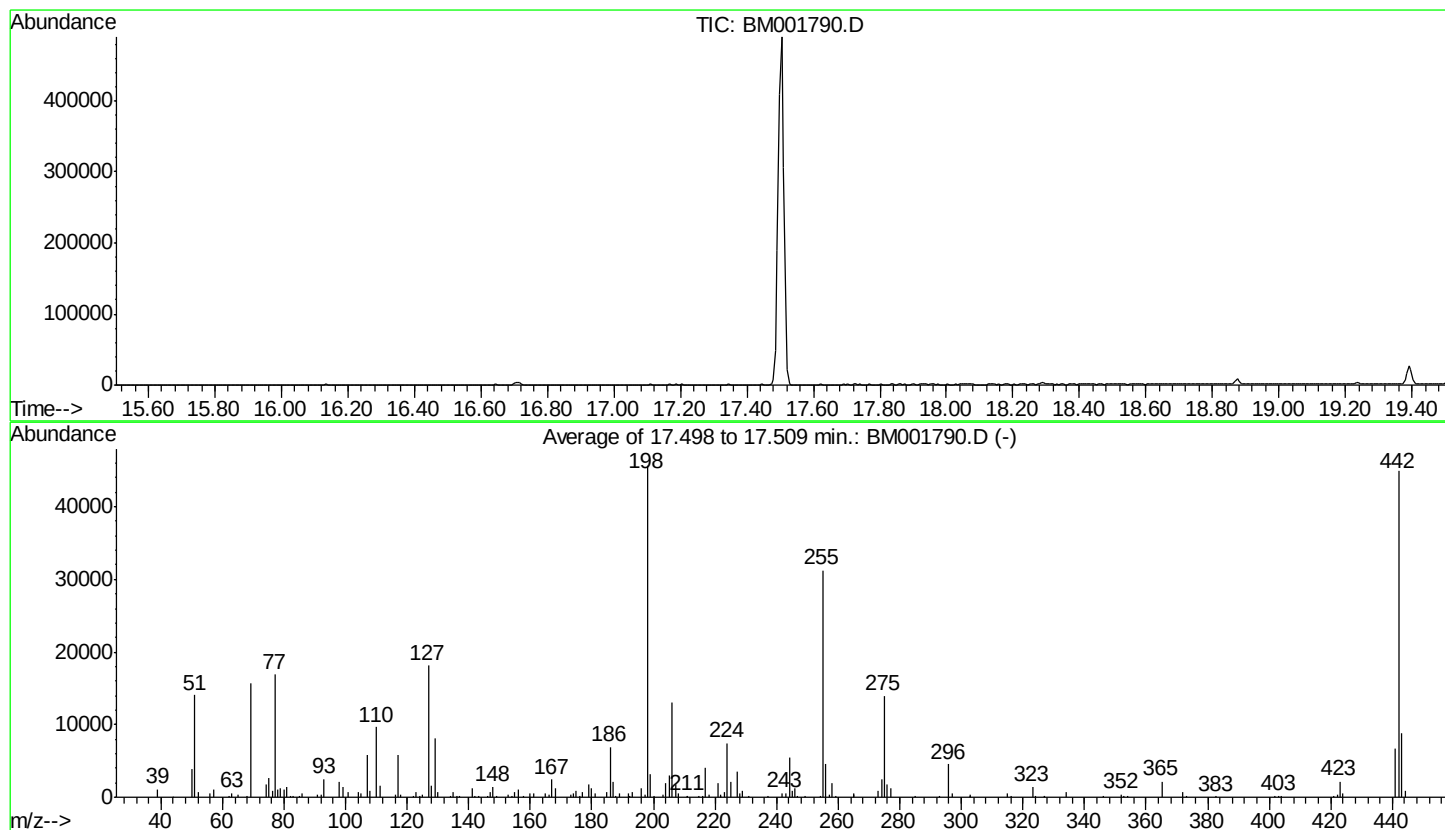

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2513

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.8	14052	PASS
68	69	0.00	2	1.6	242	PASS
69	198	0.00	100	34.2	15611	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	39.7	18137	PASS
197	198	0.00	2	0.9	400	PASS
198	198	100	100	100.0	45653	PASS
199	198	5	9	6.9	3157	PASS
275	198	10	60	30.5	13942	PASS
365	198	1	100	4.8	2173	PASS
441	443	0.01	100	76.4	6738	PASS
442	198	50	100	98.4	44917	PASS
443	442	15	24	19.6	8814	PASS

m/z	Abundance
39.10	1361.0
44.00	735.0
50.10	4501.0
51.10	15921.0
52.00	1052.0
56.00	584.0
57.00	1145.0
63.00	650.0
65.10	354.0
68.00	363.0
69.00	18224.0
74.00	2171.0
75.00	2853.0
76.10	1091.0
77.10	20008.0
78.00	1272.0
78.90	1476.0
80.00	1086.0
80.90	1791.0
82.00	349.0
83.00	311.0
84.90	304.0
85.90	598.0
90.90	434.0
92.10	506.0
93.00	2983.0
98.00	2537.0
99.00	1563.0
101.00	760.0
103.90	852.0
105.00	584.0
107.00	6912.0
108.00	945.0
110.00	10745.0
111.00	1605.0
116.00	445.0
117.00	6511.0
118.10	367.0
122.00	304.0
122.90	837.0
123.90	314.0
125.10	328.0
127.00	19080.0
128.00	1752.0
129.00	8578.0
130.00	756.0
135.00	776.0
136.00	402.0
137.10	304.0
140.90	1297.0
141.90	361.0
147.00	816.0
147.90	1783.0
148.90	331.0
152.90	488.0
154.00	302.0
155.00	659.0
155.90	1124.0
159.90	504.0
160.90	589.0
164.90	539.0
165.90	505.0
167.00	2648.0
168.00	1253.0
173.10	440.0
173.90	572.0
175.00	1034.0
175.90	323.0
176.90	720.0
178.90	1741.0
180.00	1028.0
181.00	642.0
185.00	873.0
186.00	7295.0
187.00	2157.0
189.00	516.0
191.90	553.0
192.90	802.0
195.90	1218.0
197.10	303.0
197.90	46880.0
199.00	3241.0
200.00	418.0
202.90	425.0
204.00	2069.0
205.00	2945.0
206.00	13321.0
207.00	1764.0
207.90	600.0
210.90	420.0
216.90	4471.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

218.00	597.0
221.00	1913.0
221.70	559.0
223.00	707.0
224.00	7791.0
225.00	2085.0
227.00	3676.0
228.00	582.0
229.10	776.0
237.10	362.0
242.10	351.0
243.00	521.0
244.10	5534.0
245.10	704.0
246.00	1249.0
255.00	32008.0
256.00	4633.0
257.10	342.0
258.00	1840.0
264.90	744.0
272.90	722.0
274.00	2354.0
275.00	13070.0
276.00	1638.0
276.90	1184.0
296.00	4529.0
296.90	419.0
302.80	384.0
314.90	382.0
323.10	1401.0
334.00	921.0
352.00	349.0
365.10	1871.0
372.00	673.0
403.20	308.0
422.10	359.0
423.00	1554.0
424.00	599.0
441.10	5266.0
442.10	35752.0
443.10	7456.0
444.10	710.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

m/z	Abundance
39.00	1233.0
44.00	744.0
50.10	4676.0
51.10	16648.0
52.00	746.0
56.00	629.0
57.00	1313.0
62.00	338.0
63.00	725.0
64.90	466.0
68.00	365.0
69.00	18400.0
74.00	1798.0
75.00	3382.0
76.10	1072.0
77.10	19464.0
78.00	1387.0
79.00	1408.0
80.00	1321.0
81.00	1719.0
81.90	382.0
83.00	392.0
85.00	427.0
86.00	561.0
91.00	417.0
92.00	418.0
93.00	2922.0
98.00	2133.0
99.00	1632.0
100.90	816.0
104.00	536.0
104.90	621.0
107.00	6662.0
108.00	1063.0
110.00	11610.0
111.00	2042.0
116.00	518.0
117.00	6996.0
117.90	472.0
122.00	445.0
122.90	715.0
124.00	383.0
125.00	488.0
127.00	21768.0
128.00	1840.0
129.00	9964.0
129.90	898.0
134.00	322.0
134.90	894.0
136.10	302.0
136.90	398.0
141.00	1484.0
141.90	405.0
143.00	370.0
146.00	369.0
147.00	937.0
148.00	1484.0
153.00	584.0
154.00	416.0
155.00	889.0
155.90	1228.0
157.90	362.0
160.00	598.0
160.90	653.0
165.00	575.0
165.90	382.0
167.00	2673.0
168.00	1545.0
173.10	401.0
173.90	619.0
175.00	1026.0
176.90	736.0
179.00	1937.0
179.90	1628.0
181.00	854.0
185.00	876.0
186.00	8193.0
187.00	2533.0
187.90	309.0
189.00	649.0
191.90	681.0
193.00	833.0
196.00	1717.0
197.10	446.0
198.00	55464.0
198.90	3964.0
200.00	347.0
202.90	500.0
204.00	2405.0
205.00	3995.0
206.00	15863.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

207.00	2143.0
208.00	778.0
211.10	702.0
214.90	363.0
215.90	314.0
217.00	4953.0
218.00	612.0
221.00	2196.0
221.90	585.0
223.00	991.0
224.00	8756.0
225.00	2380.0
227.00	4329.0
227.90	671.0
229.00	1021.0
231.00	526.0
241.90	631.0
243.00	676.0
244.00	7045.0
245.00	1008.0
245.90	1508.0
246.90	414.0
249.10	308.0
254.10	342.0
255.00	36776.0
256.00	5552.0
257.10	382.0
258.00	2661.0
259.10	475.0
265.10	864.0
273.00	1045.0
274.00	2935.0
275.00	16992.0
276.00	2484.0
277.00	1623.0
285.00	304.0
292.90	450.0
296.00	5500.0
297.00	575.0
303.00	644.0
315.00	600.0
316.00	351.0
323.00	1577.0
326.90	363.0
334.00	870.0
346.00	417.0
352.00	415.0
352.90	349.0
354.00	572.0
365.00	2928.0
372.00	1026.0
373.10	314.0
382.90	338.0
401.90	337.0
403.10	463.0
404.00	385.0
421.00	394.0
422.00	338.0
423.00	2966.0
424.00	650.0
441.10	8149.0
442.10	54408.0
443.10	10137.0
444.10	1138.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

m/z	Abundance
39.00	685.0
44.00	649.0
50.00	2545.0
51.00	9589.0
52.00	538.0
56.00	321.0
57.00	675.0
63.10	311.0
69.00	10209.0
74.00	1102.0
75.00	1603.0
76.00	448.0
77.10	11073.0
78.00	754.0
78.90	789.0
80.00	626.0
81.00	963.0
85.90	314.0
93.00	1669.0
98.00	1435.0
99.00	855.0
100.90	371.0
104.00	509.0
105.00	410.0
107.00	3915.0
107.90	593.0
110.00	6579.0
111.00	991.0
117.00	3881.0
122.80	510.0
127.00	13565.0
128.00	948.0
129.00	5609.0
130.10	462.0
135.00	524.0
140.90	763.0
147.10	438.0
147.90	1119.0
155.00	377.0
155.90	800.0
159.90	331.0
160.90	343.0
165.00	384.0
167.00	1904.0
168.00	1001.0
174.00	419.0
175.00	850.0
177.00	531.0
179.00	1513.0
180.00	1009.0
180.90	358.0
184.90	584.0
186.00	5231.0
187.00	1612.0
188.90	387.0
191.80	301.0
192.10	304.0
193.00	667.0
195.90	944.0
197.10	453.0
197.90	34616.0
199.00	2268.0
204.00	1197.0
205.00	2300.0
206.00	10172.0
207.10	1590.0
207.90	459.0
217.00	2941.0
221.00	1480.0
222.00	403.0
223.00	541.0
224.00	5759.0
225.00	1678.0
227.00	2508.0
228.00	413.0
229.00	647.0
241.90	381.0
243.00	401.0
244.10	3980.0
245.10	757.0
246.00	1149.0
255.00	25048.0
256.00	3690.0
257.00	315.0
257.90	1496.0
264.90	760.0
273.00	788.0
274.00	1907.0
275.00	11764.0
276.00	1195.0
277.00	1139.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

296.00	3705.0
297.00	468.0
303.10	520.0
314.90	441.0
323.00	1286.0
324.00	324.0
327.10	305.0
334.00	568.0
345.90	307.0
352.10	407.0
365.00	1720.0
372.10	539.0
422.00	301.0
423.00	1921.0
424.00	568.0
441.10	6799.0
442.10	44592.0
443.10	8851.0
444.00	717.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65

m/z	Abundance
43.90	707.0

Instrument :
BNA_M
ClientSampleId :
DFTPP65