

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
 Data File : BM026552.D
 Acq On : 25 Jun 2020 09:44
 Operator : JU/CG
 Sample : L3064-03
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET156

Manual Integrations
 APPROVED

mohammad
 6/26/2020 12:19:41 PM

Quant Time: Jun 25 10:59:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 25 10:53:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	94884	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	437842	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	301775	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	691091	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	732240	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	650228	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.98	96	4305	1.59	ng/uL	0.01
5) Phenol-d5	6.58	99	61688	7.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	47778	8.64	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	53515	7.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	55785	8.11	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	25083	6.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.23	143	26463	6.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	46162	5.86	ng/ul	0.01
29) 4-Chloroaniline-d4	10.29	131	66304	8.07	ng/ul	0.01
44) Dimethylphthalate-d6	13.46	166	197577	7.79	ng/ul	0.00
47) Acenaphthylene-d8	13.72	160	197566	6.49	ng/ul	0.00
52) 4-Nitrophenol-d4	14.34	143	3145m	0.75	ng/ul	0.07
58) Fluorene-d10	15.03	176	151737	6.97	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.20	200	2512	0.56	ng/ul	0.02
71) Anthracene-d10	16.89	188	242036	6.88	ng/ul	0.00
79) Pyrene-d10	19.19	212	274069	6.83	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.96	264	235235	6.54	ng/ul	0.00

Target Compounds					Ovalue	
45) Dimethylphthalate	13.50	163	71463	2.712	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
Data File : BM026552.D
Acq On : 25 Jun 2020 09:44
Operator : JU/CG
Sample : L3064-03
Misc :
ALS Vial : 3 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
ET156

Manual Integrations
APPROVED

mohammad
6/26/2020 12:19:41 PM

Quant Time: Jun 25 10:59:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 25 10:53:13 2020
Response via : Initial Calibration

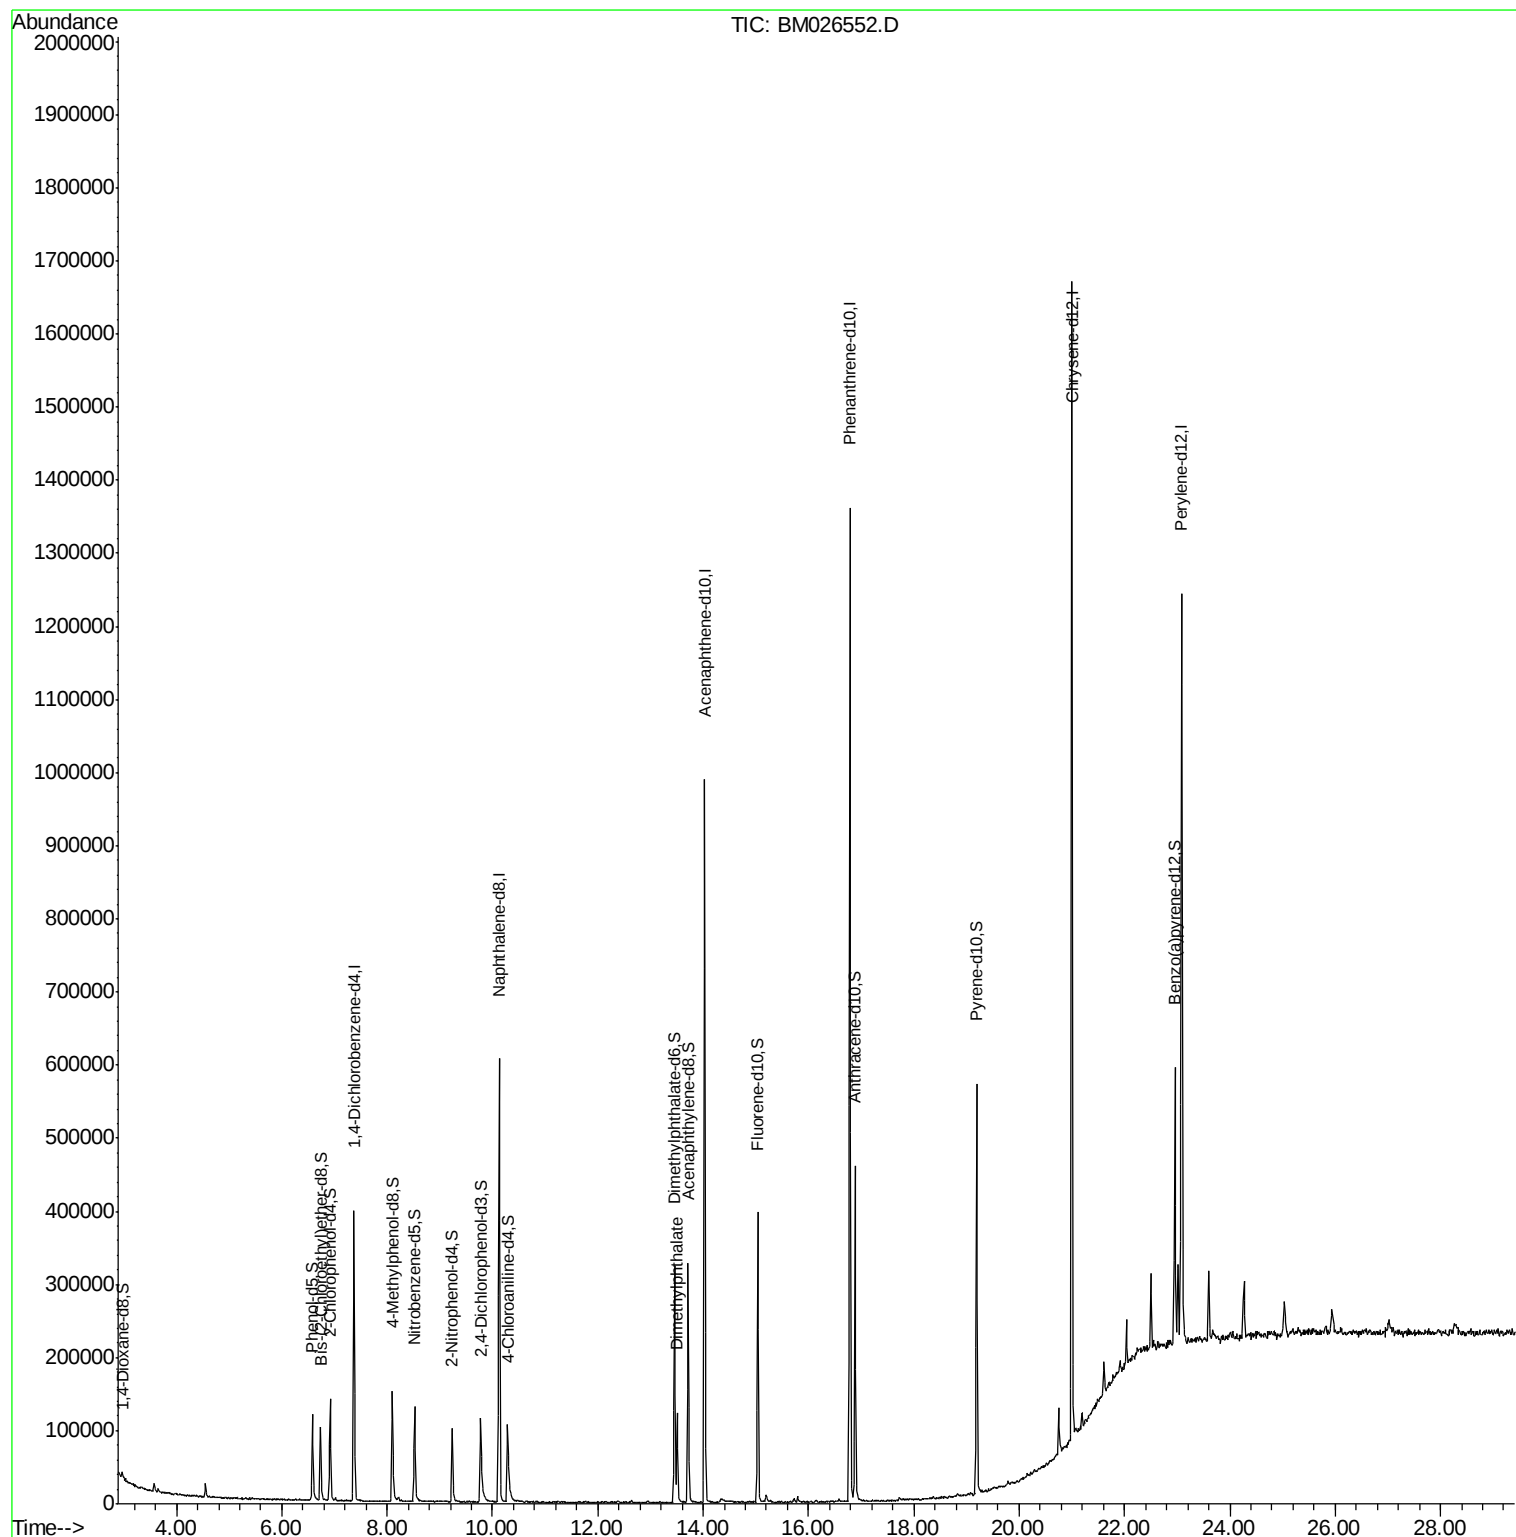

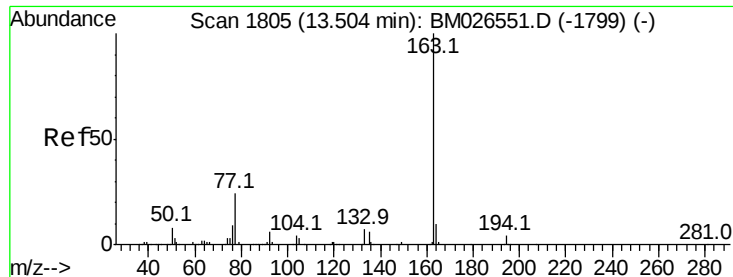

#45
 Dimethylphthalate
 Concen: 2.712 ng/ul
 RT: 13.50 min Scan# 1805
 Delta R.T. -0.00 min
 Lab File: BM026552.D
 Acq: 25 Jun 2020 09:44

Instrument :
 BNA_M
 ClientSampleId :
 ET156

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.4	5.2
164	10.4	7.8	11.6

Manual Integrations
 APPROVED

mohammad
 6/26/2020 12:19:41 PM

