

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
 Data File : BM026553.D
 Acq On : 25 Jun 2020 10:20
 Operator : JU/CG
 Sample : L3064-09
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET163

Quant Time: Jun 25 11:00:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 25 10:53:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	79547	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	372782	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	255925	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	591769	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	649452	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	611795	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.98	96	1431	0.63	ng/uL	0.01
5) Phenol-d5	6.59	99	28782	3.93	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	19650	4.24	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	21296	3.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	31589	5.48	ng/ul	0.00
19) Nitrobenzene-d5	8.53	128	12584	3.80	ng/ul	0.01
22) 2-Nitrophenol-d4	9.24	143	13924	3.82	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.78	165	29451	4.39	ng/ul	0.01
29) 4-Chloroaniline-d4	10.29	131	40073	5.73	ng/ul	0.01
44) Dimethylphthalate-d6	13.46	166	198893	9.24	ng/ul	0.00
47) Acenaphthylene-d8	13.72	160	163812	6.35	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	16732	4.69	ng/ul	0.02
58) Fluorene-d10	15.03	176	133118	7.21	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	16278	4.20	ng/ul	0.00
71) Anthracene-d10	16.89	188	232047	7.70	ng/ul	0.00
79) Pyrene-d10	19.19	212	268818	7.55	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.96	264	199934	5.91	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.50	163	63879	2.859	ng/ul 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
Data File : BM026553.D
Acq On : 25 Jun 2020 10:20
Operator : JU/CG
Sample : L3064-09
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET163

Quant Time: Jun 25 11:00:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 25 10:53:13 2020
Response via : Initial Calibration

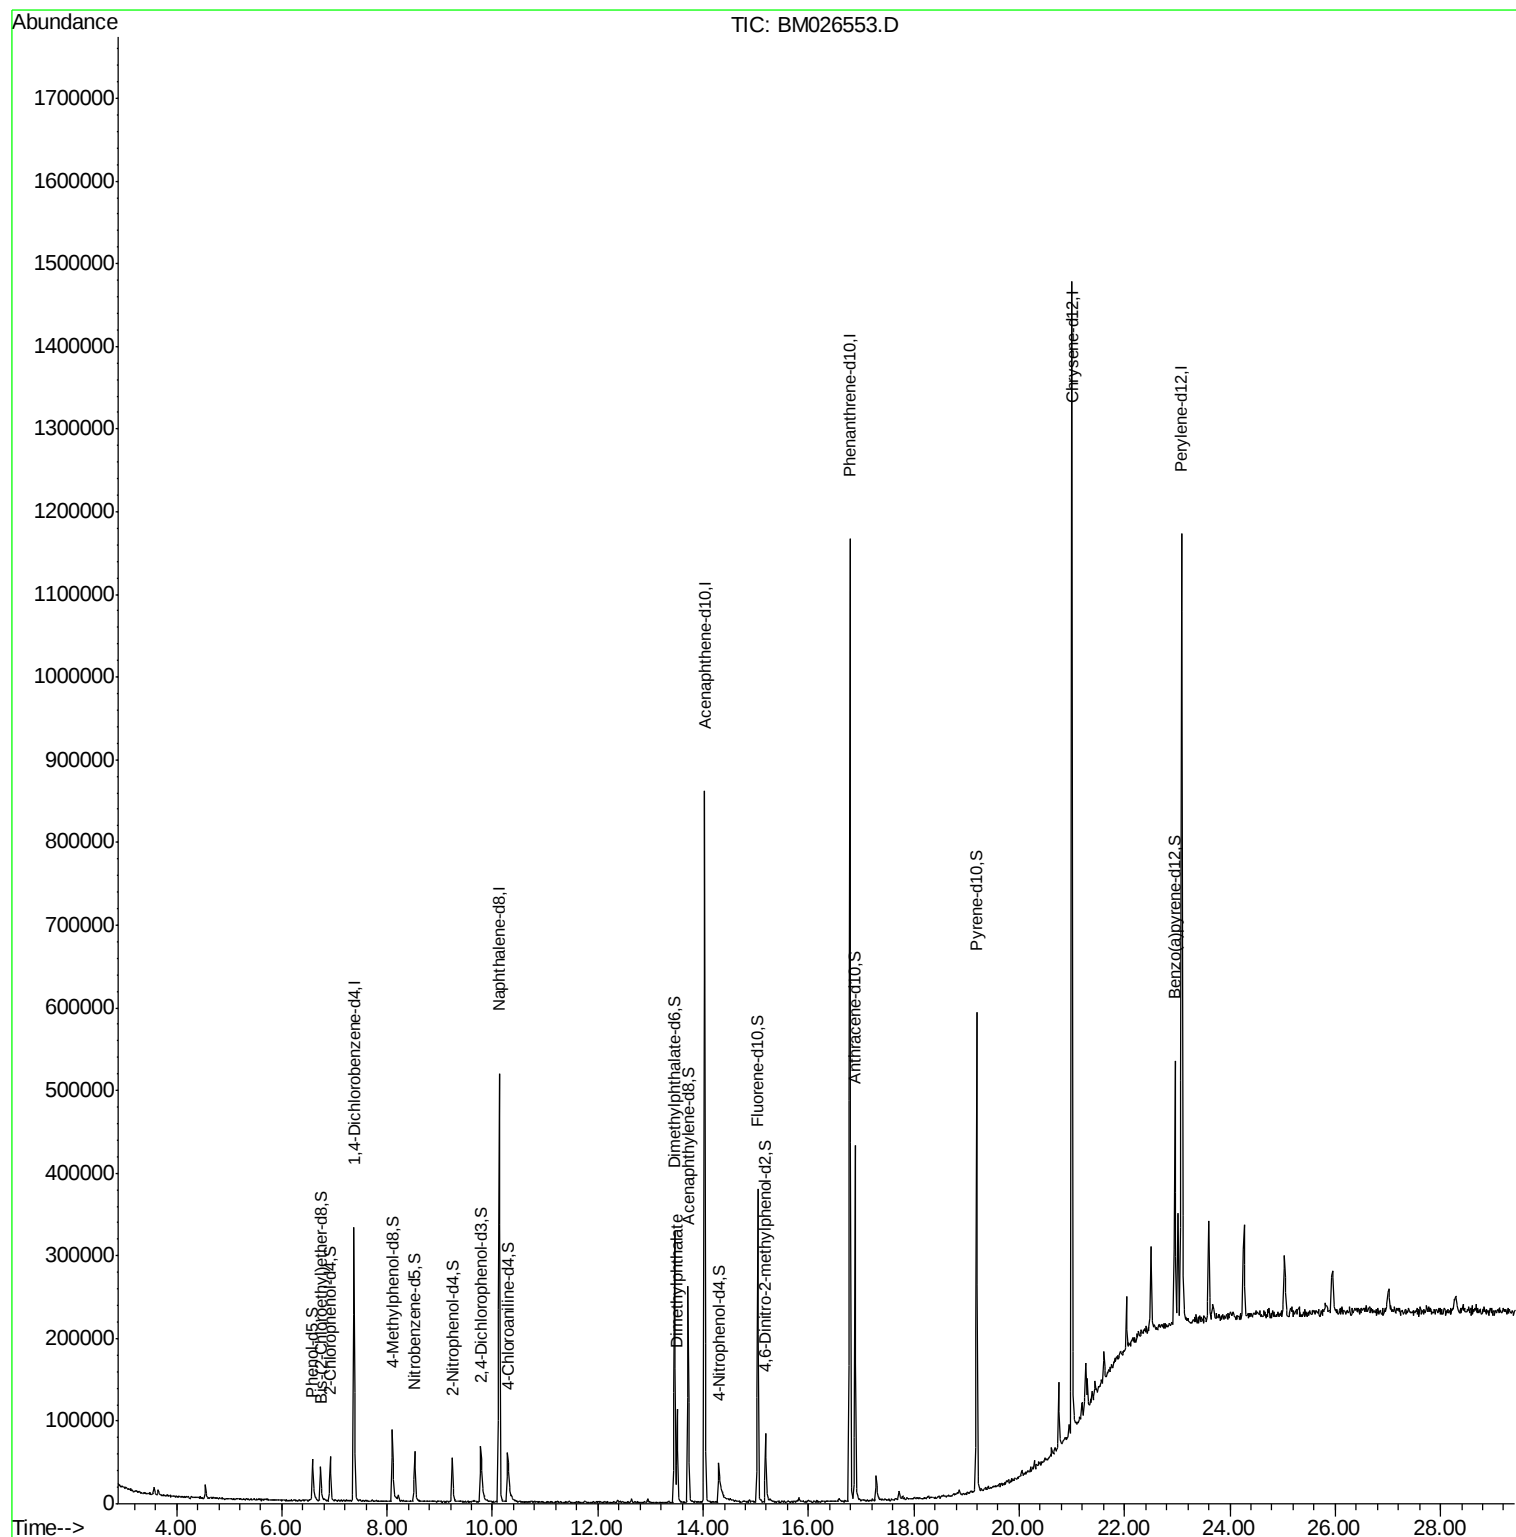

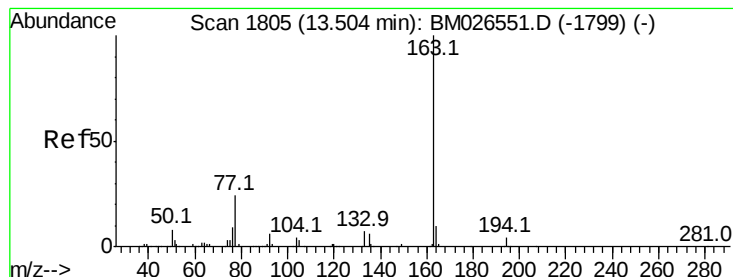

#45

Dimethylphthalate

Concen: 2.859 ng/ul

RT: 13.50 min Scan# 1805

Delta R.T. -0.00 min

Lab File: BM026553.D

Acq: 25 Jun 2020 10:20

Instrument :

BNA_M

ClientSampleId :

ET163

Tot Ion:163 Resp: 63879

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.2

164 11.1 7.8 11.6

