

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
 Data File : BM026559.D
 Acq On : 25 Jun 2020 15:24
 Operator : JU/CG
 Sample : L3062-21
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET152

Quant Time: Jun 25 15:55:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 25 10:53:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	81759	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	391689	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	268600	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	624539	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	719231	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	746484	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.97	96	3681	1.58	ng/uL	0.00
5) Phenol-d5	6.58	99	64927	8.62	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	74657	15.67	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	74678	12.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	78305	13.21	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	35403	10.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.24	143	24995	6.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.77	165	71624	10.16	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	111993	15.23	ng/ul	0.00
44) Dimethylphthalate-d6	13.46	166	322198	14.27	ng/ul	0.00
47) Acenaphthylene-d8	13.72	160	241243	8.91	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.03	176	154236	7.96	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.22	200	248	0.06	ng/ul	0.04
71) Anthracene-d10	16.89	188	209263	6.58	ng/ul	0.00
79) Pyrene-d10	19.19	212	222623	5.64	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.95	264	194361	4.71	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.50	163	304962	13.003	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
Data File : BM026559.D
Acq On : 25 Jun 2020 15:24
Operator : JU/CG
Sample : L3062-21
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET152

Quant Time: Jun 25 15:55:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 25 10:53:13 2020
Response via : Initial Calibration

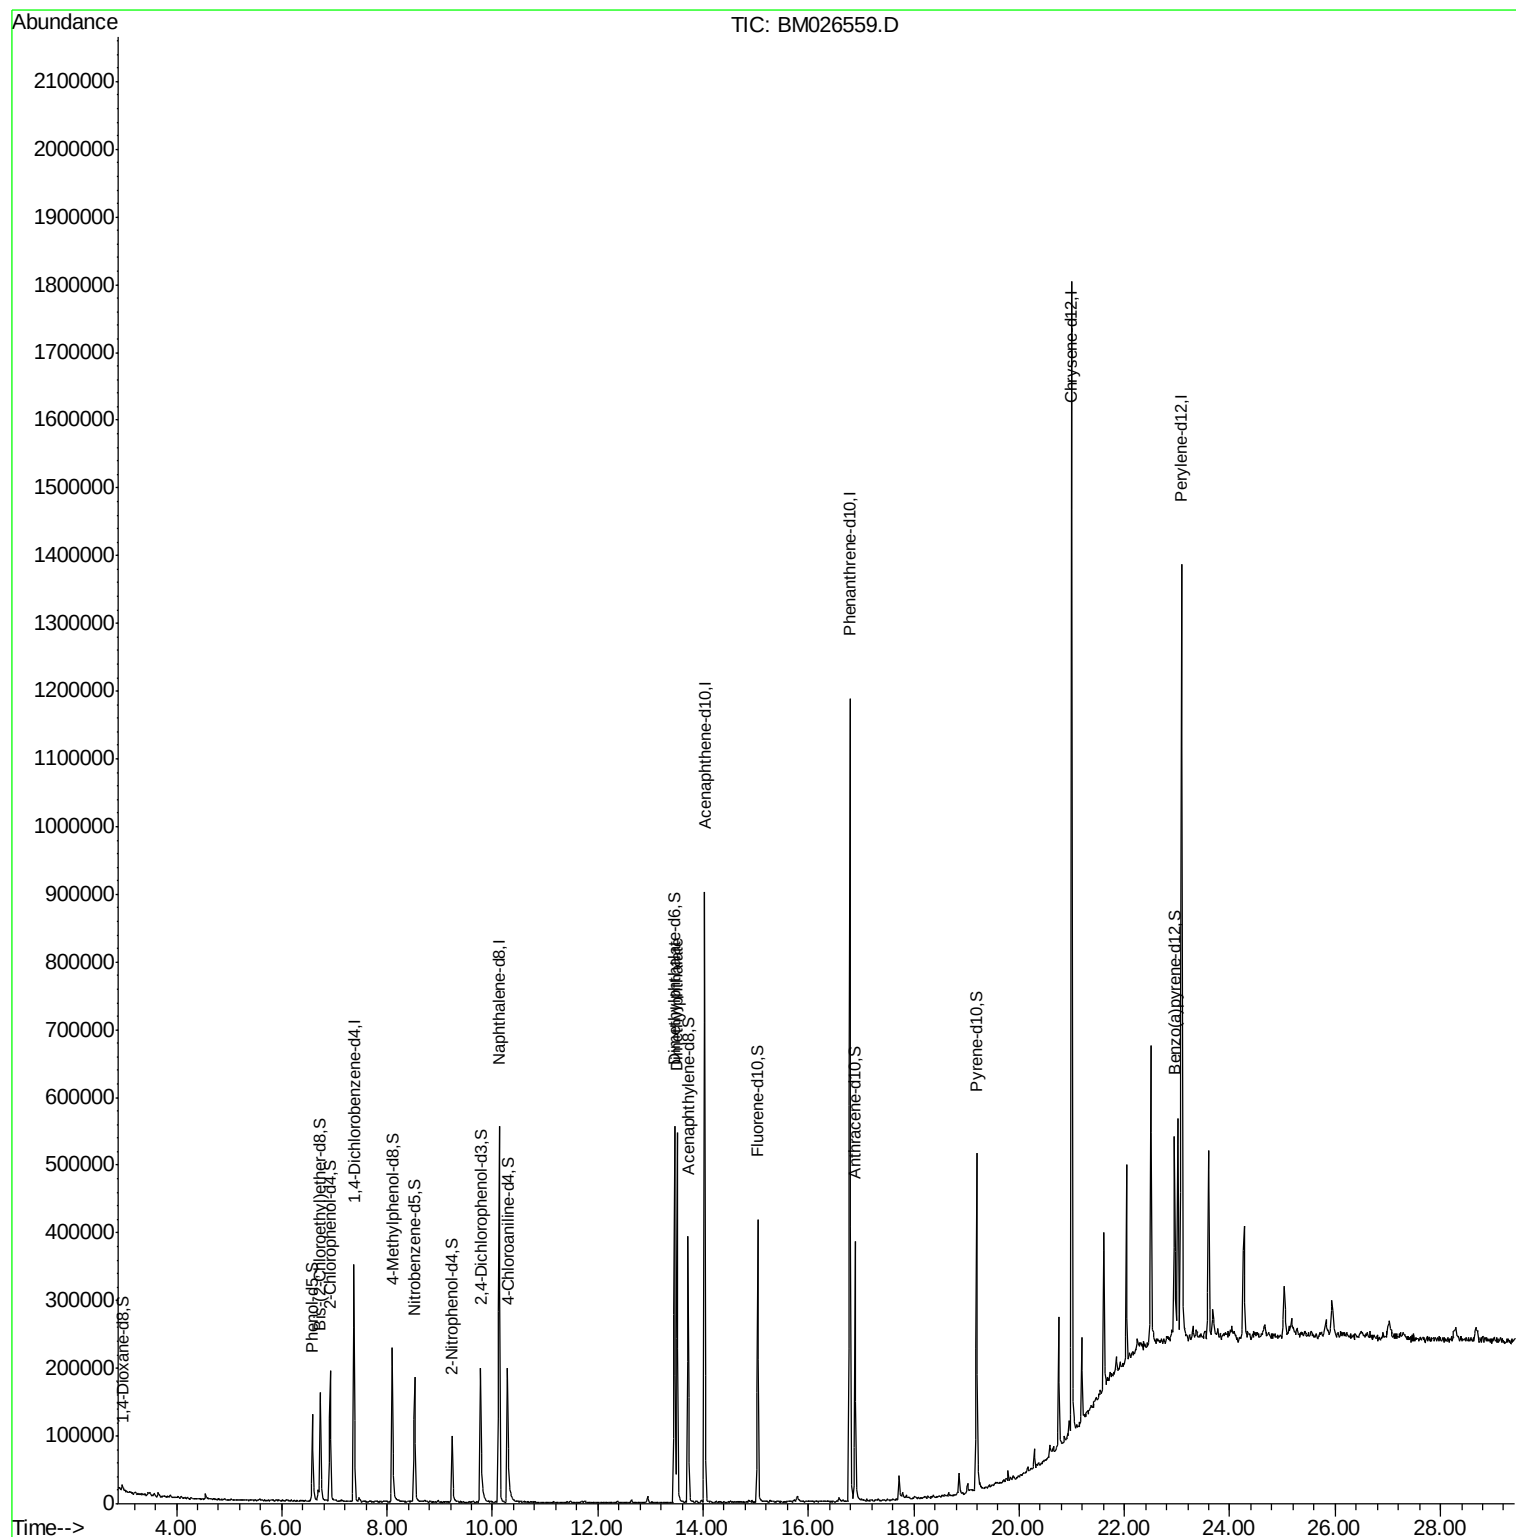

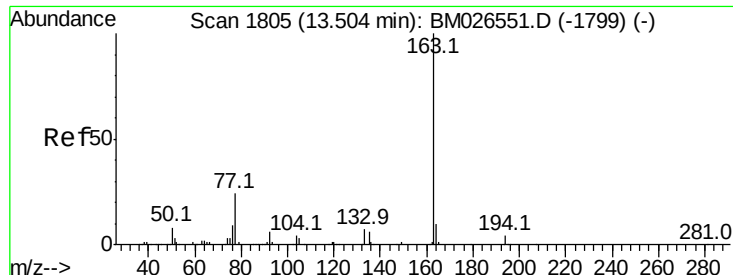

#45

Dimethylphthalate

Concen: 13.003 ng/ul

RT: 13.50 min Scan# 1805

Delta R.T. -0.00 min

Lab File: BM026559.D

Acq: 25 Jun 2020 15:24

Instrument :

BNA_M

ClientSampleId :

ET152


Tot Ion:163 Resp: 304962

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.2

164 10.2 7.8 11.6

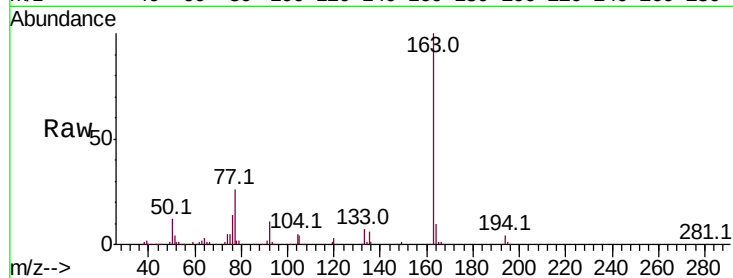

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

