

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
 Data File : BM026561.D
 Acq On : 25 Jun 2020 16:37
 Operator : JU/CG
 Sample : L3062-12
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET145

Manual Integrations
 APPROVED

mohammad
 6/26/2020 12:19:59 PM

Quant Time: Jun 25 17:08:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 25 10:53:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	91384	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	426766	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	284846	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	657428	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	781389	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	799850	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.96	96	11594	4.45	ng/uL	0.00
5) Phenol-d5	6.57	99	208648	24.78	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	178689	33.55	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	183998	26.81	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	196869	29.71	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	90398	23.84	ng/ul	0.00
22) 2-Nitrophenol-d4	9.23	143	80559	19.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.77	165	184443	24.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.28	131	265141	33.10	ng/ul	0.00
44) Dimethylphthalate-d6	13.46	166	676740	28.26	ng/ul	0.00
47) Acenaphthylene-d8	13.72	160	625580	21.78	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	28128m	7.08	ng/ul	0.02
58) Fluorene-d10	15.03	176	434767	21.15	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.18	200	29255	6.80	ng/ul	0.00
71) Anthracene-d10	16.89	188	675429	20.18	ng/ul	0.00
79) Pyrene-d10	19.19	212	778981	18.18	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.96	264	833425	18.84	ng/ul	0.00

Target Compounds					Ovalue
45) Dimethylphthalate	13.50	163	199318	8.014	ng/ul 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
Data File : BM026561.D
Acq On : 25 Jun 2020 16:37
Operator : JU/CG
Sample : L3062-12
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
ET145

Manual Integrations
APPROVED

mohammad
6/26/2020 12:19:59 PM

Quant Time: Jun 25 17:08:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 25 10:53:13 2020
Response via : Initial Calibration

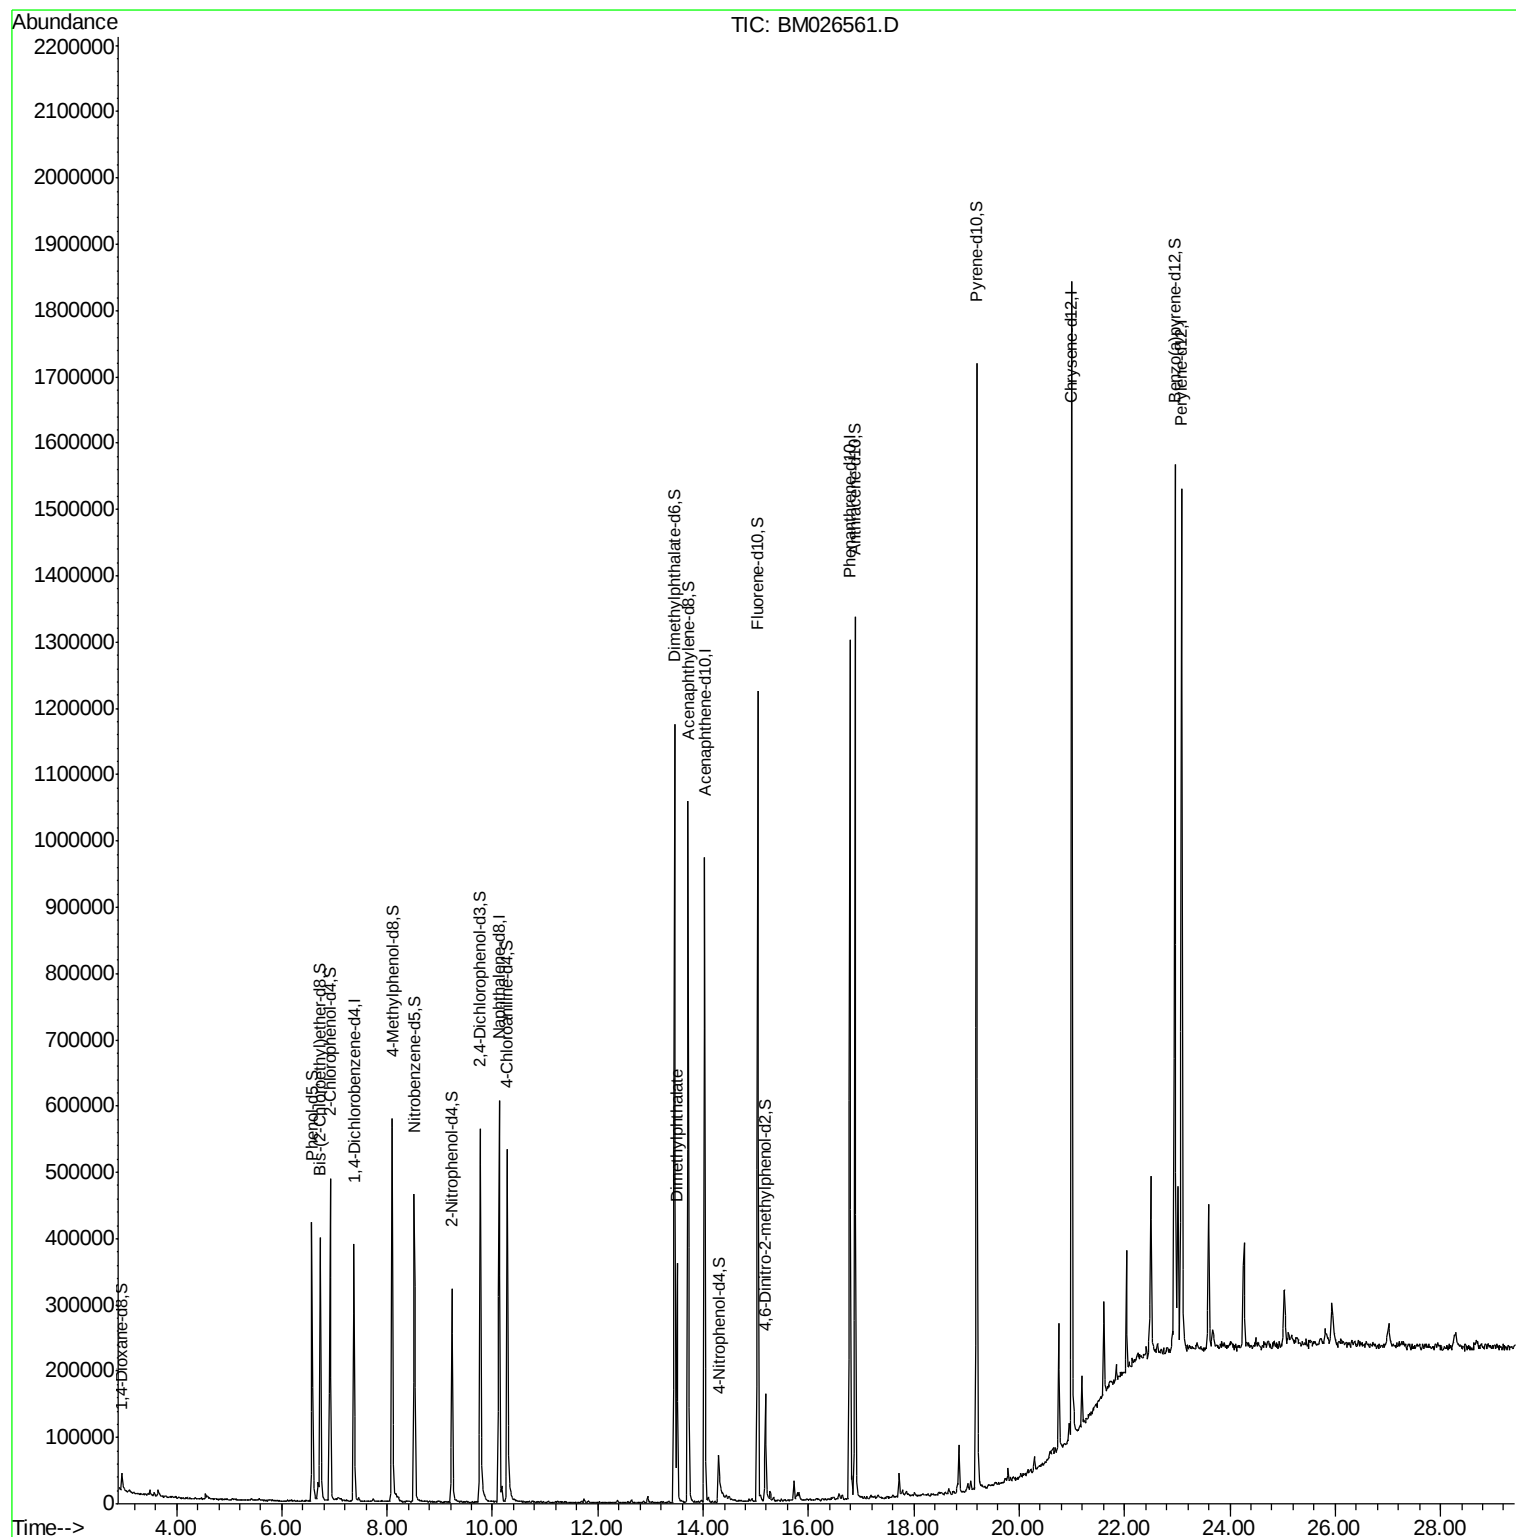

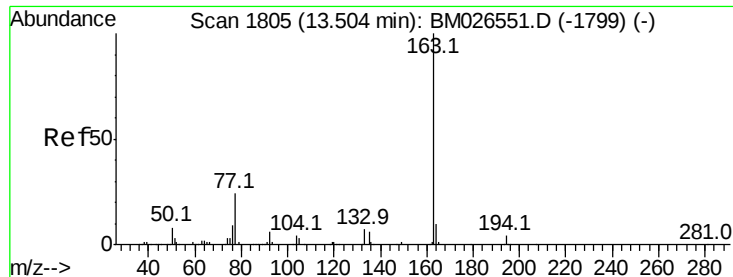

#45
 Dimethylphthalate
 Concen: 8.014 ng/ul
 RT: 13.50 min Scan# 1805
 Delta R.T. -0.00 min
 Lab File: BM026561.D
 Acq: 25 Jun 2020 16:37

Instrument :
 BNA_M
 ClientSampleId :
 ET145

Tot Ion:	163	Resp:	199318
Ion Ratio		Lower	Upper
163	100		
194	4.2	3.4	5.2
164	10.0	7.8	11.6

Manual Integrations
 APPROVED

mohammad
 6/26/2020 12:19:59 PM

