

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
 Data File : BM026562.D
 Acq On : 25 Jun 2020 17:13
 Operator : JU/CG
 Sample : L3062-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET142

Manual Integrations
 APPROVED

mohammad
 6/26/2020 12:20:06 PM

Quant Time: Jun 25 17:45:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 25 10:53:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	87859	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	409529	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	279455	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	647335	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	727266	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	739884	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.97	96	6105	2.44	ng/uL	0.00
5) Phenol-d5	6.58	99	114555	14.15	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	101981	19.92	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	104852	15.89	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	109486	17.19	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	52222	14.35	ng/ul	0.00
22) 2-Nitrophenol-d4	9.23	143	46460	11.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.77	165	102859	13.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.29	131	145360	18.91	ng/ul	0.00
44) Dimethylphthalate-d6	13.46	166	407332	17.34	ng/ul	0.00
47) Acenaphthylene-d8	13.72	160	373154	13.24	ng/ul	0.00
52) 4-Nitrophenol-d4	14.32	143	5864m	1.50	ng/ul	0.05
58) Fluorene-d10	15.03	176	271583	13.47	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	4122	0.97	ng/ul	0.01
71) Anthracene-d10	16.89	188	433457	13.15	ng/ul	0.00
79) Pyrene-d10	19.19	212	490345	12.29	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.95	264	498698	12.19	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.50	163	381356	15.629	ng/ul	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
Data File : BM026562.D
Acq On : 25 Jun 2020 17:13
Operator : JU/CG
Sample : L3062-09
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
ET142

Quant Time: Jun 25 17:45:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 25 10:53:13 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/26/2020 12:20:06 PM

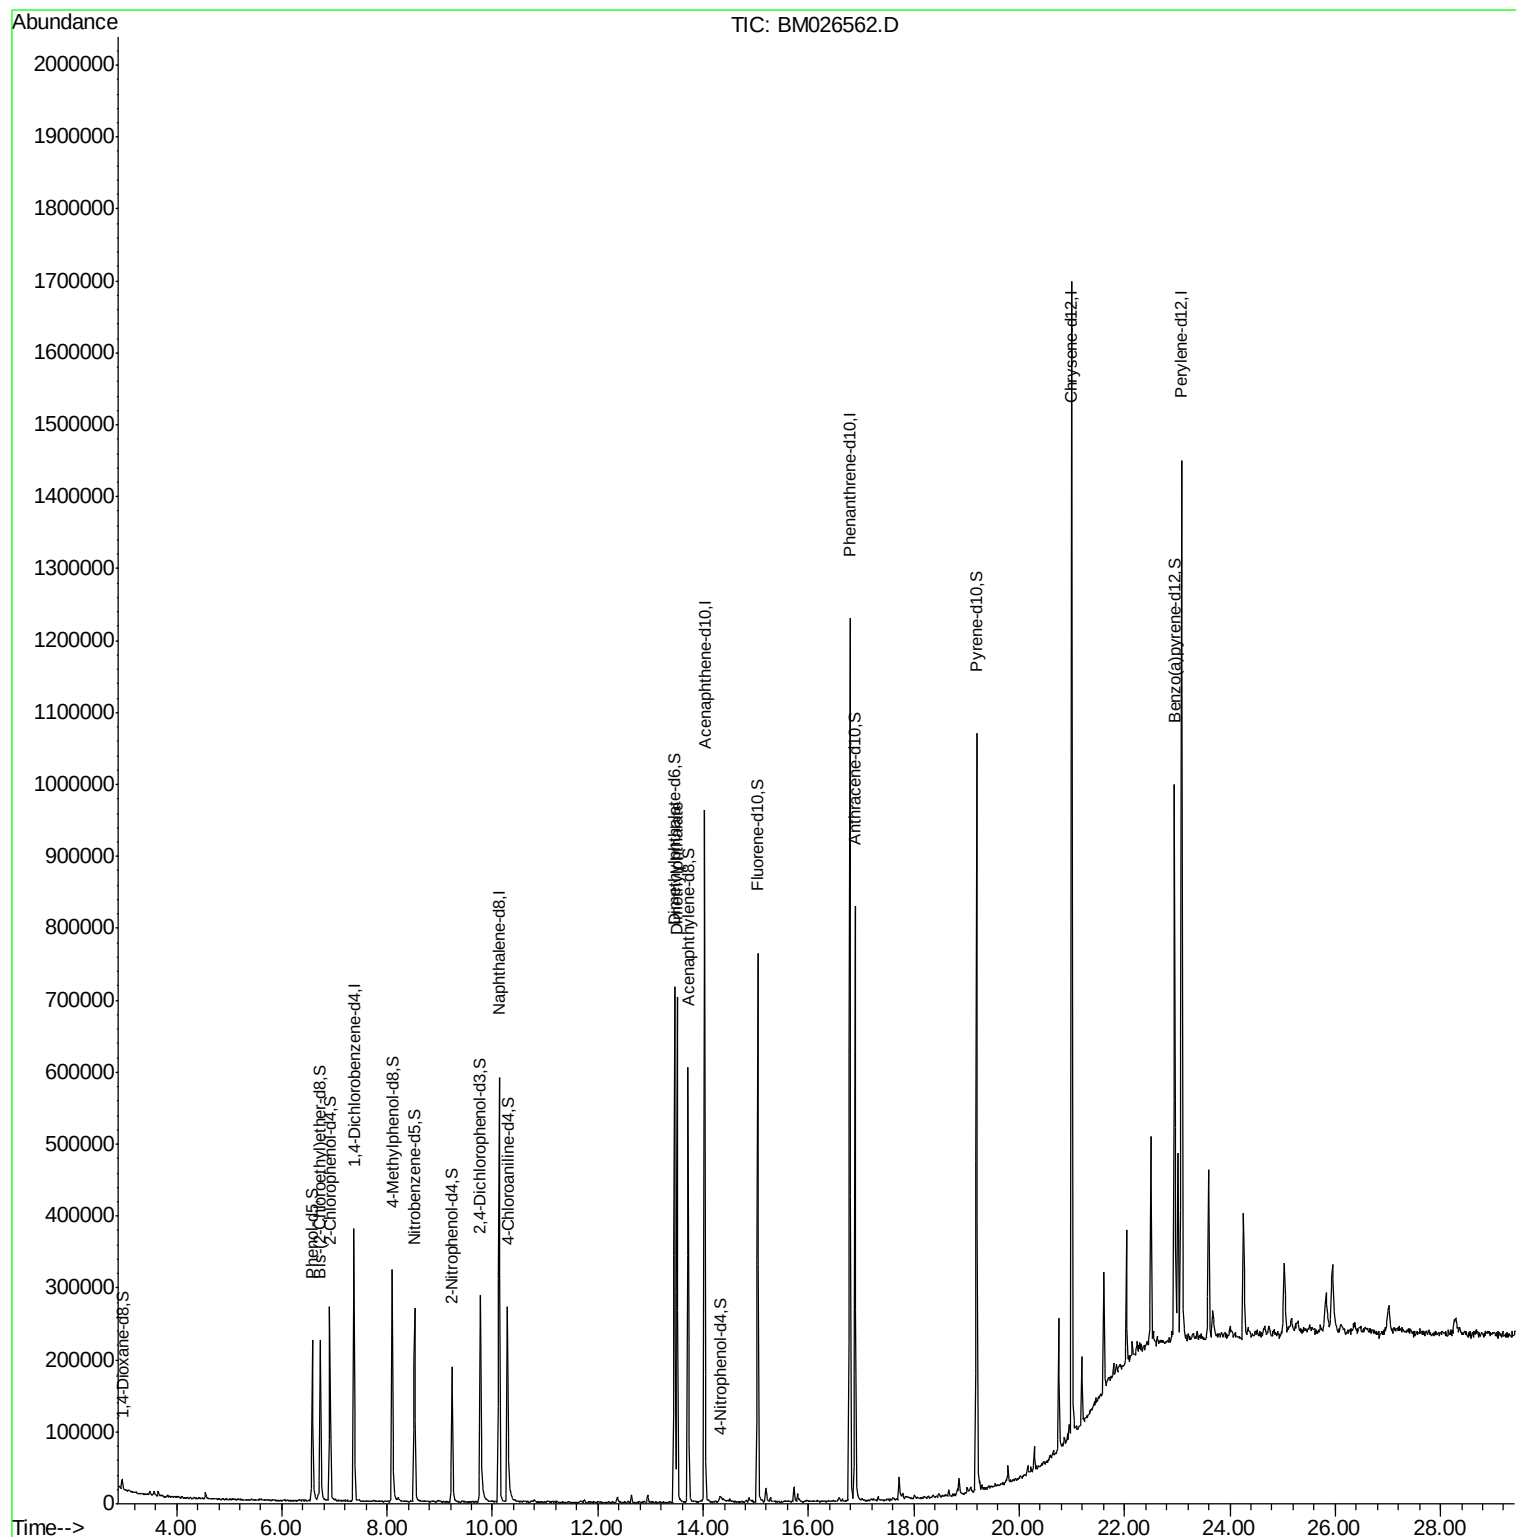

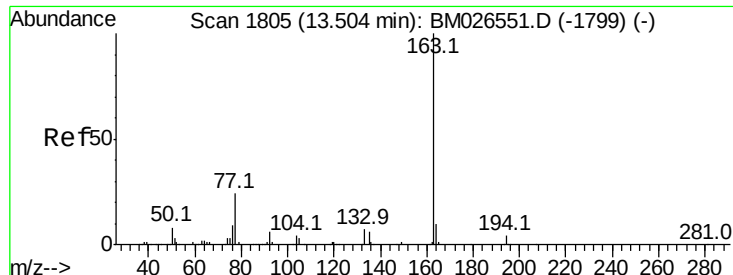

#45
 Dimethylphthalate
 Concen: 15.629 ng/ul
 RT: 13.50 min Scan# 1805
 Delta R.T. -0.00 min
 Lab File: BM026562.D
 Acq: 25 Jun 2020 17:13

Instrument :
 BNA_M
 ClientSampleId :
 ET142

Tot Ion	Ratio	Resp Lower	Upper
163	100		
194	4.3	3.4	5.2
164	9.5	7.8	11.6

Manual Integrations
 APPROVED

mohammad
 6/26/2020 12:20:06 PM

