

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
 Data File : BM026567.D
 Acq On : 25 Jun 2020 20:51
 Operator : JU/CG
 Sample : L3062-22
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET153

Manual Integrations
 APPROVED

mohammad
 6/26/2020 12:20:14 PM

Quant Time: Jun 26 00:48:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 26 00:37:06 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	97147	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	460439	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	316698	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.79	188	724321	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	787403	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	800598	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.96	96	9421	3.40	ng/uL	0.00
5) Phenol-d5	6.57	99	144064	16.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	114472	20.22	ng/ul	0.00
9) 2-Chlorophenol-d4	6.91	132	119928	16.44	ng/ul	0.00
13) 4-Methylphenol-d8	8.09	113	126295	17.93	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	59754	14.61	ng/ul	0.00
22) 2-Nitrophenol-d4	9.23	143	56383	12.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.77	165	120836	14.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.28	131	164217	19.00	ng/ul	0.00
44) Dimethylphthalate-d6	13.46	166	457061	17.16	ng/ul	0.00
47) Acenaphthylene-d8	13.71	160	451561	14.14	ng/ul	0.00
52) 4-Nitrophenol-d4	14.31	143	14726m	3.33	ng/ul	0.04
58) Fluorene-d10	15.03	176	315162	13.79	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.19	200	12542	2.65	ng/ul	0.00
71) Anthracene-d10	16.88	188	487921	13.23	ng/ul	0.00
79) Pyrene-d10	19.19	212	524664	12.15	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.95	264	443913	10.03	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.50	163	161814	5.852	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
Data File : BM026567.D
Acq On : 25 Jun 2020 20:51
Operator : JU/CG
Sample : L3062-22
Misc :
ALS Vial : 18 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
ET153

Quant Time: Jun 26 00:48:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 26 00:37:06 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/26/2020 12:20:14 PM

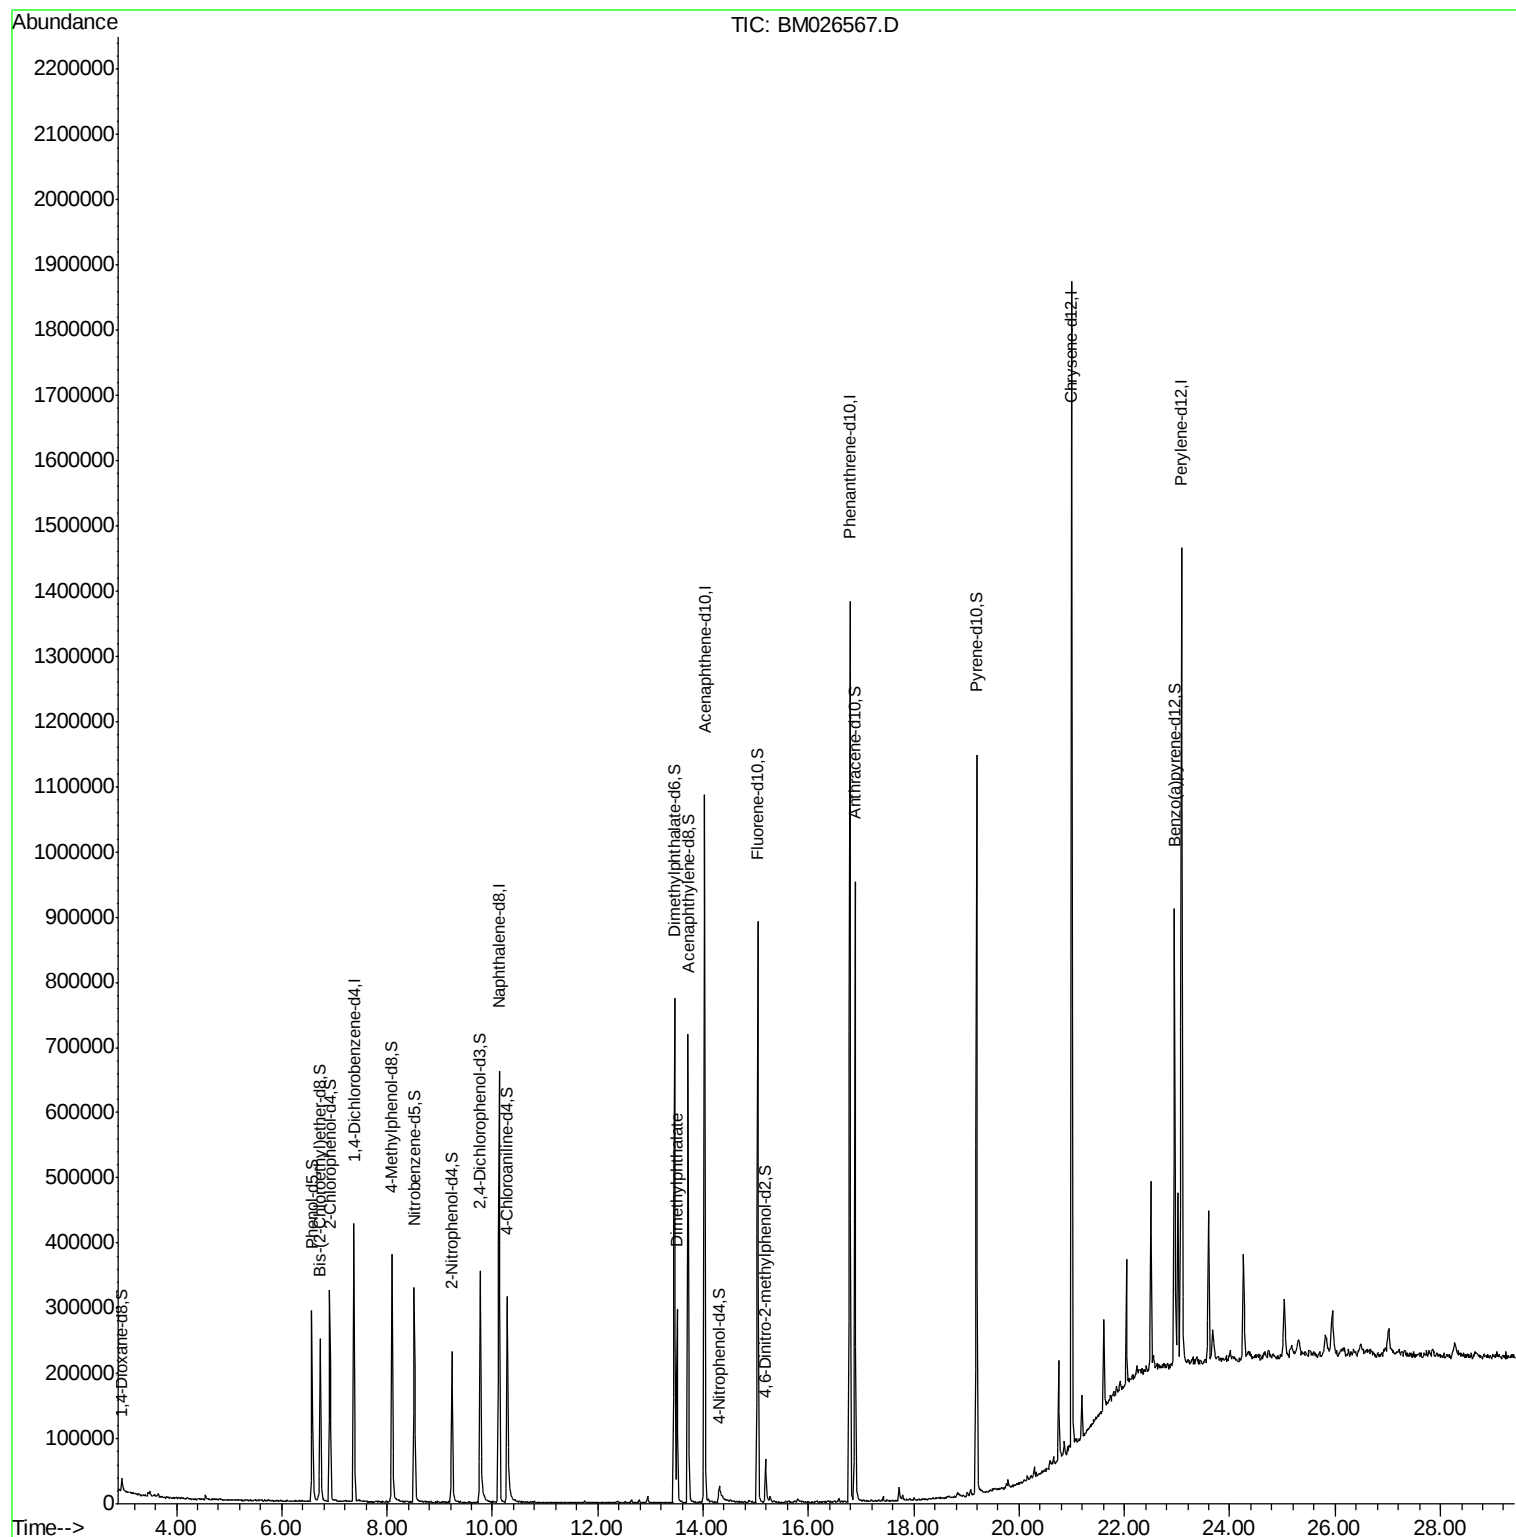

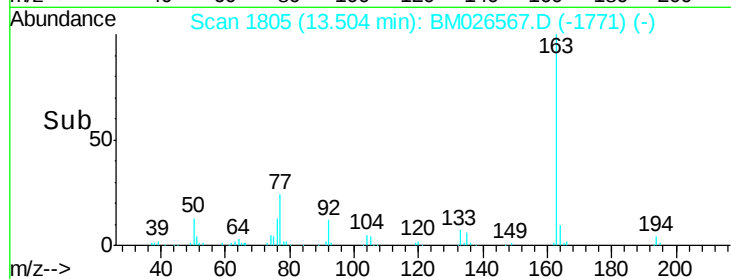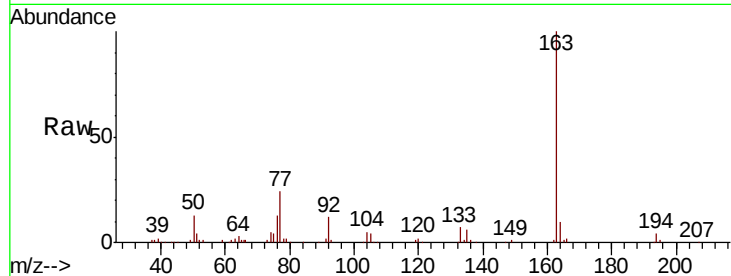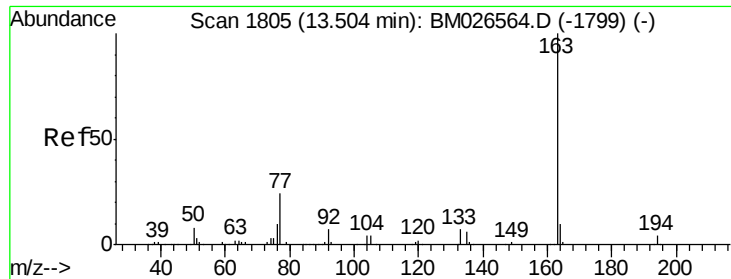

#45
 Dimethylphthalate
 Concen: 5.852 ng/ul
 RT: 13.50 min Scan# 1805
 Delta R.T. -0.00 min
 Lab File: BM026567.D
 Acq: 25 Jun 2020 20:51

Instrument :
 BNA_M
 ClientSampleId :
 ET153

Tot Ion	Ratio	Resp	Lower	Upper
163	100	161814		
194	4.2		3.4	5.2
164	10.2		7.8	11.6

Manual Integrations
 APPROVED

mohammad
 6/26/2020 12:20:14 PM

