

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
 Data File : BM06252.D
 Acq On : 25 Jun 2020 09:44
 Operator : JU/CG
 Sample : L3064-03
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET156

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.575	113	117	122	rVB4	10477	17356	0.84%	0.116%
2	3.657	129	131	136	rVB5	5243	6632	0.32%	0.044%
3	3.916	173	175	177	rBV3	2179	2125	0.10%	0.014%
4	4.551	279	283	292	rVB	18436	29279	1.41%	0.196%
5	5.440	431	434	437	rVB4	2063	2251	0.11%	0.015%
6	6.581	620	628	640	rBV	116785	217872	10.49%	1.458%
7	6.734	648	654	665	rBV	99955	166981	8.04%	1.118%
8	6.916	679	685	697	rVV	138047	225573	10.86%	1.510%
9	7.022	698	703	706	rVB5	3472	3876	0.19%	0.026%
10	7.369	755	762	772	rBV	397681	634003	30.52%	4.243%
11	8.098	879	886	900	rBV	151178	268458	12.92%	1.797%
12	8.204	900	904	912	rVB5	5015	9873	0.48%	0.066%
13	8.522	951	958	966	rBV	129735	220086	10.59%	1.473%
14	9.233	1074	1079	1090	rBV	100597	174881	8.42%	1.170%
15	9.781	1164	1172	1191	rBV	115343	263253	12.67%	1.762%
16	10.128	1224	1231	1246	rBV	606389	985955	47.46%	6.598%
17	10.292	1252	1259	1279	rBV	105221	256043	12.32%	1.714%
18	11.757	1502	1508	1516	rVB5	2016	4593	0.22%	0.031%
19	12.380	1610	1614	1618	rBV5	1576	2286	0.11%	0.015%
20	12.639	1654	1658	1661	rBV5	2479	3150	0.15%	0.021%
21	12.951	1704	1711	1716	rBV5	2478	5211	0.25%	0.035%
22	13.457	1791	1797	1802	rBV	322641	451344	21.72%	3.021%
23	13.504	1802	1805	1819	rVB	122248	184218	8.87%	1.233%
24	13.716	1835	1841	1857	rBV	327600	463534	22.31%	3.102%
25	14.027	1888	1894	1903	rBV	989554	1429383	68.80%	9.566%
26	14.339	1942	1947	1949	rBV5	4252	7967	0.38%	0.053%
27	14.357	1949	1950	1955	rVB5	3185	3433	0.17%	0.023%
28	14.868	2034	2037	2041	rBV3	1661	2301	0.11%	0.015%
29	15.033	2057	2065	2078	rBV	396834	588522	28.33%	3.939%
30	15.198	2089	2093	2100	rBV5	10381	18718	0.90%	0.125%
31	15.286	2104	2108	2112	rVB3	3496	4349	0.21%	0.029%
32	15.727	2180	2183	2188	rVV3	5017	6881	0.33%	0.046%
33	15.798	2191	2195	2198	rBV2	8611	9949	0.48%	0.067%
34	16.145	2250	2254	2259	rBV5	3432	5220	0.25%	0.035%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
 Data File : BM026552.D
 Acq On : 25 Jun 2020 09:44
 Operator : JU/CG
 Sample : L3064-03
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET156

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Title : SVOA CALIBRATION

35	16.580	2325	2328	2332	rVB5	3643	5371	0.26%	0.036%
36	16.786	2357	2363	2374	rBV	1358767	1789445	86.13%	11.976%
37	16.886	2374	2380	2393	rVB	457363	657855	31.66%	4.403%
38	17.727	2518	2523	2530	rBV5	5081	11238	0.54%	0.075%
39	17.786	2530	2533	2536	rVV3	2325	3219	0.15%	0.022%
40	18.009	2567	2571	2572	rVB4	2417	2283	0.11%	0.015%
41	18.368	2630	2632	2639	rVB8	3450	4278	0.21%	0.029%
42	18.498	2649	2654	2656	rBV5	2159	3315	0.16%	0.022%
43	18.780	2699	2702	2703	rBV3	1987	2483	0.12%	0.017%
44	18.827	2707	2710	2712	rVV2	2973	3333	0.16%	0.022%
45	19.133	2761	2762	2764	rBV2	2756	2816	0.14%	0.019%
46	19.192	2766	2772	2786	rVV	562115	783197	37.70%	5.241%
47	20.750	3033	3037	3043	rBV2	63287	103255	4.97%	0.691%
48	21.003	3074	3080	3089	rBV	1583563	2077569	100.00%	13.904%
49	22.039	3253	3256	3260	rVB	60642	71490	3.44%	0.478%
50	22.503	3332	3335	3340	rVB2	100381	119171	5.74%	0.798%
51	22.956	3407	3412	3418	rBV	368535	573453	27.60%	3.838%
52	23.021	3420	3423	3427	rVV	100536	131473	6.33%	0.880%
53	23.086	3428	3434	3449	rVB	1021241	1776915	85.53%	11.892%
54	23.603	3518	3522	3528	rVB	92009	144545	6.96%	0.967%


Sum of corrected areas: 14942260

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
Data File : BM026552.D
Acq On : 25 Jun 2020 09:44
Operator : JU/CG
Sample : L3064-03
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET156

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

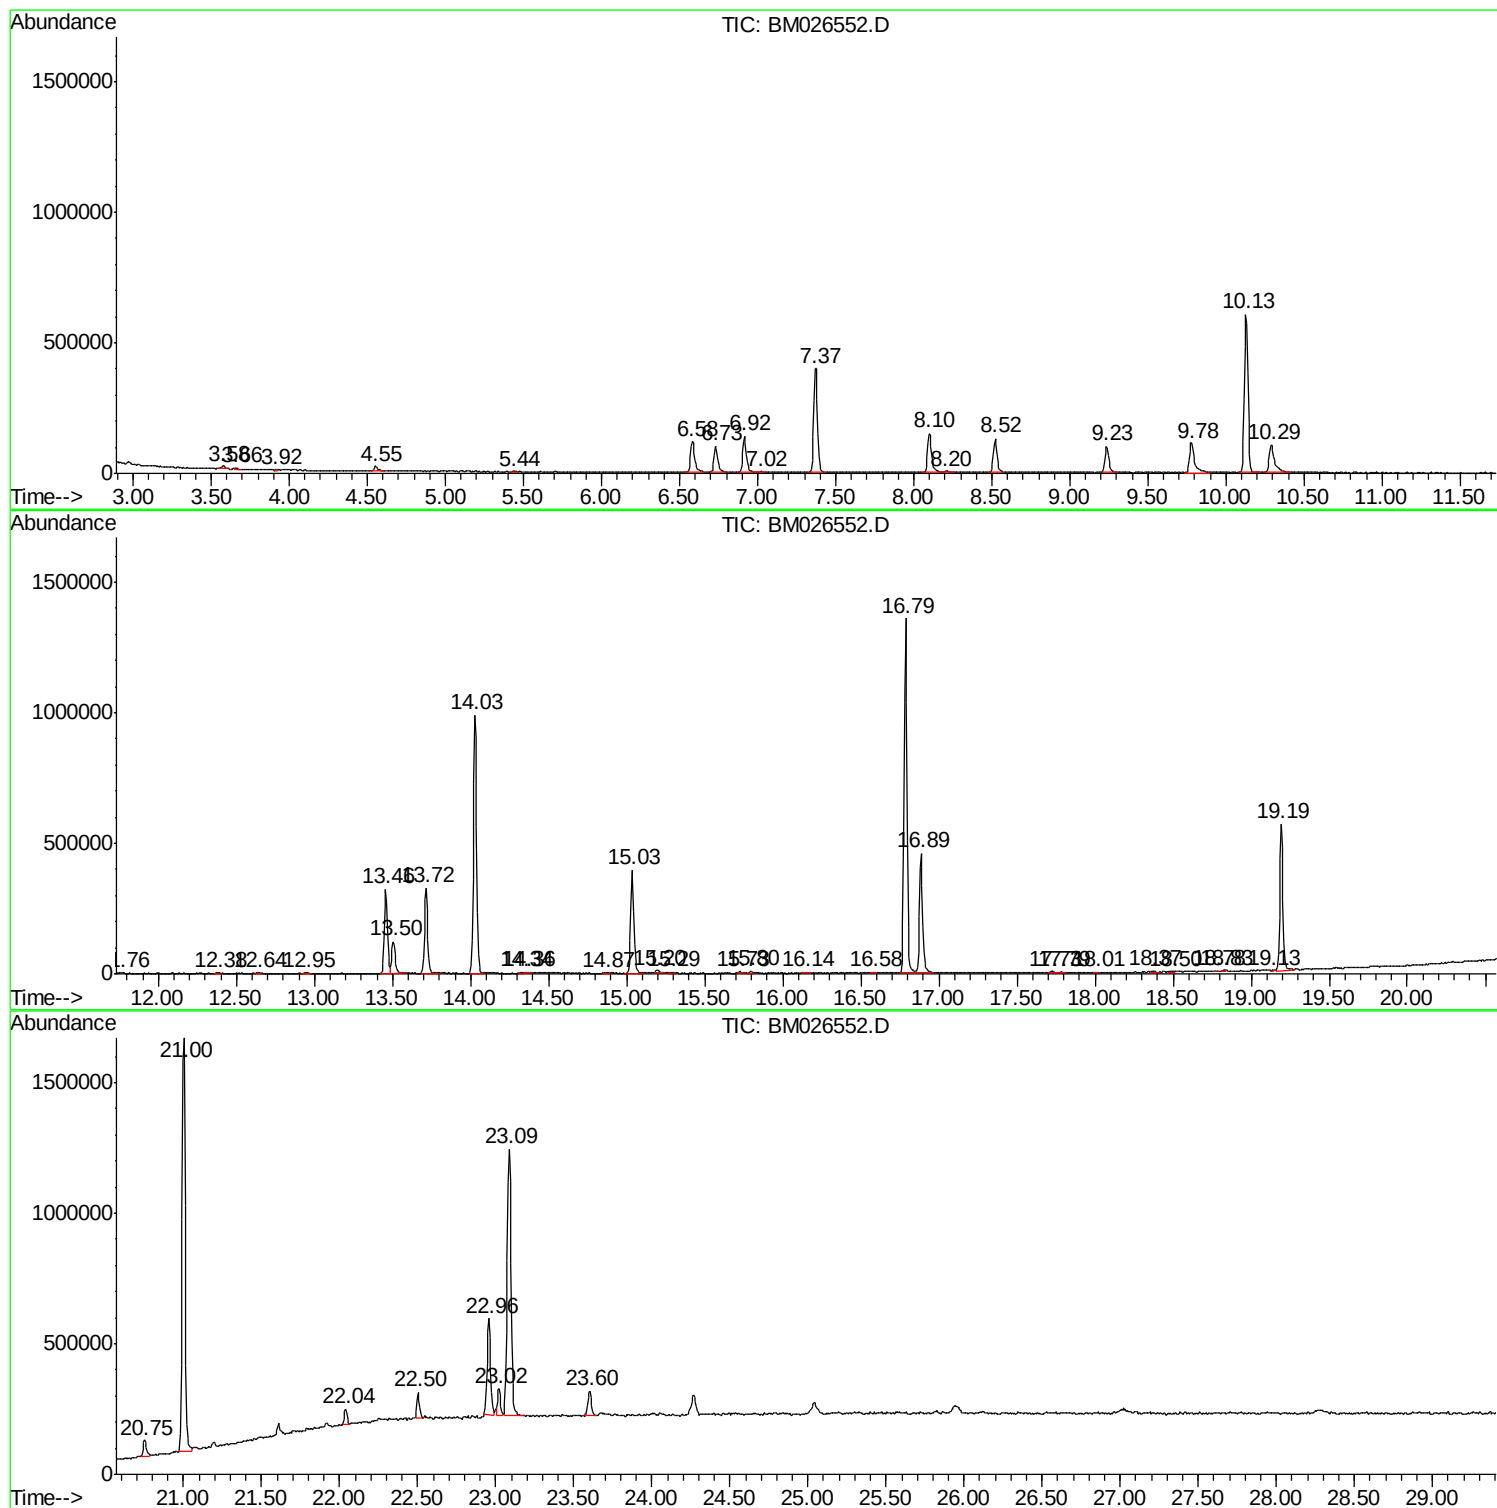

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062520\
Data File : BM026552.D
Acq On : 25 Jun 2020 09:44
Operator : JU/CG
Sample : L3064-03
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET156

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062520\
Data File : BM026552.D
Acq On : 25 Jun 2020 09:44
Operator : JU/CG
Sample : L3064-03
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET156

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc