

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
 Data File : BM026568.D
 Acq On : 25 Jun 2020 21:27
 Operator : JU/CG
 Sample : L3062-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET138

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.963	10	13	21	rVB	20628	29307	1.08%	0.102%
2	3.099	33	36	40	rBV4	2775	4506	0.17%	0.016%
3	3.463	94	98	101	rBV3	8985	12402	0.46%	0.043%
4	3.493	101	103	108	rVB4	8031	9642	0.35%	0.034%
5	3.569	113	116	123	rVB6	4222	9254	0.34%	0.032%
6	3.657	128	131	136	rVB2	6706	8011	0.29%	0.028%
7	4.557	280	284	286	rBV2	7101	10323	0.38%	0.036%
8	4.581	286	288	295	rVB4	4490	7982	0.29%	0.028%
9	4.781	319	322	327	rVB6	1938	3389	0.12%	0.012%
10	5.881	506	509	513	rBV4	1600	3052	0.11%	0.011%
11	6.357	585	590	592	rBV6	2065	3241	0.12%	0.011%
12	6.575	619	627	640	rBV	339630	568612	20.86%	1.987%
13	6.687	642	646	648	rVV2	13286	17937	0.66%	0.063%
14	6.728	648	653	664	rVB	279482	431353	15.83%	1.507%
15	6.910	678	684	695	rVB	362730	580080	21.28%	2.027%
16	7.010	698	701	708	rVB8	3328	5388	0.20%	0.019%
17	7.098	712	716	718	rBV5	3287	3609	0.13%	0.013%
18	7.369	756	762	770	rBV	454561	691840	25.39%	2.417%
19	7.728	815	823	827	rBV7	2953	5329	0.20%	0.019%
20	7.904	849	853	859	rVB6	5046	10617	0.39%	0.037%
21	8.092	879	885	894	rBV	418586	691359	25.37%	2.416%
22	8.516	951	957	972	rVB	353889	562715	20.65%	1.966%
23	8.675	980	984	987	rBV6	1970	3745	0.14%	0.013%
24	8.716	987	991	997	rVB4	3495	5972	0.22%	0.021%
25	9.016	1037	1042	1046	rBV7	2590	4216	0.15%	0.015%
26	9.057	1046	1049	1054	rVB5	4314	5438	0.20%	0.019%
27	9.233	1071	1079	1087	rBV	259357	435510	15.98%	1.522%
28	9.310	1089	1092	1102	rVB9	6080	12204	0.45%	0.043%
29	9.769	1163	1170	1184	rBV	421373	745500	27.35%	2.605%
30	9.886	1188	1190	1196	rVB5	4255	7105	0.26%	0.025%
31	10.128	1219	1231	1237	rBV	683732	1098428	40.30%	3.838%
32	10.175	1237	1239	1246	rVB	24093	34799	1.28%	0.122%
33	10.280	1249	1257	1280	rBV	361022	733721	26.92%	2.564%
34	10.533	1298	1300	1306	rVB7	2562	4368	0.16%	0.015%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
 Data File : BM026568.D
 Acq On : 25 Jun 2020 21:27
 Operator : JU/CG
 Sample : L3062-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET138

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Title : SVOA CALIBRATION

35	10.622	1311	1315	1320	rVB6	4480	6815	0.25%	0.024%
36	10.810	1343	1347	1349	rBV5	3095	4368	0.16%	0.015%
37	10.886	1357	1360	1364	rBV4	3426	5077	0.19%	0.018%
38	11.069	1388	1391	1399	rVB7	3014	5608	0.21%	0.020%
39	11.180	1403	1410	1419	rBV8	10797	25012	0.92%	0.087%
40	11.310	1428	1432	1437	rBV6	4526	7241	0.27%	0.025%
41	11.422	1446	1451	1455	rVB6	7032	10018	0.37%	0.035%
42	11.504	1462	1465	1470	rVB6	3600	5274	0.19%	0.018%
43	11.563	1470	1475	1478	rBV6	4962	9852	0.36%	0.034%
44	11.592	1478	1480	1488	rVB7	4186	9085	0.33%	0.032%
45	11.733	1497	1504	1508	rVB6	6318	11561	0.42%	0.040%
46	11.810	1513	1517	1524	rVB5	13720	27613	1.01%	0.096%
47	11.880	1524	1529	1533	rBV6	3779	7724	0.28%	0.027%
48	11.992	1544	1548	1549	rVB4	3552	4468	0.16%	0.016%
49	12.033	1551	1555	1557	rBV3	4248	6881	0.25%	0.024%
50	12.192	1579	1582	1583	rBV2	3640	3257	0.12%	0.011%
51	12.251	1590	1592	1594	rVB3	3681	3254	0.12%	0.011%
52	12.298	1594	1600	1606	rVB6	6602	13978	0.51%	0.049%
53	12.374	1608	1613	1617	rBV6	4510	7673	0.28%	0.027%
54	12.427	1619	1622	1629	rVB7	6013	10746	0.39%	0.038%
55	12.480	1629	1631	1634	rBV4	2832	3128	0.11%	0.011%
56	12.521	1636	1638	1641	rVB4	3519	3436	0.13%	0.012%
57	12.574	1643	1647	1650	rBV	12952	19662	0.72%	0.069%
58	12.786	1678	1683	1684	rBV4	4977	7140	0.26%	0.025%
59	12.833	1687	1691	1693	rBV4	9054	12194	0.45%	0.043%
60	12.945	1704	1710	1715	rBV3	15079	27967	1.03%	0.098%
61	13.174	1745	1749	1753	rBV7	3222	6565	0.24%	0.023%
62	13.286	1764	1768	1773	rBV7	6445	10467	0.38%	0.037%
63	13.345	1774	1778	1780	rBV5	4214	4337	0.16%	0.015%
64	13.380	1782	1784	1788	rVB5	5376	5397	0.20%	0.019%
65	13.457	1791	1797	1801	rBV	911344	1260533	46.25%	4.404%
66	13.504	1801	1805	1810	rVB	696199	920297	33.77%	3.216%
67	13.716	1834	1841	1853	rBV	903538	1398791	51.33%	4.888%
68	13.851	1861	1864	1869	rVB5	12634	16446	0.60%	0.057%
69	13.898	1870	1872	1877	rVB5	4622	4818	0.18%	0.017%
70	14.027	1881	1894	1901	rBV	1071405	1535442	56.34%	5.365%
71	14.086	1901	1904	1911	rVB2	37768	58202	2.14%	0.203%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
 Data File : BM026568.D
 Acq On : 25 Jun 2020 21:27
 Operator : JU/CG
 Sample : L3062-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET138

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Title : SVOA CALIBRATION

72	14.280	1931	1937	1949	rBV	151608	370601	13.60%	1.295%
73	14.439	1960	1964	1967	rVB	24352	29048	1.07%	0.101%
74	14.592	1986	1990	1995	rVB6	18932	27448	1.01%	0.096%
75	14.763	2015	2019	2020	rBV4	8677	8301	0.30%	0.029%
76	14.827	2026	2030	2034	rVB5	17554	22803	0.84%	0.080%
77	14.886	2038	2040	2045	rBV6	8101	11416	0.42%	0.040%
78	15.033	2058	2065	2071	rBV	1252932	1733329	63.60%	6.056%
79	15.086	2071	2074	2079	rVB3	23837	37228	1.37%	0.130%
80	15.174	2085	2089	2100	rBV	246883	382330	14.03%	1.336%
81	15.539	2147	2151	2157	rBV6	16379	31615	1.16%	0.110%
82	15.762	2185	2189	2192	rBV2	49456	66972	2.46%	0.234%
83	15.815	2196	2198	2203	rVB3	26105	32035	1.18%	0.112%
84	16.639	2335	2338	2342	rVB2	38724	52976	1.94%	0.185%
85	16.786	2357	2363	2367	rBV	1378981	1865898	68.47%	6.520%
86	16.827	2367	2370	2374	rVV	89250	118334	4.34%	0.413%
87	16.880	2374	2379	2389	rVV	1372877	1905648	69.92%	6.659%
88	18.856	2712	2715	2719	rVB	166837	187222	6.87%	0.654%
89	19.192	2767	2772	2781	rVB	1761778	2461193	90.31%	8.600%
90	20.997	3075	3079	3084	rBV	1956198	2389892	87.69%	8.351%
91	22.956	3407	3412	3417	rBV	1234522	1918749	70.40%	6.704%
92	23.086	3429	3434	3454	rVB	1384609	2725320	100.00%	9.523%


Sum of corrected areas: 28619639

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062520\
Data File : BM026568.D
Acq On : 25 Jun 2020 21:27
Operator : JU/CG
Sample : L3062-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET138

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

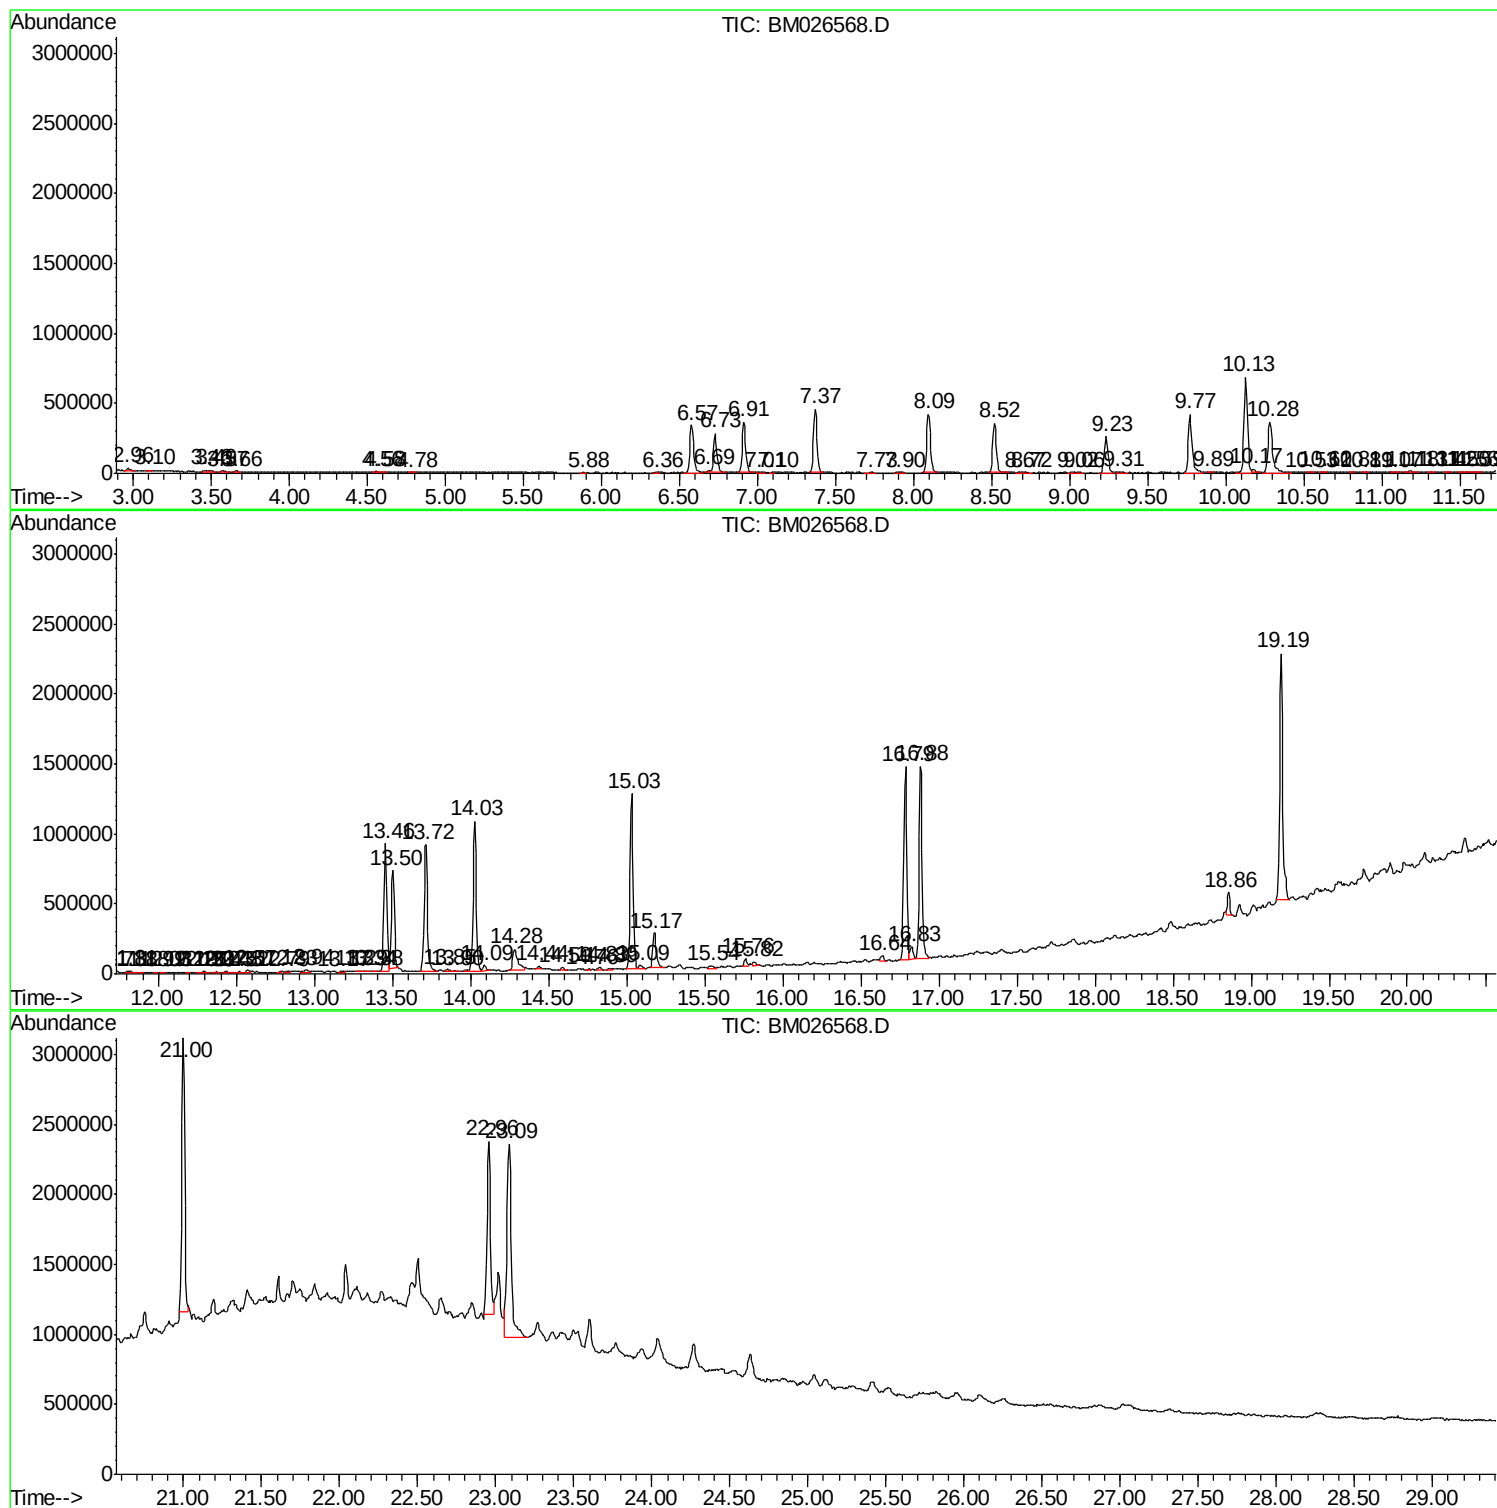

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062520\
Data File : BM026568.D
Acq On : 25 Jun 2020 21:27
Operator : JU/CG
Sample : L3062-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET138

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062520\
Data File : BM026568.D
Acq On : 25 Jun 2020 21:27
Operator : JU/CG
Sample : L3062-07
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET138

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc