


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062521\
Data File : BM030619.D
Acq On : 26 Jun 2021 03:01
Operator : CG/JU
Sample : PB137215BL
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK215

Manual Integrations
APPROVED

mohammad
6/28/2021 1:22:01 PM

Quant Time: Jun 26 04:11:31 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jun 26 01:33:06 2021
Response via : Initial Calibration

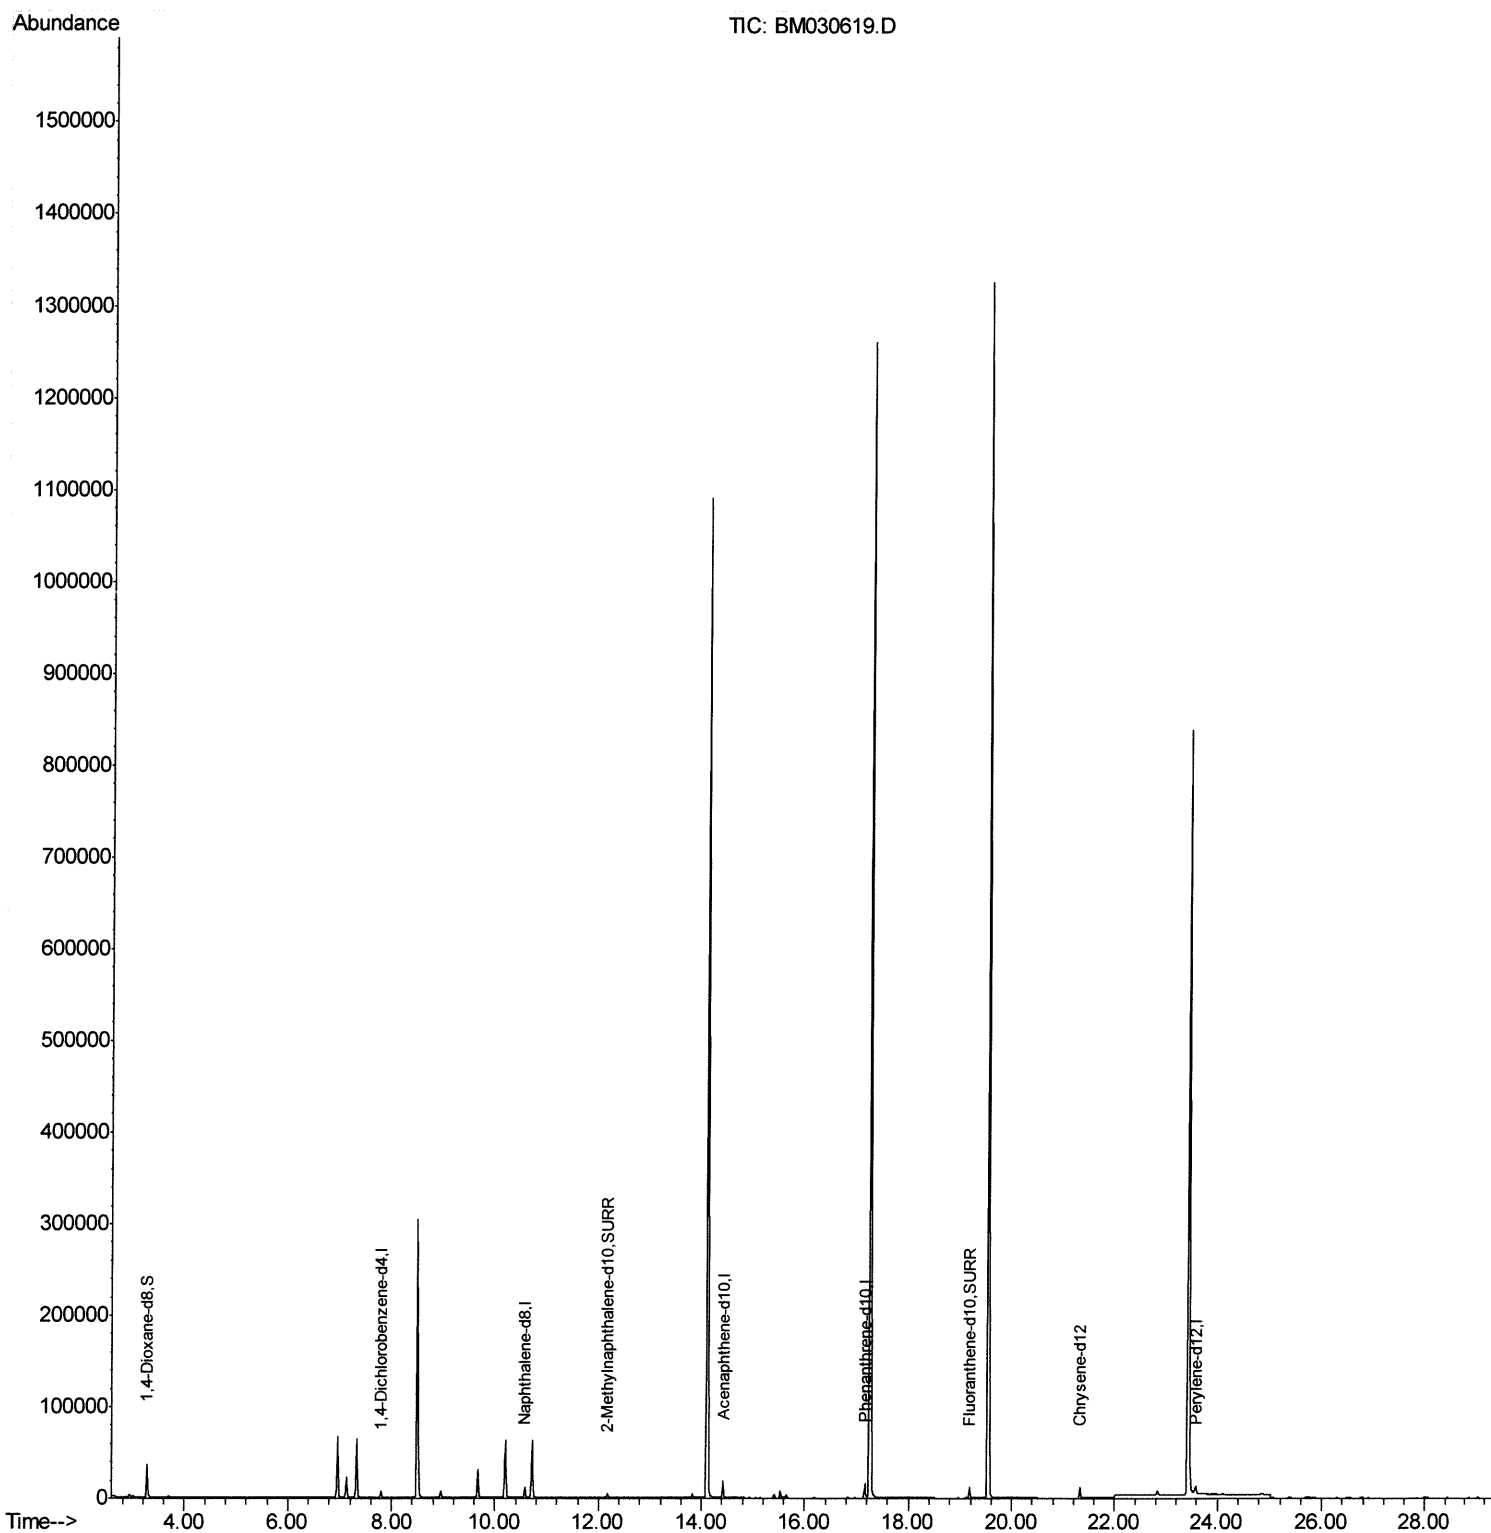




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062521\
 Data File : BM030619.D
 Acq On : 26 Jun 2021 03:01
 Operator : CG/JU
 Sample : PB137215BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK215

Manual Integrations
 APPROVED

mohammad
 6/28/2021 1:22:01 PM

Quant Time: Jun 26 03:47:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 26 01:33:06 2021
 Response via : Initial Calibration

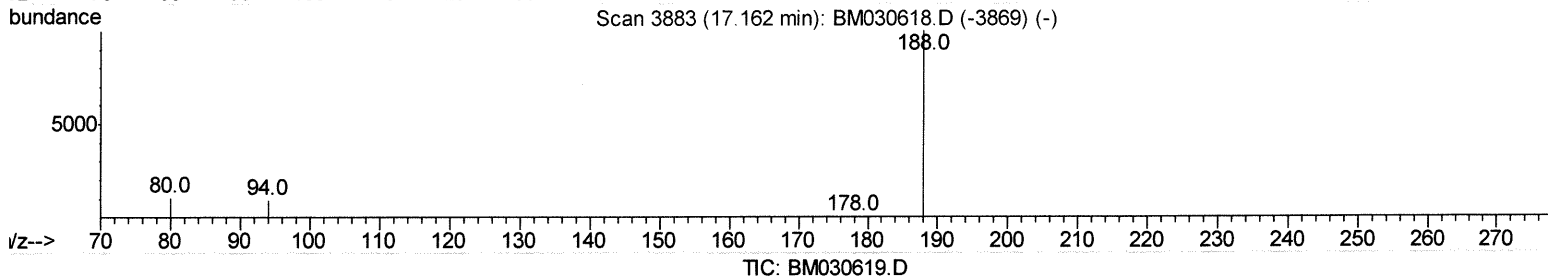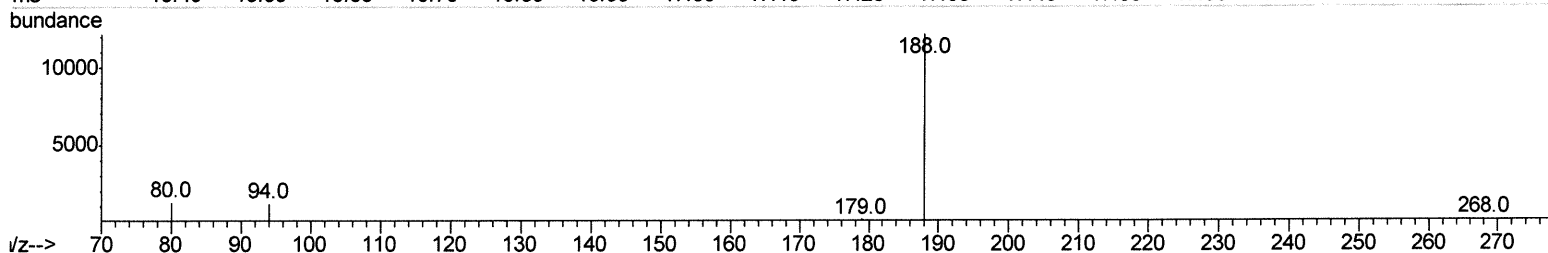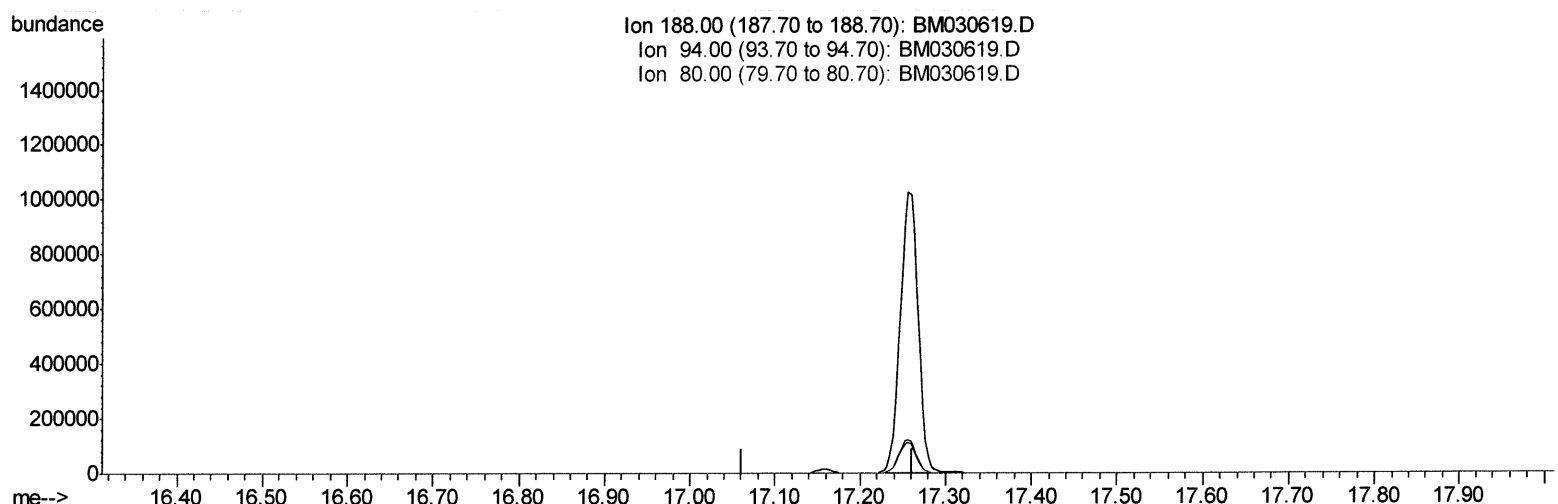

(13) Phenanthrene-d10 (I)

17.162min (-17.162) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.30	0.00#
80.00	11.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062521\
 Data File : BM030619.D
 Acq On : 26 Jun 2021 03:01
 Operator : CG/JU
 Sample : PB137215BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK215

Manual Integrations
 APPROVED

mohammad
 6/28/2021 1:22:01 PM

Quant Time: Jun 26 03:47:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 26 01:33:06 2021
 Response via : Initial Calibration

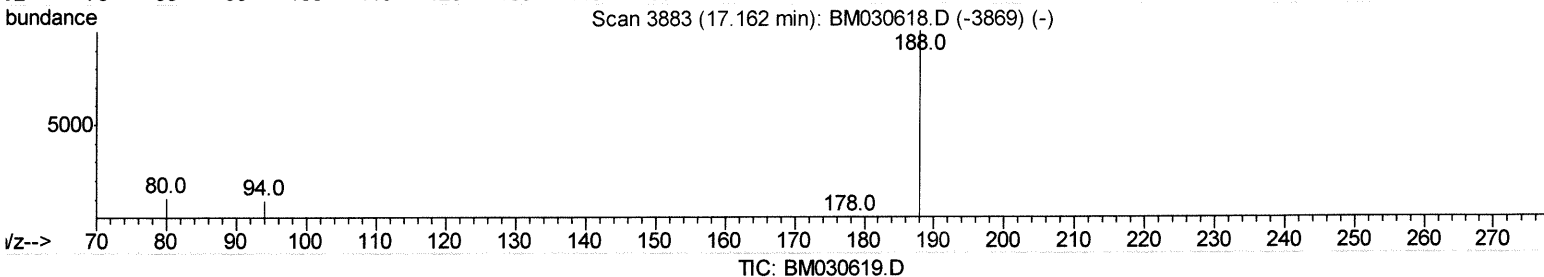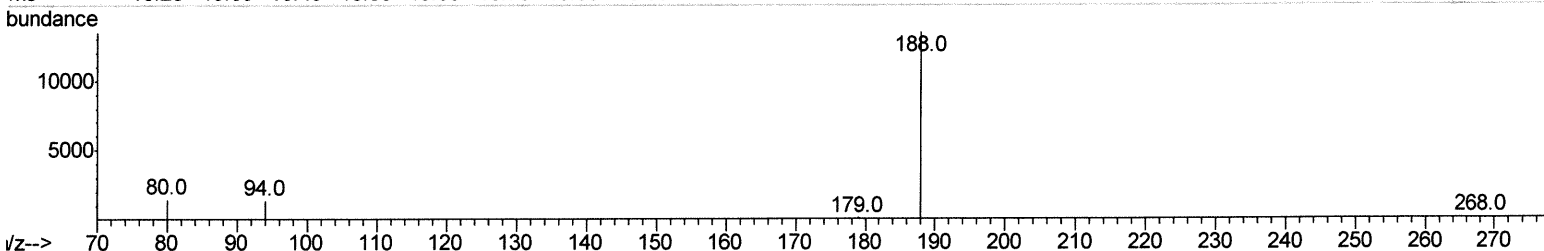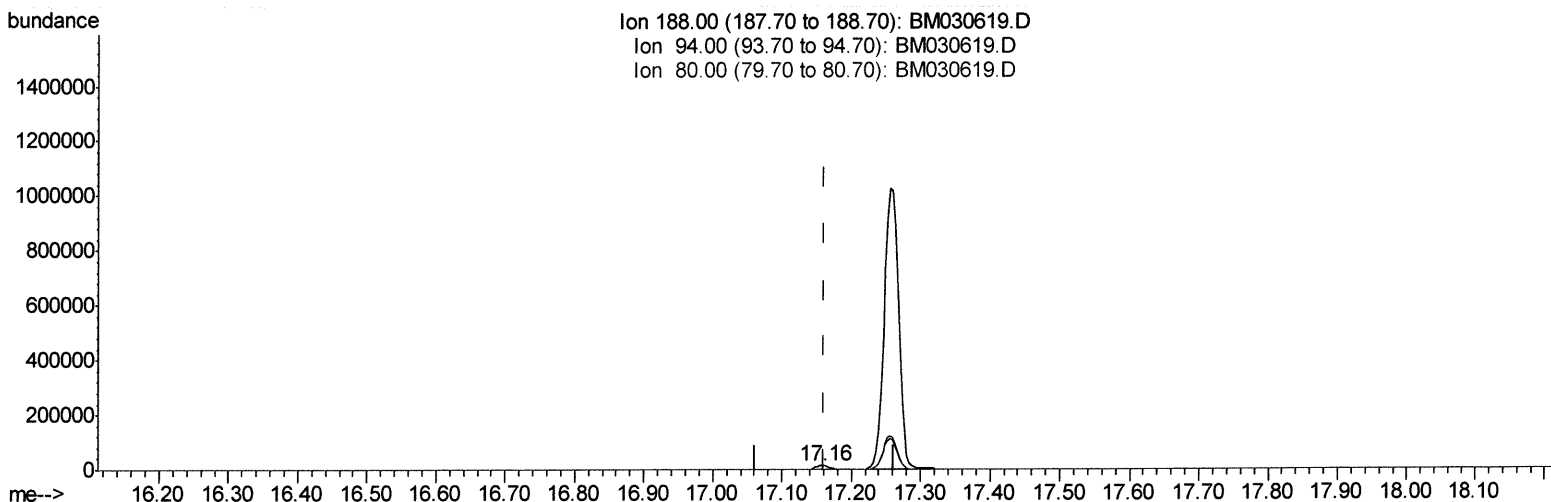

(13) Phenanthrene-d10 (I)

17.159min (-0.003) 0.40ng/ul m

response 18725

Ion	Exp%	Act%
188.00	100	100
94.00	10.30	10.27
80.00	11.60	10.89
0.00	0.00	0.00

JU 6/28/21

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062521\
 Data File : BM030619.D
 Acq On : 26 Jun 2021 03:01
 Operator : CG/JU
 Sample : PB137215BL
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK215

Manual Integrations
 APPROVED

mohammad
 6/28/2021 1:22:01 PM

Quant Time: Jun 26 04:11:31 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jun 26 01:33:06 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	3917	0.40	ng/ul	0.00
4) Naphthalene-d8	10.58	136	16460	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.42	164	10096	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.16	188	18725m	0.40	ng/ul	0.00
17) Chrysene-d12	21.33	240	11421	0.40	ng/ul	0.00
23) Perylene-d12	23.58	264	12719	0.40	ng/ul	-0.01

5/6/39/21

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.28	96	23939	5.71	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.17	152	7999	0.30	ng/ul	0.00
18) Fluoranthene-d10	19.18	212	13375	0.38	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed