


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062521\
Data File : BM030633.D
Acq On : 26 Jun 2021 12:13
Operator : CG/JU
Sample : PB137215BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK215

Quant Time: Jun 27 02:50:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 25 10:09:59 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/28/2021 1:22:41 PM

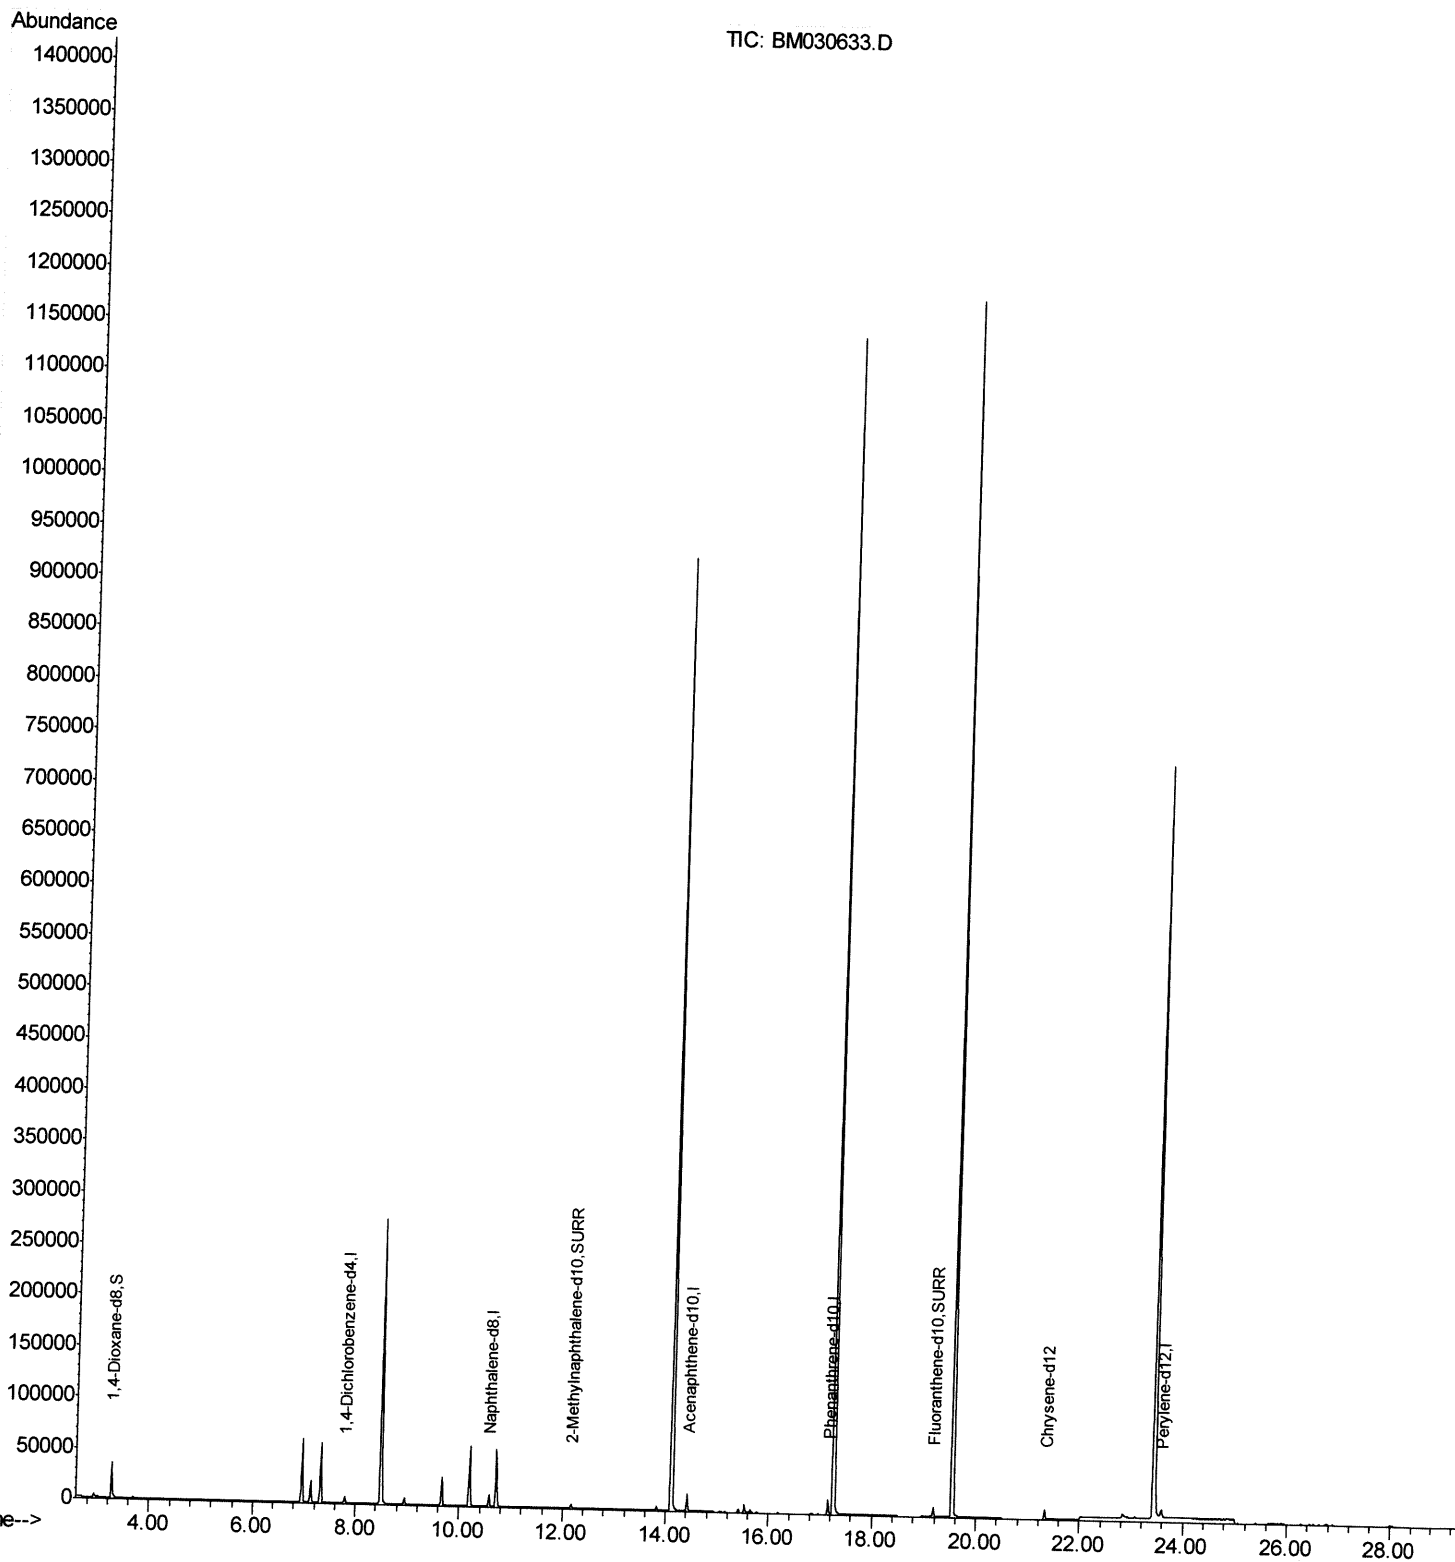



Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062521\
 Data File : BM030633.D
 Acq On : 26 Jun 2021 12:13
 Operator : CG/JU
 Sample : PB137215BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK215

Manual Integrations
 APPROVED

mohammad
 6/28/2021 1:22:41 PM

Quant Time: Jun 27 02:45:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 25 10:09:59 2021
 Response via : Initial Calibration

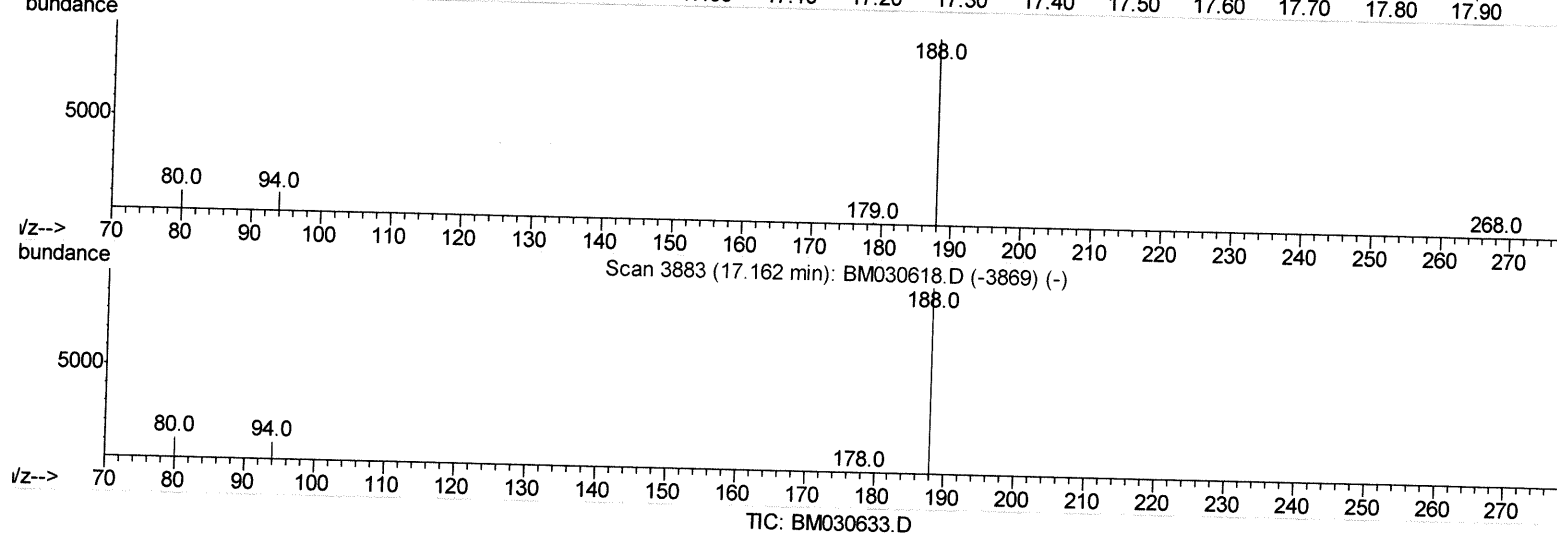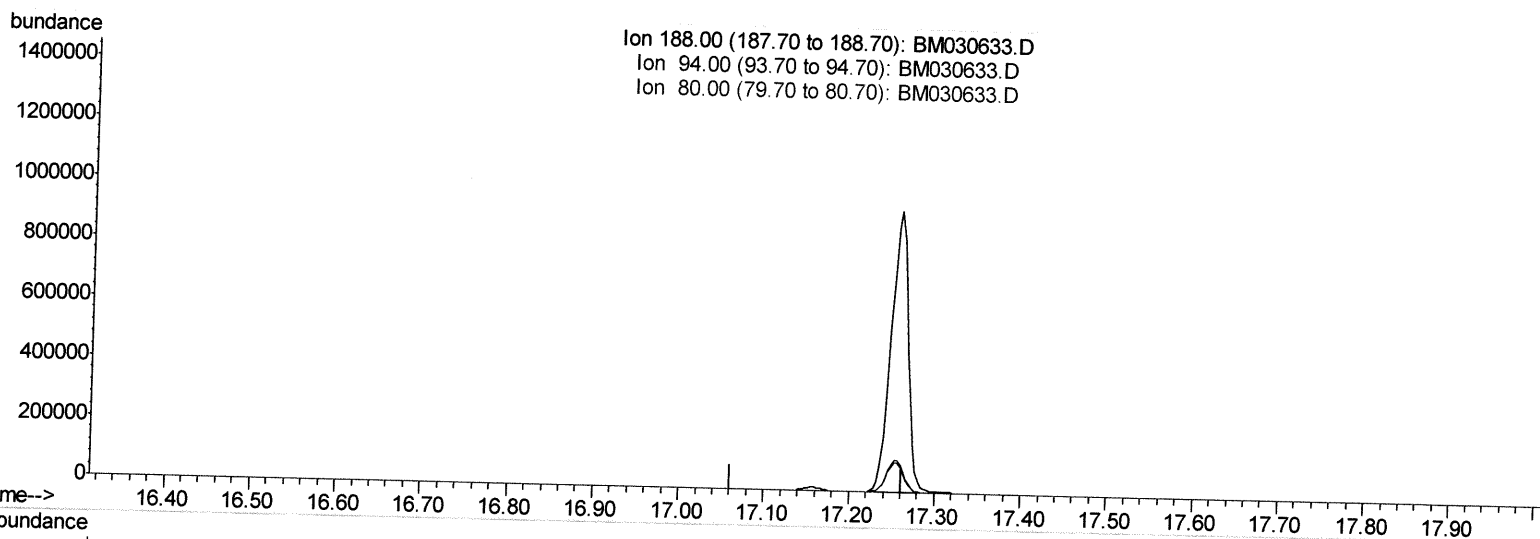

TIC: BM030633.D

(13) Phenanthrene-d10 (I)

17.162min (-17.162) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	10.30	0.00#
80.00	11.60	0.00#
0.00	0.00	0.00


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062521\
 Data File : BM030633.D
 Acq On : 26 Jun 2021 12:13
 Operator : CG/JU
 Sample : PB137215BL
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK215

Manual Integrations
 APPROVED

mohammad
 6/28/2021 1:22:41 PM

Quant Time: Jun 27 02:45:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jun 25 10:09:59 2021
 Response via : Initial Calibration

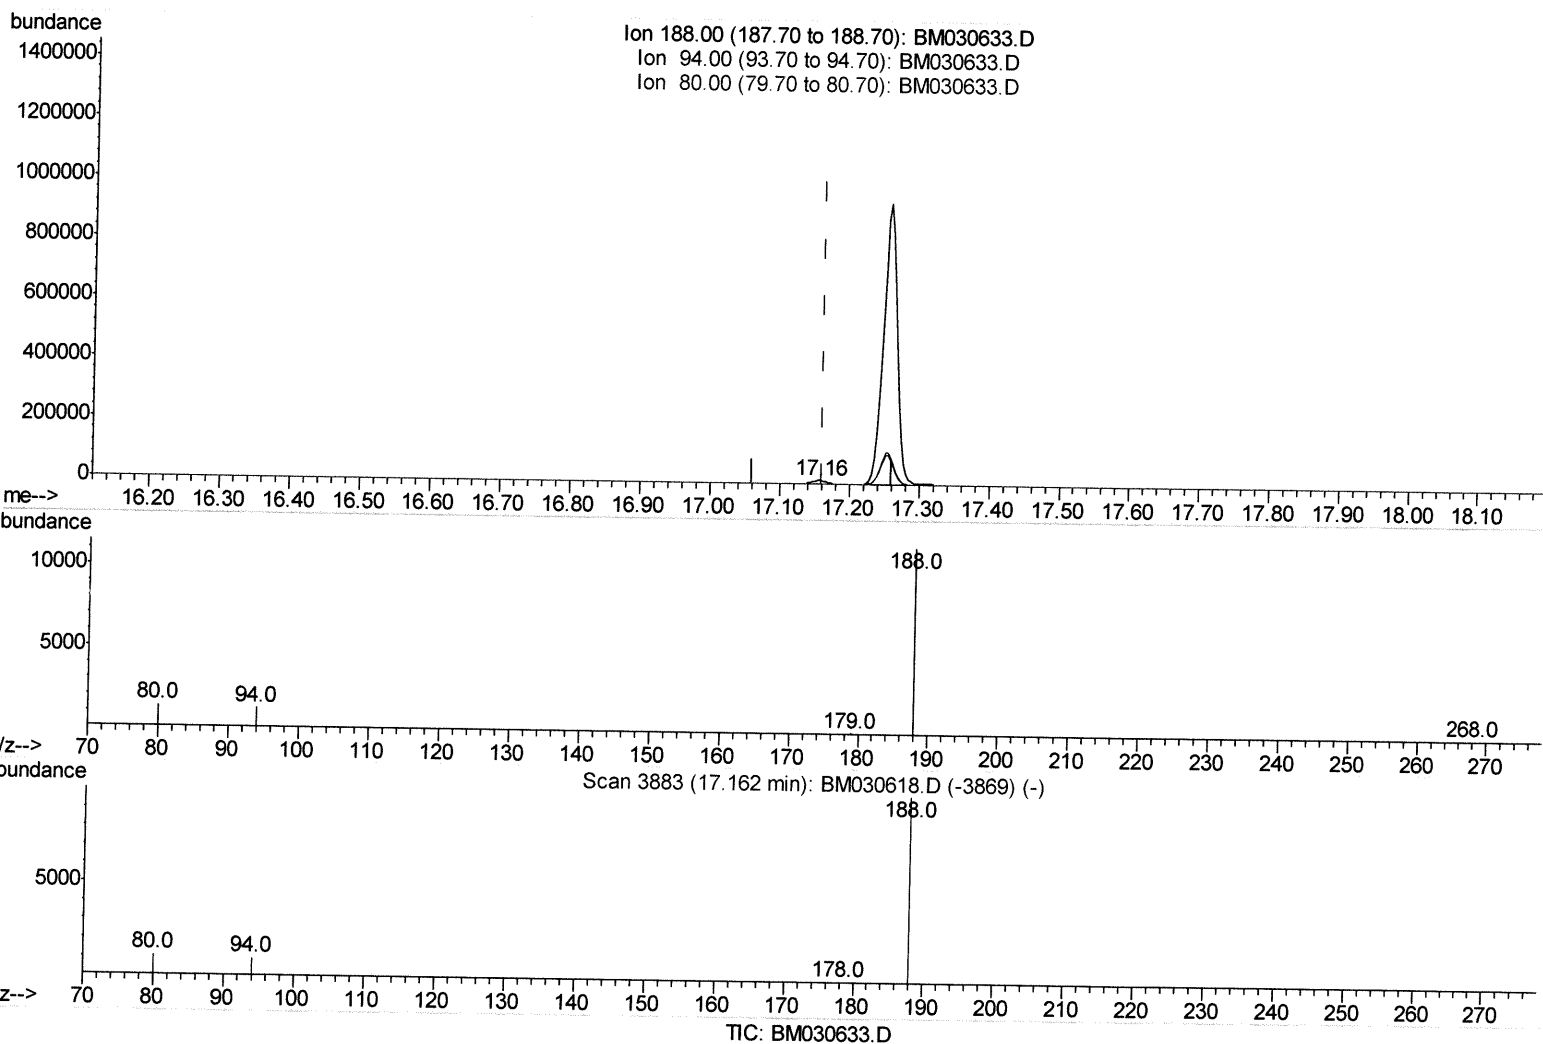

(13) Phenanthrene-d10 (I)

17.155min (-0.007) 0.40ng/ul m

response 16434

Ion	Exp%	Act%
188.00	100	100
94.00	10.30	10.42
80.00	11.60	11.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062521\
Data File : BM030633.D
Acq On : 26 Jun 2021 12:13
Operator : CG/JU
Sample : PB137215BL
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK215

Quant Time: Jun 27 02:50:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SFAM-EPA-SIM-BM062321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jun 25 10:09:59 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/28/2021 1:22:41 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.79	152	3631	0.40	ng/ul	0.00
4) Naphthalene-d8	10.58	136	15093	0.40	ng/ul	0.00
9) Acenaphthene-d10	14.42	164	9083	0.40	ng/ul	0.00
13) Phenanthrene-d10	17.16	188	16434m	0.40	ng/ul	0.00
17) Chrysene-d12	21.33	240	10083	0.40	ng/ul	0.00
23) Perylene-d12	23.58	264	11475	0.40	ng/ul	0.00

JU 6/30/21

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.27	96	22315	5.74	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	12.17	152	7243	0.30	ng/ul	0.00
18) Fluoranthene-d10	19.18	212	11474	0.37	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed