
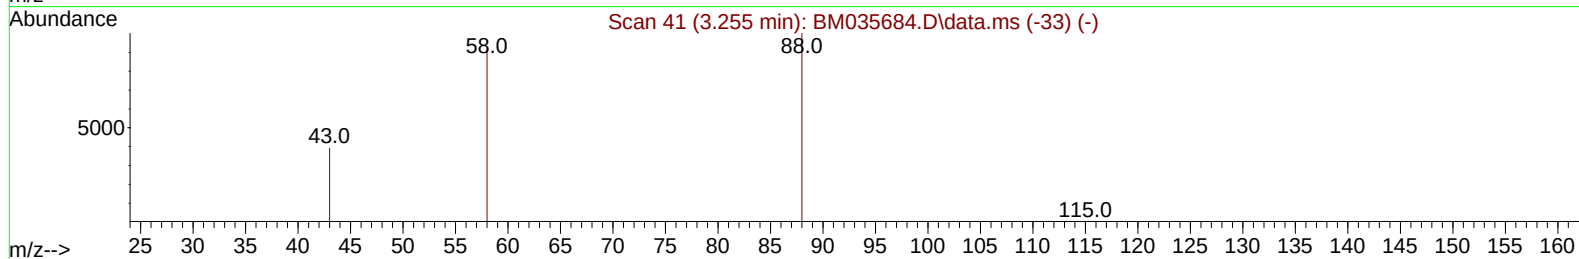
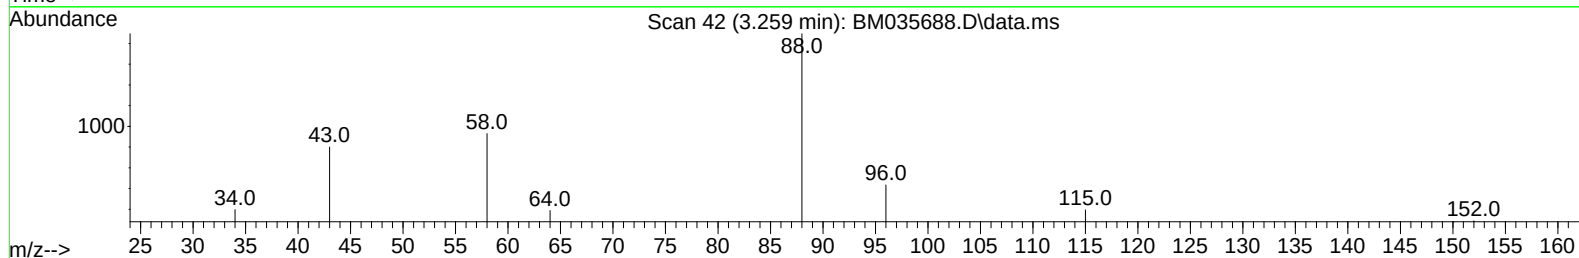


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062522\
Data File : BM035688.D
Acq On : 25 Jun 2022 15:38
Operator : CG/JU
Sample : SSTDICV0.4
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Jun 28 02:34:33 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM062522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 28 02:33:21 2022
Response via : Initial Calibration

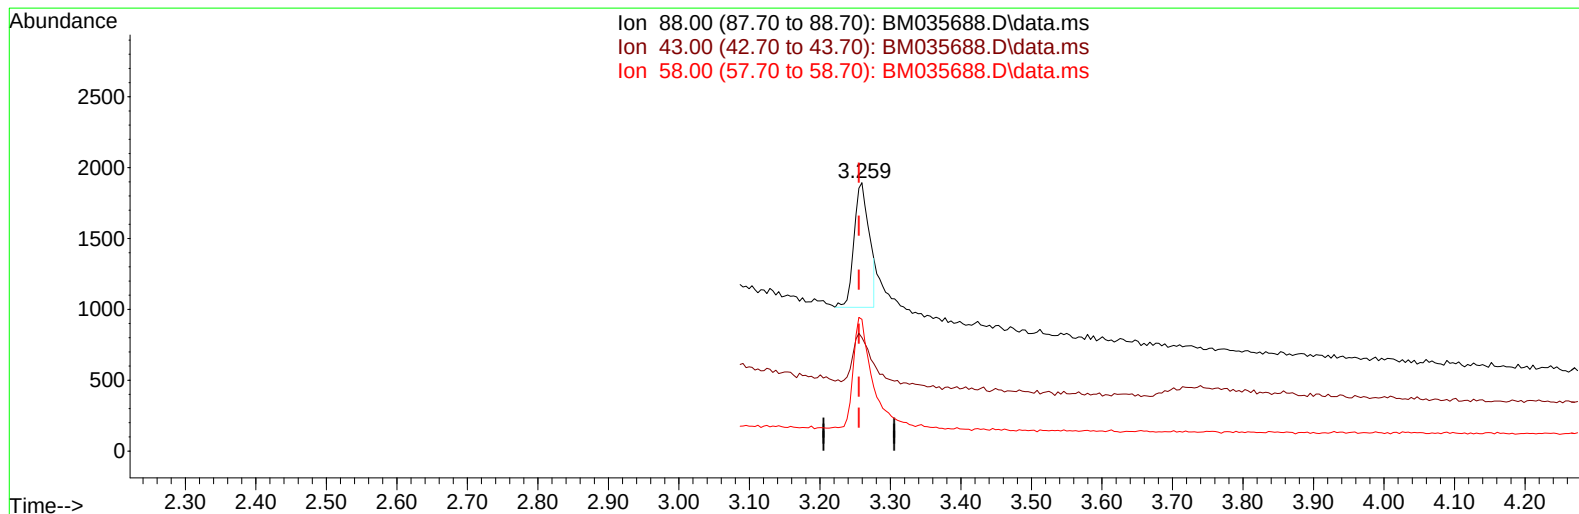

TIC: BM035688.D\data.ms

(2) 1,4-Dioxane

3.259min (+ 0.004) 0.31 ng/u1

response 1312

Ion	Exp%	Act%
88.00	100.00	100.00
43.00	47.20	42.29
58.00	53.20	49.10
0.00	0.00	0.00