

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062616\
 Data File : BM006053.D
 Acq On : 26 Jun 2016 23:23
 Operator : UM/SJ
 Sample : H3670-19
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 D9YA1

Manual Integrations
 APPROVED

sohil
 6/27/2016 8:07:05 PM

Quant Time: Jun 27 06:09:00 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM062516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jun 27 05:15:31 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	208679	20.00	ng/ul	0.00
7) Naphthalene-d8	10.44	136	1026184	20.00	ng/ul	0.00
15) Acenaphthene-d10	14.31	164	643679	20.00	ng/ul	0.00
23) Phenanthrene-d10	17.06	188	1580631	20.00	ng/ul	0.00
29) Chrysene-d12	21.25	240	1709627	20.00	ng/ul	0.00
34) Perylene-d12	23.47	264	1598585	20.00	ng/ul	0.00


System Monitoring Compounds

2) 1,4-Dioxane-d8	3.17	96	7170	1.53	ng/uL	0.00
3) Phenol-d5	6.83	99	303026	13.80	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	7.00	67	207194	16.97	ng/ul	0.00
5) 2-Chlorophenol-d4	7.19	132	244765	16.01	ng/ul	0.00
6) 4-Methylphenol-d8	8.36	113	157287	8.49	ng/ul	0.00
8) Nitrobenzene-d5	8.81	128	137738	17.63	ng/ul	0.00
9) 2-Nitrophenol-d4	9.53	143	153037	17.60	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	10.06	165	274457	16.46	ng/ul	0.00
12) 4-Chloroaniline-d4	10.58	131	305404	16.88	ng/ul	0.00
16) Dimethylphthalate-d6	13.72	166	946239	17.17	ng/ul	0.00
17) Acenaphthylene-d8	14.00	160	1223713	19.15	ng/ul	0.00
20) 4-Nitrophenol-d4	14.51	143	162646	13.84	ng/ul	0.00
21) Fluorene-d10	15.30	176	879472	18.69	ng/ul	0.00
24) 4,6-Dinitro-2-methylphenol	15.43	200	80632	9.19	ng/ul	0.00
26) Anthracene-d10	17.16	188	1398109	19.26	ng/ul	0.00
30) Pyrene-d10	19.46	212	1625424	21.70	ng/ul	0.01
37) Benzo(a)pyrene-d12	23.33	264	1405617	19.48	ng/ul	0.01

Target Compounds

					Qvalue
11) Naphthalene	10.49	128	224243	4.37 ng/ul	100
13) 2-Methylnaphthalene	12.10	142	45064	1.09 ng/ul	91
18) Acenaphthylene	14.03	152	195171	2.90 ng/ul	99
19) Acenaphthene	14.37	153	173953	4.06 ng/ul	97
22) Fluorene	15.36	166	238064	4.62 ng/ul	96
25) Phenanthrene	17.10	178	4021147	47.30 ng/ul	100
27) Anthracene	17.19	178	901335	10.27 ng/ul	99
28) Fluoranthene	19.12	202	5318906	48.84 ng/ul	99
31) Pyrene	19.49	202	4520340	46.19 ng/ul	98
32) Benzo(a)anthracene	21.23	228	2069000	20.37 ng/ul	98
33) Chrysene	21.29	228	1959462	21.12 ng/ul	96
35) Benzo(b)fluoranthene	22.81	252	2512277	27.05 ng/ul	98
36) Benzo(k)fluoranthene	22.85	252	717575m	8.31 ng/ul	
38) Benzo(a)pyrene	23.37	252	1595462	17.92 ng/ul	98
39) Indeno(1,2,3-cd)pyrene	25.69	276	1223114	11.52 ng/ul	96
40) Dibenzo(a,h)anthracene	25.69	278	255339	2.89 ng/ul#	80
41) Benzo(g,h,i)perylene	26.37	276	1213583	13.22 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

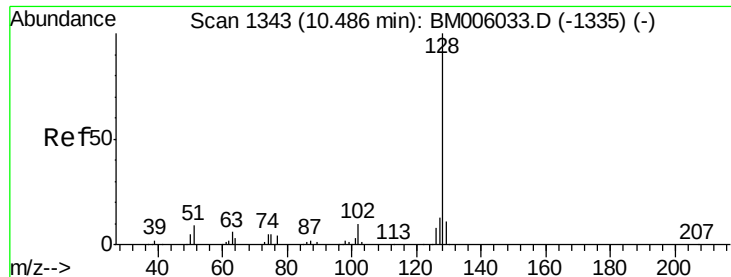





#11
Naphthalene
Concen: 4.37 ng/ul
RT: 10.49 min Scan# 1343
Delta R.T. -0.00 min
Lab File: BM006053.D
Acq: 26 Jun 2016 23:23

Instrument :
BNA_M
ClientSampleId :
D9YA1

Tgt Ion	Ratio	Resp	Lower	Upper
128	100	224243		
129	10.7	8.6	13.0	
127	12.6	10.2	15.4	




Manual Integrations
APPROVED


sohil
6/27/2016 8:07:05 PM

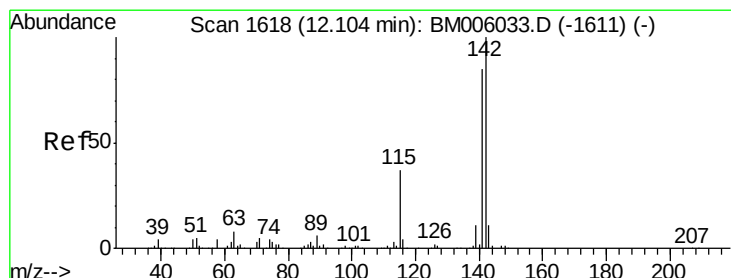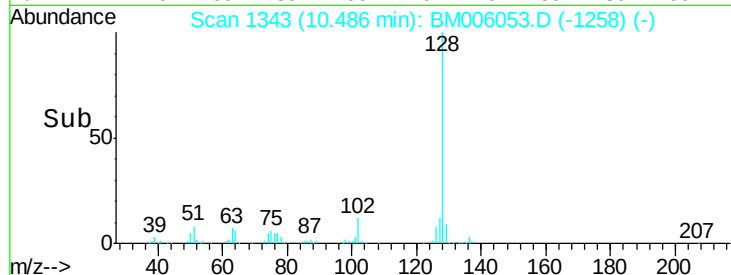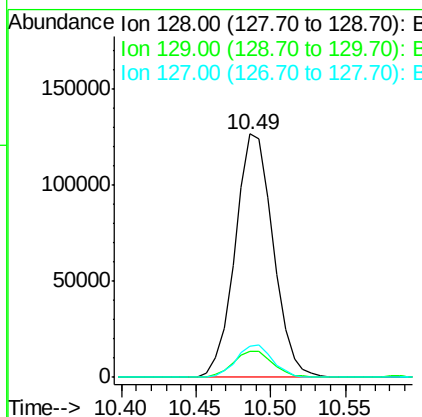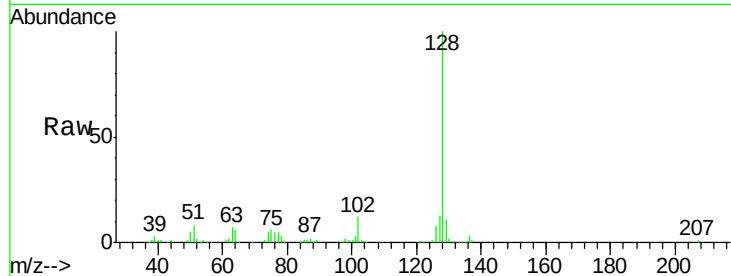

#13
2-Methylnaphthalene
Concen: 1.09 ng/ul
RT: 12.10 min Scan# 1618
Delta R.T. -0.00 min
Lab File: BM006053.D
Acq: 26 Jun 2016 23:23

Tgt Ion	Ratio	Resp	Lower	Upper
142	100	45064		
141	95.1	69.4	104.2	

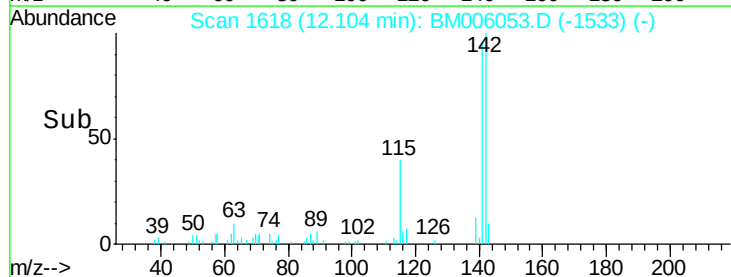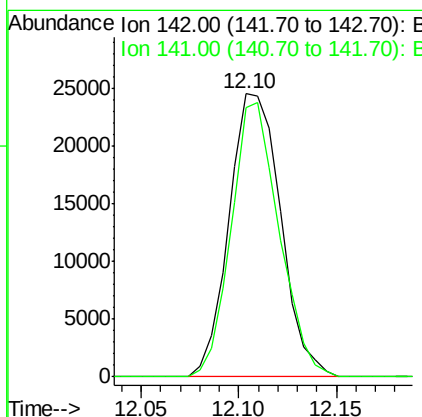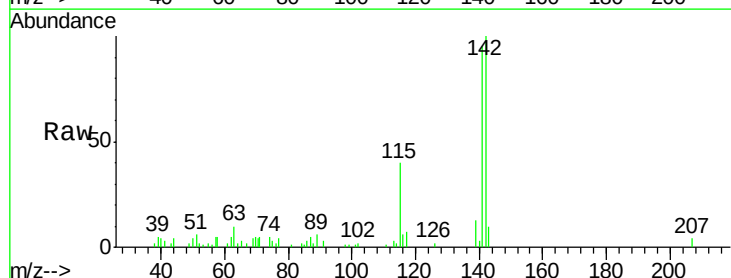

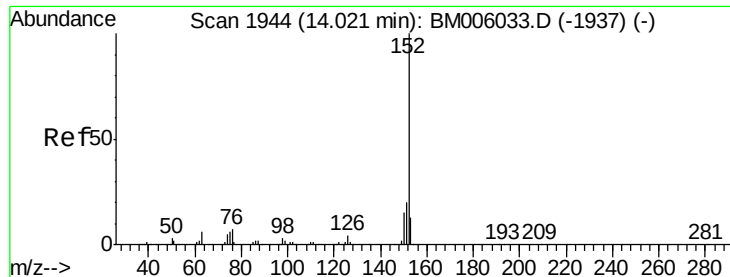





#18
 Acenaphthylene
 Concen: 2.90 ng/ul
 RT: 14.03 min Scan# 1945
 Delta R.T. 0.01 min
 Lab File: BM006053.D
 Acq: 26 Jun 2016 23:23

Instrument :
 BNA_M
 ClientSampleId :
 D9YA1

Tgt Ion	Ratio	Resp	Lower	Upper
152	100	195171		
151	18.9	15.5	23.3	
153	13.6	10.5	15.7	




Manual Integrations
 APPROVED


sohil
 6/27/2016 8:07:05 PM

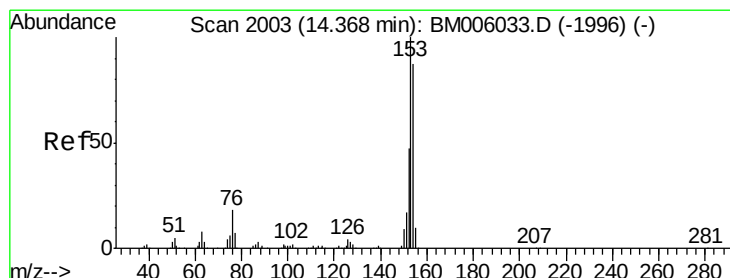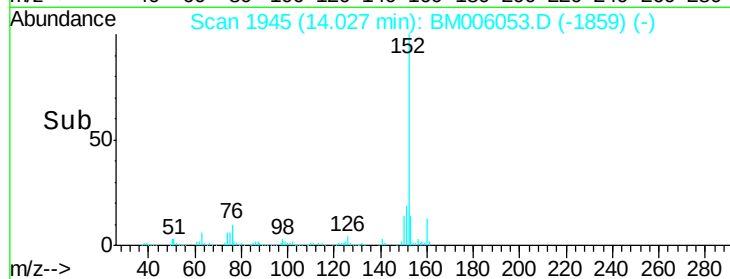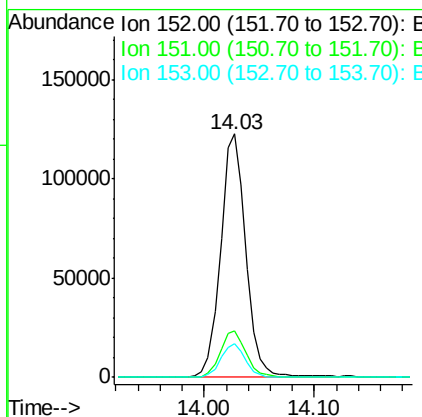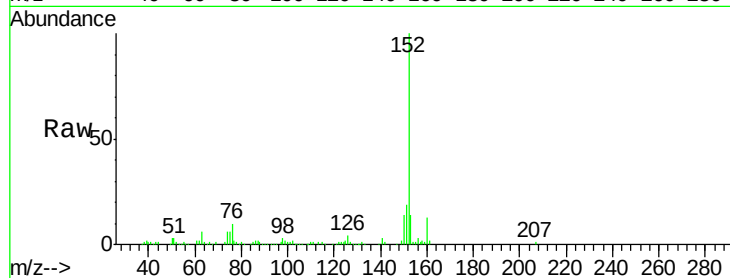

#19
 Acenaphthene
 Concen: 4.06 ng/ul
 RT: 14.37 min Scan# 2003
 Delta R.T. -0.00 min
 Lab File: BM006053.D
 Acq: 26 Jun 2016 23:23

Tgt Ion	Ratio	Resp	Lower	Upper
153	100	173953		
152	51.4	38.6	57.8	
154	89.8	70.7	106.1	

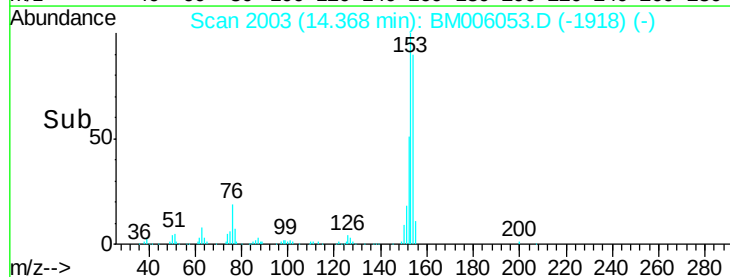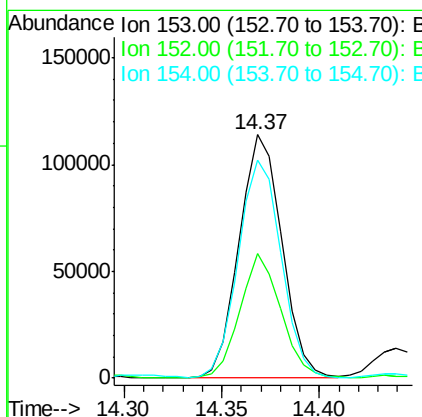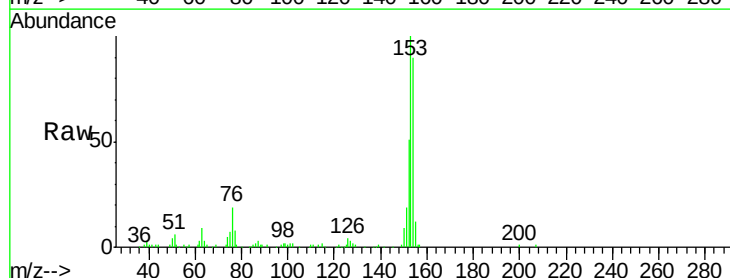

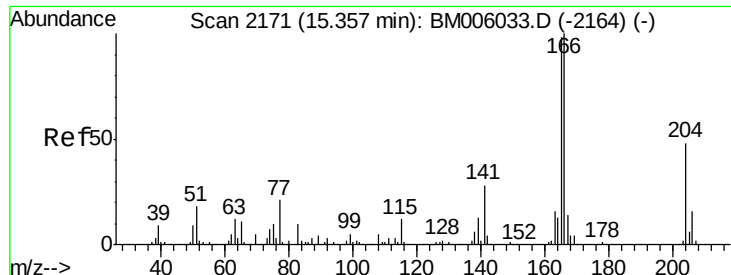

#22

Fluorene

Concen: 4.62 ng/ul

RT: 15.36 min Scan# 2171

Delta R.T. -0.00 min

Lab File: BM006053.D


Acq: 26 Jun 2016 23:23

Instrument :

BNA_M

ClientSampleId :




D9YA1

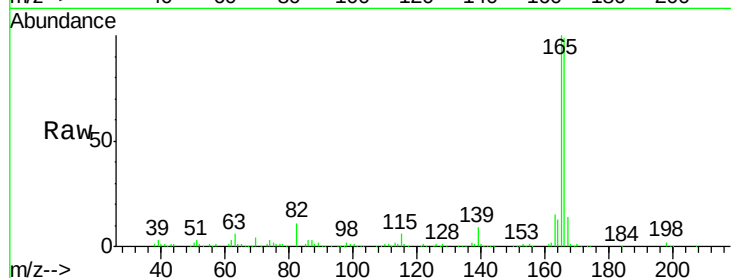

Tgt Ion:	166	Resp:	238064
Ion Ratio	Lower	Upper	
166	100		
165	100.6	76.8	115.2
167	14.6	10.8	16.2

Manual Integrations
APPROVED

sohil
6/27/2016 8:07:05 PM

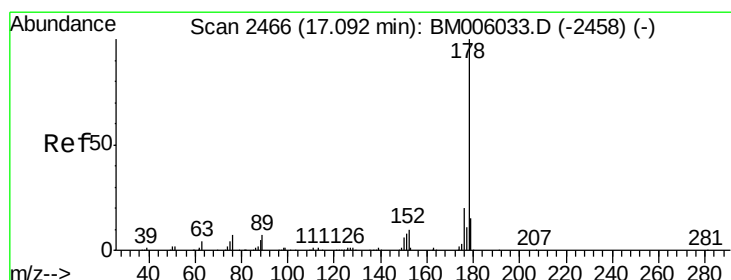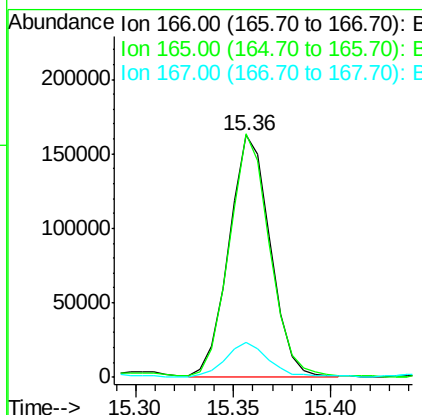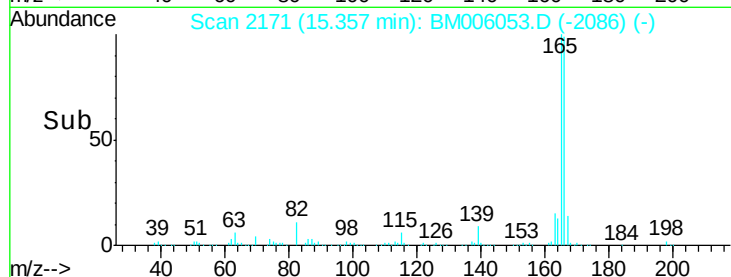

#25

Phenanthrene

Concen: 47.30 ng/ul




RT: 17.10 min Scan# 2468


Delta R.T. 0.01 min

Lab File: BM006053.D

Acq: 26 Jun 2016 23:23

Tgt Ion:	178	Resp:	4021147
Ion Ratio	Lower	Upper	
178	100		
179	15.3	12.1	18.1
176	19.4	15.4	23.0

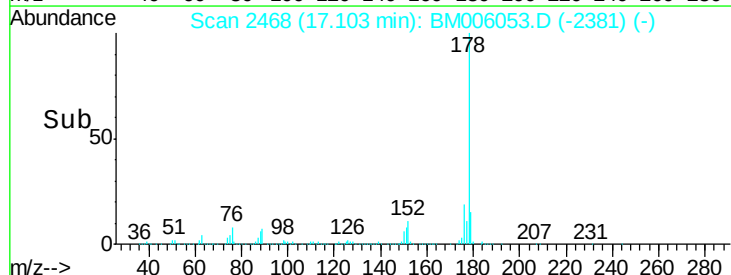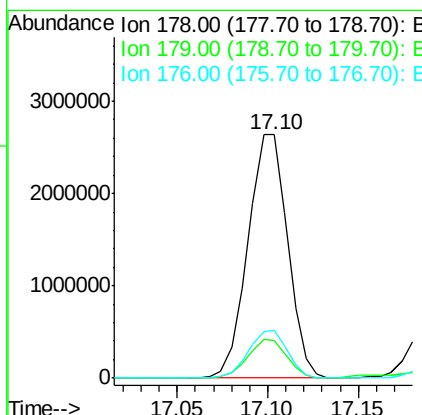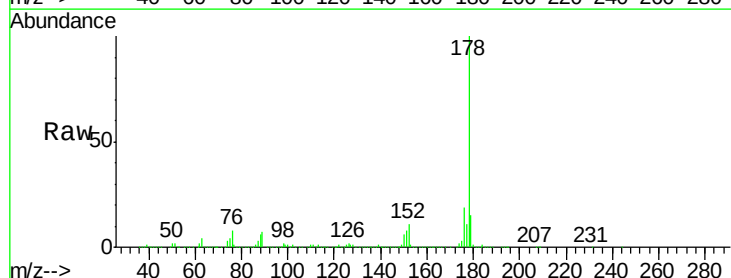

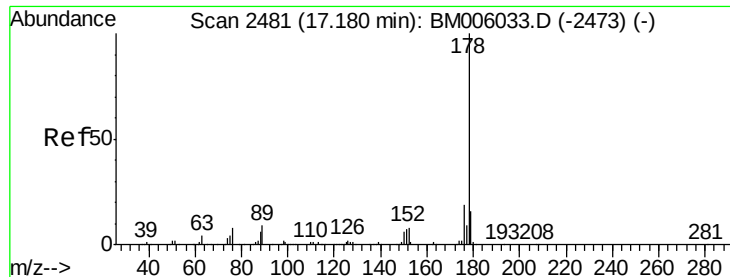





#27
 Anthracene
 Concen: 10.27 ng/ul
 RT: 17.19 min Scan# 2483
 Delta R.T. 0.01 min
 Lab File: BM006053.D
 Acq: 26 Jun 2016 23:23

Instrument :
 BNA_M
 ClientSampleId :
 D9YA1

Tgt Ion	Ratio	Resp Lower	Resp Upper
178	100		
179	15.4	12.2	18.4
176	18.0	14.9	22.3




Manual Integrations
 APPROVED


sohil
 6/27/2016 8:07:05 PM

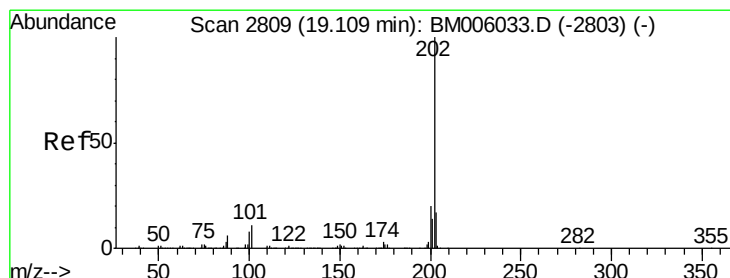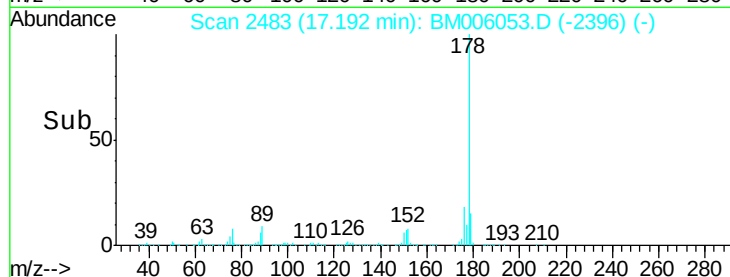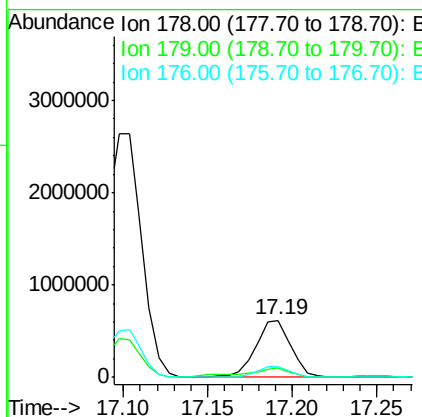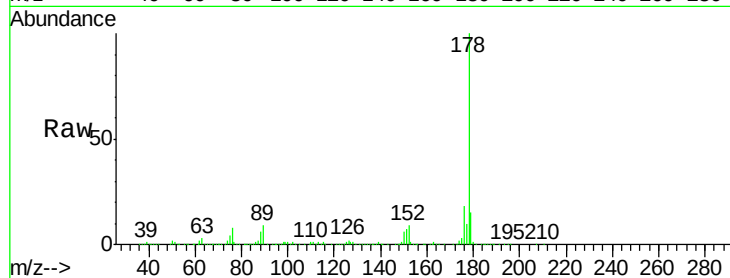

#28
 Fluoranthene
 Concen: 48.84 ng/ul
 RT: 19.12 min Scan# 2811
 Delta R.T. 0.01 min
 Lab File: BM006053.D
 Acq: 26 Jun 2016 23:23

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	9.7	8.2	12.4
100	7.4	6.3	9.5

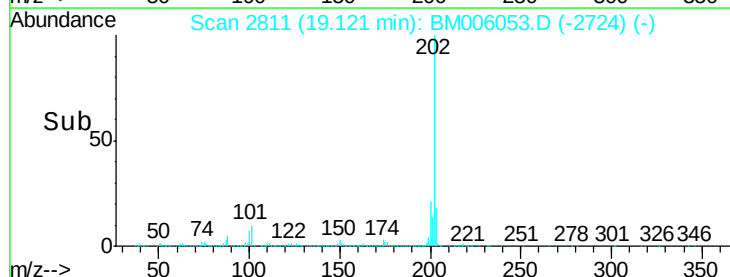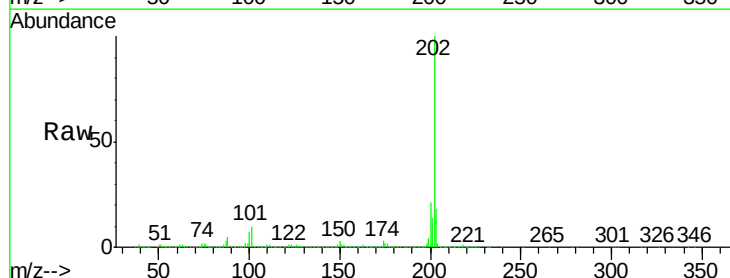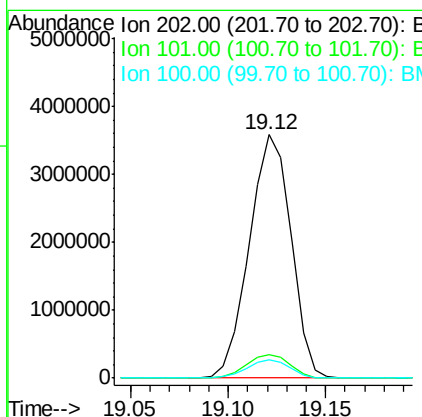

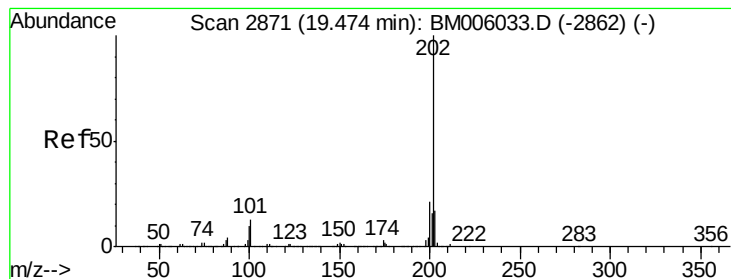

#31

Pyrene

Concen: 46.19 ng/ul

RT: 19.49 min Scan# 2873

Delta R.T. 0.01 min

Lab File: BM006053.D

Acq: 26 Jun 2016 23:23

Instrument :

BNA_M





ClientSampleId :

D9YA1

Tgt Ion:	202	Resp:	4520340
Ion	Ratio	Lower	Upper
202	100		
101	11.8	9.8	14.6
100	9.1	8.2	12.2

Manual Integrations
APPROVED

sohil
6/27/2016 8:07:05 PM

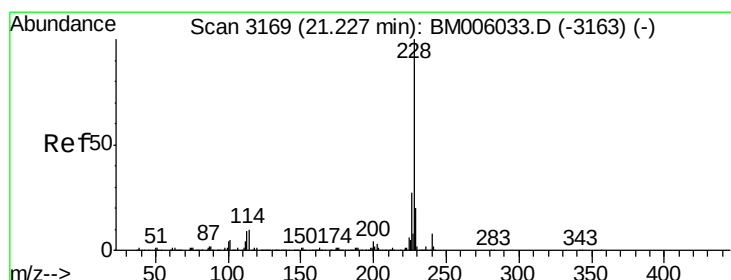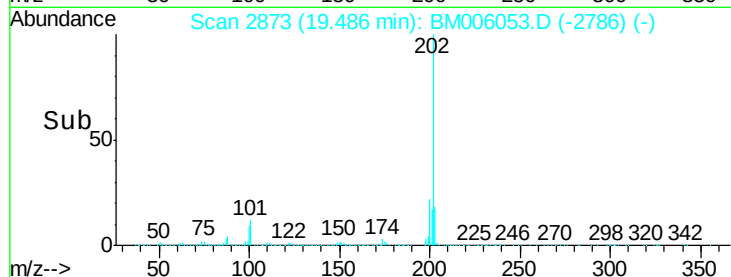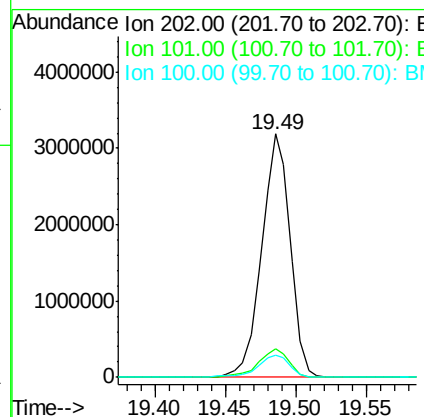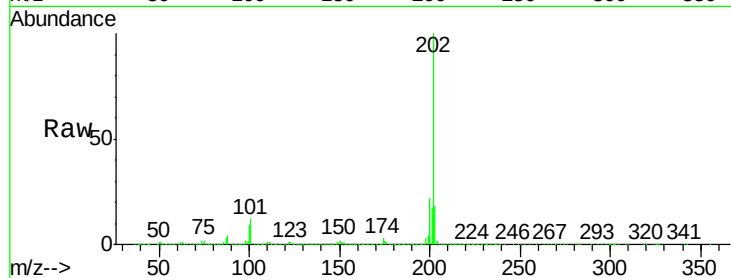

#32

Benzo(a)anthracene

Concen: 20.37 ng/ul




RT: 21.23 min Scan# 3170


Delta R.T. 0.01 min

Lab File: BM006053.D

Acq: 26 Jun 2016 23:23

Tgt Ion:	228	Resp:	2069000
Ion	Ratio	Lower	Upper
228	100		
229	20.4	15.8	23.6
226	28.0	21.5	32.3

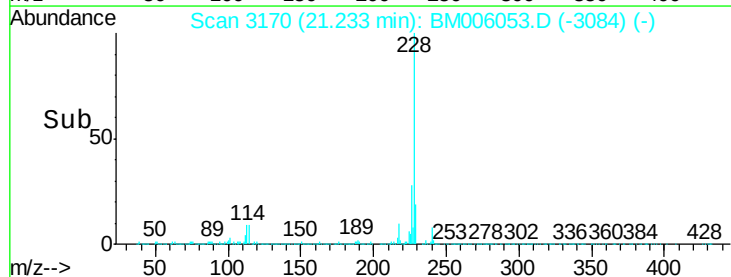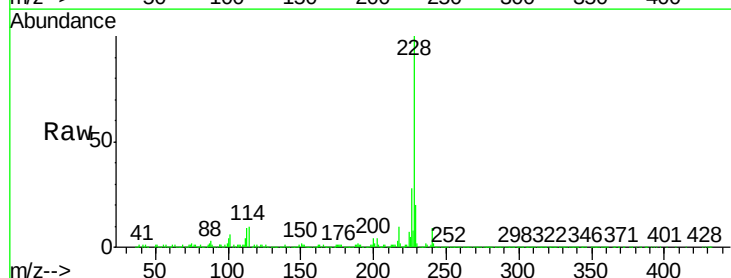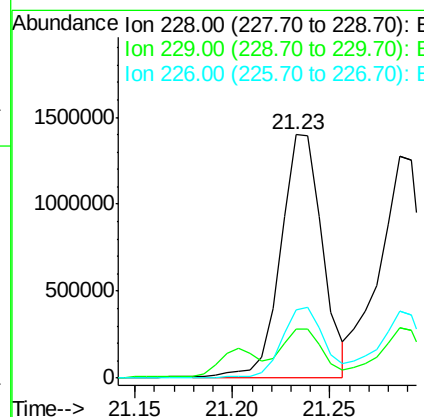

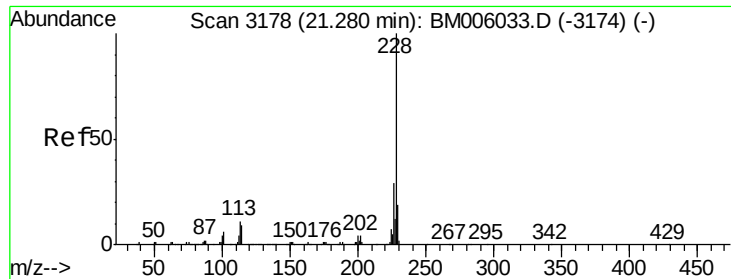

#33

Chrysene

Concen: 21.12 ng/ul

RT: 21.29 min Scan# 3179

Delta R.T. 0.01 min

Lab File: BM006053.D

Acq: 26 Jun 2016 23:23

Instrument :

BNA_M





ClientSampled :

D9YA1

Tgt Ion:	228	Resp:	1959462
Ion Ratio	Lower	Upper	
228	100		
226	29.9	24.3	36.5
229	22.8	15.4	23.2

Manual Integrations
APPROVED

sohil
6/27/2016 8:07:05 PM

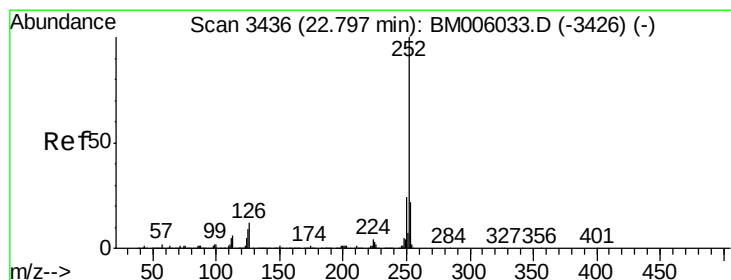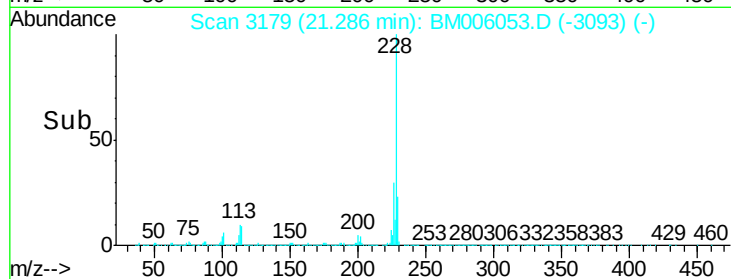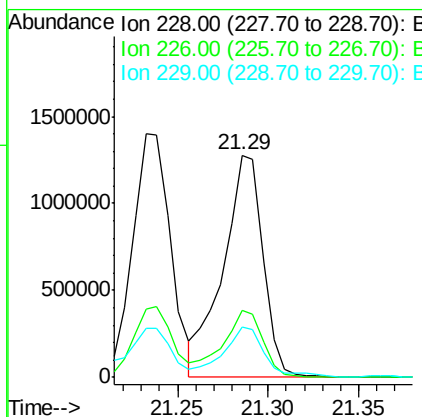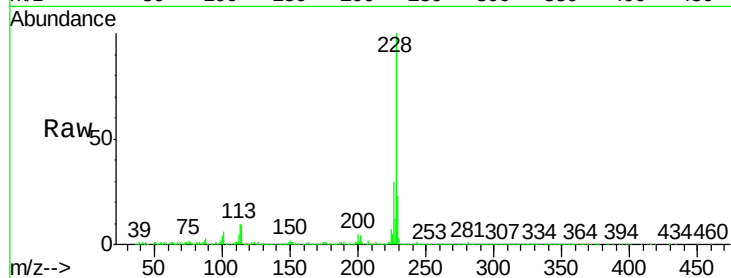

#35

Benzo(b)fluoranthene

Concen: 27.05 ng/ul




RT: 22.81 min Scan# 3438


Delta R.T. 0.01 min

Lab File: BM006053.D

Acq: 26 Jun 2016 23:23

Tgt Ion:	252	Resp:	2512277
Ion Ratio	Lower	Upper	
252	100		
253	22.5	17.2	25.8
125	9.8	6.8	10.2

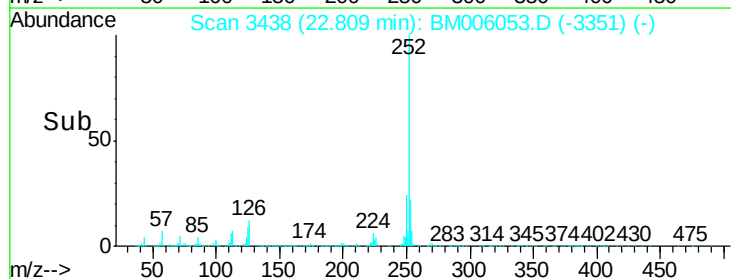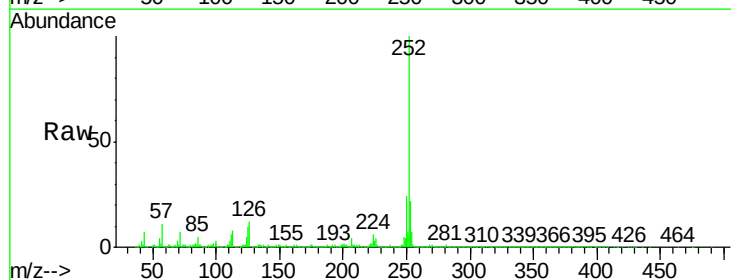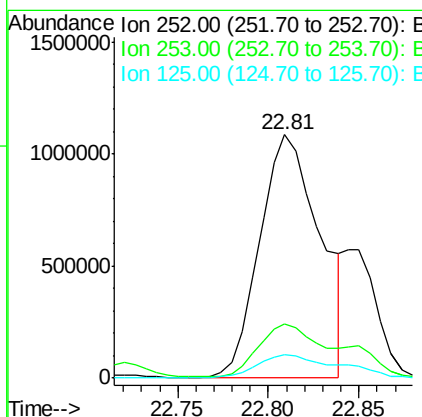

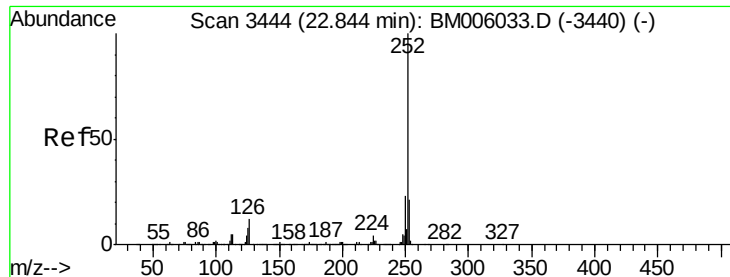


#36
Benzo(k)fluoranthene
Concen: 8.31 ng/ul m
RT: 22.85 min Scan# 3445
Delta R.T. 0.01 min
Lab File: BM006053.D
Acq: 26 Jun 2016 23:23

Instrument :
BNA_M
ClientSampled :
D9YA1




Tgt Ion	Ratio	Lower	Upper
252	100		
253	24.8	17.3	25.9
125	9.3	7.0	10.4

Manual Integrations
APPROVED

sohil
6/27/2016 8:07:05 PM

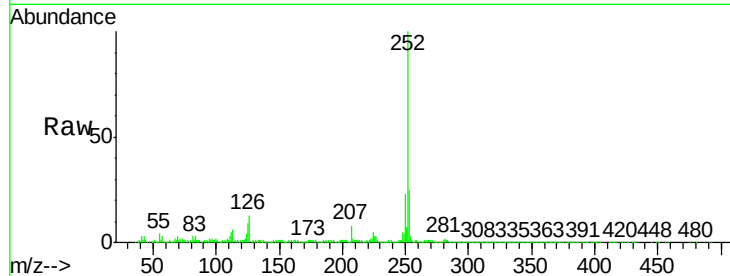




Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

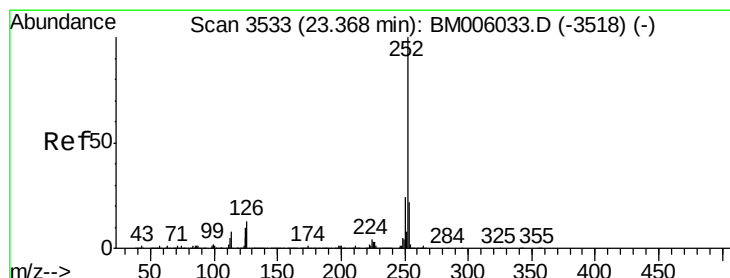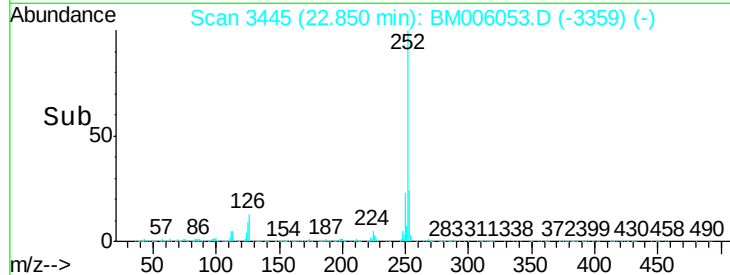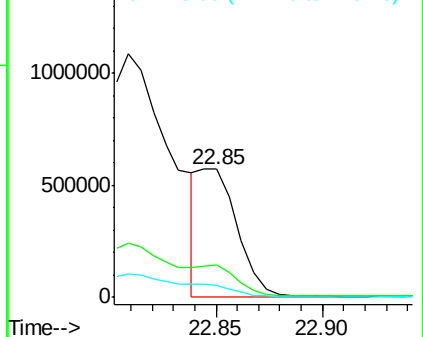


#38
Benzo(a)pyrene
Concen: 17.92 ng/ul
RT: 23.37 min Scan# 3534
Delta R.T. 0.01 min
Lab File: BM006053.D
Acq: 26 Jun 2016 23:23

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.4	17.6	26.4
125	9.8	7.8	11.6

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

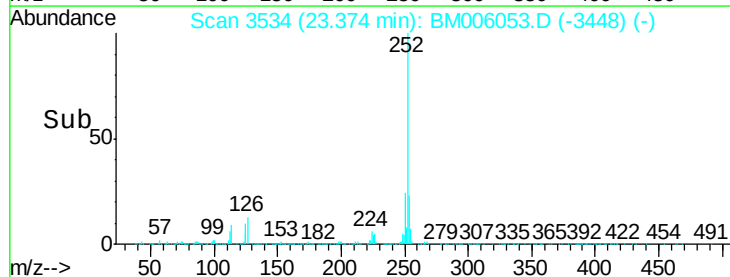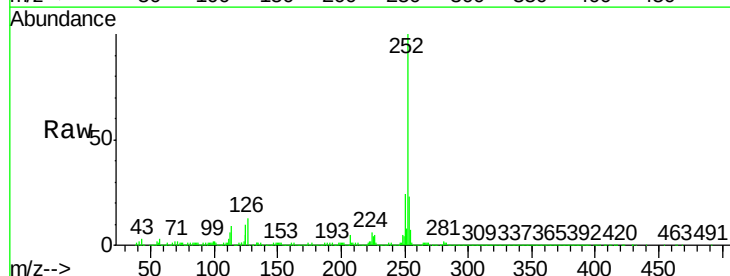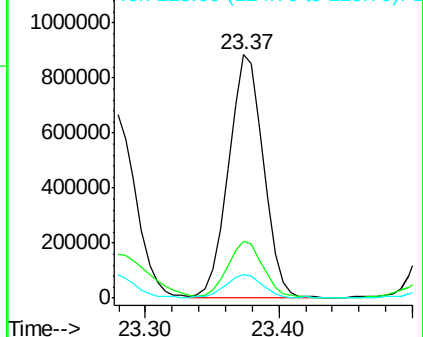

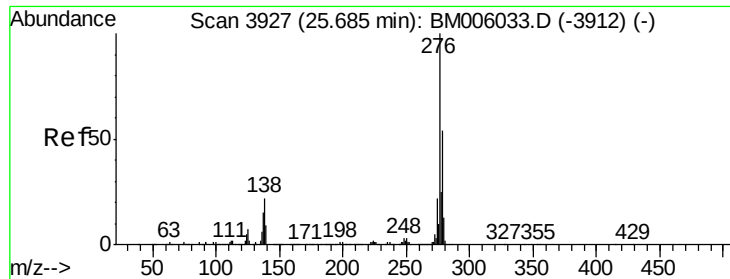

#39

Indeno(1,2,3-cd)pyrene

Concen: 11.52 ng/ul

RT: 25.69 min Scan# 3928

Delta R.T. 0.01 min

Lab File: BM006053.D


Acq: 26 Jun 2016 23:23

Instrument :

BNA_M

ClientSampleId :

D9YA1

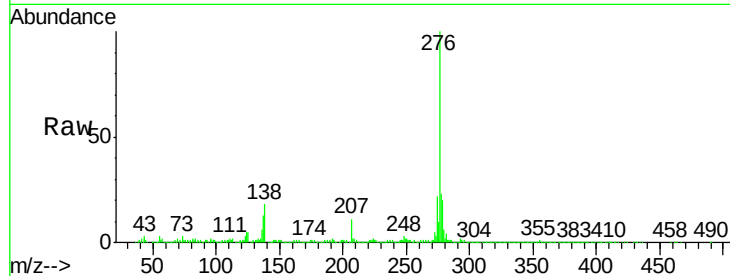

Tgt Ion: 276 Resp: 1223114

Ion Ratio Lower Upper


276 100

138 17.9 16.6 25.0

277 23.4 19.6 29.4

Manual Integrations
APPROVED



sohil
6/27/2016 8:07:05 PM

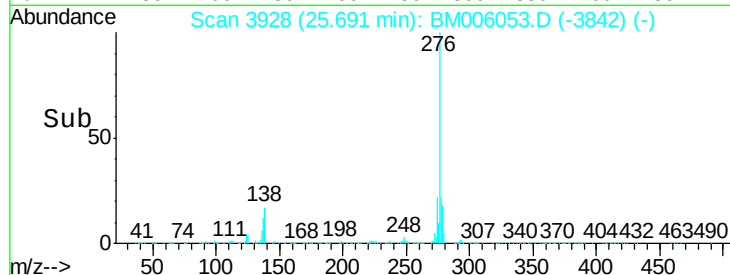

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

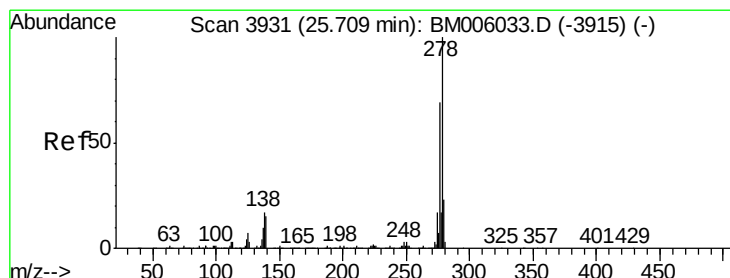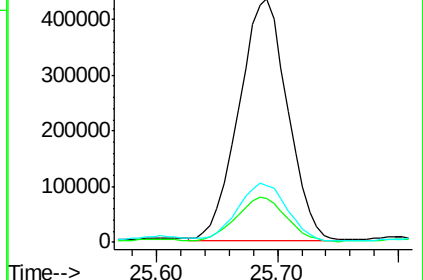

#40

Dibenzo(a,h)anthracene

Concen: 2.89 ng/ul

RT: 25.69 min Scan# 3928

Delta R.T. -0.02 min

Lab File: BM006053.D

Acq: 26 Jun 2016 23:23


Tgt Ion: 278 Resp: 255339

Ion Ratio Lower Upper

278 100

139 0.0 11.4 17.2#



279 28.8 18.8 28.2#

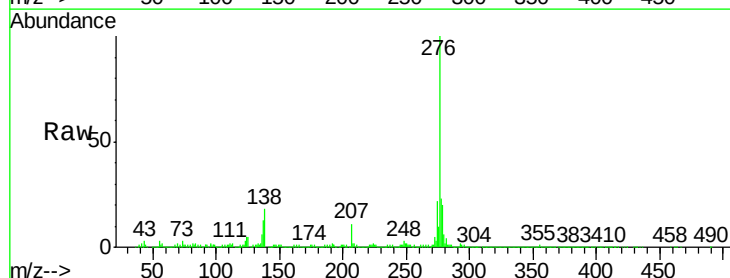


Abundance Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

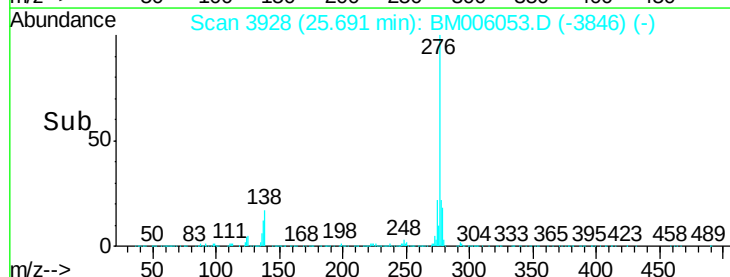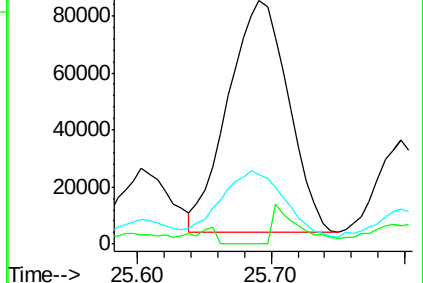

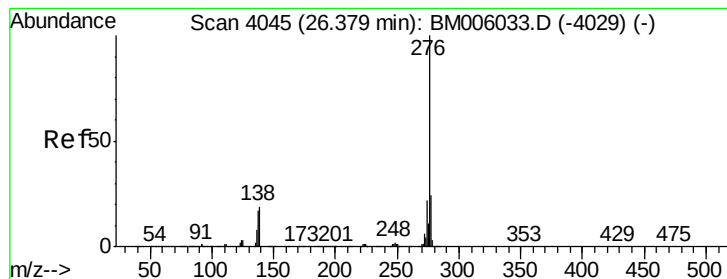

#41

Benzo(g,h,i)perylene

Concen: 13.22 ng/ul

RT: 26.37 min Scan# 4044

Delta R.T. -0.01 min

Lab File: BM006053.D


Acq: 26 Jun 2016 23:23

Instrument :

BNA_M

ClientSampleId :

D9YA1

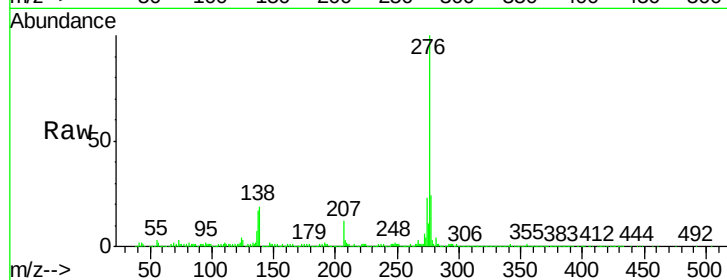

Tgt Ion: 276 Resp: 1213583

Ion Ratio Lower Upper


276 100

138 18.5 15.9 23.9

277 24.3 19.2 28.8

Manual Integrations
APPROVED

sohil
6/27/2016 8:07:05 PM

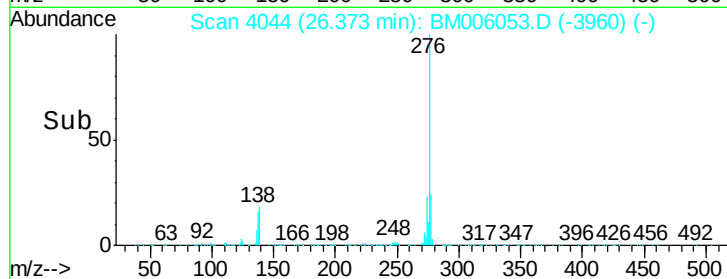

Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

