

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062617\
 Data File : BM010757.D
 Acq On : 26 Jun 2017 22:15
 Operator : SJ/JU
 Sample : I3756-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AD9

Quant Time: Jun 27 01:31:47 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 01:28:19 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	133917	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	626714	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.11	164	458990	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.86	188	1185348	20.00	ng/ul	0.00
75) Chrysene-d12	21.08	240	1376808	20.00	ng/ul	0.00
83) Perylene-d12	23.22	264	997606	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.07	96	4448	1.90	ng/uL	0.00
5) Phenol-d5	6.65	99	128681	10.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.80	67	70878	9.73	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	97560	10.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	114773	10.85	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	51247	11.46	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	59507	11.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	120366	11.10	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	144248	12.62	ng/ul	0.00
43) Dimethylphthalate-d6	13.53	166	462566	11.48	ng/ul	0.00
46) Acenaphthylene-d8	13.79	160	521480	11.13	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	63140	8.90	ng/ul	0.00
57) Fluorene-d10	15.11	176	392775	11.28	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.23	200	68808	9.45	ng/ul	0.00
70) Anthracene-d10	16.96	188	678948	11.86	ng/ul	0.00
76) Pyrene-d10	19.27	212	810010	12.66	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.08	264	581468	12.06	ng/ul	0.00


Target Compounds					Qvalue	
44) Dimethylphthalate	13.57	163	117544	2.976	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM062617\
Data File : BM010757.D
Acq On : 26 Jun 2017 22:15
Operator : SJ/JU
Sample : I3756-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AD9

Quant Time: Jun 27 01:31:47 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 27 01:28:19 2017
Response via : Initial Calibration

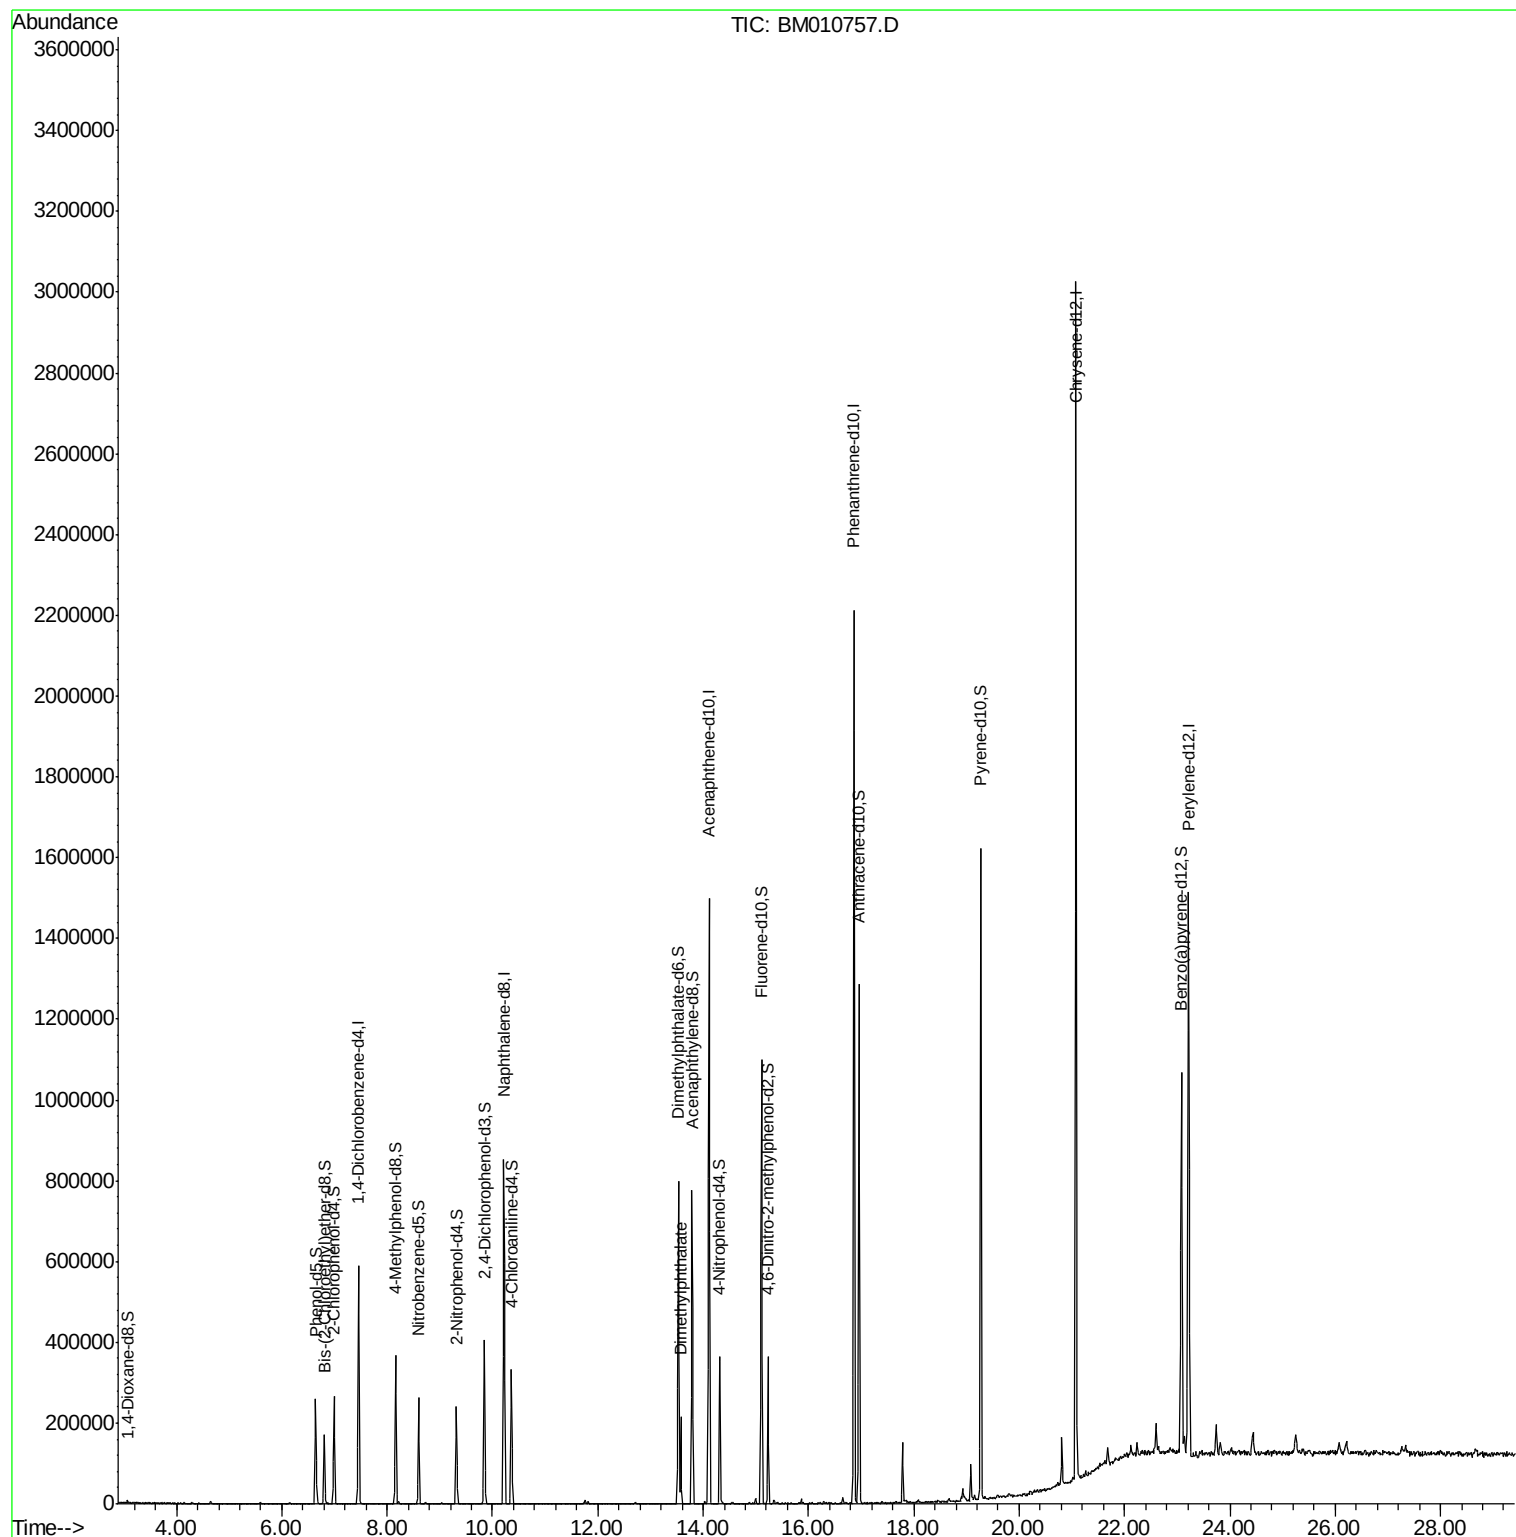

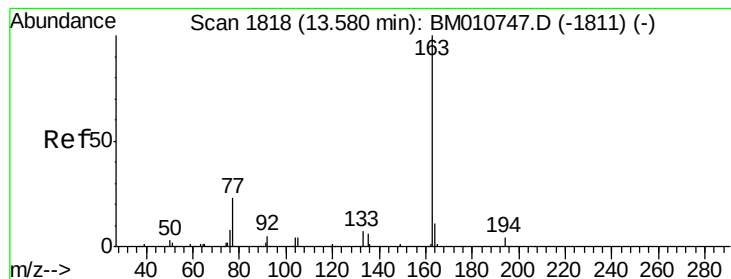

#44

Dimethylphthalate

Concen: 2.976 ng/ul

RT: 13.57 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BM010757.D

Acq: 26 Jun 2017 22:15

Instrument :

BNA_M

ClientSampleId :

C0AD9

Tgt Ion:163 Resp: 117544

Ion Ratio Lower Upper

163 100

194 4.2 3.5 5.3

164 10.1 8.2 12.4

