

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_M\DATA\BM062617\
 Data File : BM010759.D
 Acq On : 26 Jun 2017 23:27
 Operator : SJ/JU
 Sample : I3756-10
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AE1

Quant Time: Jun 27 01:32:08 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jun 27 01:28:19 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.46	152	68144	20.00	ng/ul	0.00
18) Naphthalene-d8	10.22	136	321830	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.11	164	224085	20.00	ng/ul	0.00
61) Phenanthrene-d10	16.86	188	559854	20.00	ng/ul	0.00
75) Chrysene-d12	21.07	240	656708	20.00	ng/ul	0.00
83) Perylene-d12	23.21	264	510817	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.07	96	3669	3.09	ng/uL	0.00
5) Phenol-d5	6.65	99	109784	16.91	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.81	67	61278	16.54	ng/ul	0.00
9) 2-Chlorophenol-d4	6.99	132	80903	17.77	ng/ul	0.00
13) 4-Methylphenol-d8	8.16	113	93640	17.40	ng/ul	0.00
19) Nitrobenzene-d5	8.60	128	45371	19.76	ng/ul	0.00
22) 2-Nitrophenol-d4	9.32	143	50640	19.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.85	165	102968	18.49	ng/ul	0.00
29) 4-Chloroaniline-d4	10.36	131	116225	19.81	ng/ul	0.00
43) Dimethylphthalate-d6	13.53	166	381276	19.38	ng/ul	0.00
46) Acenaphthylene-d8	13.79	160	426657	18.65	ng/ul	0.00
51) 4-Nitrophenol-d4	14.32	143	58678	16.95	ng/ul	0.00
57) Fluorene-d10	15.11	176	320829	18.87	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.23	200	56680	16.48	ng/ul	0.00
70) Anthracene-d10	16.96	188	528029	19.53	ng/ul	0.00
76) Pyrene-d10	19.27	212	662902	21.73	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.08	264	502019	20.33	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	13.57	163	96395	4.999	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA_M\DATA\BM062617\
Data File : BM010759.D
Acq On : 26 Jun 2017 23:27
Operator : SJ/JU
Sample : I3756-10
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AE1

Quant Time: Jun 27 01:32:08 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM062017.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jun 27 01:28:19 2017
Response via : Initial Calibration

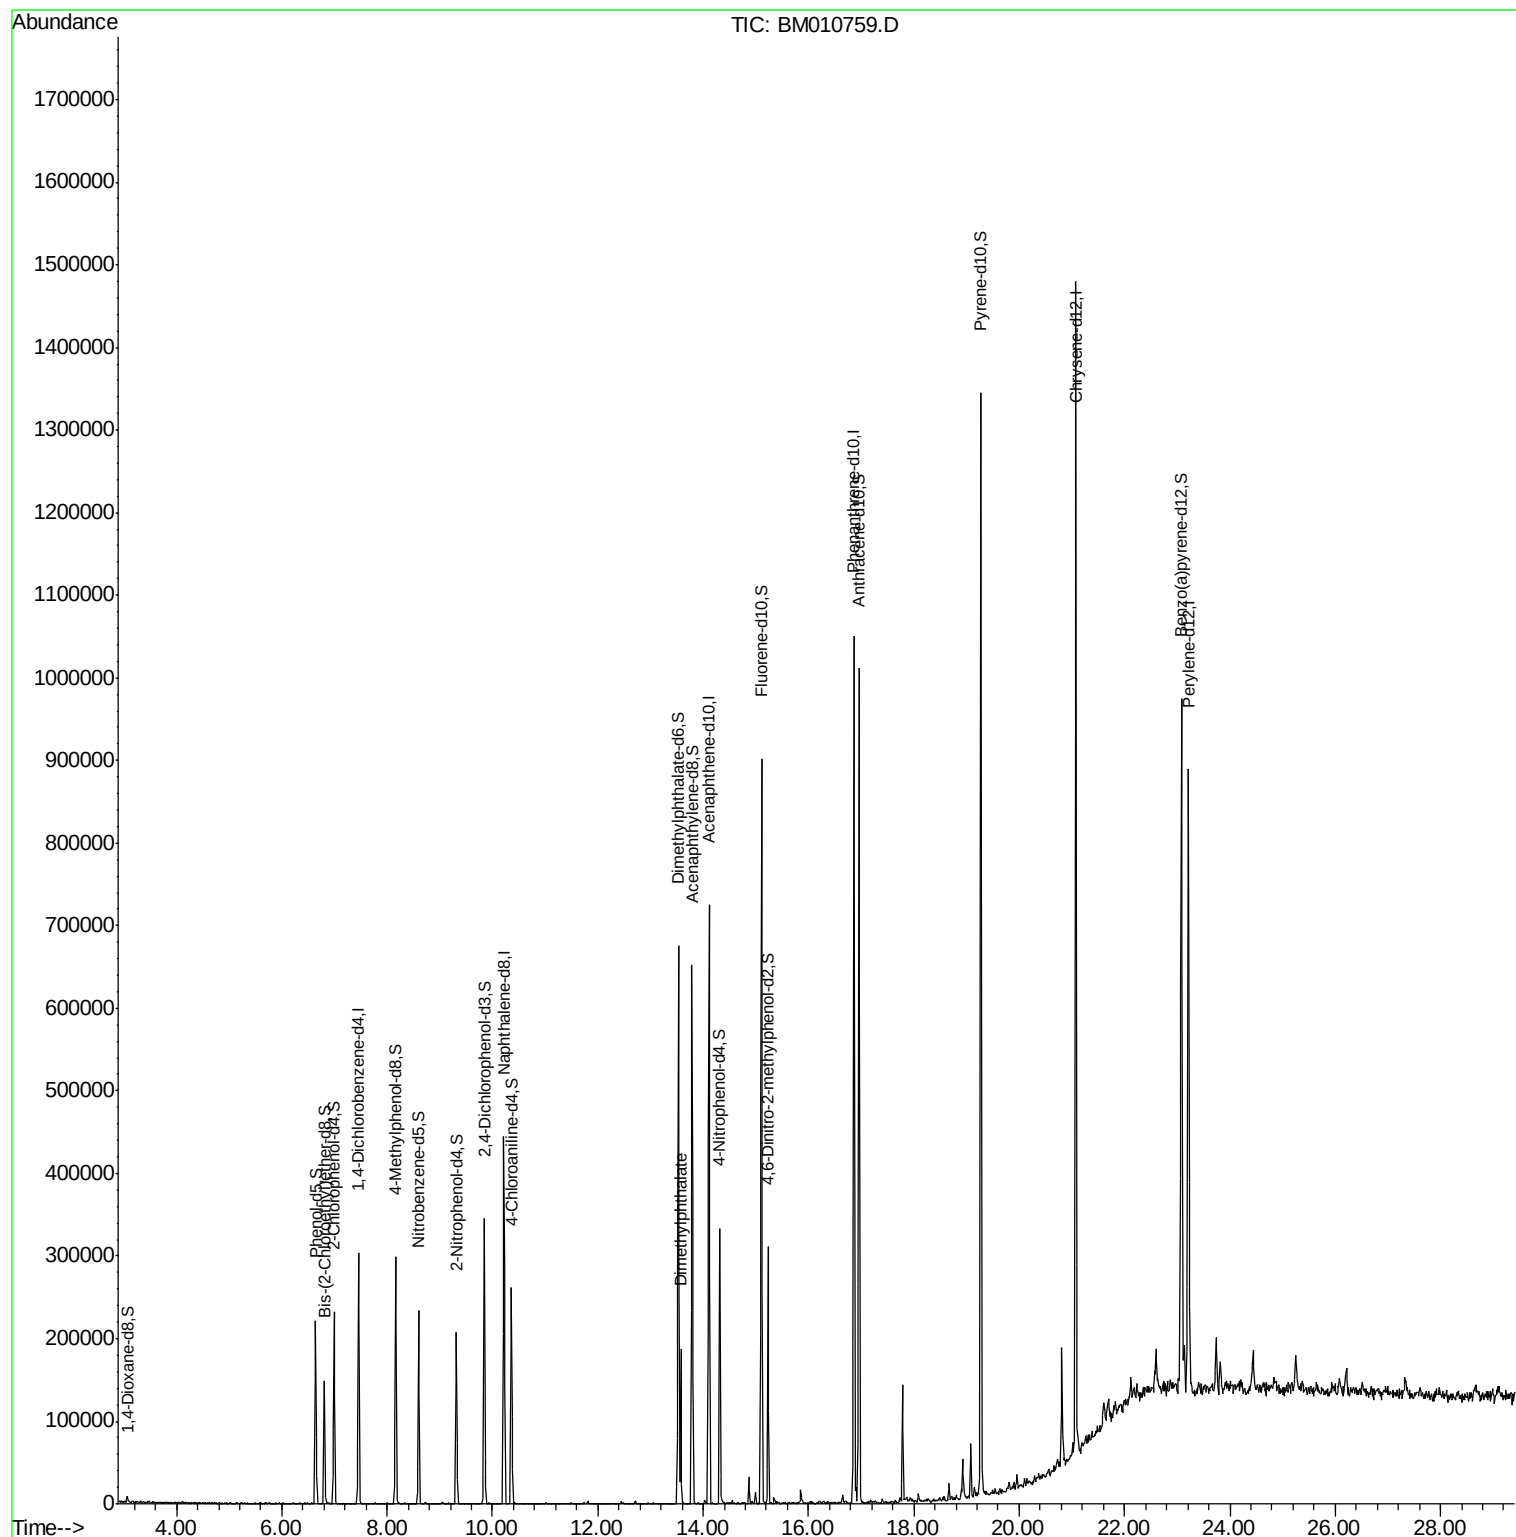

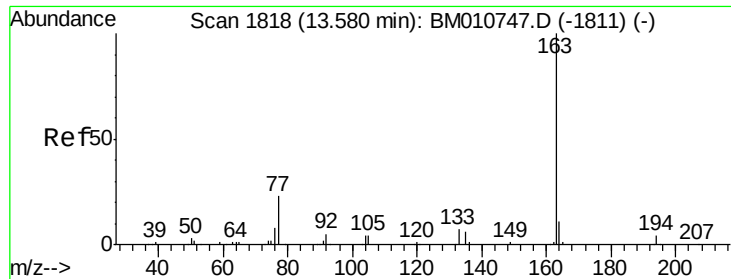

#44

Dimethylphthalate

Concen: 4.999 ng/ul

RT: 13.57 min Scan# 1817

Delta R.T. -0.01 min

Lab File: BM010759.D


Acq: 26 Jun 2017 23:27

Instrument :

BNA_M

ClientSampleId :

C0AE1

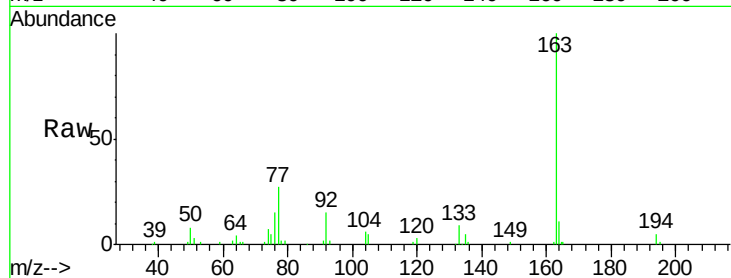


Tgt Ion:163 Resp: 96395

Ion Ratio Lower Upper

163 100

194 4.7 3.5 5.3

164 11.3 8.2 12.4

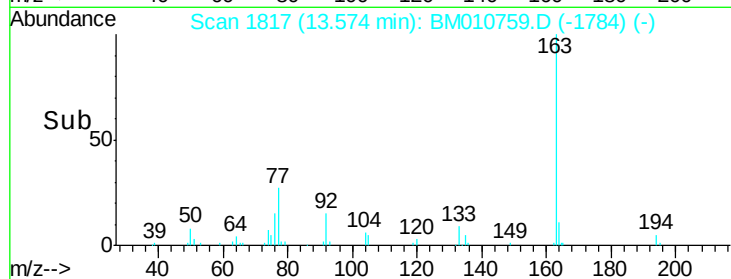

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

