


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062620\
Data File : BM026601.D
Acq On : 26 Jun 2020 22:30
Operator : JU/CG
Sample : L3062-10
Misc :
ALS Vial : 21 Sample Multiplier: 1




Quant Time: Jun 26 23:43:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 26 22:52:41 2020
Response via : Initial Calibration

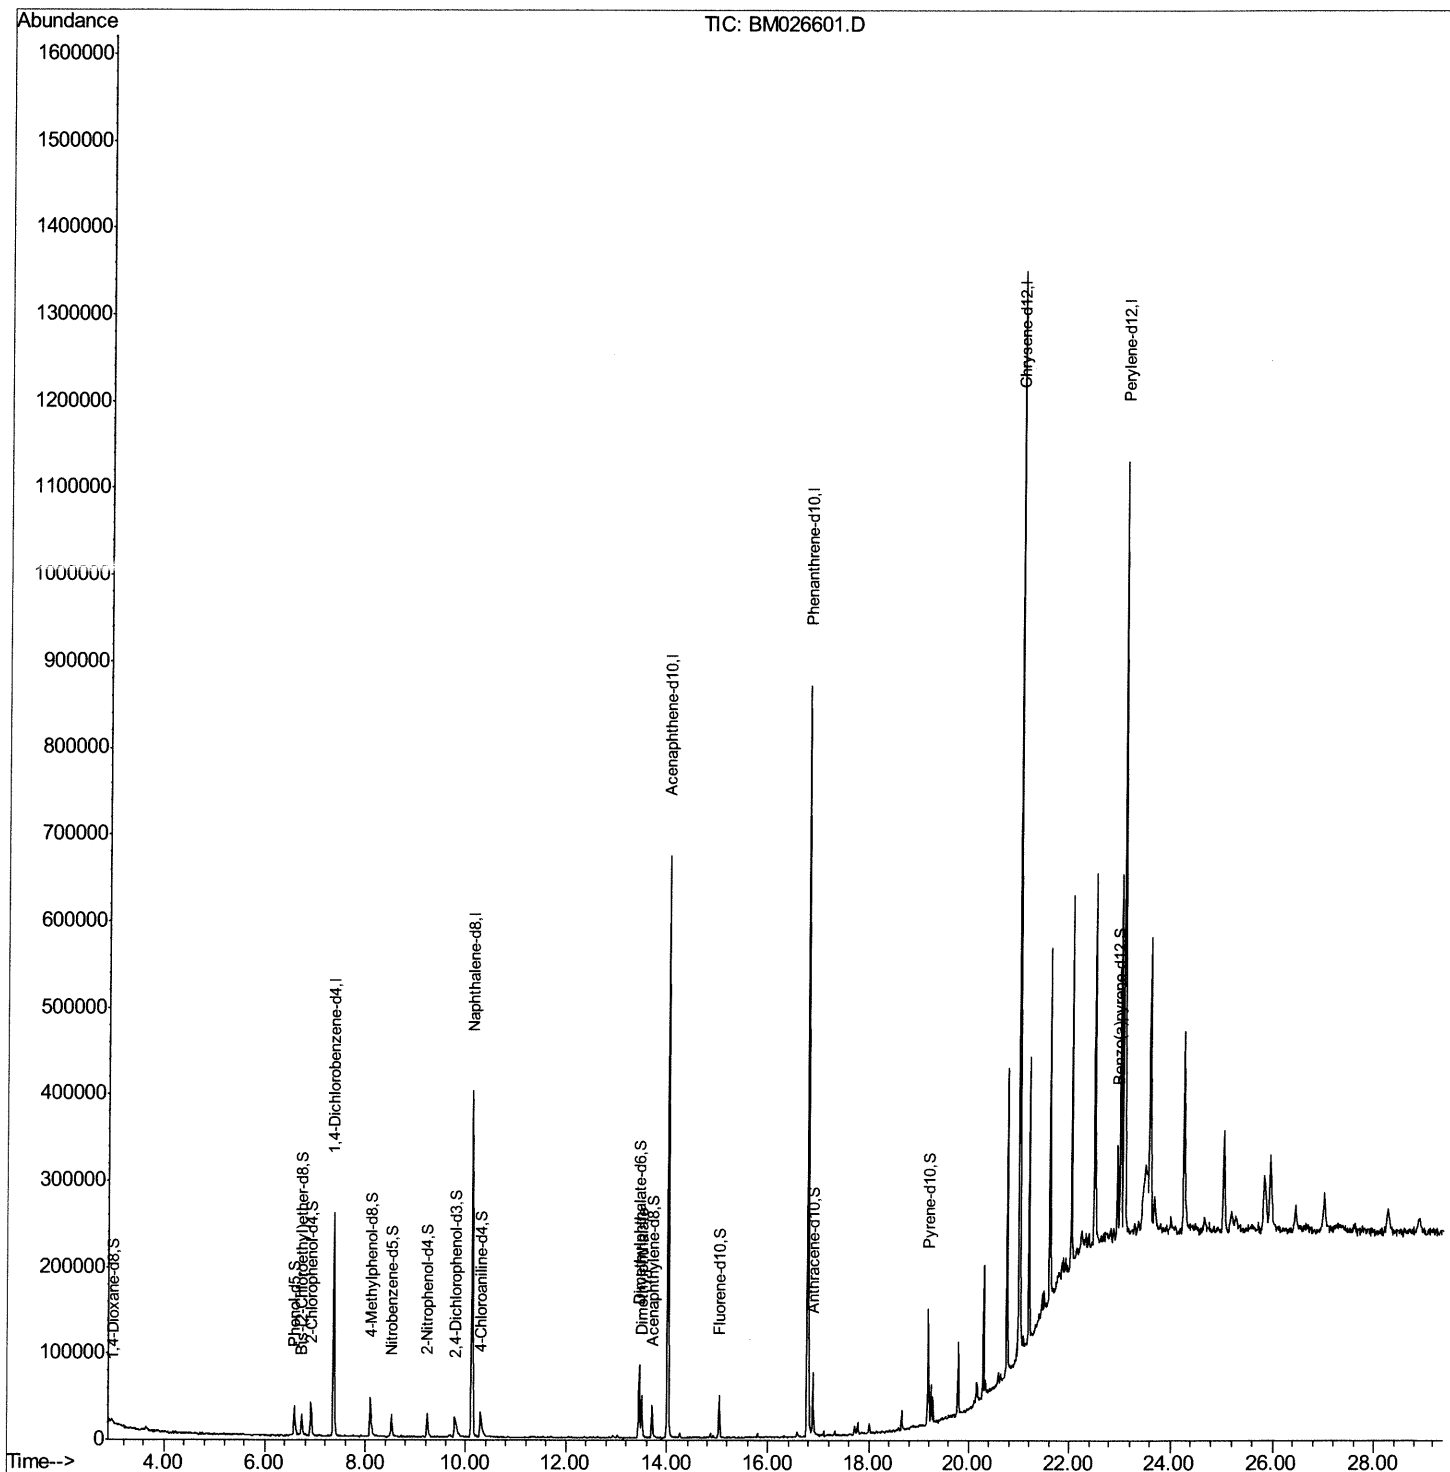

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062620\
 Data File : BM026601.D
 Acq On : 26 Jun 2020 22:30
 Operator : JU/CG
 Sample : L3062-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 26 23:42:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 26 22:52:41 2020
 Response via : Initial Calibration

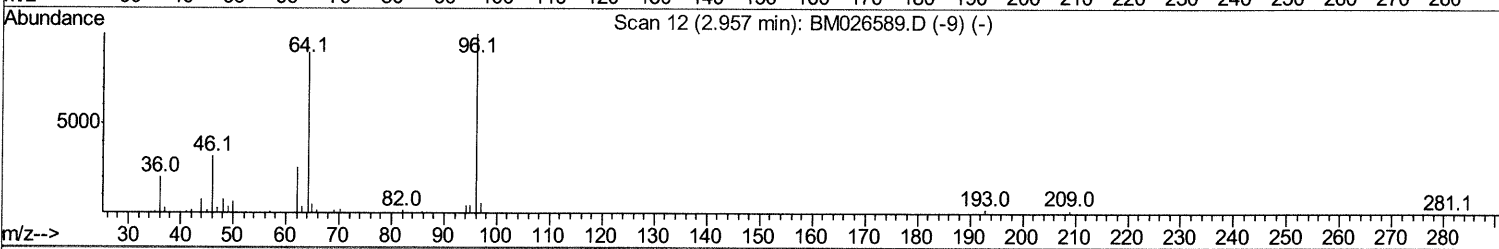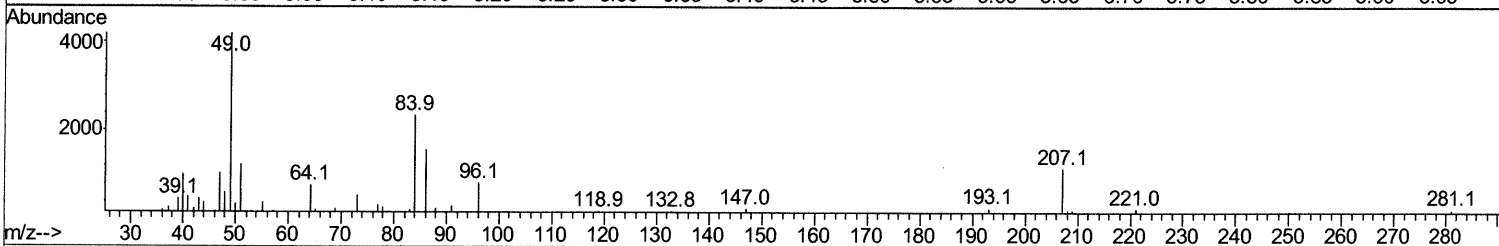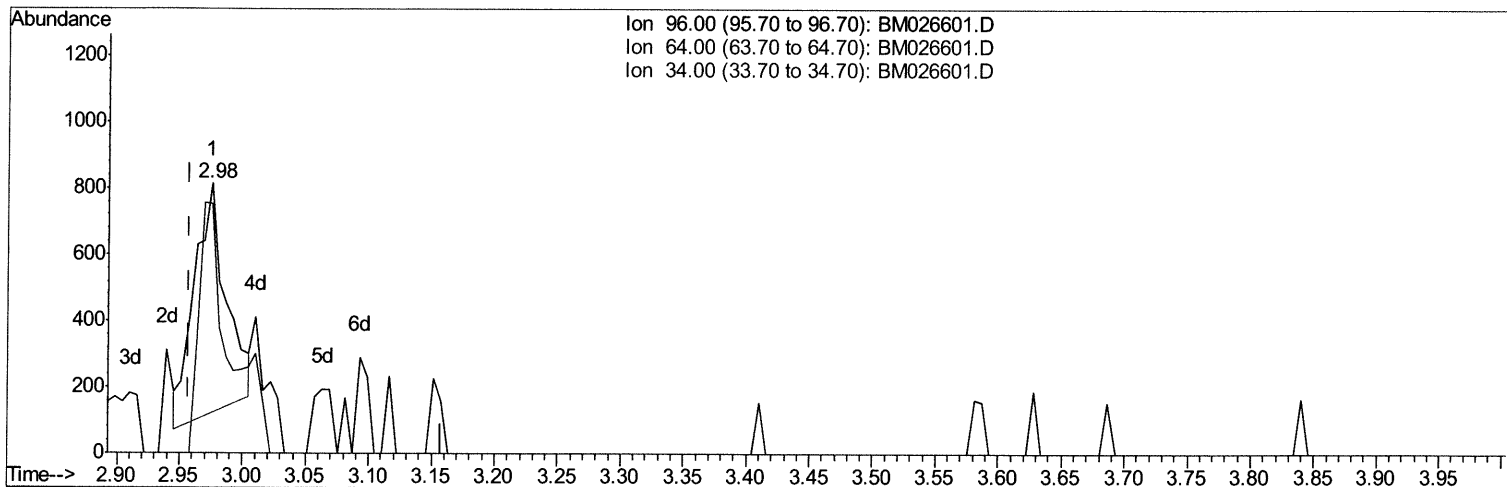

TIC: BM026601.D

(3) 1,4-Dioxane-d8 (S)

2.975min (+0.017) 0.66ng/uL




response 1234

Ion	Exp%	Act%
96.00	100	100
64.00	84.50	92.38
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062620\
 Data File : BM026601.D
 Acq On : 26 Jun 2020 22:30
 Operator : JU/CG
 Sample : L3062-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 26 23:42:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 26 22:52:41 2020
 Response via : Initial Calibration

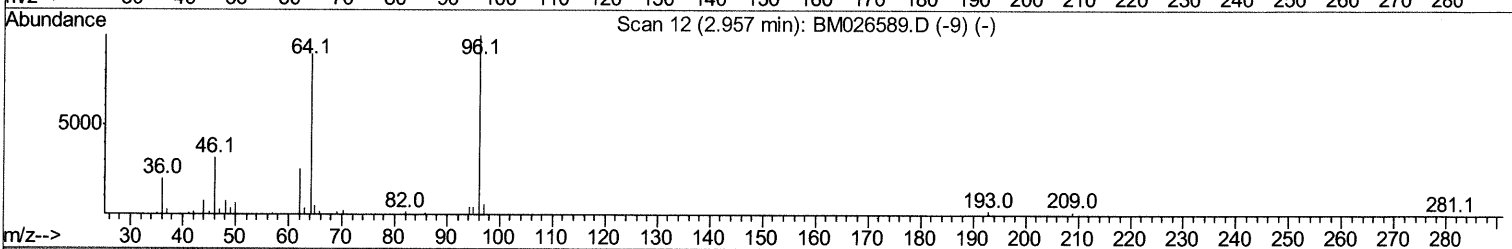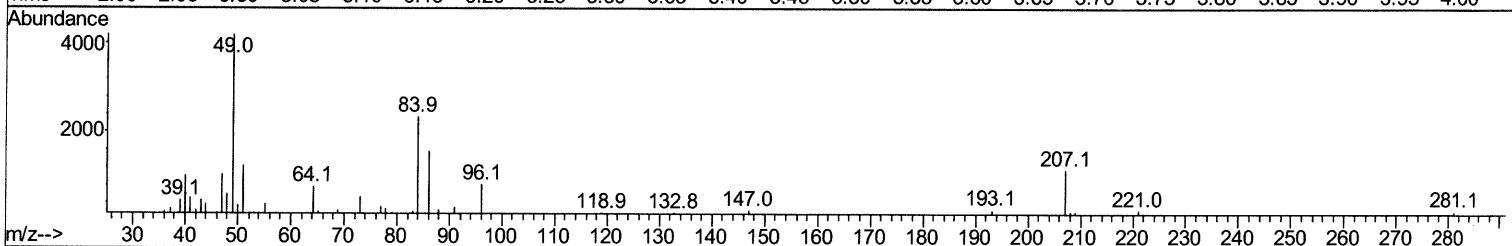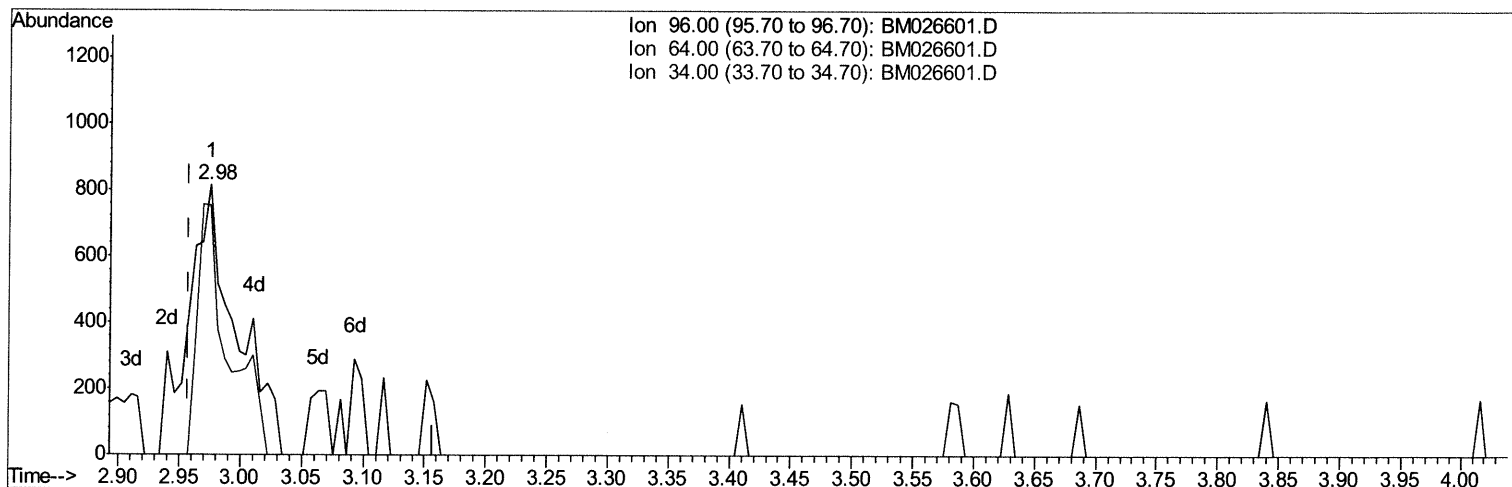

TIC: BM026601.D

(3) 1,4-Dioxane-d8 (S)

2.975min (+0.017) 1.16ng/uL m 06/30/20 JU




response 2180

Ion	Exp%	Act%
96.00	100	100
64.00	84.50	92.38
34.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062620\
 Data File : BM026601.D
 Acq On : 26 Jun 2020 22:30
 Operator : JU/CG
 Sample : L3062-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 26 23:42:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 26 22:52:41 2020
 Response via : Initial Calibration

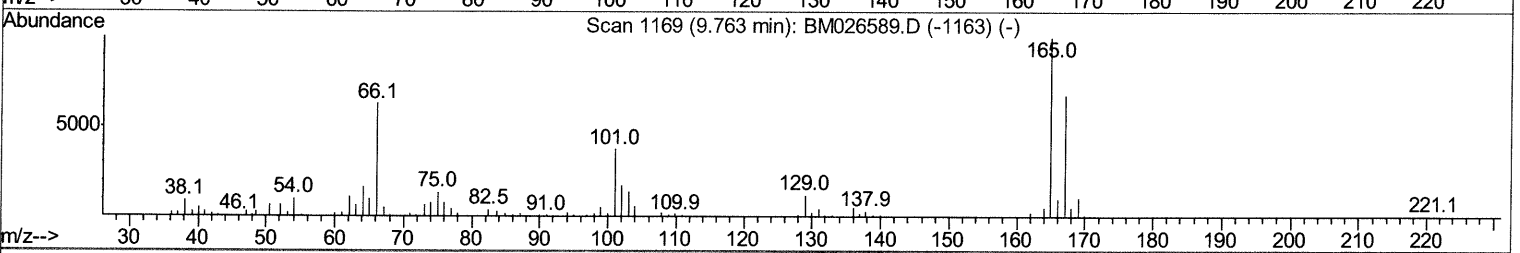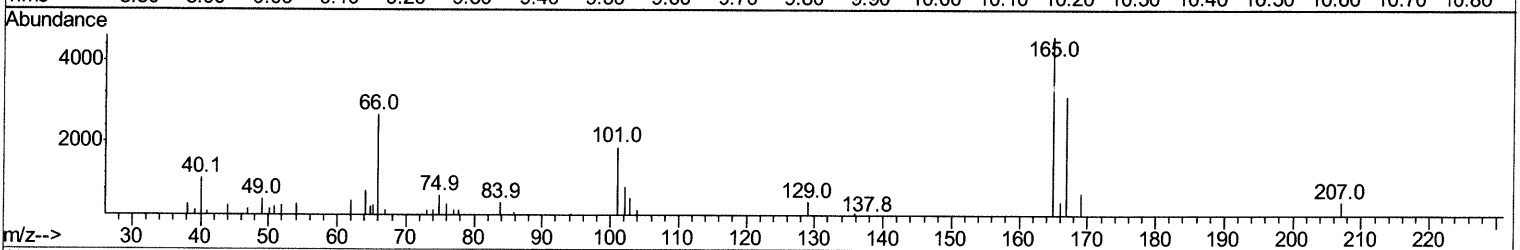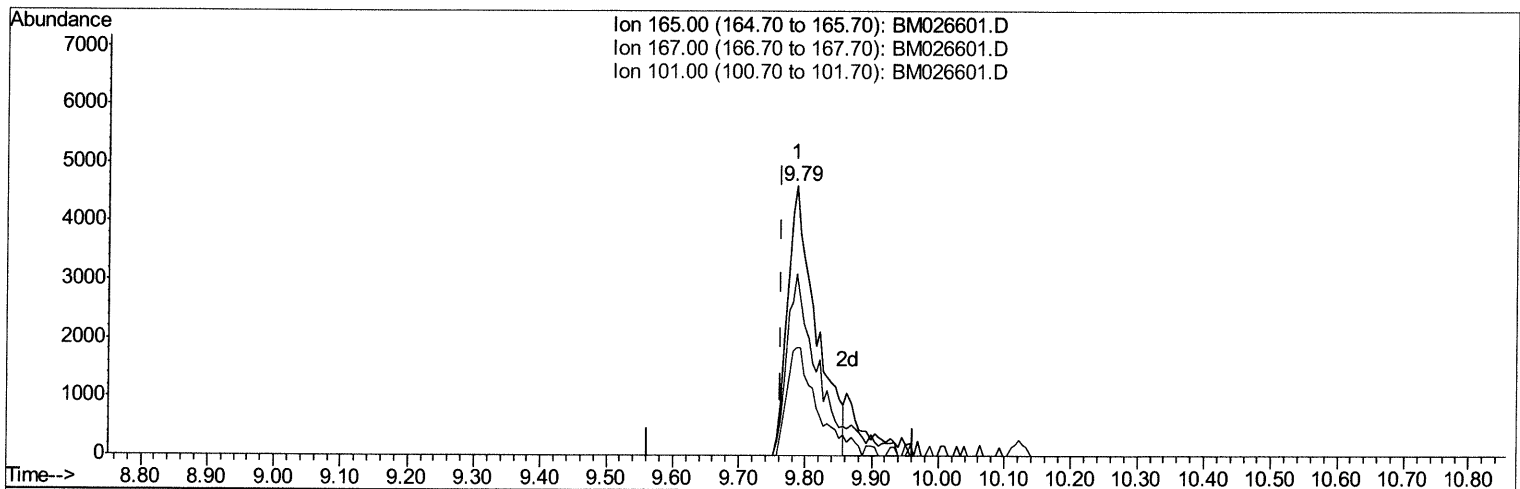

TIC: BM026601.D

(26) 2,4-Dichlorophenol-d3 (S)

9.786min (+0.023) 2.58ng/ul




response 13710

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	67.35
101.00	35.50	39.95
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062620\
Data File : BM026601.D
Acq On : 26 Jun 2020 22:30
Operator : JU/CG
Sample : L3062-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 26 23:42:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 26 22:52:41 2020
Response via : Initial Calibration

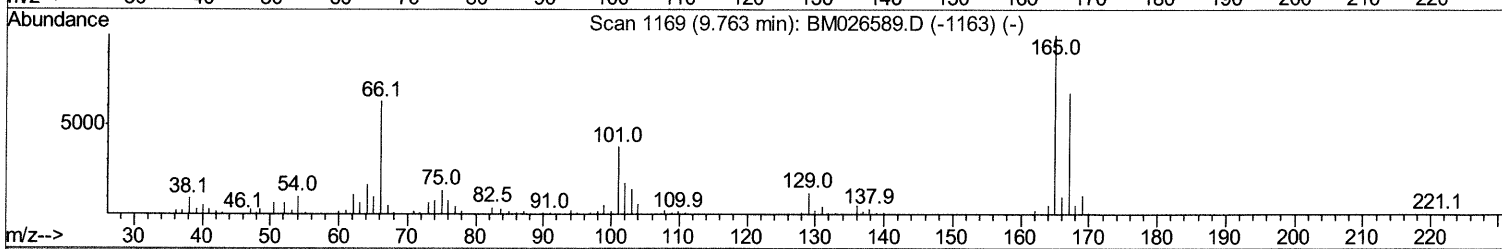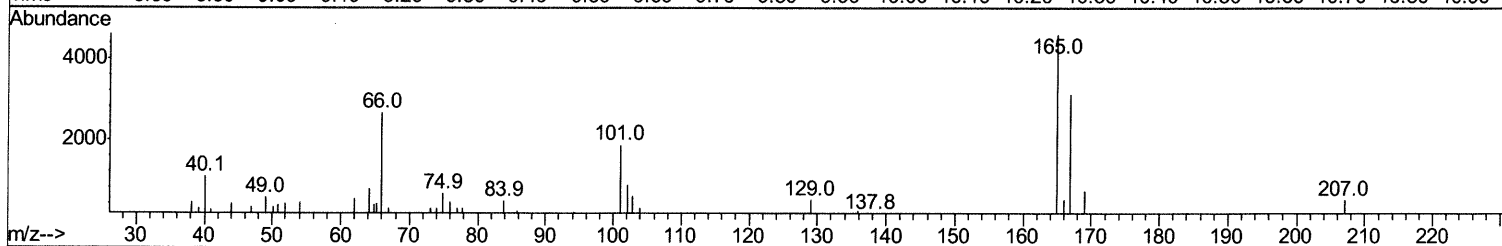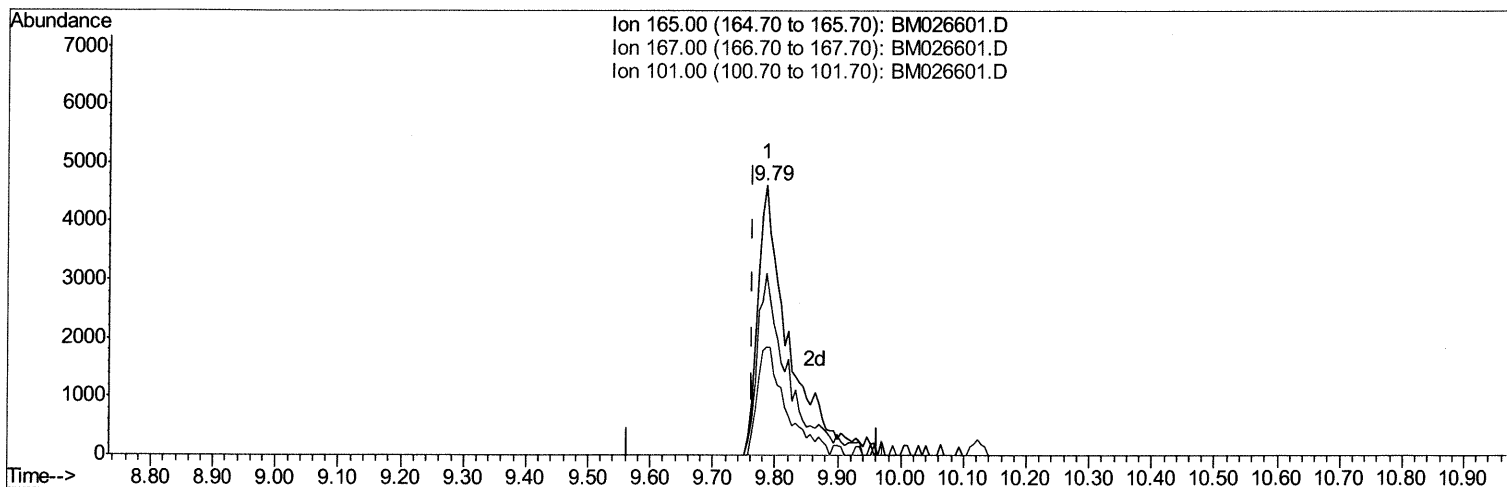

TIC: BM026601.D

(26) 2,4-Dichlorophenol-d3 (S)

9.786min (+0.023) 3.05ng/ul m 06/30/2024




response 16163

Ion	Exp%	Act%
165.00	100	100
167.00	63.60	67.35
101.00	35.50	39.95
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062620\
 Data File : BM026601.D
 Acq On : 26 Jun 2020 22:30
 Operator : JU/CG
 Sample : L3062-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 26 23:42:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 26 22:52:41 2020
 Response via : Initial Calibration

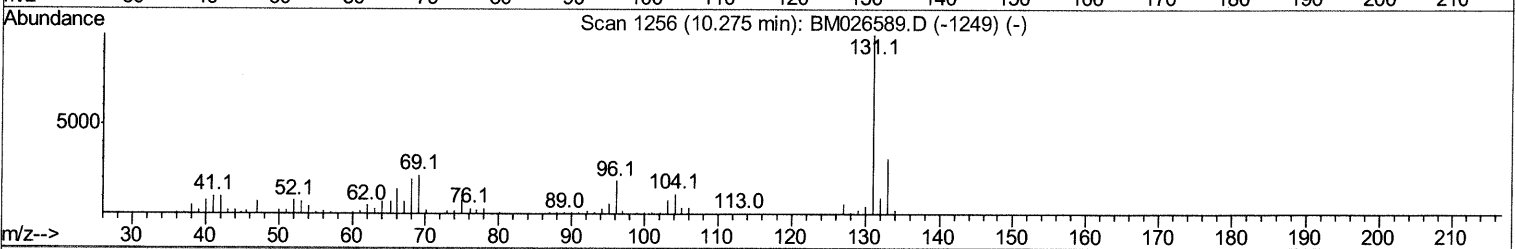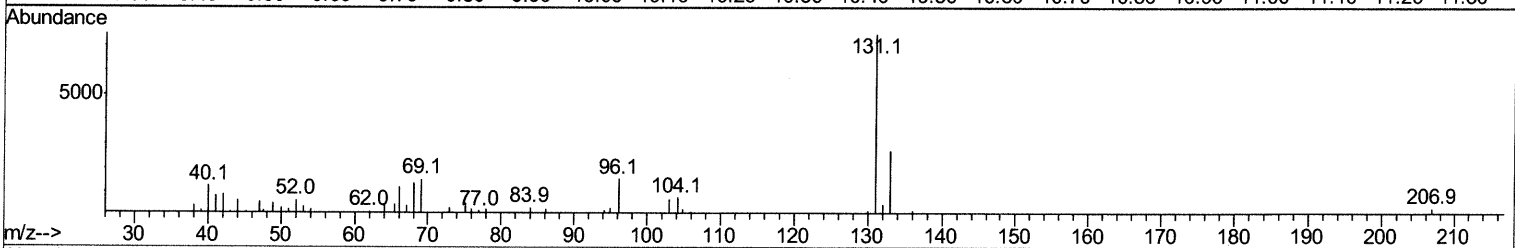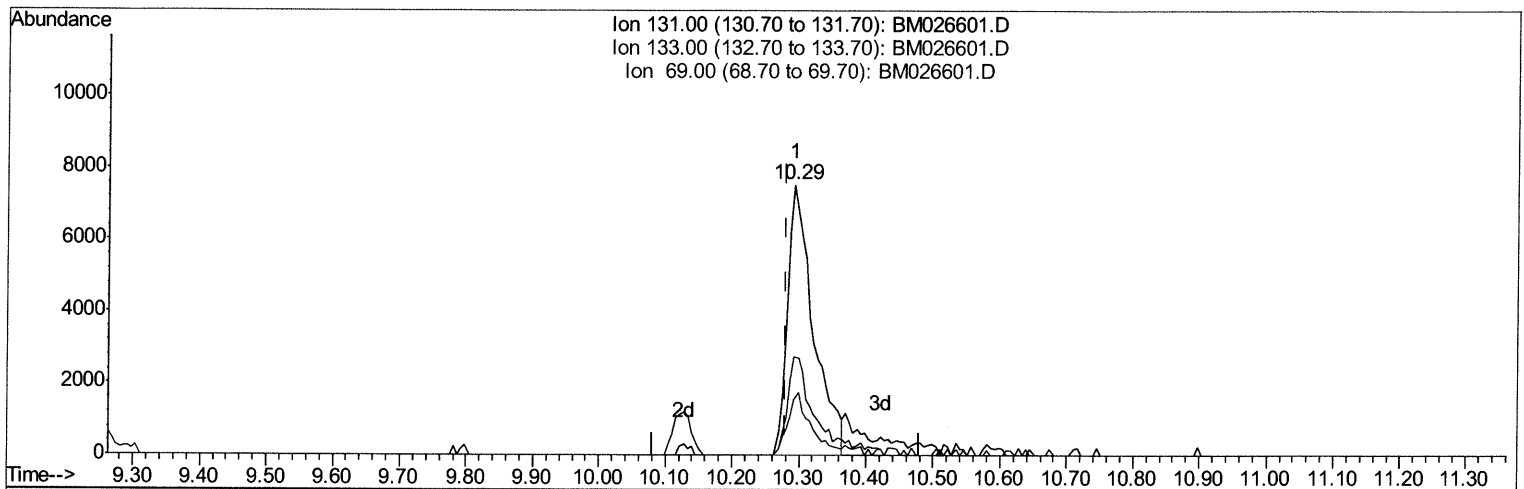

TIC: BM026601.D

(29) 4-Chloroaniline-d4 (S)

10.292min (+0.012) 3.64ng/ul




response 20133

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	36.46
69.00	18.60	20.31
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062620\
Data File : BM026601.D
Acq On : 26 Jun 2020 22:30
Operator : JU/CG
Sample : L3062-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 26 23:42:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 26 22:52:41 2020
Response via : Initial Calibration

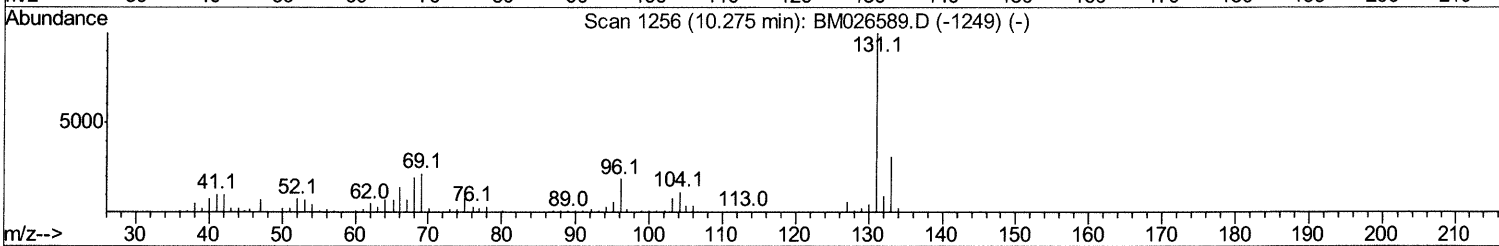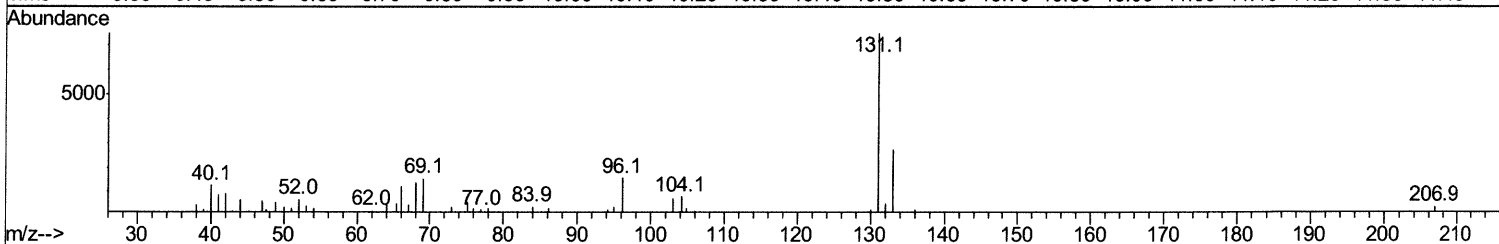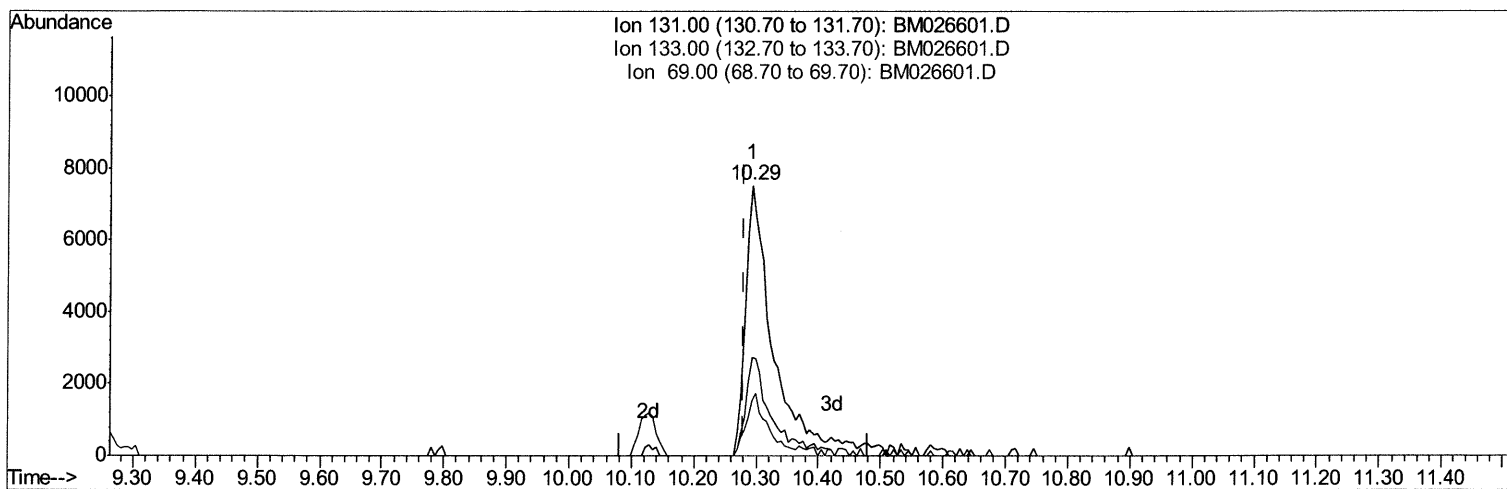

TIC: BM026601.D

(29) 4-Chloroaniline-d4 (S)

10.292min (+0.012) 4.34ng/ul m 06/30/20 JU

response 23985

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	36.46
69.00	18.60	20.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM062620\
 Data File : BM026601.D
 Acq On : 26 Jun 2020 22:30
 Operator : JU/CG
 Sample : L3062-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Quant Time: Jun 26 23:43:32 2020

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Fri Jun 26 22:52:41 2020

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	65748	20.00	ng/ul	0.00
18) Naphthalene-d8	10.12	136	294694	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.02	164	202616	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.78	188	470150	20.00	ng/ul	0.00
78) Chrysene-d12	20.99	240	565711	20.00	ng/ul	-0.01
86) Perylene-d12	23.07	264	566795	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.98	96	2180m>	1.16	ng/uL>	0.02	06/30/2020
5) Phenol-d5	6.58	99	21692	3.58	ng/ul	0.00	
7) Bis-(2-Chloroethyl)ether-d	6.73	67	12594	3.29	ng/ul	0.00	
9) 2-Chlorophenol-d4	6.92	132	17396	3.52	ng/ul	0.00	
13) 4-Methylphenol-d8	8.10	113	18701	3.92	ng/ul	0.00	
19) Nitrobenzene-d5	8.52	128	5325	2.03	ng/ul	0.00	
22) 2-Nitrophenol-d4	9.23	143	8043	2.79	ng/ul	0.00	
26) 2,4-Dichlorophenol-d3	9.79	165	16163m}	3.05	ng/ul}	0.02	06/30/2020
29) 4-Chloroaniline-d4	10.29	131	23985m}	4.34	ng/ul}	0.01	
44) Dimethylphthalate-d6	13.46	166	58515	3.43	ng/ul	0.00	
47) Acenaphthylene-d8	13.71	160	25934	1.27	ng/ul	0.00	
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul		
58) Fluorene-d10	15.03	176	20890	1.43	ng/ul	0.00	
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul		
71) Anthracene-d10	16.89	188	44936	1.88	ng/ul	0.00	
79) Pyrene-d10	19.19	212	68309	2.20	ng/ul	0.00	
90) Benzo(a)pyrene-d12	22.94	264	69261	2.21	ng/ul	-0.01	

Target Compounds

					Ovalue	
45) Dimethylphthalate	13.50	163	30217	1.708	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed