

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062620\
 Data File : BM026584.D
 Acq On : 26 Jun 2020 12:12
 Operator : JU/CG
 Sample : L3062-21
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET152

Manual Integrations
 APPROVED

mohammad
 6/29/2020 3:17:26 PM

Quant Time: Jun 26 12:59:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 26 11:31:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	55976	20.00	ng/ul	0.00
18) Naphthalene-d8	10.13	136	251458	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	171006	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.78	188	386842	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	449449	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	442981	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.96	96	4767	2.99	ng/uL	0.00
5) Phenol-d5	6.57	99	108358	21.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.72	67	101013	30.96	ng/ul	0.00
9) 2-Chlorophenol-d4	6.91	132	102574	24.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.09	113	118832	29.28	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	53481	23.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.23	143	47078	19.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.77	165	114190	25.23	ng/ul	0.00
29) 4-Chloroaniline-d4	10.28	131	168342	35.67	ng/ul	0.00
44) Dimethylphthalate-d6	13.46	166	456701	31.76	ng/ul	0.00
47) Acenaphthylene-d8	13.71	160	416603	24.15	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	12301m	5.16	ng/ul	0.03
58) Fluorene-d10	15.03	176	273869	22.20	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.18	200	12737	5.03	ng/ul	0.00
71) Anthracene-d10	16.88	188	398967	20.26	ng/ul	0.00
79) Pyrene-d10	19.19	212	448610	18.20	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.95	264	422981	17.27	ng/ul	0.00

Target Compounds					Ovalue	
45) Dimethylphthalate	13.50	163	295336	19.779	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062620\
Data File : BM026584.D
Acq On : 26 Jun 2020 12:12
Operator : JU/CG
Sample : L3062-21
Misc :
ALS Vial : 5 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
ET152

Manual Integrations
APPROVED

mohammad
6/29/2020 3:17:26 PM

Quant Time: Jun 26 12:59:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 26 11:31:11 2020
Response via : Initial Calibration

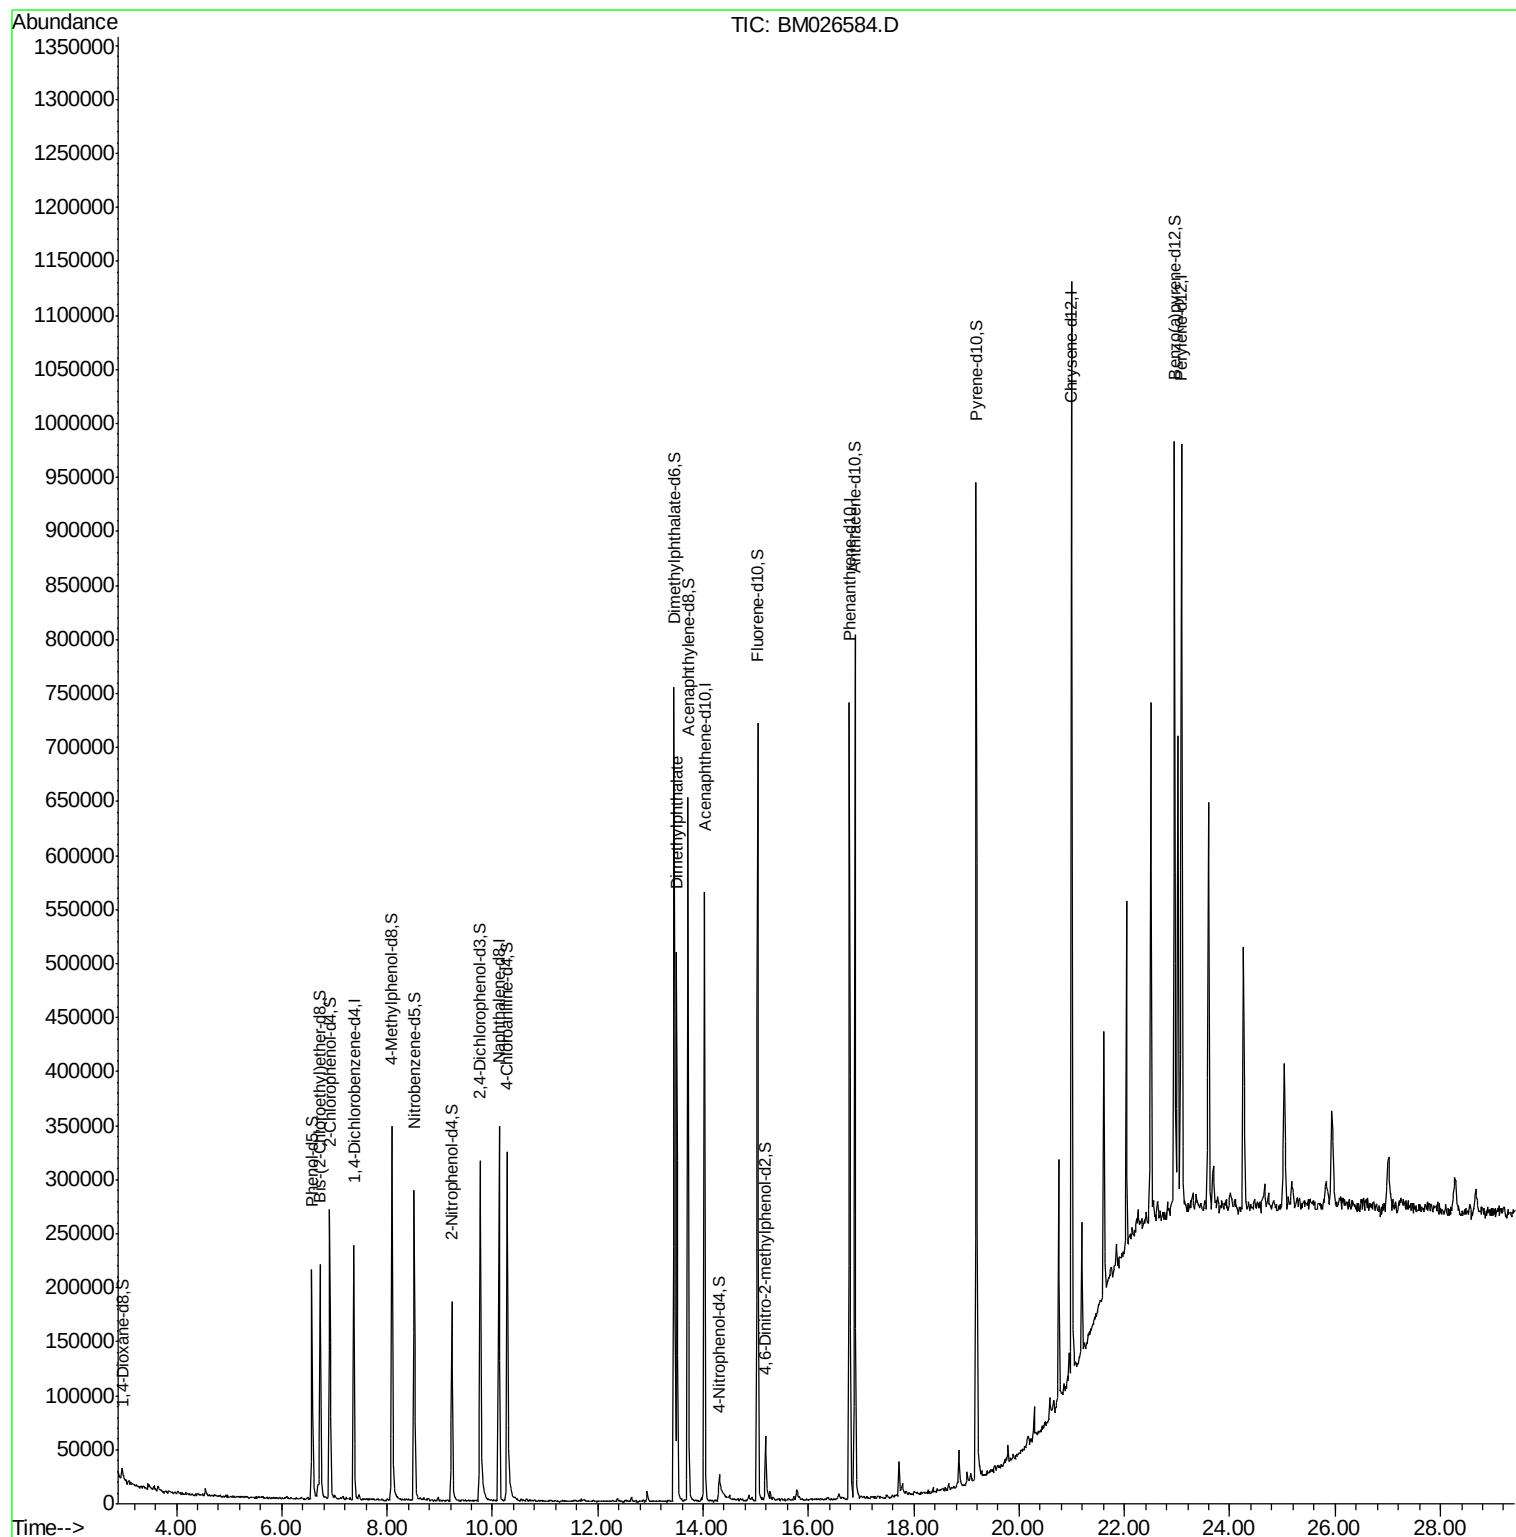

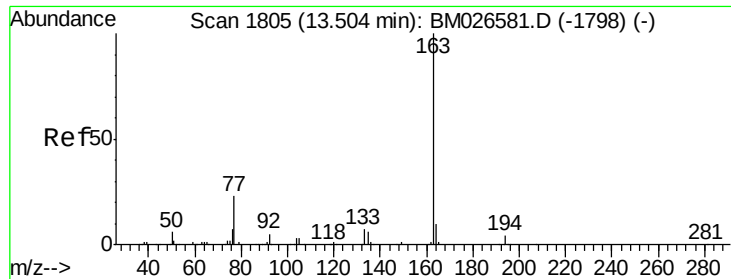

#45
 Dimethylphthalate
 Concen: 19.779 ng/ul
 RT: 13.50 min Scan# 1805
 Delta R.T. -0.00 min
 Lab File: BM026584.D
 Acq: 26 Jun 2020 12:12

Instrument :
 BNA_M
 ClientSampleId :
 ET152

Tot Ion:	163	Resp:	295336
Ion Ratio	Lower	Upper	
163	100		
194	4.6	3.4	5.2
164	10.1	7.8	11.6

Manual Integrations
 APPROVED

mohammad
 6/29/2020 3:17:26 PM

