

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062620\
 Data File : BM026587.D
 Acq On : 26 Jun 2020 14:01
 Operator : JU/CG
 Sample : L3118-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F57

Manual Integrations
 APPROVED

mohammad
 6/29/2020 3:17:33 PM

Quant Time: Jun 26 15:36:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 26 11:31:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	79413	20.00	ng/ul	0.00
18) Naphthalene-d8	10.12	136	359800	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	247119	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.78	188	560530	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	627501	20.00	ng/ul	0.00
86) Perylene-d12	23.09	264	586146	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.96	96	11723	5.18	ng/uL	0.00
5) Phenol-d5	6.57	99	44928	6.14	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.72	67	148828	32.16	ng/ul	0.00
9) 2-Chlorophenol-d4	6.91	132	130820	21.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.09	113	91376	15.87	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	84649m	26.48	ng/ul	0.00
22) 2-Nitrophenol-d4	9.23	143	95339	27.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.77	165	158735	24.51	ng/ul	0.00
29) 4-Chloroaniline-d4	10.30	131	14559m	2.16	ng/ul	0.02
44) Dimethylphthalate-d6	13.46	166	649949	31.28	ng/ul	0.00
47) Acenaphthylene-d8	13.71	160	741181	29.74	ng/ul	0.00
52) 4-Nitrophenol-d4	14.30	143	13123m	3.81	ng/ul	0.03
58) Fluorene-d10	15.03	176	572753	32.12	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.18	200	93789	25.57	ng/ul	0.00
71) Anthracene-d10	16.88	188	988230	34.63	ng/ul	0.00
79) Pyrene-d10	19.19	212	1174758	34.14	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.96	264	1077292	33.24	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.50	163	65892	3.054	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062620\
Data File : BM026587.D
Acq On : 26 Jun 2020 14:01
Operator : JU/CG
Sample : L3118-01
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0F57

Manual Integrations
APPROVED

mohammad
6/29/2020 3:17:33 PM

Quant Time: Jun 26 15:36:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 26 11:31:11 2020
Response via : Initial Calibration

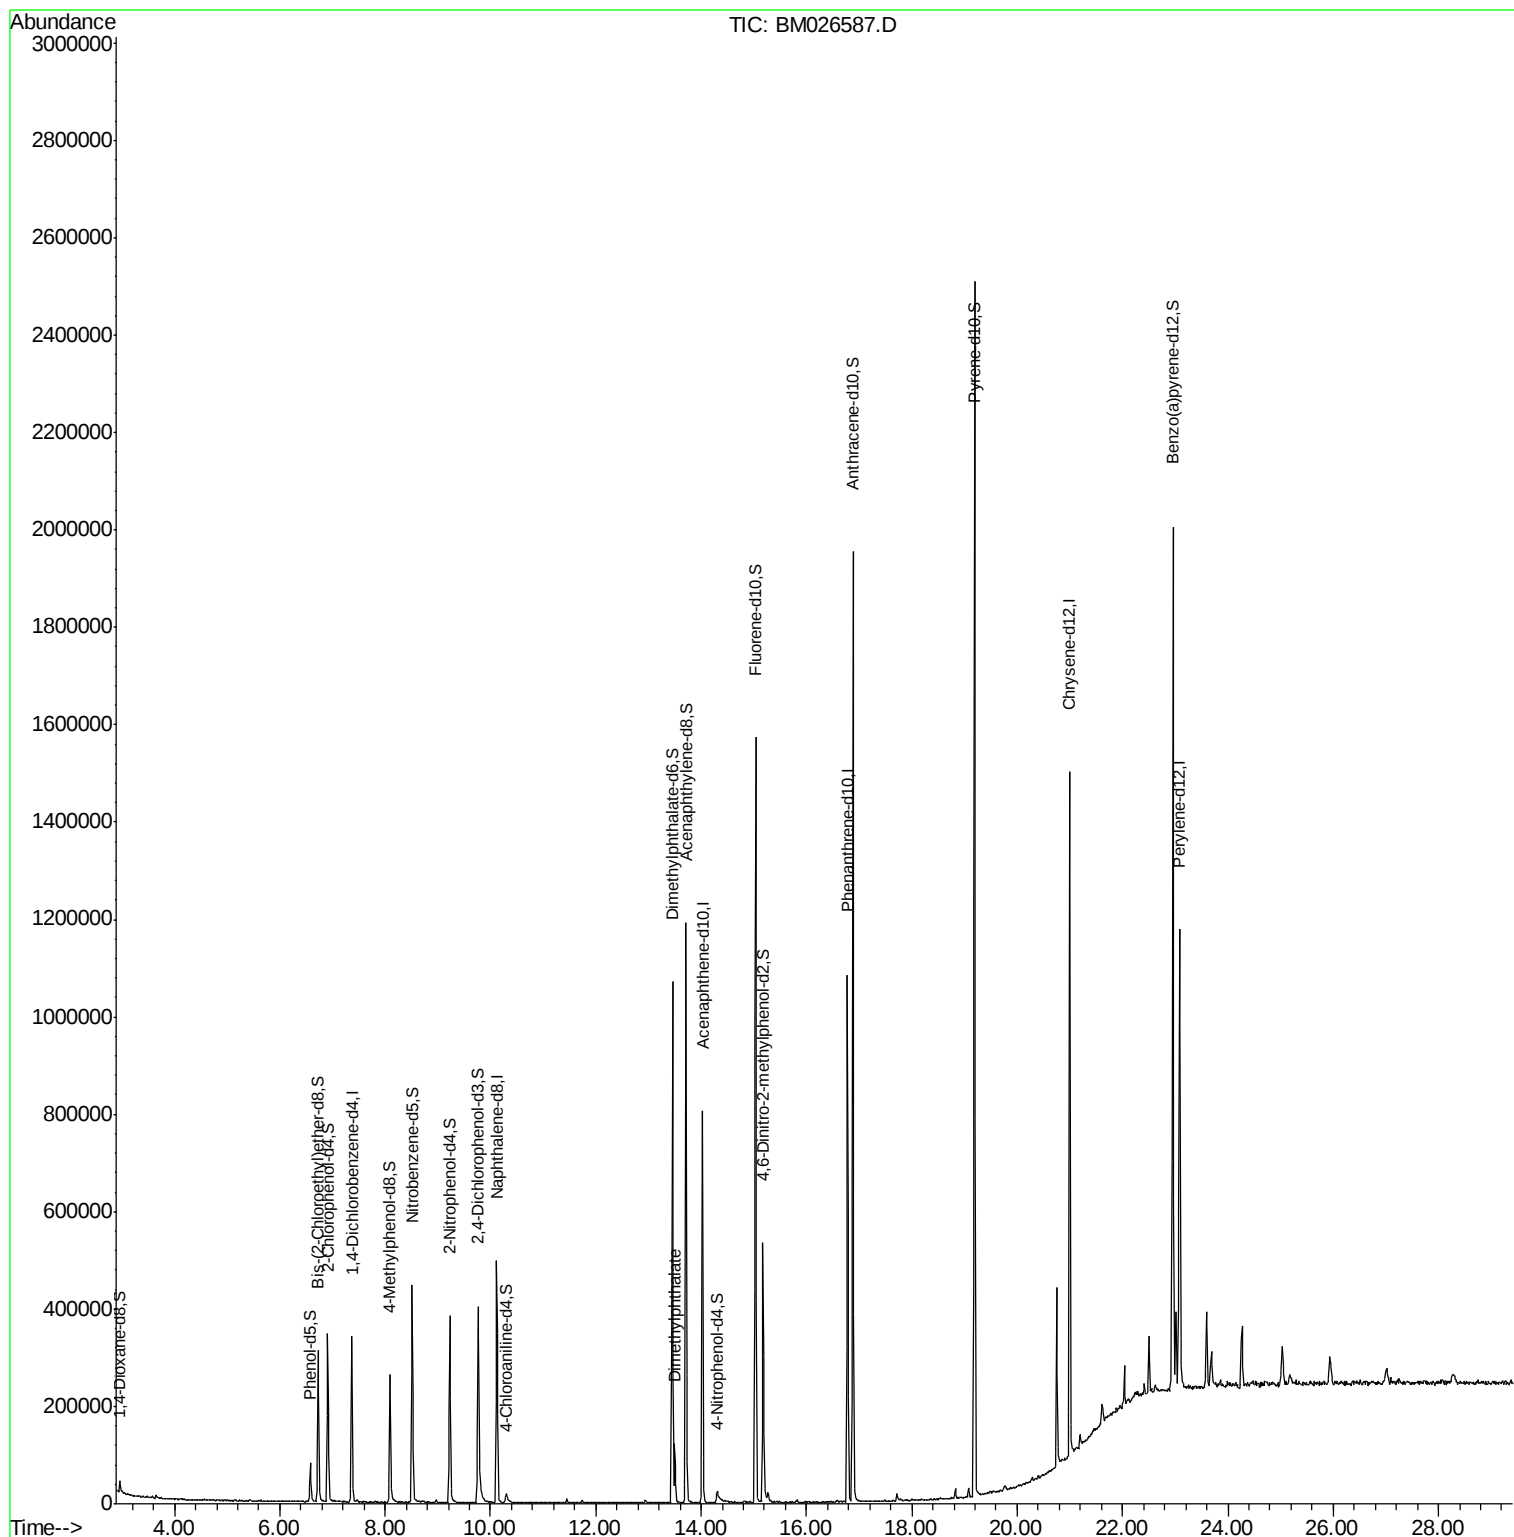

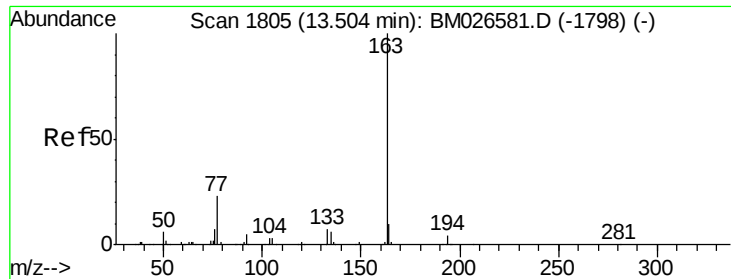

#45
 Dimethylphthalate
 Concen: 3.054 ng/ul
 RT: 13.50 min Scan# 1805
 Delta R.T. -0.00 min
 Lab File: BM026587.D
 Acq: 26 Jun 2020 14:01

Instrument :
 BNA_M
 ClientSampleId :
 C0F57

Tot Ion	Ratio	Resp	Lower	Upper
163	100	65892		
194	4.8		3.4	5.2
164	9.6		7.8	11.6

Manual Integrations
 APPROVED

mohammad
 6/29/2020 3:17:33 PM

