

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062620\
 Data File : BM026593.D
 Acq On : 26 Jun 2020 17:39
 Operator : JU/CG
 Sample : L3064-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET156

Manual Integrations
 APPROVED

mohammad
 6/29/2020 3:17:42 PM

Quant Time: Jun 26 18:20:00 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 26 11:31:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	51530	20.00	ng/ul	0.00
18) Naphthalene-d8	10.12	136	235582	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.03	164	162612	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.78	188	390052	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	456592	20.00	ng/ul	0.00
86) Perylene-d12	23.08	264	445800	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.96	96	5788	3.94	ng/uL	0.00
5) Phenol-d5	6.57	99	91425	19.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	67913	22.61	ng/ul	0.00
9) 2-Chlorophenol-d4	6.91	132	72295	18.68	ng/ul	0.00
13) 4-Methylphenol-d8	8.09	113	78029	20.88	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	38024m	18.17	ng/ul	0.00
22) 2-Nitrophenol-d4	9.23	143	39842	17.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.77	165	74484	17.57	ng/ul	0.00
29) 4-Chloroaniline-d4	10.28	131	102298	23.14	ng/ul	0.00
44) Dimethylphthalate-d6	13.45	166	293822	21.49	ng/ul	0.00
47) Acenaphthylene-d8	13.71	160	309371	18.86	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	18359	8.10	ng/ul	0.02
58) Fluorene-d10	15.03	176	230254	19.62	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.18	200	20921	8.20	ng/ul	0.00
71) Anthracene-d10	16.88	188	378013	19.04	ng/ul	0.00
79) Pyrene-d10	19.19	212	451535	18.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.95	264	456855	18.53	ng/ul	0.00

Target Compounds					Ovalue	
45) Dimethylphthalate	13.50	163	120664	8.498	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062620\
Data File : BM026593.D
Acq On : 26 Jun 2020 17:39
Operator : JU/CG
Sample : L3064-03
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
ET156

Quant Time: Jun 26 18:20:00 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 26 11:31:11 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/29/2020 3:17:42 PM

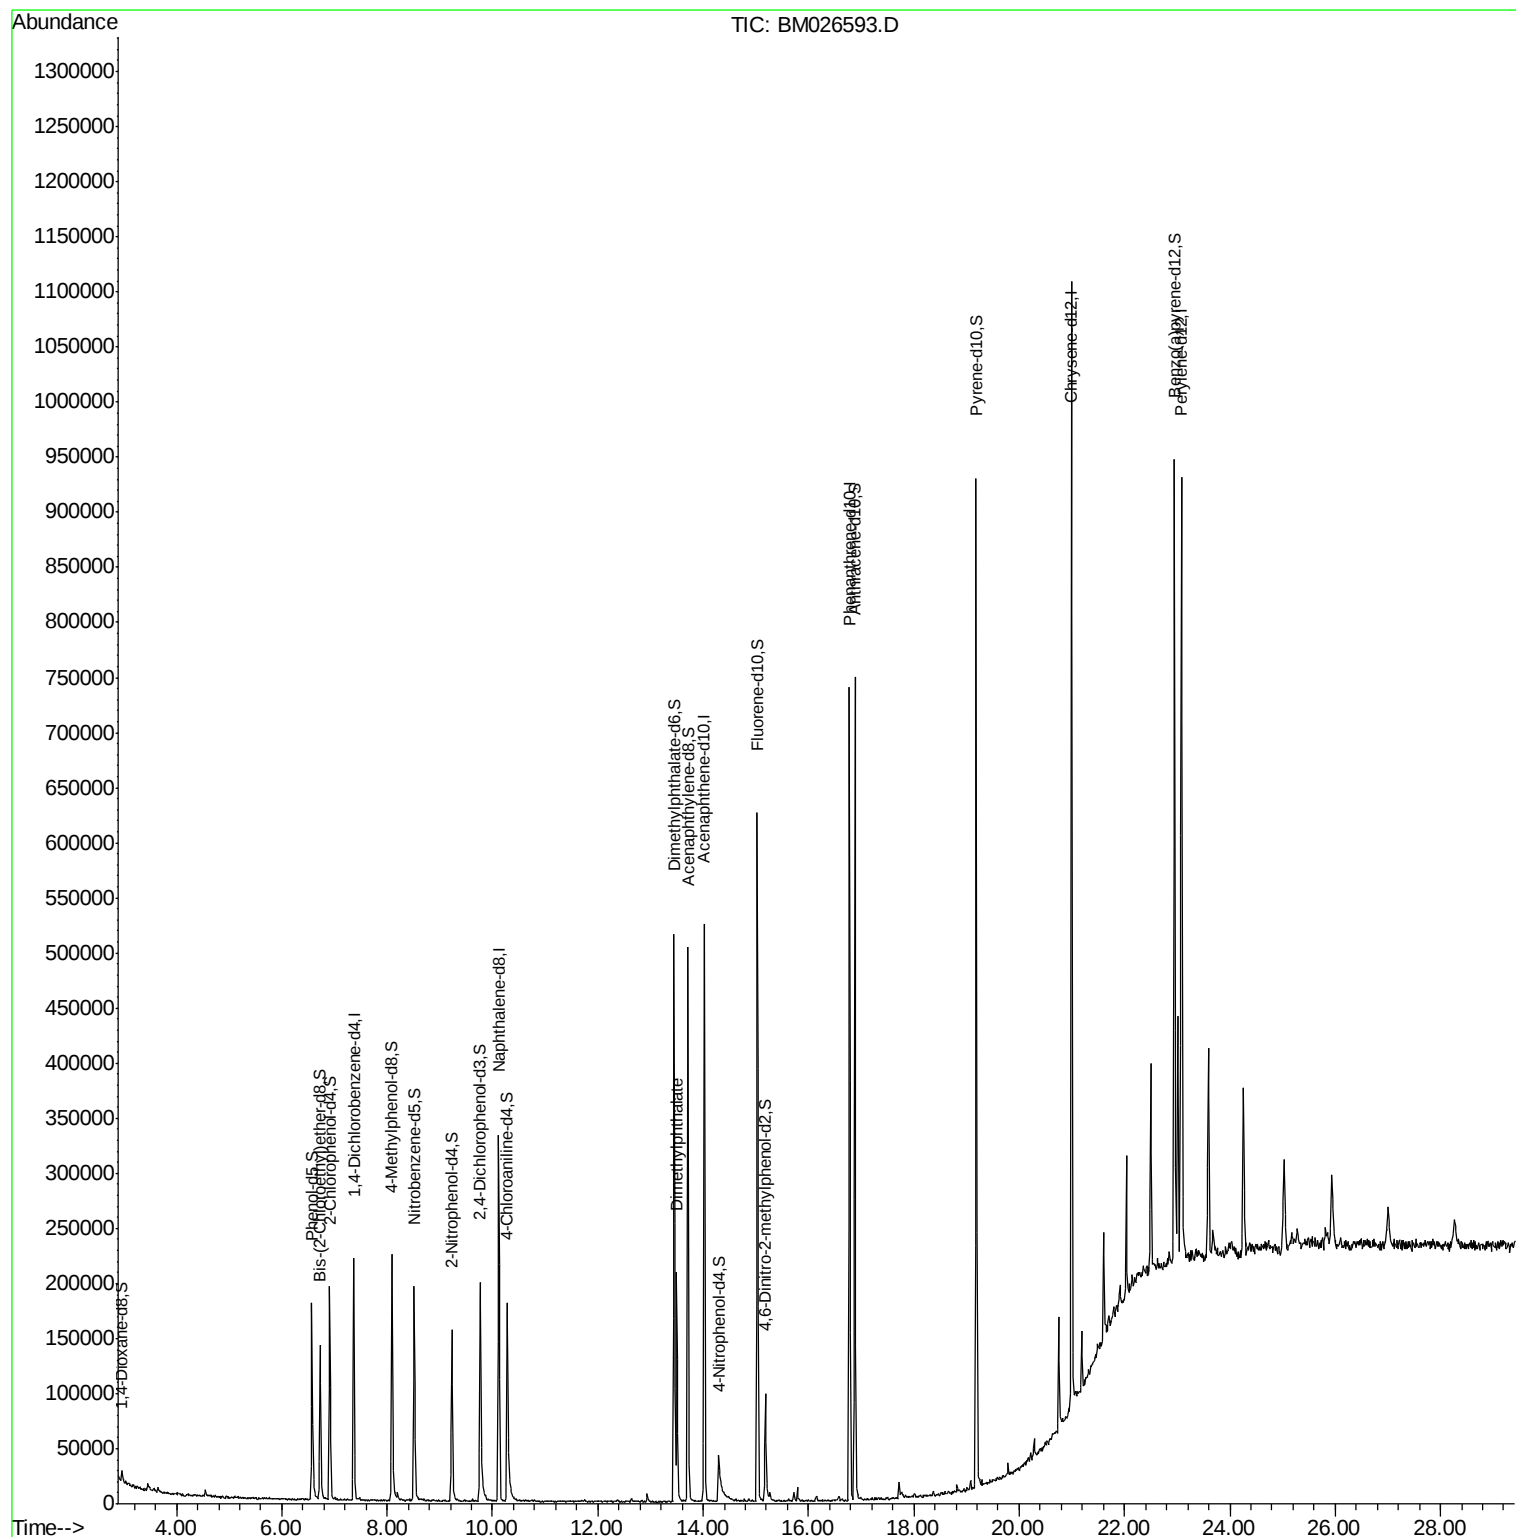

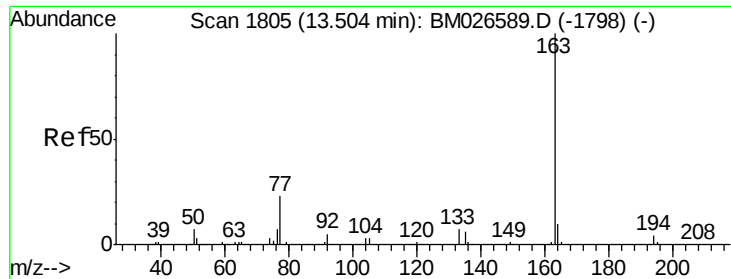

#45
 Dimethylphthalate
 Concen: 8.498 ng/ul
 RT: 13.50 min Scan# 1805
 Delta R.T. -0.00 min
 Lab File: BM026593.D
 Acq: 26 Jun 2020 17:39

Instrument :
 BNA_M
 ClientSampleId :
 ET156

Tot Ion:	163	Resp:	120664
Ion Ratio	Lower	Upper	
163	100		
194	4.9	3.4	5.2
164	9.3	7.8	11.6

Manual Integrations
 APPROVED

mohammad
 6/29/2020 3:17:42 PM

