

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062620\
 Data File : BM026595.D
 Acq On : 26 Jun 2020 18:52
 Operator : JU/CG
 Sample : L3064-09
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET163

Manual Integrations
 APPROVED

mohammad
 6/29/2020 3:17:48 PM

Quant Time: Jun 26 22:54:52 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 26 11:31:11 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	61085	20.00	ng/ul	0.00
18) Naphthalene-d8	10.12	136	281076	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.02	164	192898	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.78	188	442600	20.00	ng/ul	0.00
78) Chrysene-d12	21.00	240	553199	20.00	ng/ul	0.00
86) Perylene-d12	23.08	264	564088	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.96	96	7048	4.05	ng/uL	0.00
5) Phenol-d5	6.58	99	128283	22.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.72	67	90978	25.56	ng/ul	0.00
9) 2-Chlorophenol-d4	6.91	132	100878	21.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.09	113	110199	24.88	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	49944	20.00	ng/ul	0.00
22) 2-Nitrophenol-d4	9.23	143	53023	19.30	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.77	165	104398	20.64	ng/ul	0.00
29) 4-Chloroaniline-d4	10.28	131	126284	23.94	ng/ul	0.00
44) Dimethylphthalate-d6	13.45	166	370576	22.85	ng/ul	0.00
47) Acenaphthylene-d8	13.71	160	415442	21.35	ng/ul	0.00
52) 4-Nitrophenol-d4	14.29	143	36259m	13.48	ng/ul	0.01
58) Fluorene-d10	15.03	176	305217	21.93	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.17	200	32842	11.34	ng/ul	0.00
71) Anthracene-d10	16.88	188	461075	20.46	ng/ul	0.00
79) Pyrene-d10	19.19	212	554102	18.26	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.95	264	563742	18.07	ng/ul	0.00

Target Compounds					Ovalue	
45) Dimethylphthalate	13.50	163	279646	16.603	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062620\
Data File : BM026595.D
Acq On : 26 Jun 2020 18:52
Operator : JU/CG
Sample : L3064-09
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampled :
ET163

Quant Time: Jun 26 22:54:52 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 26 11:31:11 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
6/29/2020 3:17:48 PM

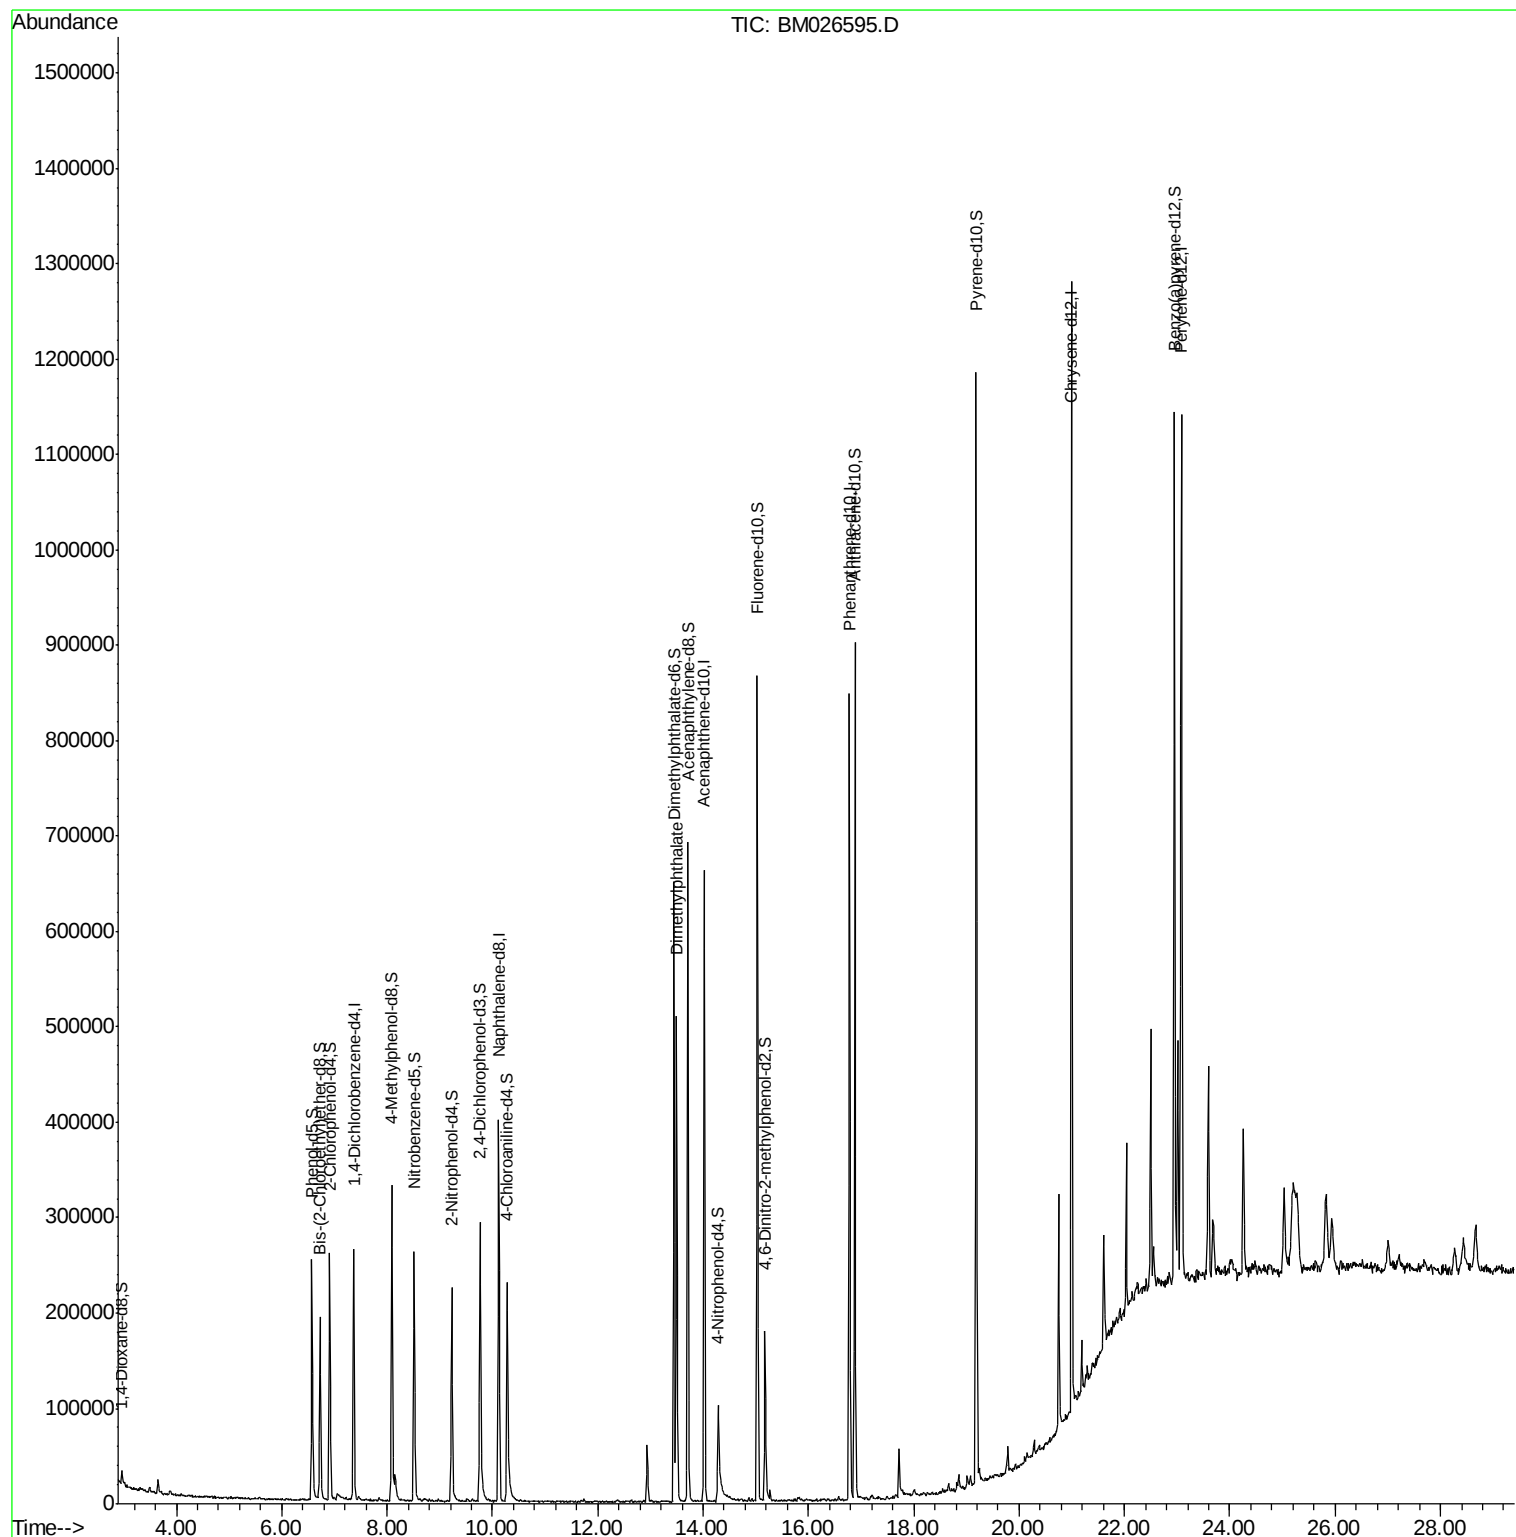

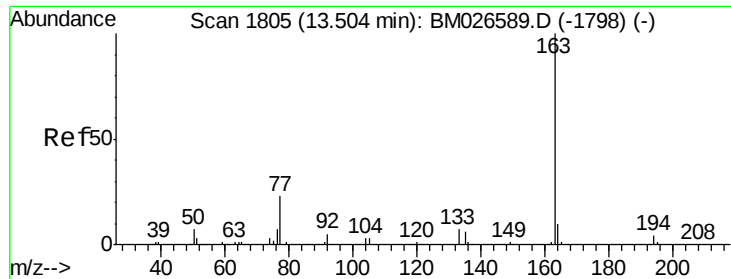

#45
 Dimethylphthalate
 Concen: 16.603 ng/ul
 RT: 13.50 min Scan# 1804
 Delta R.T. -0.01 min
 Lab File: BM026595.D
 Acq: 26 Jun 2020 18:52

Instrument :
 BNA_M
 ClientSampleId :
 ET163

Tot Ion:	163	Resp:	279646
Ion Ratio	Lower	Upper	
163	100		
194	4.4	3.4	5.2
164	10.0	7.8	11.6

Manual Integrations
 APPROVED

mohammad
 6/29/2020 3:17:48 PM

