

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062620\
 Data File : BM026601.D
 Acq On : 26 Jun 2020 22:30
 Operator : JU/CG
 Sample : L3062-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 ET143

Quant Time: Jun 26 23:43:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 26 22:52:41 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.37	152	65748	20.00	ng/ul	0.00
18) Naphthalene-d8	10.12	136	294694	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.02	164	202616	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.78	188	470150	20.00	ng/ul	0.00
78) Chrysene-d12	20.99	240	565711	20.00	ng/ul	-0.01
86) Perylene-d12	23.07	264	566795	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	2.98	96	2180m	1.16	ng/uL	0.02
5) Phenol-d5	6.58	99	21692	3.58	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.73	67	12594	3.29	ng/ul	0.00
9) 2-Chlorophenol-d4	6.92	132	17396	3.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.10	113	18701	3.92	ng/ul	0.00
19) Nitrobenzene-d5	8.52	128	5325	2.03	ng/ul	0.00
22) 2-Nitrophenol-d4	9.23	143	8043	2.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.79	165	16163m	3.05	ng/ul	0.02
29) 4-Chloroaniline-d4	10.29	131	23985m	4.34	ng/ul	0.01
44) Dimethylphthalate-d6	13.46	166	58515	3.43	ng/ul	0.00
47) Acenaphthylene-d8	13.71	160	25934	1.27	ng/ul	0.00
52) 4-Nitrophenol-d4	0.00	143	0	0.00	ng/ul	
58) Fluorene-d10	15.03	176	20890	1.43	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	0.00	200	0	0.00	ng/ul	
71) Anthracene-d10	16.89	188	44936	1.88	ng/ul	0.00
79) Pyrene-d10	19.19	212	68309	2.20	ng/ul	0.00
90) Benzo(a)pyrene-d12	22.94	264	69261	2.21	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.50	163	30217	1.708	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062620\
Data File : BM026601.D
Acq On : 26 Jun 2020 22:30
Operator : JU/CG
Sample : L3062-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
ET143

Quant Time: Jun 26 23:43:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 26 22:52:41 2020
Response via : Initial Calibration

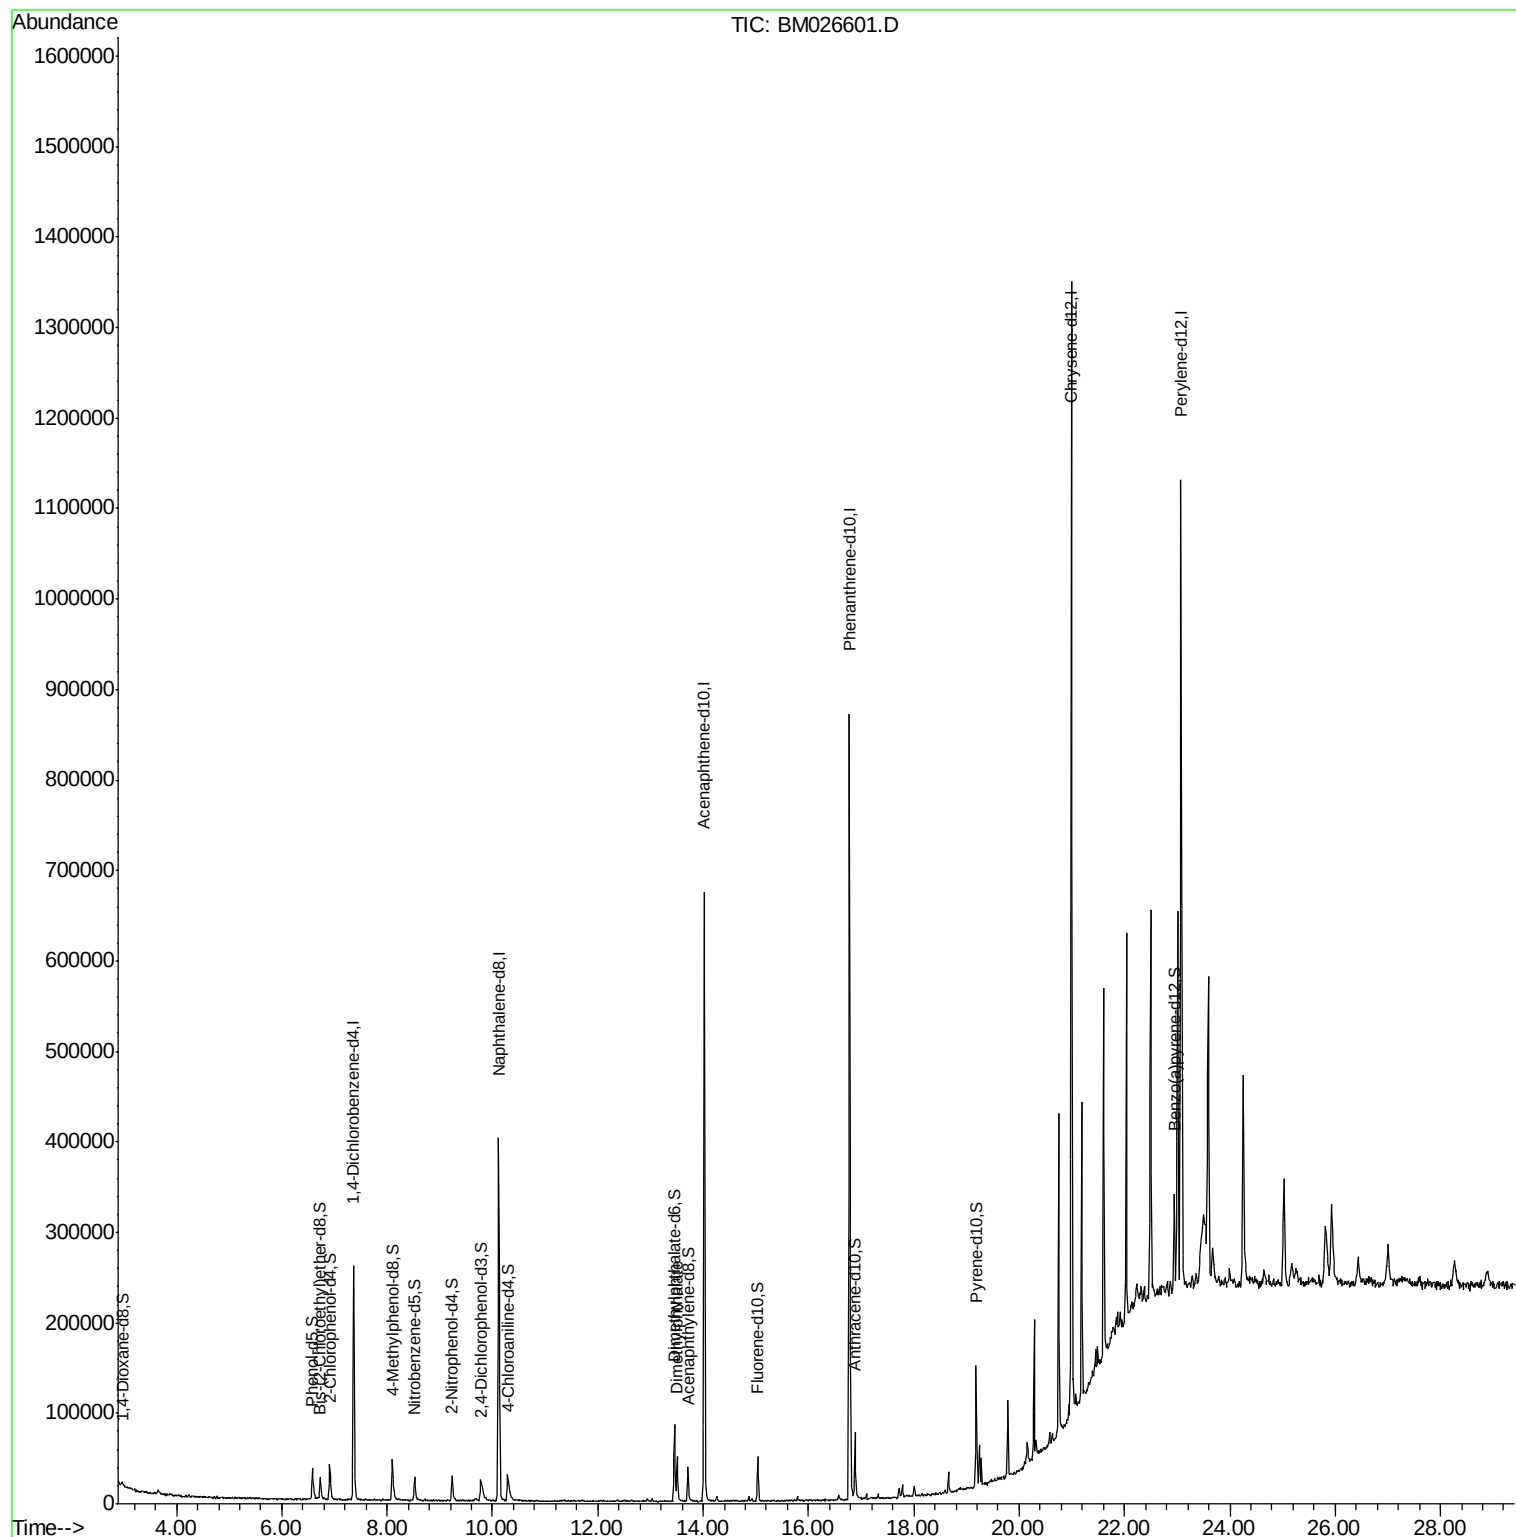

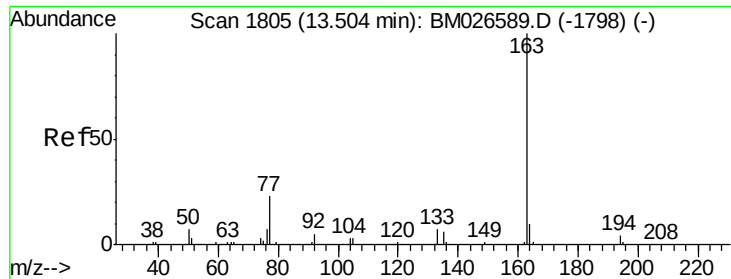

#45

Dimethylphthalate

Concen: 1.708 ng/ul

RT: 13.50 min Scan# 1805

Delta R.T. -0.00 min

Lab File: BM026601.D

Acq: 26 Jun 2020 22:30

Instrument :

BNA_M

ClientSampleId :

ET143


Tot Ion:163 Resp: 30217

Ion Ratio Lower Upper

163 100

194 4.7 3.4 5.2

164 12.0 7.8 11.6#

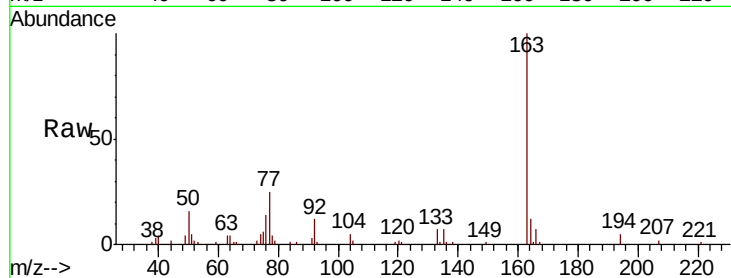

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

