

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062620\
 Data File : BM026605.D
 Acq On : 27 Jun 2020 00:55
 Operator : JU/CG
 Sample : L3118-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.958	10	12	22	rVB	22269	35172	1.11%	0.137%
2	3.652	127	130	136	rVB3	4978	7220	0.23%	0.028%
3	6.575	621	627	637	rBV	74203	133105	4.20%	0.517%
4	6.722	646	652	665	rBV	285988	455462	14.36%	1.768%
5	6.904	677	683	698	rBV	311107	514632	16.23%	1.998%
6	7.363	755	761	771	rBV	288376	461011	14.54%	1.789%
7	7.463	773	778	781	rBV3	2554	3352	0.11%	0.013%
8	7.710	816	820	826	rVB2	12161	18688	0.59%	0.073%
9	8.093	879	885	902	rBV	224636	389641	12.29%	1.512%
10	8.510	949	956	962	rBV	415592	683944	21.57%	2.655%
11	8.963	1029	1033	1038	rVB	17466	25952	0.82%	0.101%
12	9.228	1071	1078	1089	rBV	340788	573548	18.09%	2.226%
13	9.763	1163	1169	1189	rBV	382412	759716	23.96%	2.949%
14	9.987	1205	1207	1214	rVB3	4621	7556	0.24%	0.029%
15	10.122	1222	1230	1241	rVB	442173	701894	22.13%	2.724%
16	10.298	1253	1260	1273	rBV4	16639	40925	1.29%	0.159%
17	10.504	1291	1295	1300	rBV3	4829	6251	0.20%	0.024%
18	10.763	1334	1339	1344	rBV7	5716	11763	0.37%	0.046%
19	10.975	1368	1375	1377	rBV5	3432	6349	0.20%	0.025%
20	11.445	1449	1455	1462	rVB2	19908	29778	0.94%	0.116%
21	11.739	1500	1505	1510	rBV3	4731	8492	0.27%	0.033%
22	12.633	1651	1657	1661	rBV5	2501	3800	0.12%	0.015%
23	12.833	1685	1691	1699	rVB2	19032	28459	0.90%	0.110%
24	12.945	1706	1710	1714	rBV3	5107	7060	0.22%	0.027%
25	13.028	1719	1724	1731	rVB2	9140	14691	0.46%	0.057%
26	13.451	1790	1796	1801	rBV	1050697	1399597	44.13%	5.433%
27	13.498	1801	1804	1815	rVB	93739	131015	4.13%	0.509%
28	13.710	1833	1840	1850	rBV	1081310	1584749	49.97%	6.151%
29	14.022	1886	1893	1904	rBV	711188	1012413	31.93%	3.930%
30	14.298	1935	1940	1946	rBV2	24347	57431	1.81%	0.223%
31	14.927	2043	2047	2049	rBV4	3070	3205	0.10%	0.012%
32	15.027	2057	2064	2073	rBV	1555424	2099001	66.19%	8.147%
33	15.174	2083	2089	2102	rBV	531620	767383	24.20%	2.979%
34	15.269	2102	2105	2112	rVB2	18118	25527	0.80%	0.099%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062620\
 Data File : BM026605.D
 Acq On : 27 Jun 2020 00:55
 Operator : JU/CG
 Sample : L3118-03
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0F77

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
 Title : SVOA CALIBRATION

35	15.792	2187	2194	2195	rBV3	2234	3554	0.11%	0.014%
36	15.816	2195	2198	2202	rVB4	4874	6854	0.22%	0.027%
37	16.033	2232	2235	2239	rVB4	5209	5727	0.18%	0.022%
38	16.574	2322	2327	2333	rVB4	3686	8489	0.27%	0.033%
39	16.780	2356	2362	2372	rBV	947810	1275021	40.21%	4.949%
40	16.880	2372	2379	2395	rVV	1836688	2556501	80.62%	9.923%
41	17.304	2446	2451	2455	rBV6	2099	3806	0.12%	0.015%
42	17.715	2517	2521	2529	rBV2	17047	28819	0.91%	0.112%
43	17.992	2564	2568	2571	rBV6	2307	3610	0.11%	0.014%
44	18.162	2592	2597	2601	rBV4	45749	56652	1.79%	0.220%
45	18.821	2704	2709	2715	rBV2	18806	28574	0.90%	0.111%
46	19.021	2739	2743	2745	rBV4	2915	4051	0.13%	0.016%
47	19.074	2748	2752	2757	rVV2	17524	22993	0.73%	0.089%
48	19.186	2765	2771	2779	rBV	2494238	3171197	100.00%	12.309%
49	19.756	2865	2868	2869	rBV3	5255	4824	0.15%	0.019%
50	20.745	3032	3036	3046	rBV2	115429	200406	6.32%	0.778%
51	20.992	3073	3078	3086	rBV	1304792	1623181	51.19%	6.301%
52	22.492	3330	3333	3338	rVB2	58739	72346	2.28%	0.281%
53	22.945	3404	3410	3417	rBV	1801183	2897741	91.38%	11.248%
54	23.003	3418	3420	3425	rVV	89728	119283	3.76%	0.463%
55	23.074	3426	3432	3445	rVB2	879973	1538142	48.50%	5.970%
56	23.586	3516	3519	3524	rVB3	77707	121982	3.85%	0.473%


Sum of corrected areas: 25762535

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062620\
Data File : BM026605.D
Acq On : 27 Jun 2020 00:55
Operator : JU/CG
Sample : L3118-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F77

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

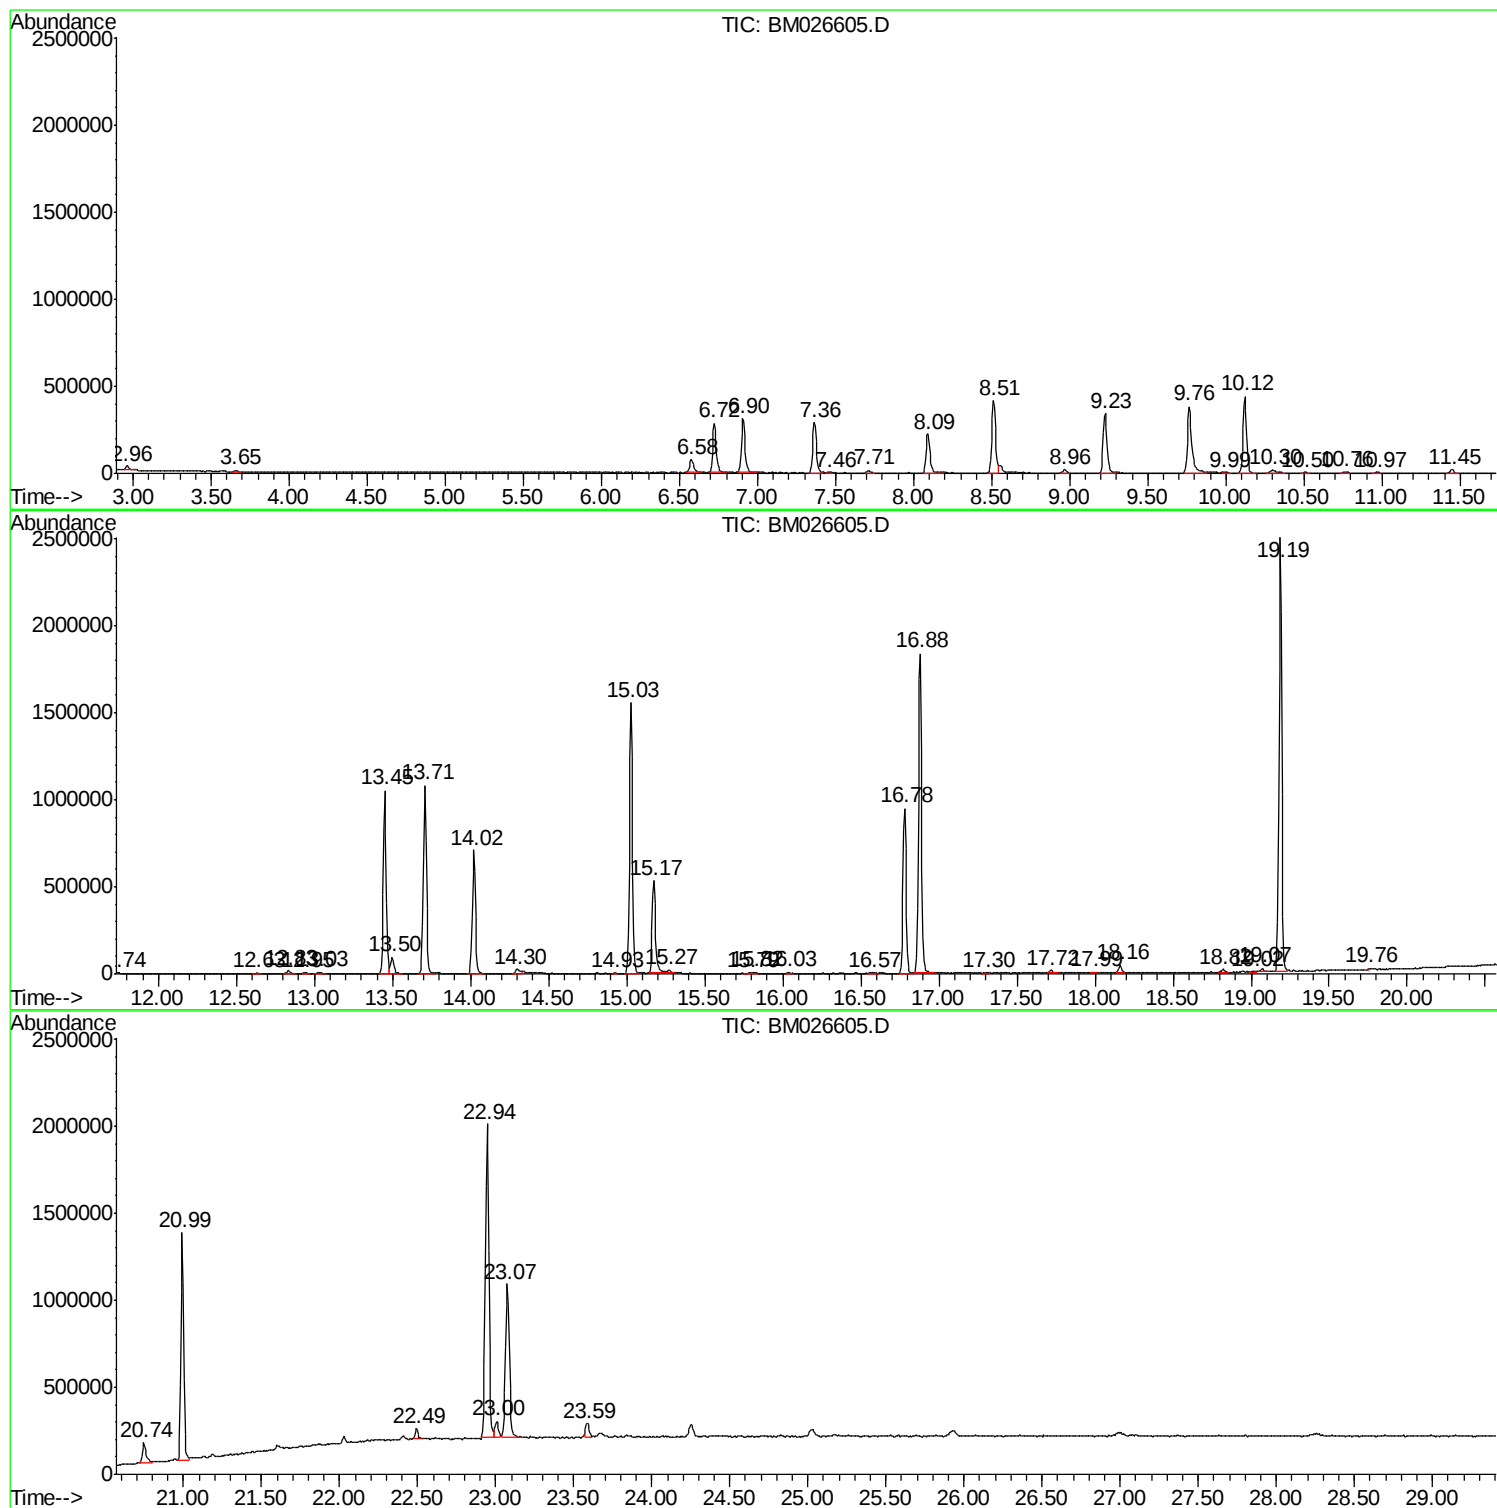

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062620\
Data File : BM026605.D
Acq On : 27 Jun 2020 00:55
Operator : JU/CG
Sample : L3118-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F77










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.74	2.47 ng/ul	200406	Chrysene-d12	20.99

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1-Nonadecene	266	C19H38	018435-45-5	97
2		17-Pentatriacontene	491	C35H70	006971-40-0	91
3		Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	91
4		3-Eicosene, (E)-	280	C20H40	074685-33-9	90
5		Octacosanol	410	C28H58O	000557-61-9	90

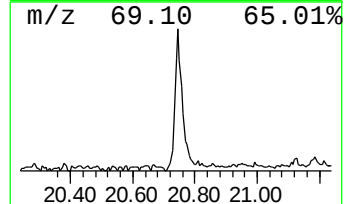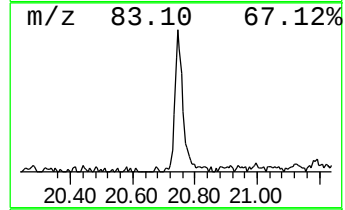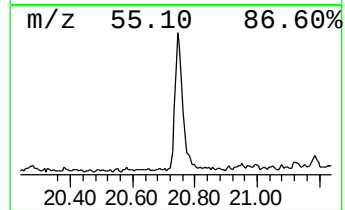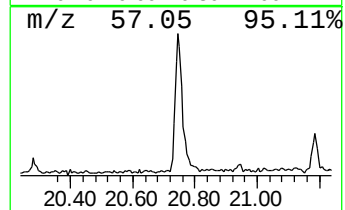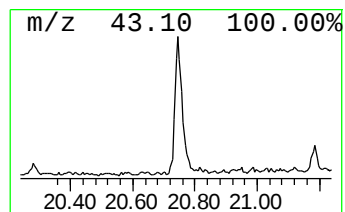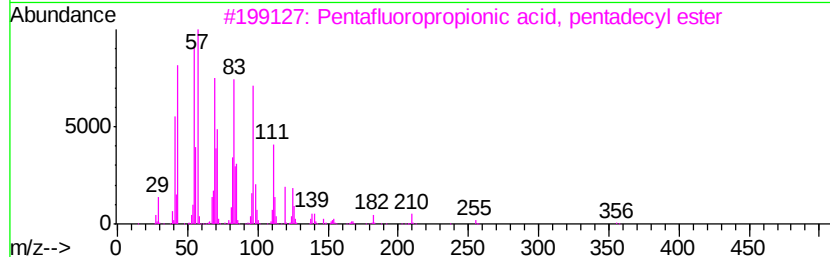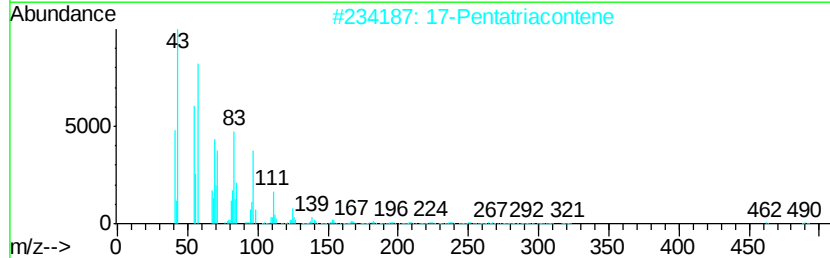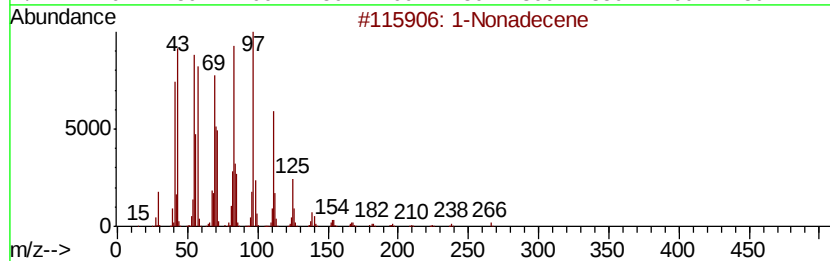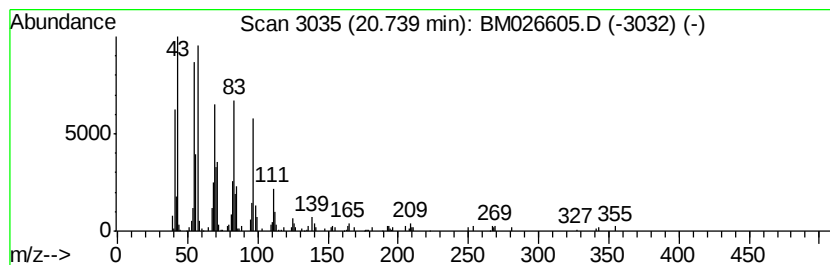

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062620\
Data File : BM026605.D
Acq On : 27 Jun 2020 00:55
Operator : JU/CG
Sample : L3118-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0F77

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061220MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc

(DEL) Alkane: Str...	20.74	2.5	ng/ul	200406	5	20.99	1623180	20.0