
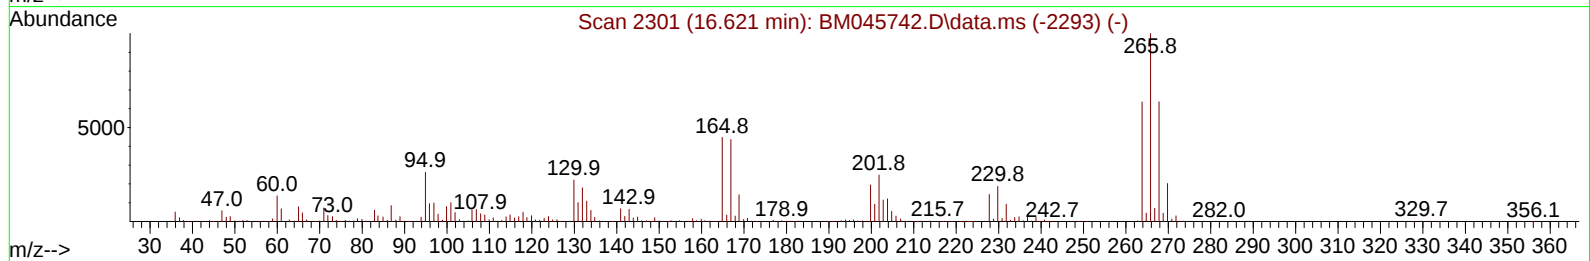
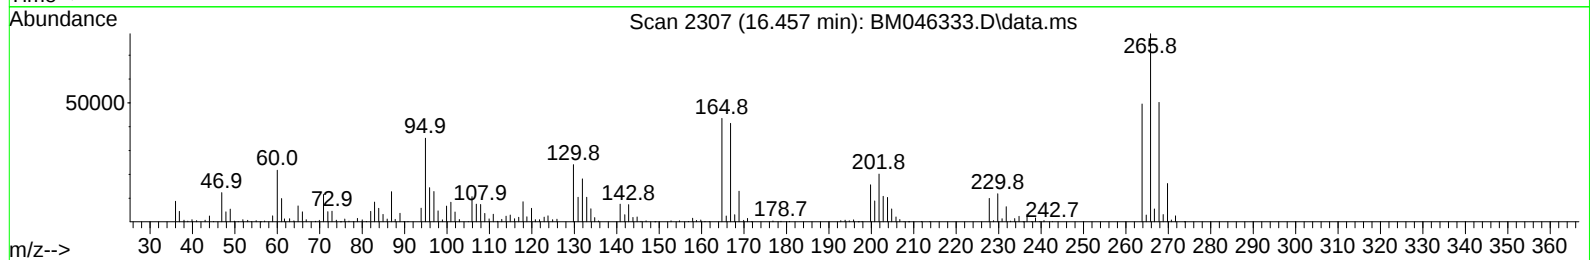


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062724\
Data File : BM046333.D
Acq On : 27 Jun 2024 15:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 16:27:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 04:12:56 2024
Response via : Initial Calibration

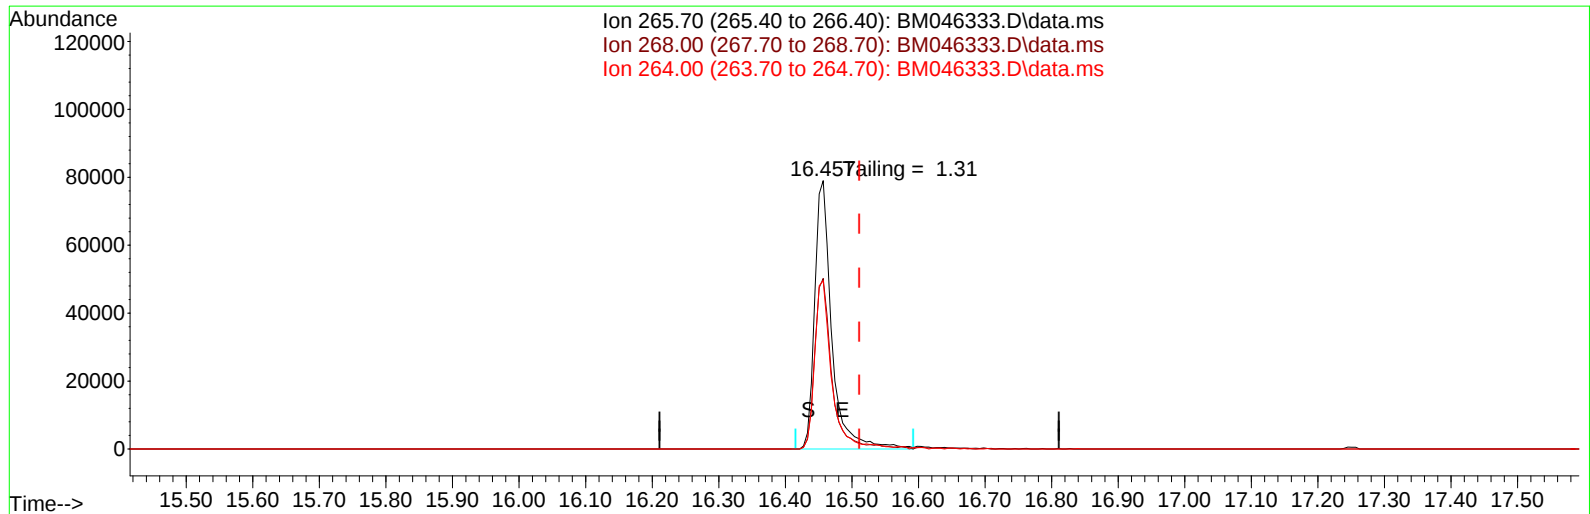

TIC: BM046333.D\data.ms

(70) Pentachlorophenol (C)




16.457min (-0.054) 0.00 ng

response 141409

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.57
264.00	63.60	62.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062724\
Data File : BM046333.D
Acq On : 27 Jun 2024 15:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 27 16:27:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 04:12:56 2024
Response via : Initial Calibration

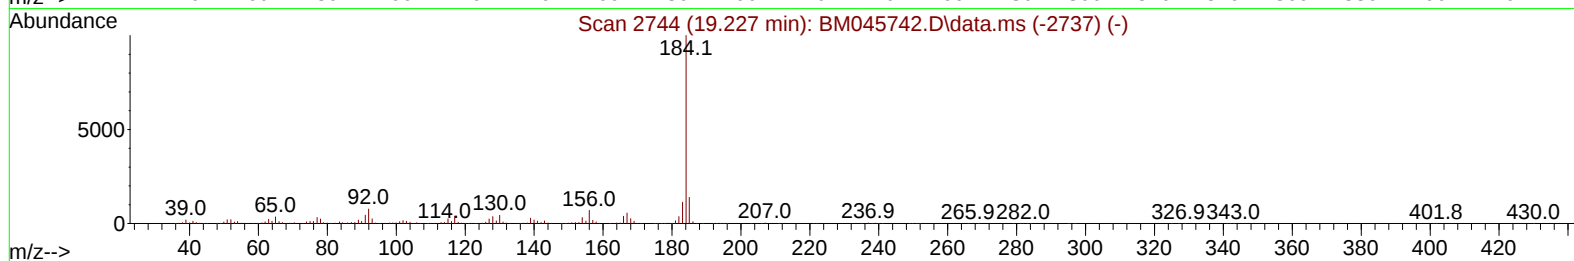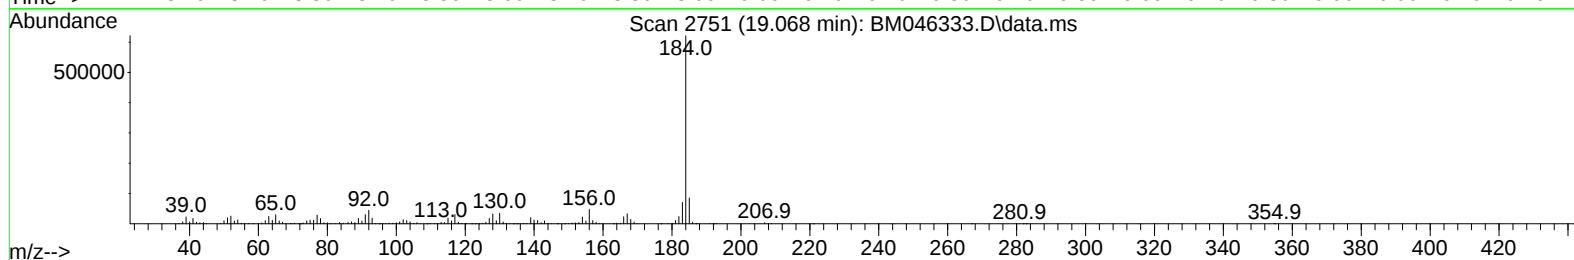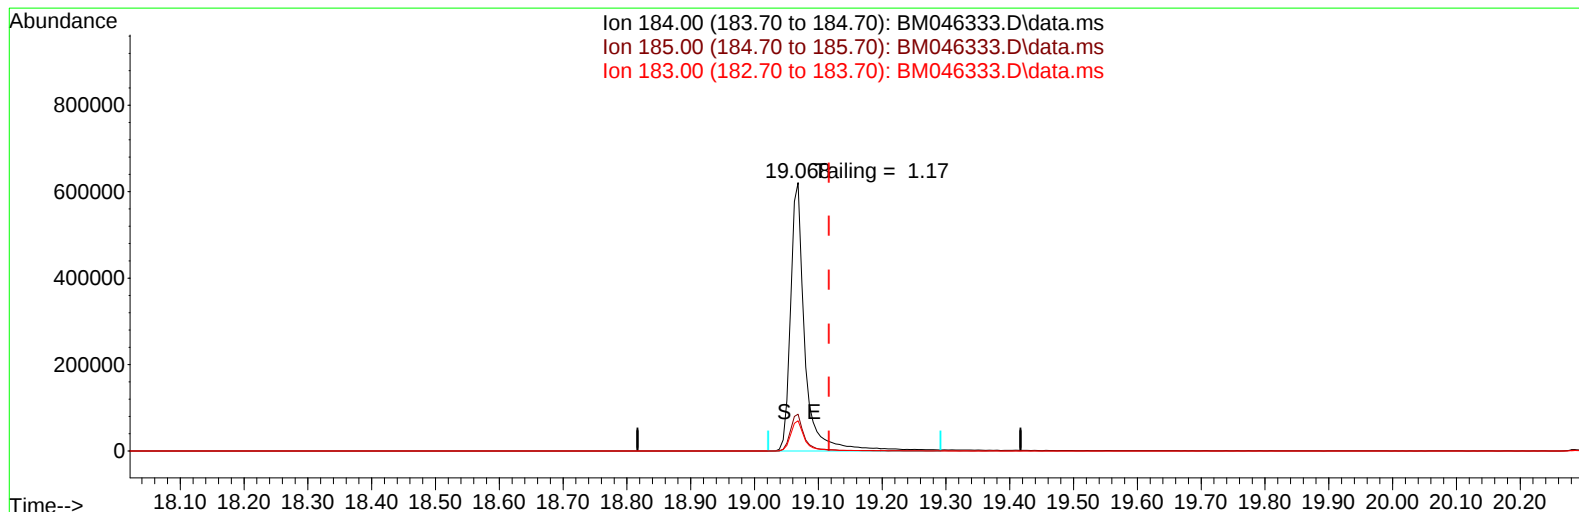

TIC: BM046333.D\data.ms

(77) Benzidine

19.068min (-0.049) 0.00 ng

response 975316

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.71
183.00	11.30	11.31
0.00	0.00	0.00