


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062724\
Data File : BM046333.D
Acq On : 27 Jun 2024 15:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270E-Tune.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 07 11:38:17 2020

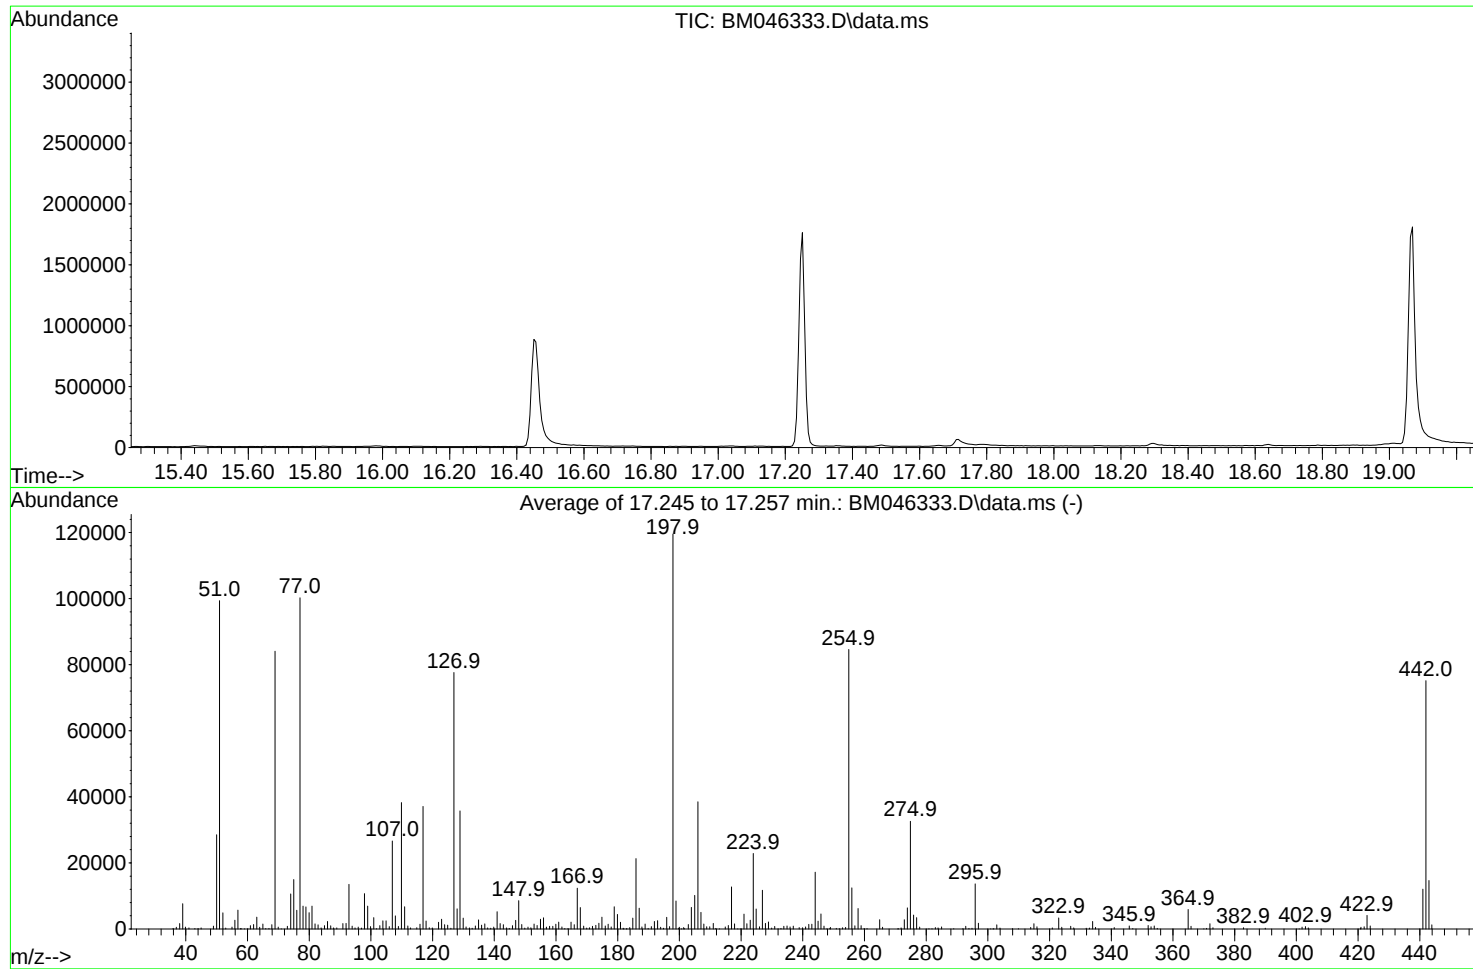




AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2434

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	1304	PASS
69	69	100	100	100.0	84093	PASS
70	69	0.00	2	0.7	589	PASS
197	198	0.00	2	0.6	707	PASS
198	198	100	100	100.0	119512	PASS
199	198	5	9	7.1	8461	PASS
365	198	1	100	4.9	5901	PASS
441	443	0.01	150	82.3	12081	PASS
442	442	100	100	100.0	75187	PASS
443	442	15	24	19.5	14676	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062724\
Data File : BM046333.D
Acq On : 27 Jun 2024 15:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 27 16:27:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 04:12:56 2024
Response via : Initial Calibration

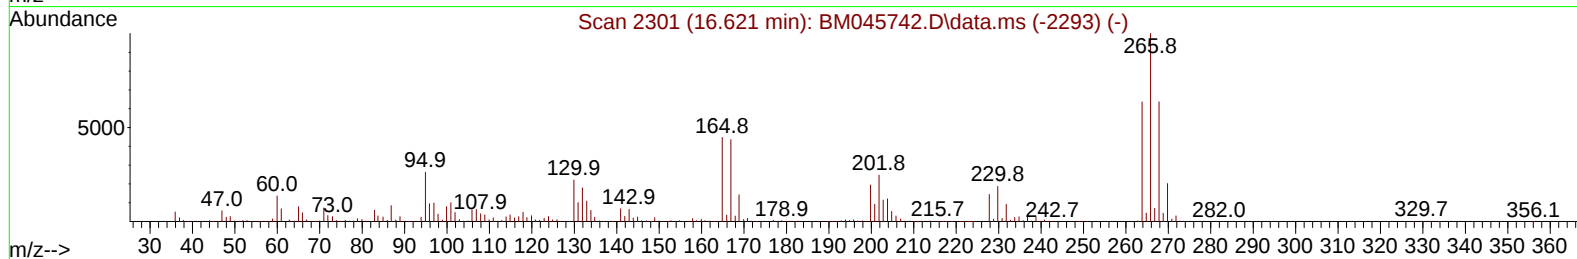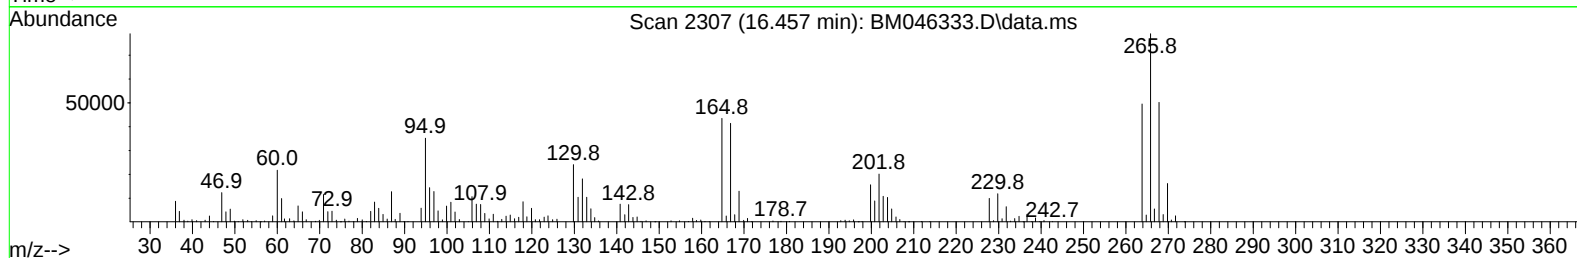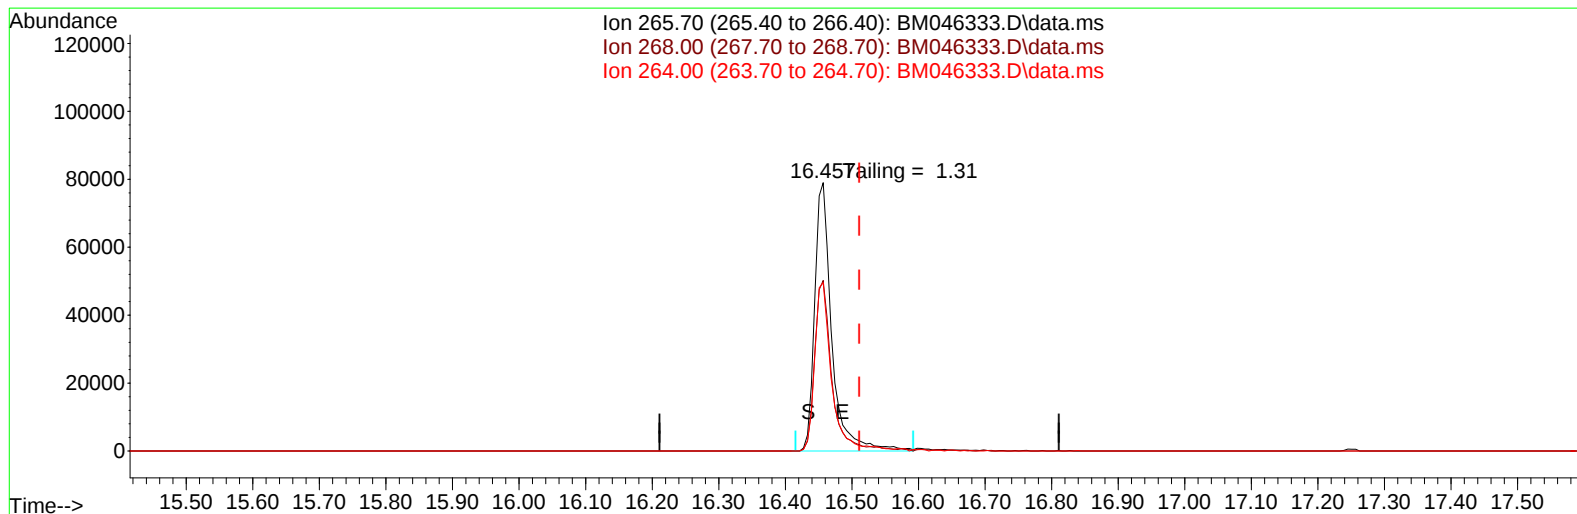

TIC: BM046333.D\data.ms

(70) Pentachlorophenol (C)

16.457min (-0.054) 0.00 ng




response 141409

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	63.57
264.00	63.60	62.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM062724\
Data File : BM046333.D
Acq On : 27 Jun 2024 15:23
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 27 16:27:47 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM062724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 23 04:12:56 2024
Response via : Initial Calibration

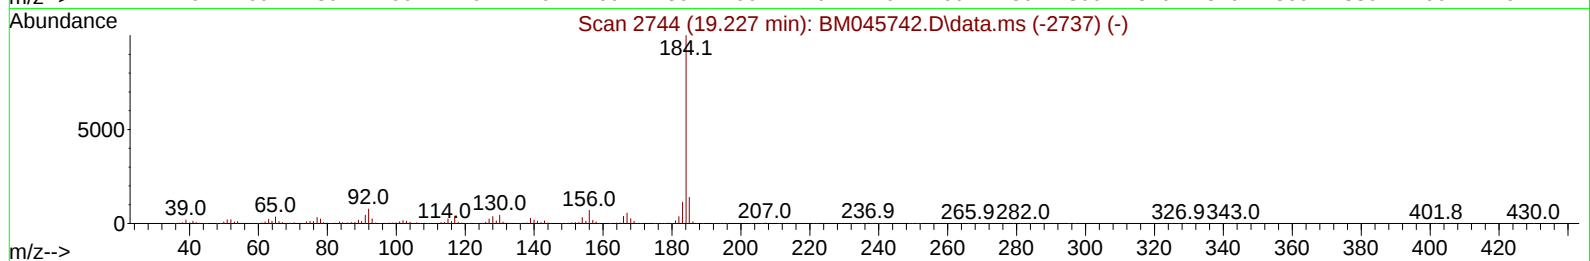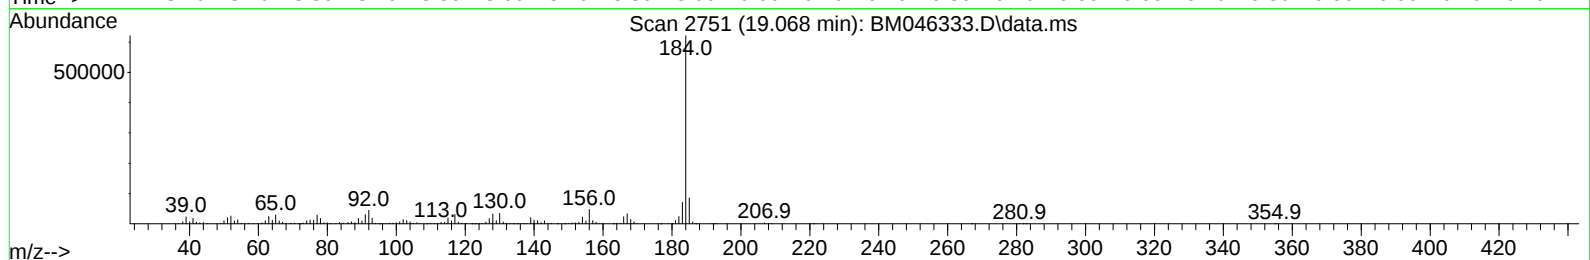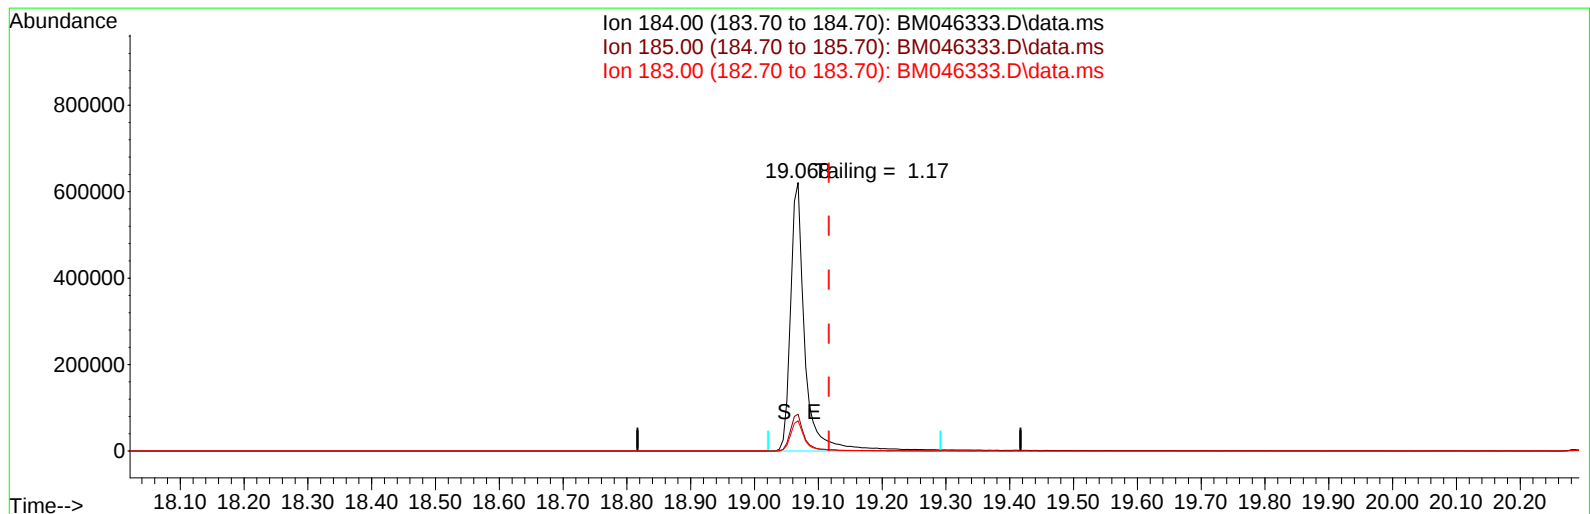

TIC: BM046333.D\data.ms

(77) Benzidine

19.068min (-0.049) 0.00 ng

response 975316

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.71
183.00	11.30	11.31
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/27/2024	BNA_M	<u>BM046333.D</u>
Compound Name	Response	Retention Time
DDT	513845	20.286
DDD	3965	19.898
DDE	0	19.492
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3965	517810	0.77

Instrument :
BNA_M
ClientSampleId :
DFTPP