

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
 Data File : BM021242.D
 Acq On : 28 Jun 2019 21:42
 Operator : HP/JU
 Sample : K3462-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Jun 28 22:57:20 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 27 05:07:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	212745	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.55	136	956450	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	622994	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	1437690	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	1110423	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1191446	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.28	96	28701	6.41	ng/uL	0.00
5) Phenol-d5	6.93	99	140903	7.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	345615	31.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	398105	26.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	282201	18.26	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	264925	34.11	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	301777	35.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	554345	31.62	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	73742	4.03	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	2081526	36.98	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	2399565	34.82	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	41611	4.54	ng/ul	0.00
57) Fluorene-d10	15.40	176	1802504	36.81	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	250179	28.31	ng/ul	-0.01
70) Anthracene-d10	17.25	188	2745596	36.75	ng/ul	0.00
78) Pyrene-d10	19.54	212	2767047	41.53	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	2647054	37.66	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.86	163	158793	3.099	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
Data File : BM021242.D
Acq On : 28 Jun 2019 21:42
Operator : HP/JU
Sample : K3462-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Jun 28 22:57:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 05:07:12 2019
Response via : Initial Calibration

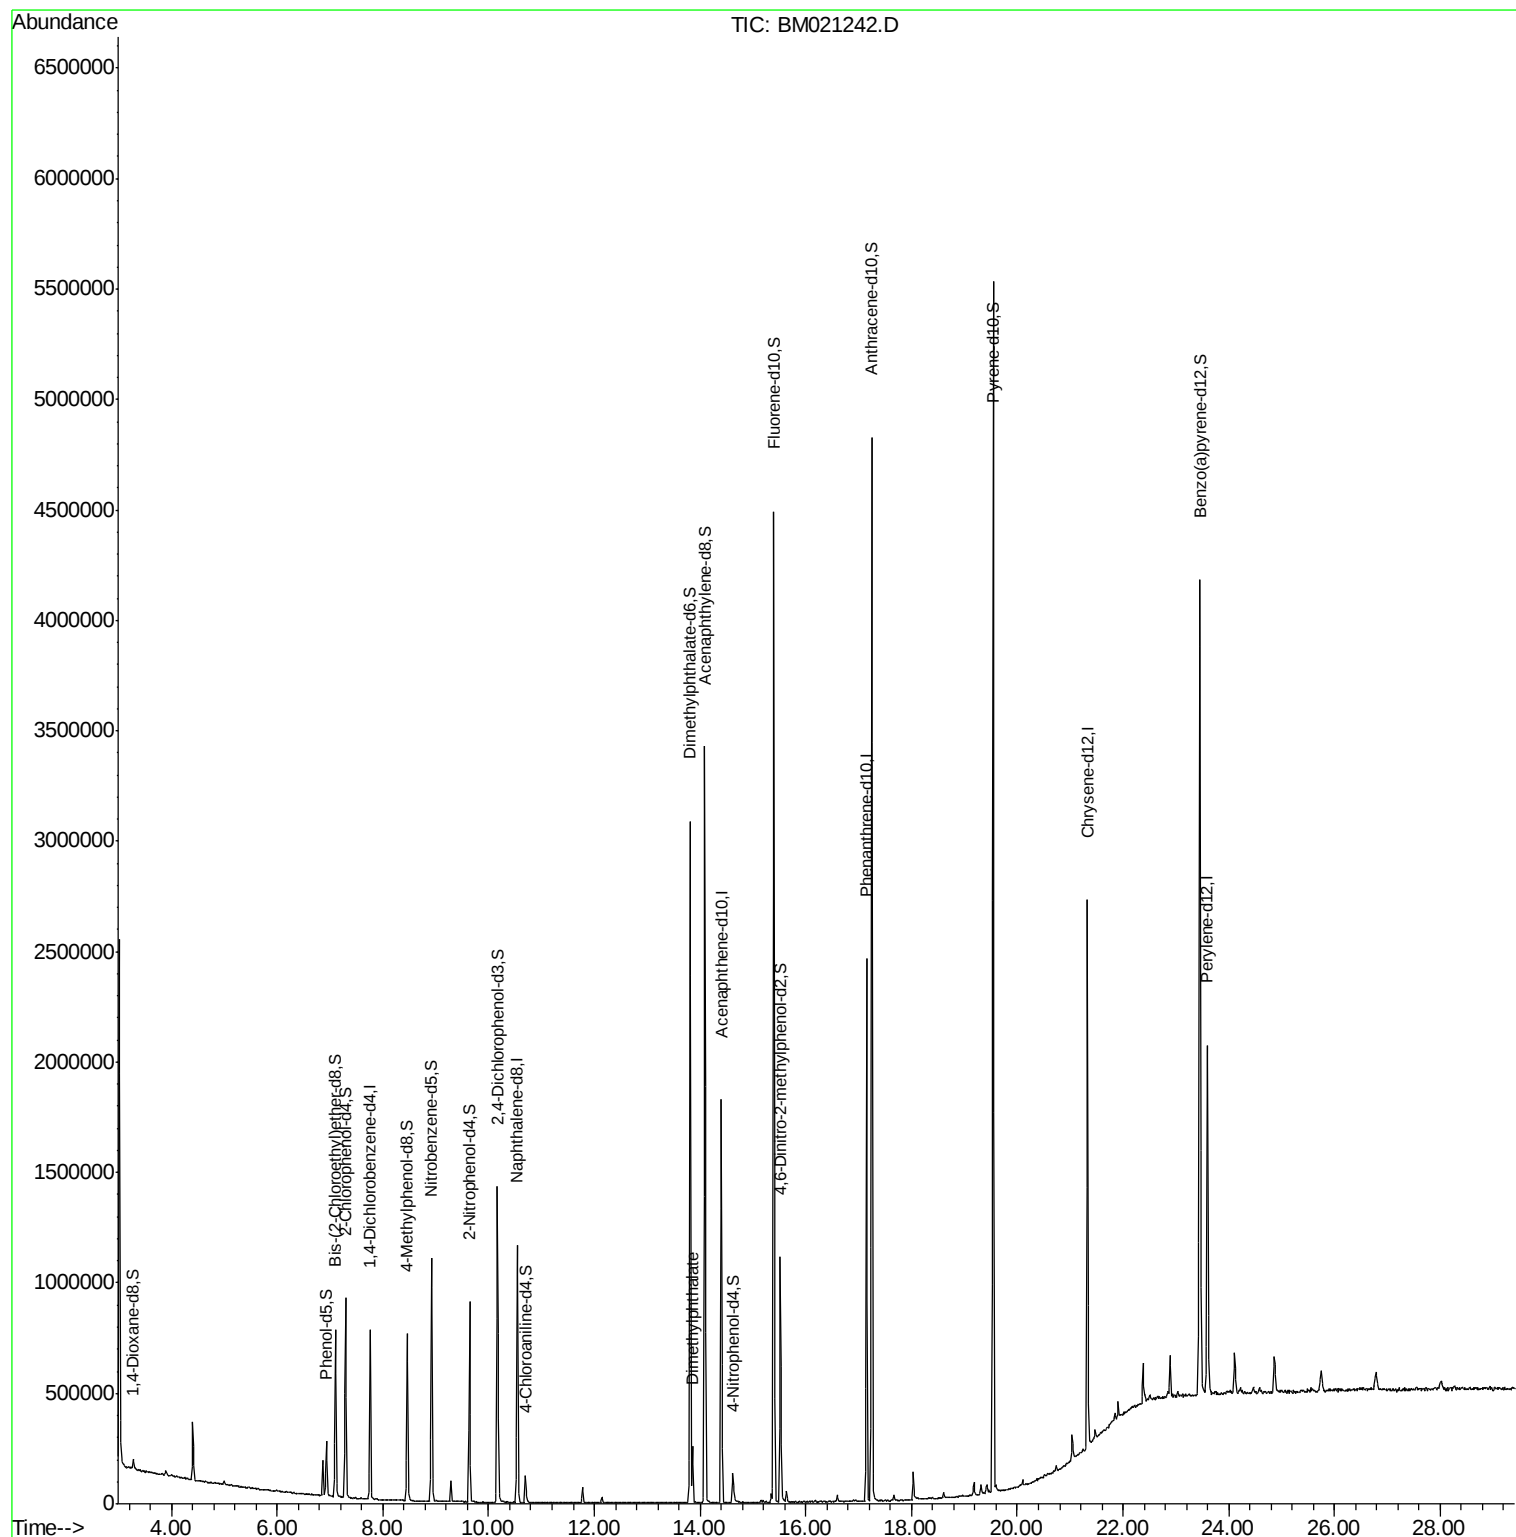

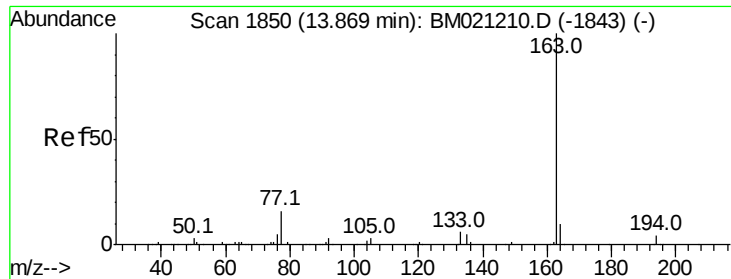

#44

Dimethylphthalate

Concen: 3.099 ng/ul

RT: 13.86 min Scan# 1849

Delta R.T. -0.01 min

Lab File: BM021242.D

Acq: 28 Jun 2019 21:42

Instrument :

BNA_M

ClientSampleId :


Tot Ion:163 Resp: 158793

Ion Ratio Lower Upper

163 100

194 4.2 3.4 5.2

164 9.6 7.7 11.5

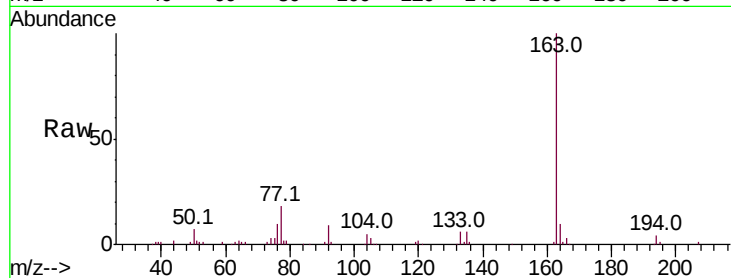

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

