


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
Data File : BM021240.D
Acq On : 28 Jun 2019 20:30
Operator : HP/JU
Sample : K3462-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Jun 28 23:20:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 05:07:12 2019
Response via : Initial Calibration

Instrument :
BNA_M
Client Sampled :
BFCM0

Manual Integrations
APPROVED

mohammad
7/1/2019 8:10:30 AM

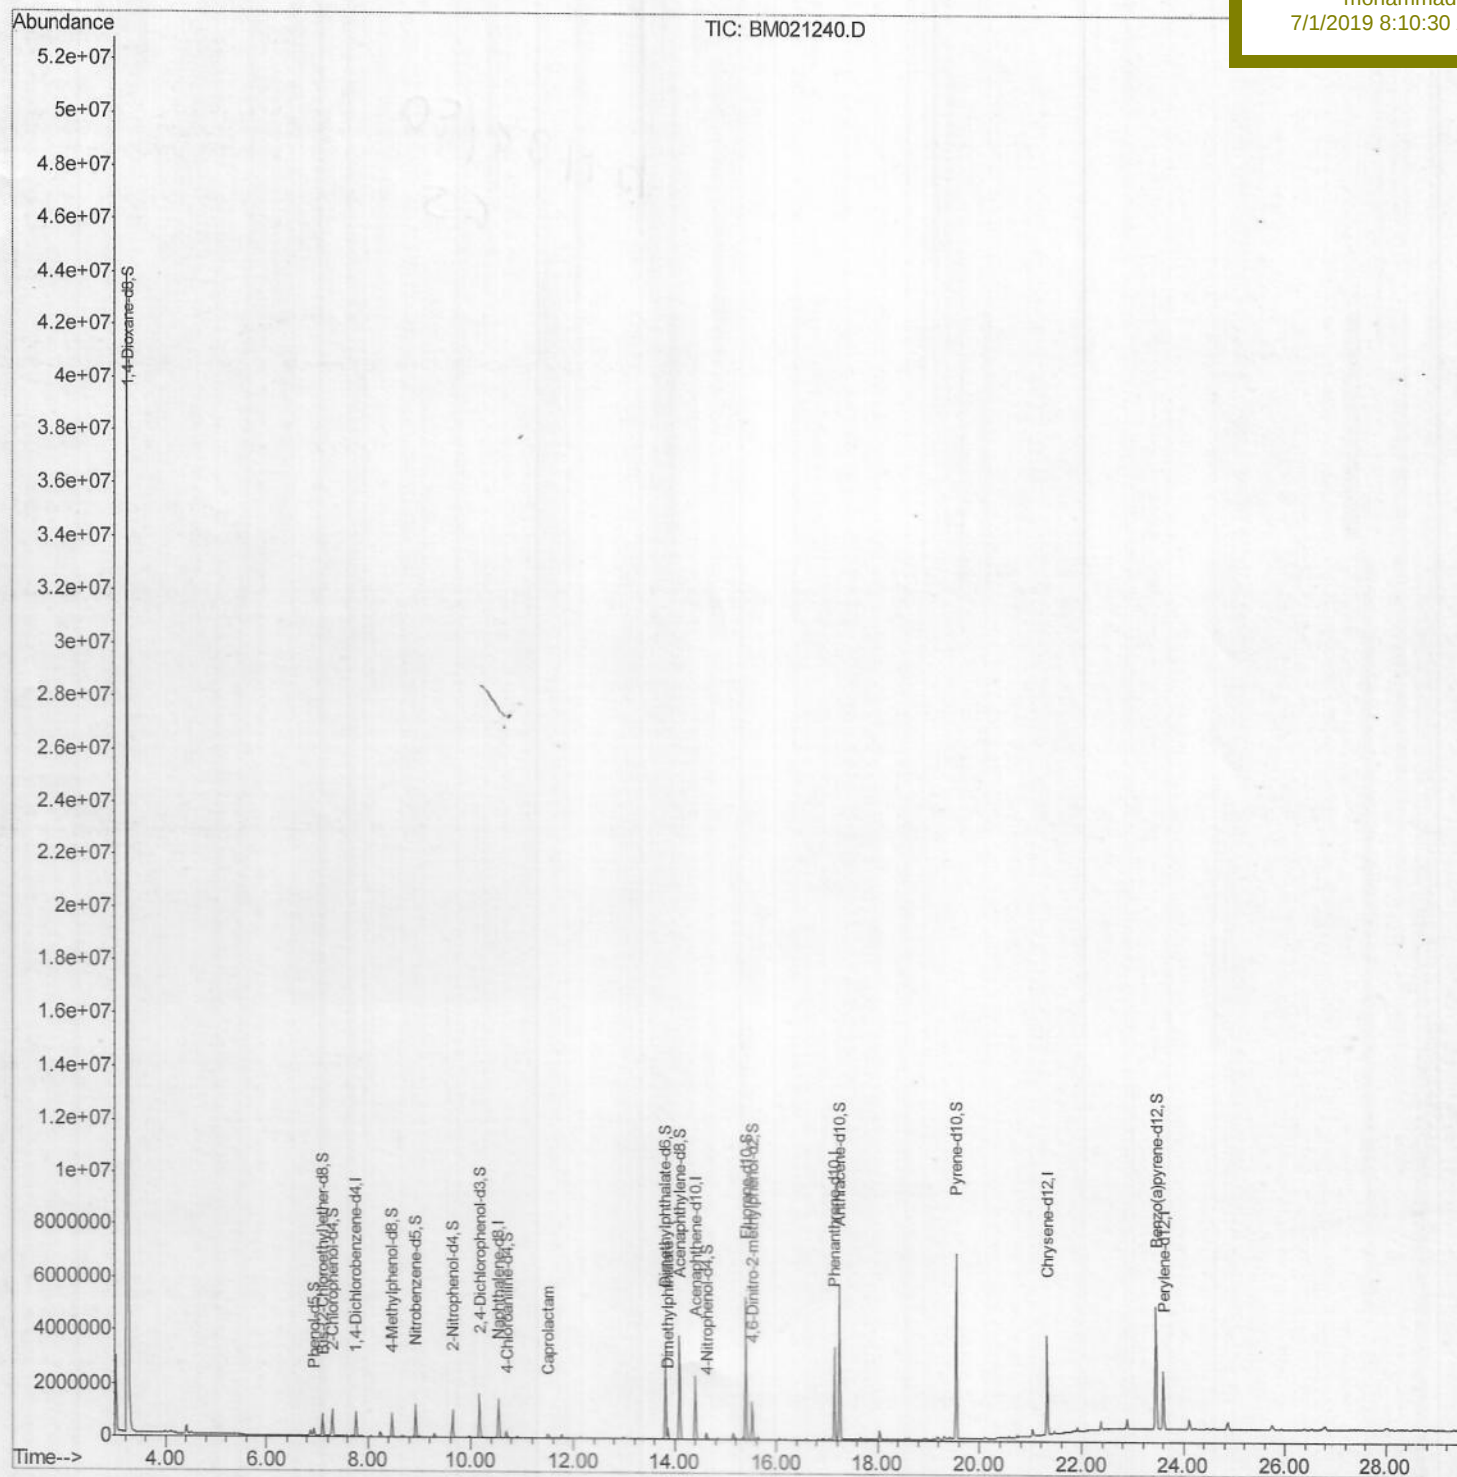

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\

Data File : BM021240.D

Acq On : 28 Jun 2019 20:30

Operator : HP/JU

Sample : K3462-02

Misc :

ALS Vial : 18 Sample Multiplier: 1

Quant Time: Jun 28 22:57:08 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Thu Jun 27 05:07:12 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




BFCM0

Manual Integrations

APPROVED

mohammad

7/1/2019 8:10:30 AM

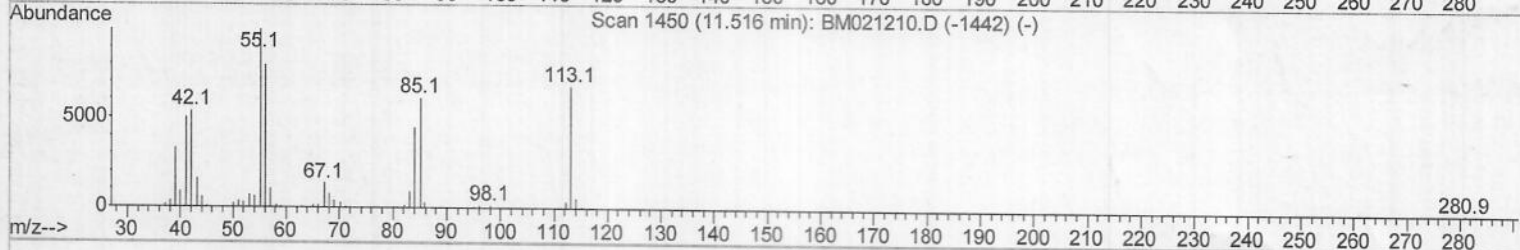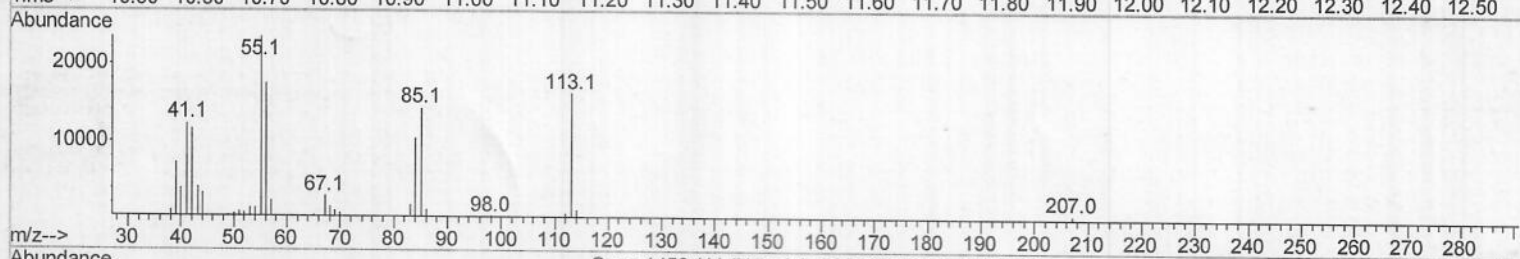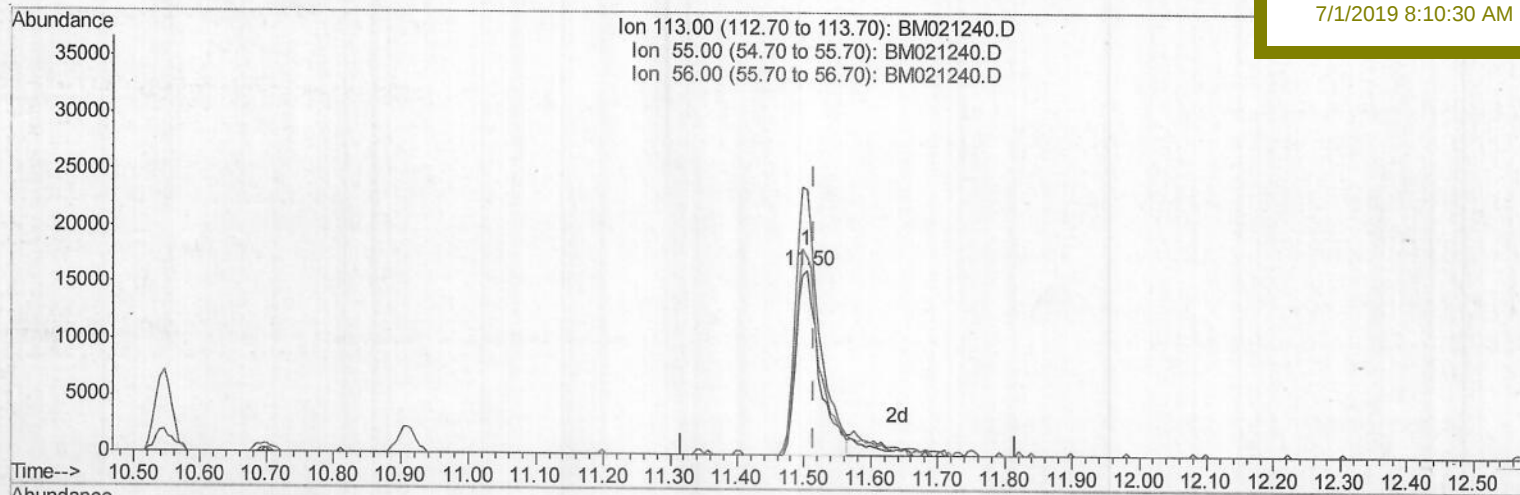

TIC: BM021240.D

(32) Caprolactam

11.504min (-0.012) 7.02ng/ul

response 39554

Ion	Exp%	Act%
113.00	100	100
55.00	144.70	144.23
56.00	113.80	107.57
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\

Data File : BM021240.D

Acq On : 28 Jun 2019 20:30

Operator : HP/JU

Sample : K3462-02

Misc :

ALS Vial : 18 Sample Multiplier: 1

Quant Time: Jun 28 22:57:08 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M

Quant Title : SVOA CALIBRATION

QLast Update : Thu Jun 27 05:07:12 2019

Response via : Initial Calibration

Instrument :

BNA_M

ClientSampleId :




BFCM0

Manual Integrations

APPROVED

mohammad

7/1/2019 8:10:30 AM

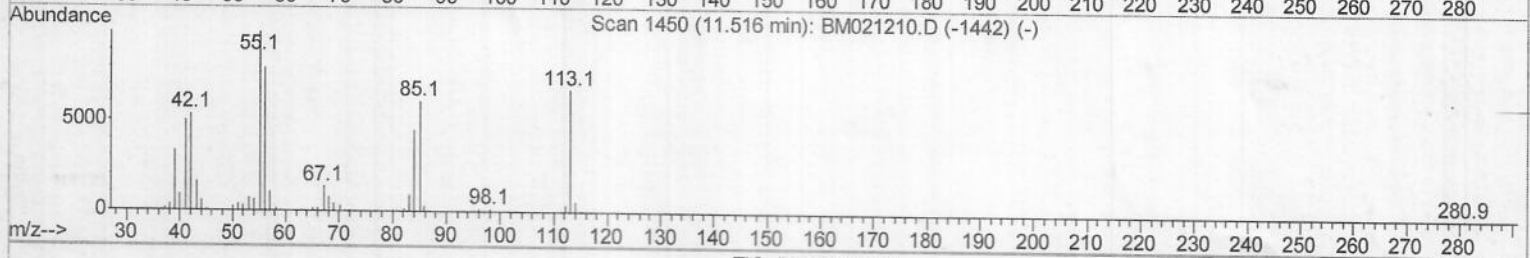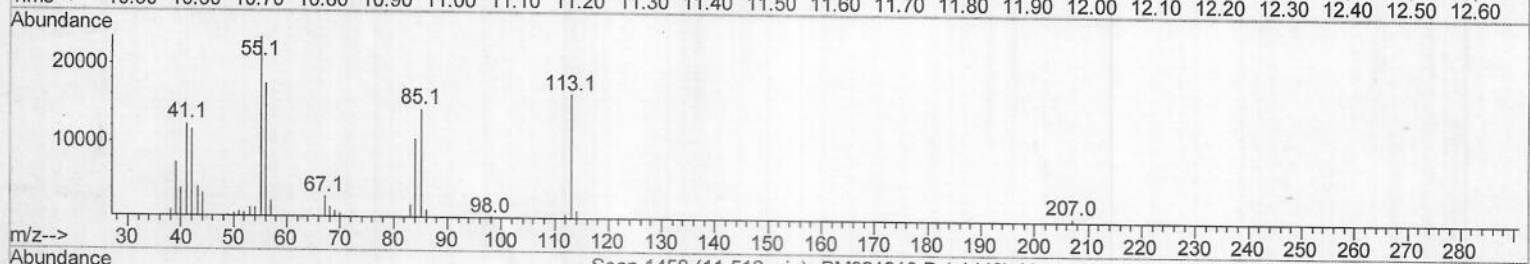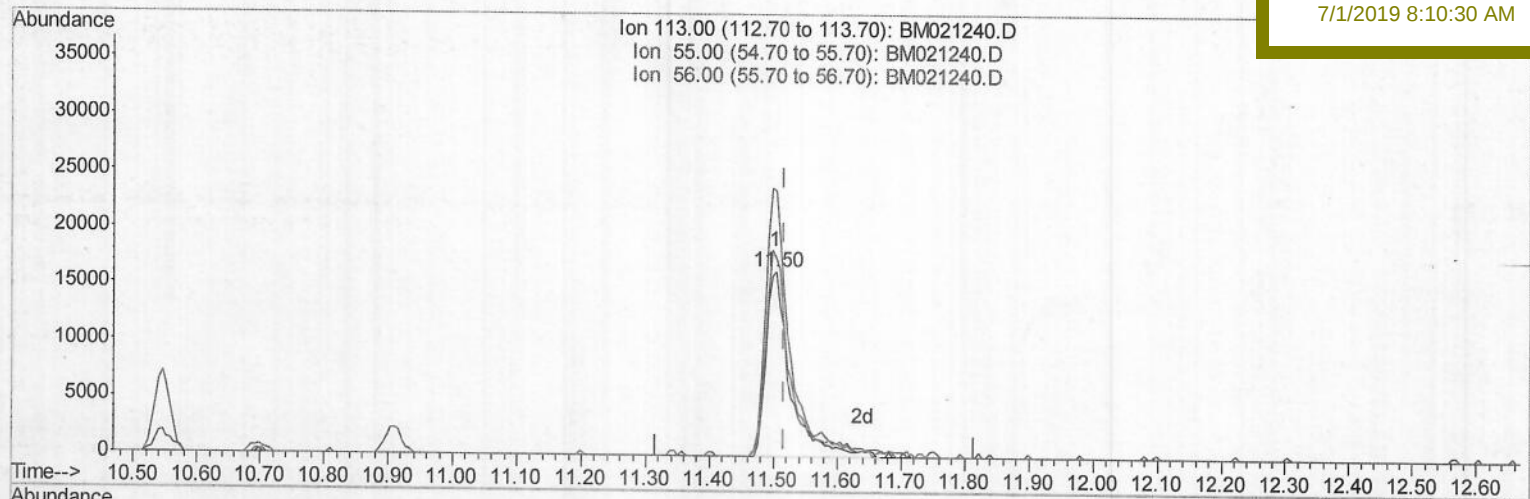

TIC: BM021240.D

(32) Caprolactam

11.504min (-0.012) 7.76ng/ul m> JU 07/03/19

response 43687

Ion	Exp%	Act%
113.00	100	100
55.00	144.70	144.23
56.00	113.80	107.57
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
 Data File : BM021240.D
 Acq On : 28 Jun 2019 20:30
 Operator : HP/JU
 Sample : K3462-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFCM0

Quant Time: Jun 28 23:20:08 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 27 05:07:12 2019
 Response via : Initial Calibration

Manual Integrations
 APPROVED

mohammad
 7/1/2019 8:10:30 AM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	266618	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.55	136	1200494	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	809095	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	1957126	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	1640205	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1643629	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.25	96	1400134	249.36	ng/uL	-0.04
5) Phenol-d5	6.93	99	177045	7.63	ng/ul	0.00
7) Bis-(2-Chloroethyl) ether-d	7.10	67	384165	27.79	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	464705	24.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	338158	17.46	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	294262	30.19	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	336647	31.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	643352	29.24	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	119068	5.19	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	2325771	31.81	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	2712718	30.31	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	62604	5.26	ng/ul	0.00
57) Fluorene-d10	15.40	176	2052753	32.28	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.52	200	331975	27.59	ng/ul	-0.01
70) Anthracene-d10	17.25	188	3303270	32.48	ng/ul	0.00
78) Pyrene-d10	19.54	212	3583966	36.41	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	3261247	33.63	ng/ul	0.00

Target Compounds

32) Caprolactam	11.50	113	43687m	7.758	ng/ul	Ovalue 30 07/03/19
44) Dimethylphthalate	13.86	163	264839	3.980	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed