

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
 Data File : BM021228.D
 Acq On : 28 Jun 2019 13:14
 Operator : HP/JU
 Sample : K3381-06
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFCM4

Quant Time: Jun 28 15:37:29 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 27 05:07:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	202841	20.00	ng/ul	-0.01
18) Naphthalene-d8	10.55	136	924577	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	635629	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	1567273	20.00	ng/ul	0.00
77) Chrysene-d12	21.34	240	1224318	20.00	ng/ul	0.00
85) Perylene-d12	23.61	264	1248177	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	28272	6.62	ng/uL	0.00
5) Phenol-d5	6.93	99	124622	7.06	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	304338	28.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	347537	24.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	247197	16.77	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	233289	31.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	267530	32.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	494407	29.18	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
43) Dimethylphthalate-d6	13.82	166	1929555	33.60	ng/ul	0.00
46) Acenaphthylene-d8	14.10	160	2248732	31.99	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	40531	4.34	ng/ul	0.00
57) Fluorene-d10	15.40	176	1703022	34.09	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	238598	24.76	ng/ul	0.00
70) Anthracene-d10	17.25	188	2709810	33.27	ng/ul	0.00
78) Pyrene-d10	19.54	212	2798992	38.10	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	2459068	33.39	ng/ul	0.00


Target Compounds				Ovalue
2) 1,4-Dioxane	3.31	88	198061	45.820 ng/uL# 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
Data File : BM021228.D
Acq On : 28 Jun 2019 13:14
Operator : HP/JU
Sample : K3381-06
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFCM4

Quant Time: Jun 28 15:37:29 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 05:07:12 2019
Response via : Initial Calibration

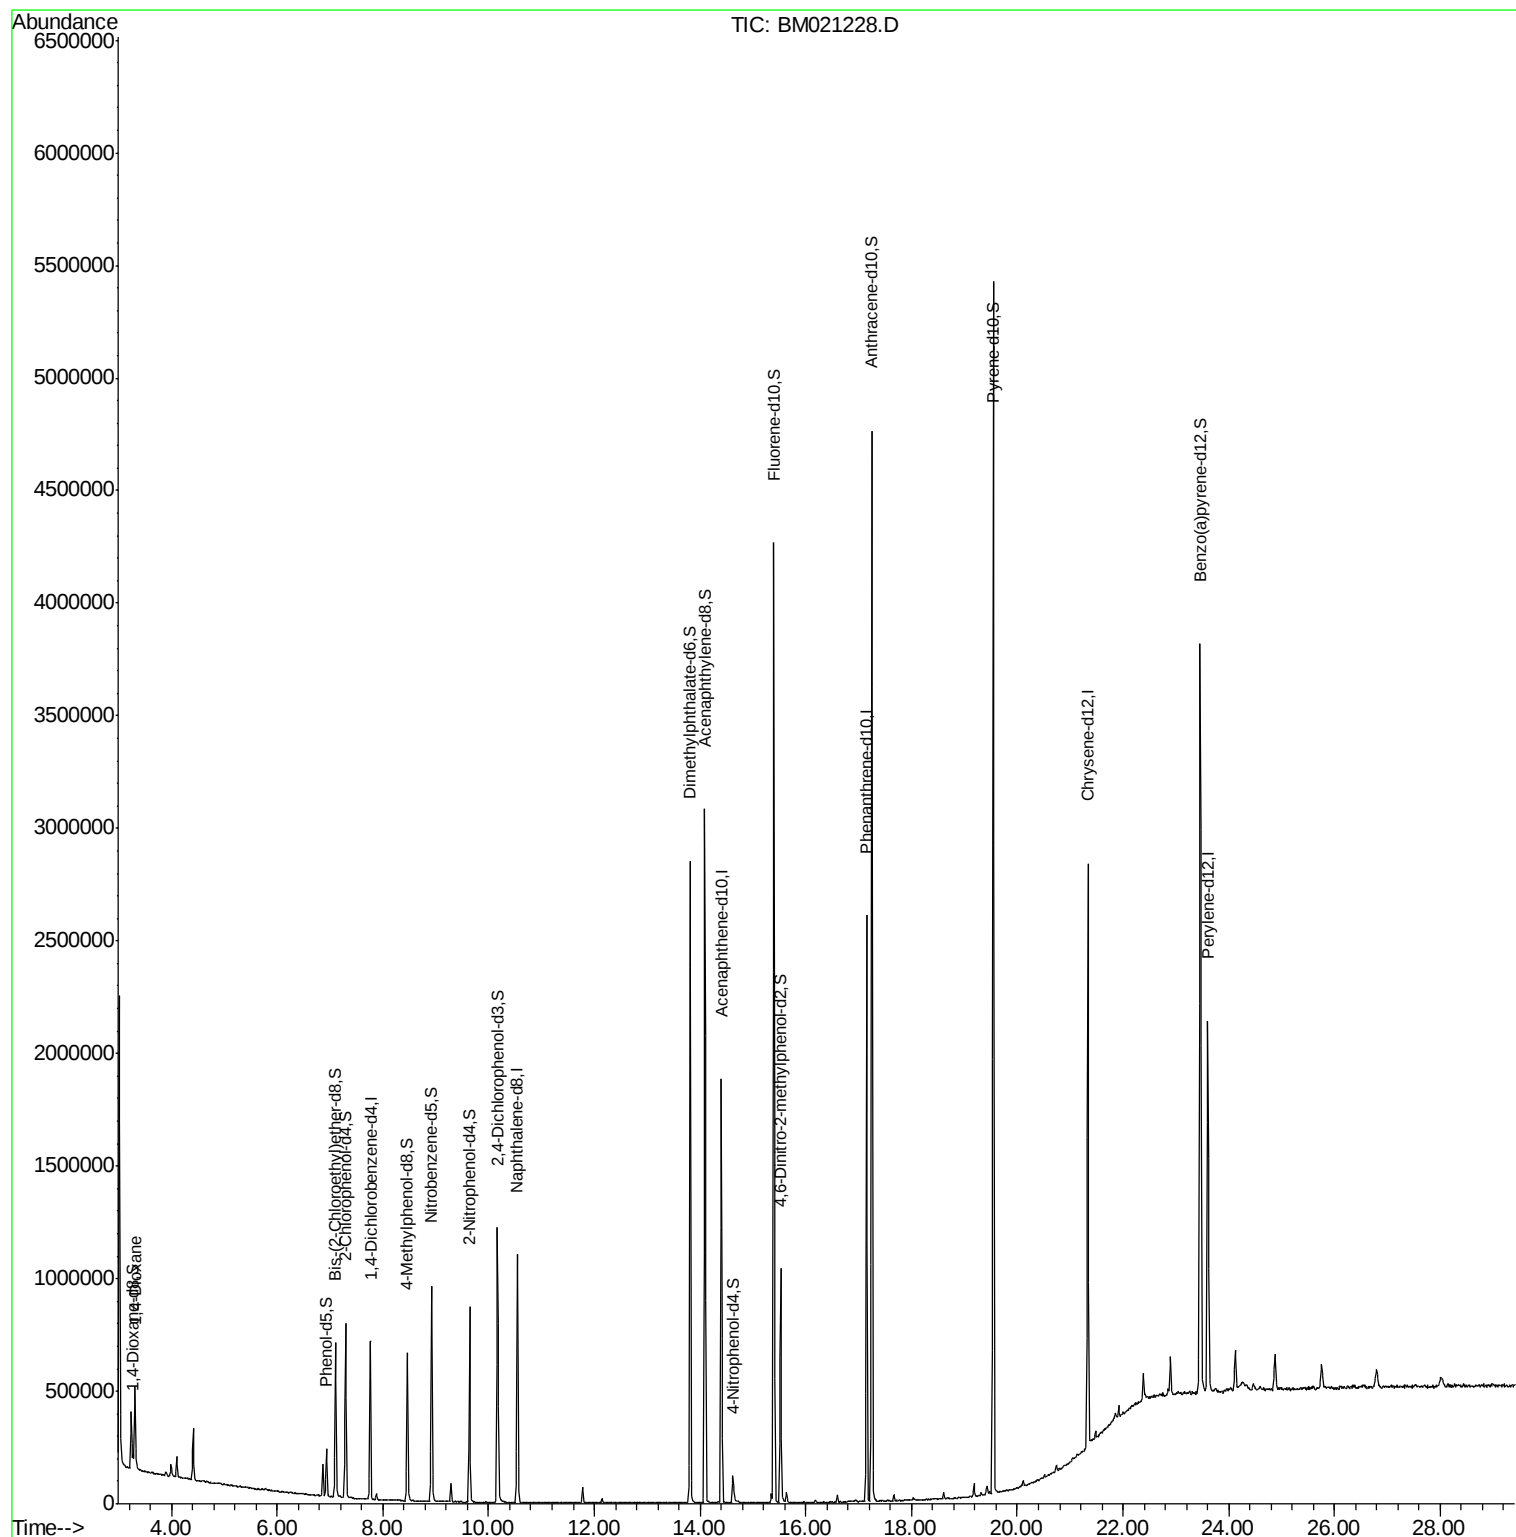

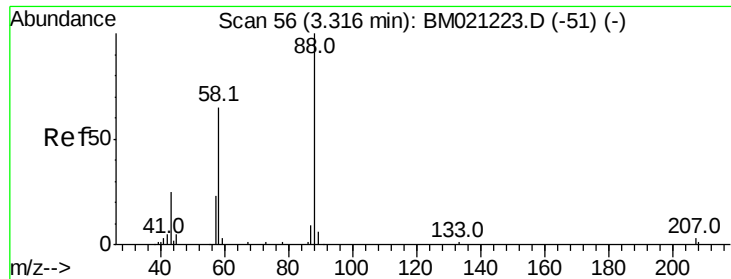

#2
 1,4-Dioxane
 Concen: 45.820 ng/uL
 RT: 3.31 min Scan# 55
 Delta R.T. -0.01 min
 Lab File: BM021228.D
 Acq: 28 Jun 2019 13:14

Instrument :
 BNA_M
 ClientSampleId :
 BFCM4

Tot Ion: 88 Resp: 198061
 Ion Ratio Lower Upper
 88 100
 43 26.5 26.7 40.1#
 58 66.2 52.6 78.8

