

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
 Data File : BM021231.D
 Acq On : 28 Jun 2019 15:03
 Operator : HP/JU
 Sample : K3381-12
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BFCM6

Quant Time: Jun 28 15:41:33 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jun 27 05:07:12 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.76	152	194115	20.00	ng/ul	0.00
18) Naphthalene-d8	10.55	136	856426	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.40	164	572236	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.15	188	1488389	20.00	ng/ul	0.00
77) Chrysene-d12	21.33	240	1582433	20.00	ng/ul	0.00
85) Perylene-d12	23.60	264	1706654	20.00	ng/ul	-0.01

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.28	96	27993	6.85	ng/uL	0.00
5) Phenol-d5	6.93	99	123169	7.29	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.10	67	323482	32.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.29	132	370297	26.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.46	113	236787	16.79	ng/ul	0.00
19) Nitrobenzene-d5	8.92	128	242813	34.92	ng/ul	0.00
22) 2-Nitrophenol-d4	9.64	143	275438	35.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.17	165	523008	33.32	ng/ul	0.00
29) 4-Chloroaniline-d4	10.70	131	30971	1.89	ng/ul	0.00
43) Dimethylphthalate-d6	13.82	166	1866890	36.11	ng/ul	0.00
46) Acenaphthylene-d8	14.09	160	2226979	35.18	ng/ul	0.00
51) 4-Nitrophenol-d4	14.62	143	43978	5.23	ng/ul	0.00
57) Fluorene-d10	15.40	176	1683782	37.44	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.53	200	258453	28.25	ng/ul	0.00
70) Anthracene-d10	17.25	188	2757551	35.65	ng/ul	0.00
78) Pyrene-d10	19.54	212	3312151	34.88	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.46	264	3587534	35.63	ng/ul	0.00


Target Compounds					Ovalue
2) 1,4-Dioxane	3.31	88	1653767	399.787	ng/uL# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
Data File : BM021231.D
Acq On : 28 Jun 2019 15:03
Operator : HP/JU
Sample : K3381-12
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BFCM6

Quant Time: Jun 28 15:41:33 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jun 27 05:07:12 2019
Response via : Initial Calibration

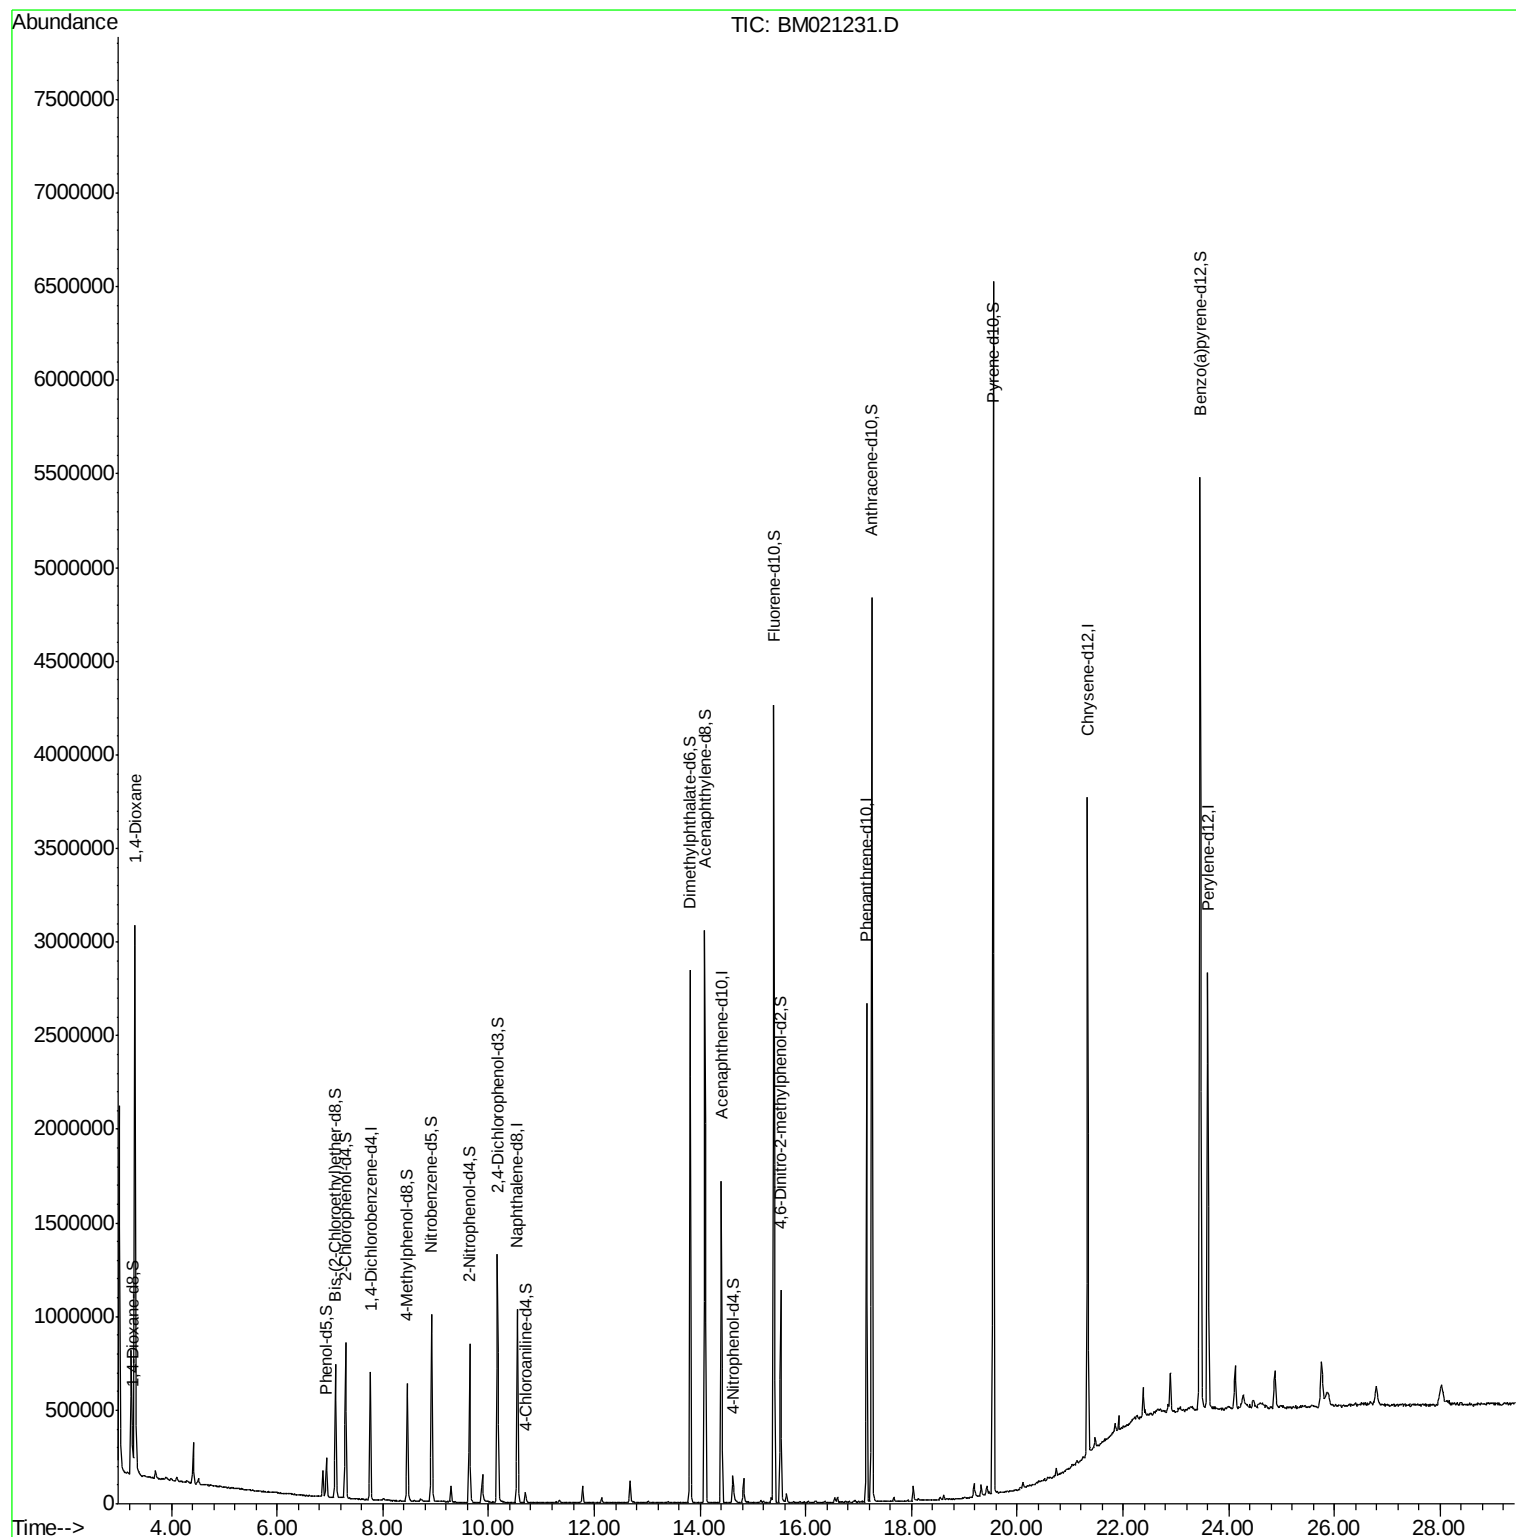

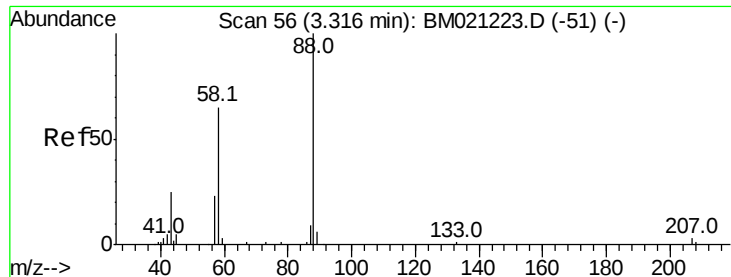

#2
 1,4-Dioxane
 Concen: 399.787 ng/uL
 RT: 3.31 min Scan# 55
 Delta R.T. -0.01 min
 Lab File: BM021231.D
 Acq: 28 Jun 2019 15:03

Instrument :
 BNA_M
 ClientSampleId :
 BFCM6

Tot Ion: 88 Resp: 1653767
 Ion Ratio Lower Upper
 88 100
 43 24.4 26.7 40.1#
 58 64.8 52.6 78.8

