

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
 Data File : BM021234.D
 Acq On : 28 Jun 2019 16:52
 Operator : HP/JU
 Sample : PB120790BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK90

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.016	3	5	10	rVB	75524	83897	1.14%	0.129%
2	3.281	47	50	56	rVB2	45845	60726	0.82%	0.093%
3	6.928	664	670	680	rBV	885861	1435785	19.50%	2.206%
4	7.104	694	700	713	rVB	725826	1143337	15.52%	1.757%
5	7.292	726	732	743	rVB	971720	1533486	20.82%	2.356%
6	7.763	805	812	820	rVB	625260	1001209	13.59%	1.538%
7	8.463	924	931	945	rBV	1221593	1929746	26.20%	2.965%
8	8.922	1002	1009	1019	rBV	960728	1589619	21.58%	2.442%
9	9.639	1124	1131	1144	rBV	804042	1348920	18.32%	2.073%
10	10.169	1213	1221	1236	rBV	1306125	2149571	29.19%	3.303%
11	10.545	1278	1285	1293	rBV	935661	1545613	20.99%	2.375%
12	10.692	1303	1310	1326	rBV	1214809	2160323	29.33%	3.319%
13	12.145	1551	1557	1564	rBV2	19688	34114	0.46%	0.052%
14	13.816	1834	1841	1855	rBV	2644073	3631184	49.30%	5.579%
15	14.092	1882	1888	1902	rBV	2939358	4305677	58.46%	6.616%
16	14.404	1933	1941	1952	rBV2	1549804	2350745	31.92%	3.612%
17	14.615	1969	1977	1992	rBV	805152	1435328	19.49%	2.205%
18	15.198	2072	2076	2080	rVB	13132	16894	0.23%	0.026%
19	15.398	2103	2110	2124	rVB	4076299	5582326	75.80%	8.577%
20	15.521	2125	2131	2144	rVV	911842	1343101	18.24%	2.064%
21	15.639	2146	2151	2156	rVB	42533	60806	0.83%	0.093%
22	16.180	2238	2243	2249	rBV6	7462	10552	0.14%	0.016%
23	16.939	2369	2372	2376	rBV3	8253	12427	0.17%	0.019%
24	17.151	2401	2408	2418	rVB2	2193553	3058549	41.53%	4.699%
25	17.251	2418	2425	2438	rBV	4382518	6112563	83.00%	9.392%
26	19.180	2749	2753	2759	rVB	51305	65105	0.88%	0.100%
27	19.433	2792	2796	2799	rBV	36175	45118	0.61%	0.069%
28	19.545	2809	2815	2824	rBV	5687426	7364806	100.00%	11.316%
29	21.121	3080	3083	3087	rBV	53139	66969	0.91%	0.103%
30	21.333	3114	3119	3128	rBV	2512705	3312027	44.97%	5.089%
31	23.462	3474	3481	3497	rVB	3908413	7100531	96.41%	10.910%
32	23.603	3499	3505	3519	rVB	1640621	3191612	43.34%	4.904%

LSC Area Percent Report

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
Data File : BM021234.D
Acq On : 28 Jun 2019 16:52
Operator : HP/JU
Sample : PB120790BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK90

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 65082666

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM062819\
Data File : BM021234.D
Acq On : 28 Jun 2019 16:52
Operator : HP/JU
Sample : PB120790BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

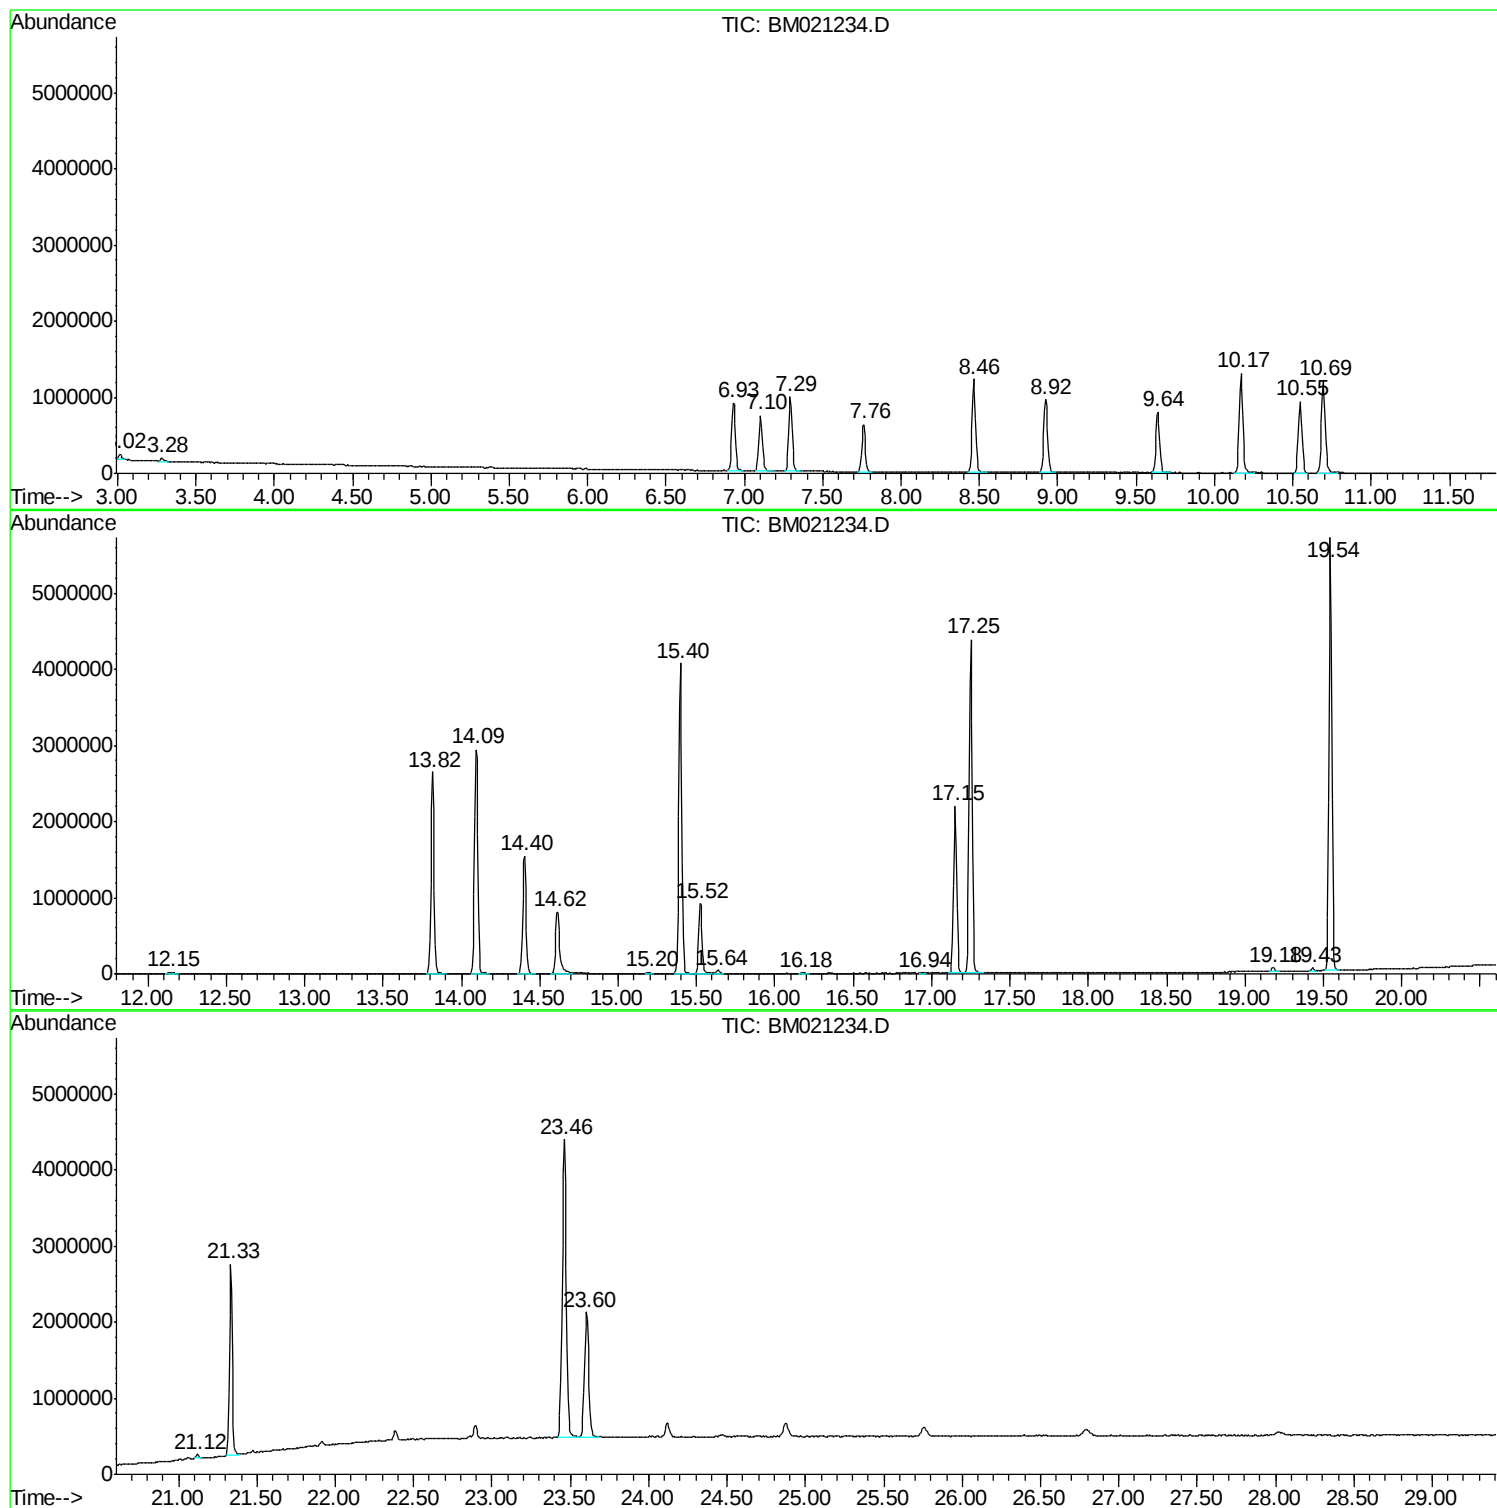

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062819\
Data File : BM021234.D
Acq On : 28 Jun 2019 16:52
Operator : HP/JU
Sample : PB120790BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM062819\
Data File : BM021234.D
Acq On : 28 Jun 2019 16:52
Operator : HP/JU
Sample : PB120790BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK90

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM061419MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc